


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN111219\  
Data File : VN059175.D  
Acq On : 12 Nov 2019 8:18  
Operator : JC/SP  
Sample : BFB  
Misc : 5.00mL/MSVOA N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N110619W.M  
Title : SW846 8260  
Last Update : Thu Nov 07 04:00:41 2019

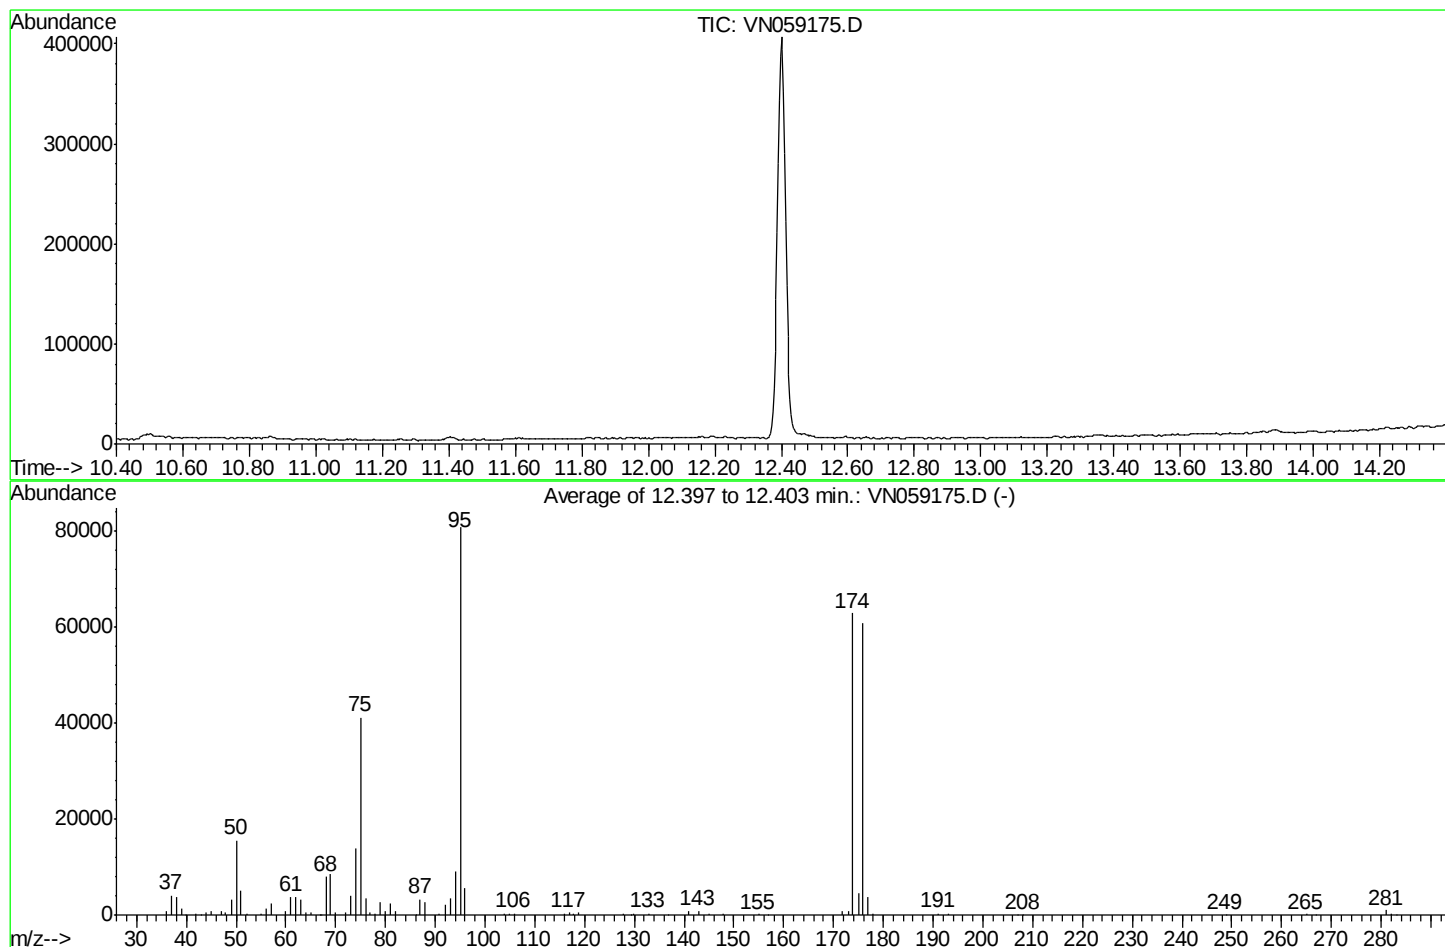

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.2      | 15517   | PASS             |
| 75          | 95           | 30           | 60           | 50.9      | 41106   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 80776   | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 5477    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.2       | 735     | PASS             |
| 174         | 95           | 50           | 100          | 77.9      | 62914   | PASS             |
| 175         | 174          | 5            | 9            | 7.2       | 4504    | PASS             |
| 176         | 174          | 95           | 101          | 96.8      | 60928   | PASS             |
| 177         | 176          | 5            | 9            | 6.3       | 3820    | PASS             |