


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN111220\  
 Data File : VN064597.D  
 Acq On : 12 Nov 2020 21:41  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 28 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N110420W.M  
 Title : SW846 8260  
 Last Update : Wed Nov 04 12:09:03 2020

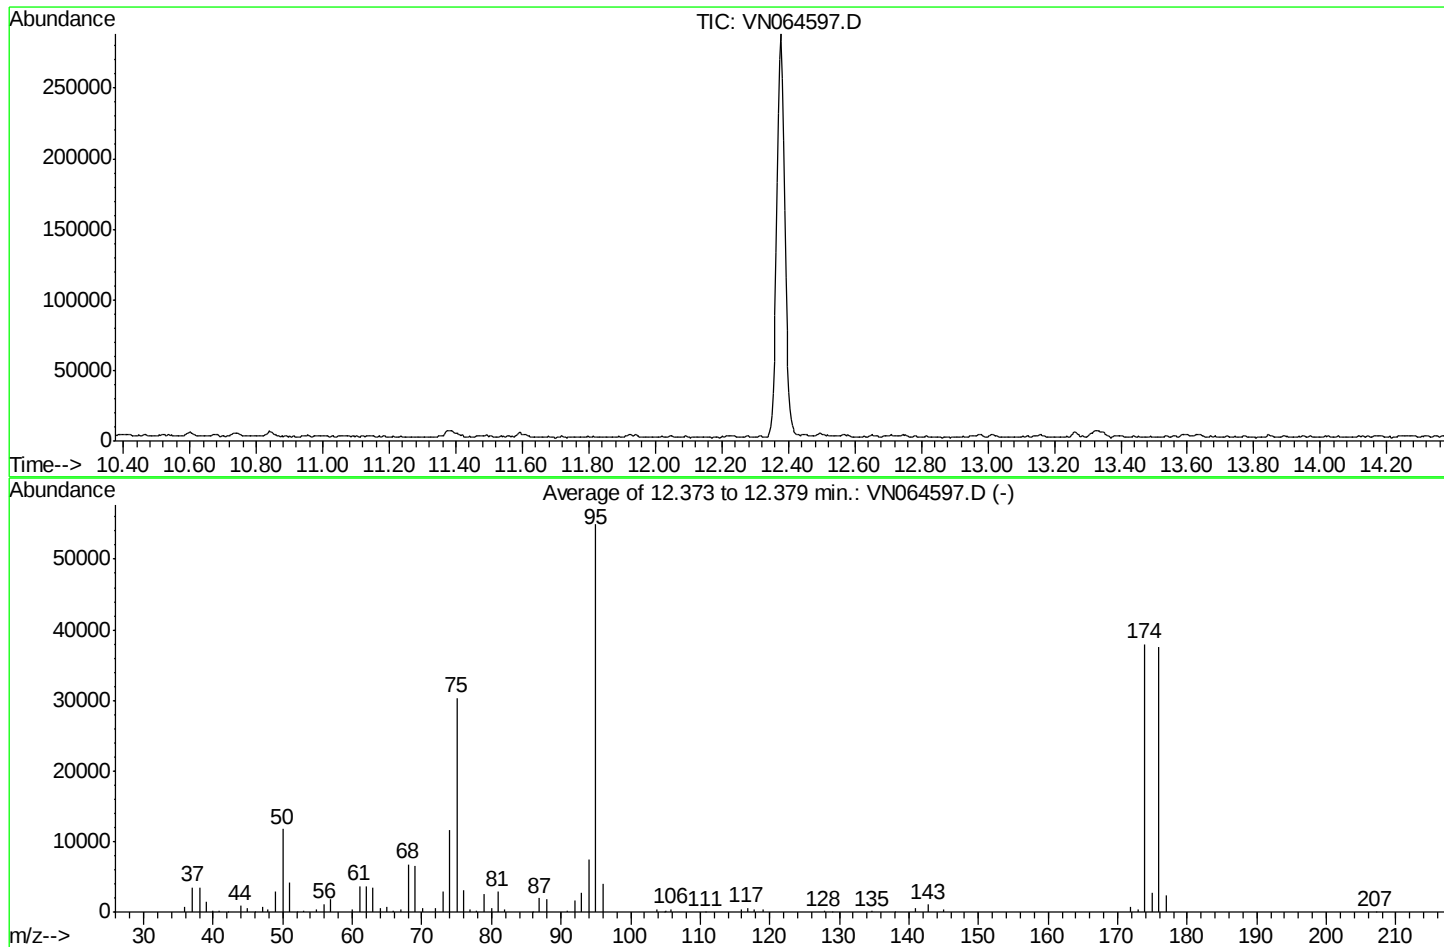

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 21.3      | 11727   | PASS             |
| 75          | 95           | 30           | 60           | 55.1      | 30306   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 54954   | PASS             |
| 96          | 95           | 5            | 9            | 7.2       | 3956    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.8       | 297     | PASS             |
| 174         | 95           | 50           | 100          | 69.0      | 37925   | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 2799    | PASS             |
| 176         | 174          | 95           | 101          | 99.1      | 37597   | PASS             |
| 177         | 176          | 5            | 9            | 6.1       | 2285    | PASS             |