
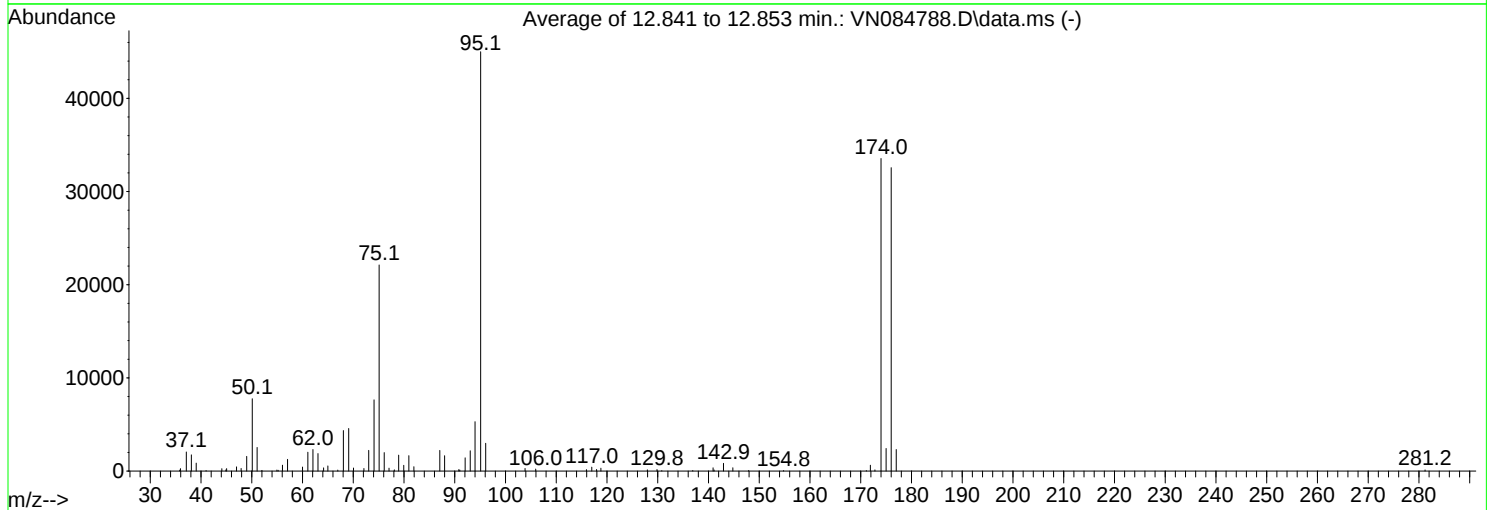


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111224\
Data File : VN084788.D
Acq On : 12 Nov 2024 10:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

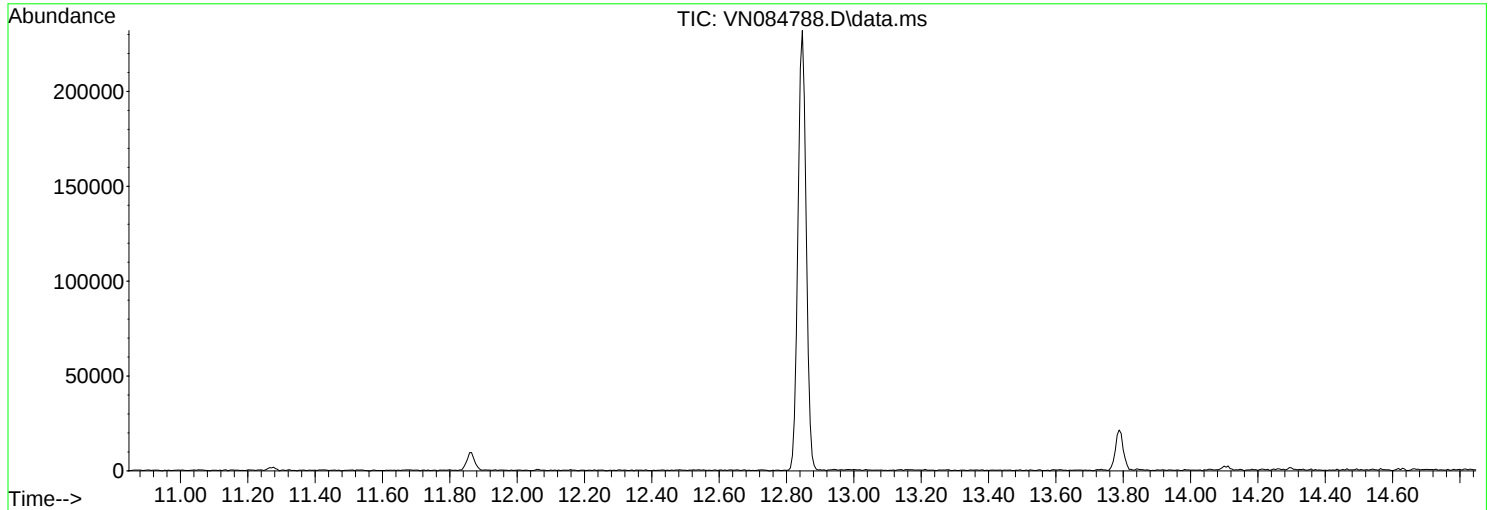

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	7763	PASS
75	95	30	60	49.2	22120	PASS
95	95	100	100	100.0	45005	PASS
96	95	5	9	6.6	2982	PASS
173	174	0.00	2	0.4	130	PASS
174	95	50	100	74.5	33547	PASS
175	174	5	9	7.2	2426	PASS
176	174	95	101	97.1	32563	PASS
177	176	5	9	7.1	2315	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	101	49.00	1579	63.05	1883	76.10	1983
35.95	263	50.10	7763	64.15	345	77.05	312
37.10	2053	51.05	2536	65.00	551	78.10	135
38.10	1741	52.00	72	66.95	111	78.95	1712
39.05	857	54.95	117	68.05	4346	79.95	617
41.00	57	55.20	86	69.10	4573	80.95	1657
44.10	261	56.05	637	70.05	328	81.95	470
44.90	127	57.05	1257	72.10	279	87.05	2214
45.05	263	60.00	434	73.05	2220	88.00	1650
47.00	454	61.05	2027	74.10	7646	90.80	159
47.90	282	62.05	2314	75.10	22120	91.00	114

Average of 12.841 to 12.853 min.: VN084788.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.05	1425	127.95	137	171.90	630		
93.05	2181	129.85	168	172.80	130		
94.00	5300	130.80	51	174.00	33547		
95.10	45005	136.90	62	175.00	2426		
96.10	2982	140.90	349	176.00	32563		
103.85	286	141.10	125	177.00	2315		
105.95	215	142.95	833	281.20	122		
115.95	156	144.80	357				
117.00	425	147.90	54				
117.95	170	154.80	50				
118.80	308	171.10	55				