
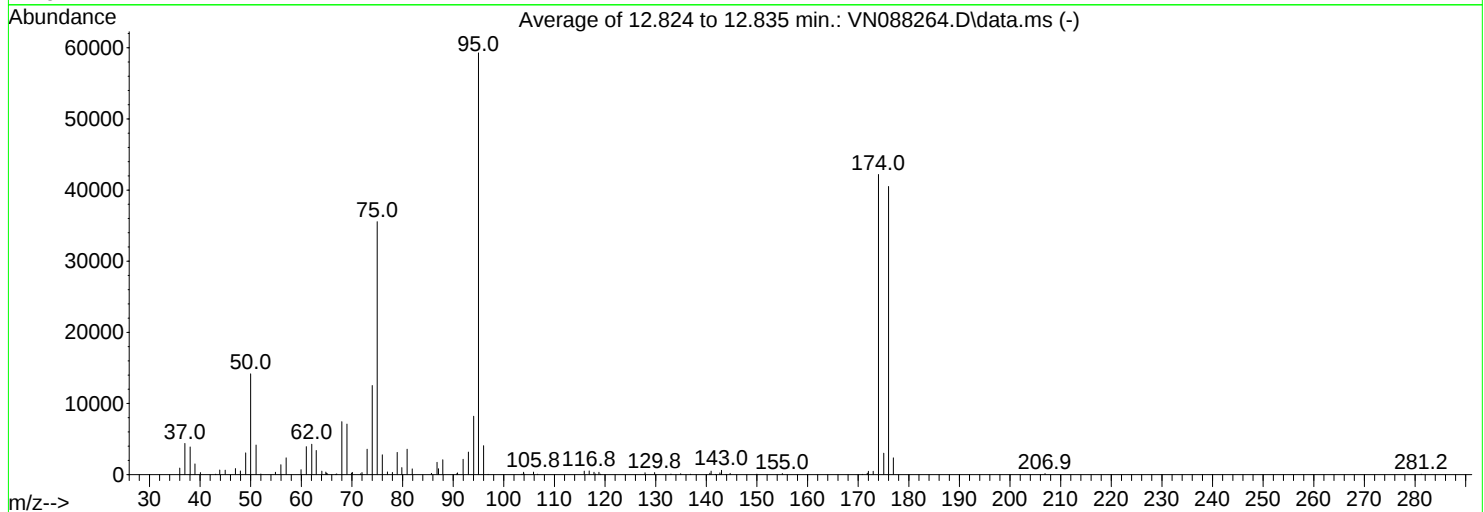


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111225\
Data File : VN088264.D
Acq On : 12 Nov 2025 09:26
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Title : SW846 8260
Last Update : Mon Nov 03 01:16:06 2025

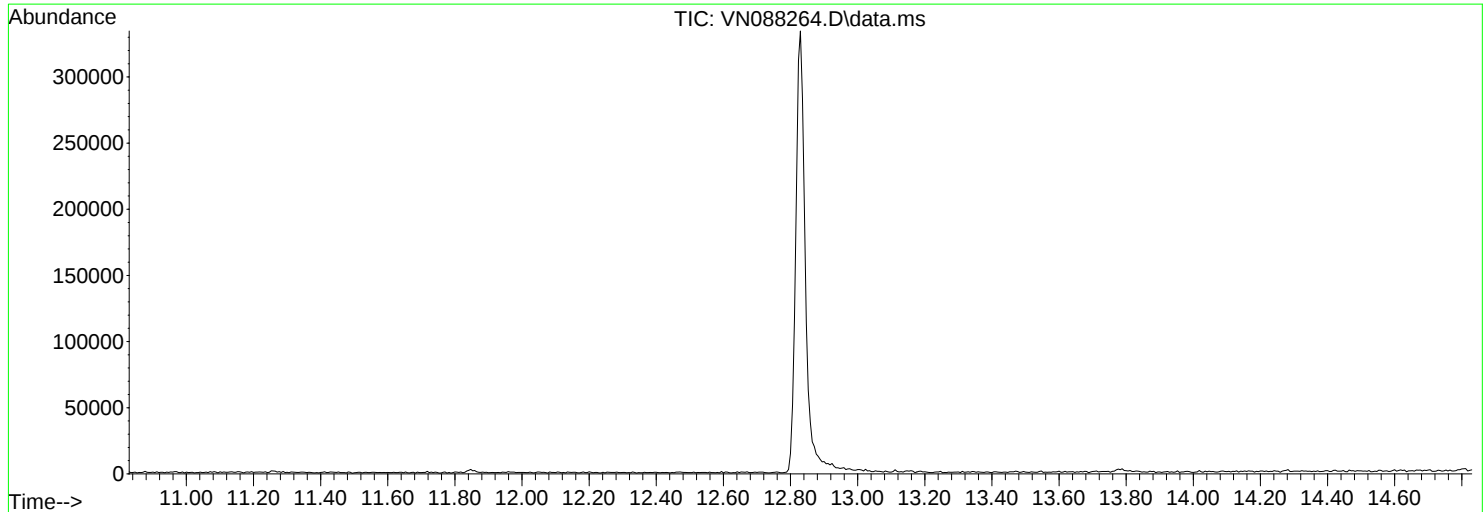

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.9	14161	PASS
75	95	30	60	60.0	35552	PASS
95	95	100	100	100.0	59291	PASS
96	95	5	9	6.9	4070	PASS
173	174	0.00	2	1.1	465	PASS
174	95	50	100	71.2	42192	PASS
175	174	5	9	7.1	3009	PASS
176	174	95	101	96.0	40499	PASS
177	176	5	9	5.8	2358	PASS

Average of 12.824 to 12.835 min.: VN088264.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	933	50.00	14161	64.85	354	73.00	356
37.00	4385	51.05	4166	65.00	213	74.00	1252
38.05	3900	52.00	92	65.20	124	75.00	3555
39.00	1502	54.90	338	66.80	53	76.00	278
40.05	291	55.95	1395	67.00	109	77.00	381
43.10	59	57.00	2352	68.00	7436	78.00	312
43.90	644	59.95	702	69.00	7099	78.95	3135
44.95	638	61.00	3942	69.90	216	79.85	986
47.00	847	62.05	4267	70.10	317	80.90	3572
47.95	522	62.95	3403	71.70	104	81.90	812
49.00	3053	64.05	497	72.00	298	85.70	183

Average of 12.824 to 12.835 min.: VN088264.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.80	1735	103.60	63	127.90	261	144.70	191
87.10	836	103.90	340	129.80	285	150.00	76
87.95	2101	104.10	78	133.00	83	155.00	156
90.70	102	105.85	365	134.95	142	170.80	53
90.85	247	106.70	72	136.90	63	171.80	206
91.95	2165	115.90	502	140.70	215	172.00	468
93.00	3181	116.85	514	140.95	487	172.95	465
94.05	8209	117.80	334	141.80	50	174.00	42192
95.00	59291	118.10	97	142.70	248	175.05	3009
96.00	4070	118.80	335	143.00	618	176.00	40499
96.90	52	119.10	71	143.90	52	176.95	2358

Average of 12.824 to 12.835 min.: VN088264.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
206.90	156						
281.20	78						