


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN111318\
 Data File : VN052276.D
 Acq On : 13 Nov 2018 10:02
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110918W.M
 Title : SW846 8260
 Last Update : Mon Nov 12 00:34:27 2018

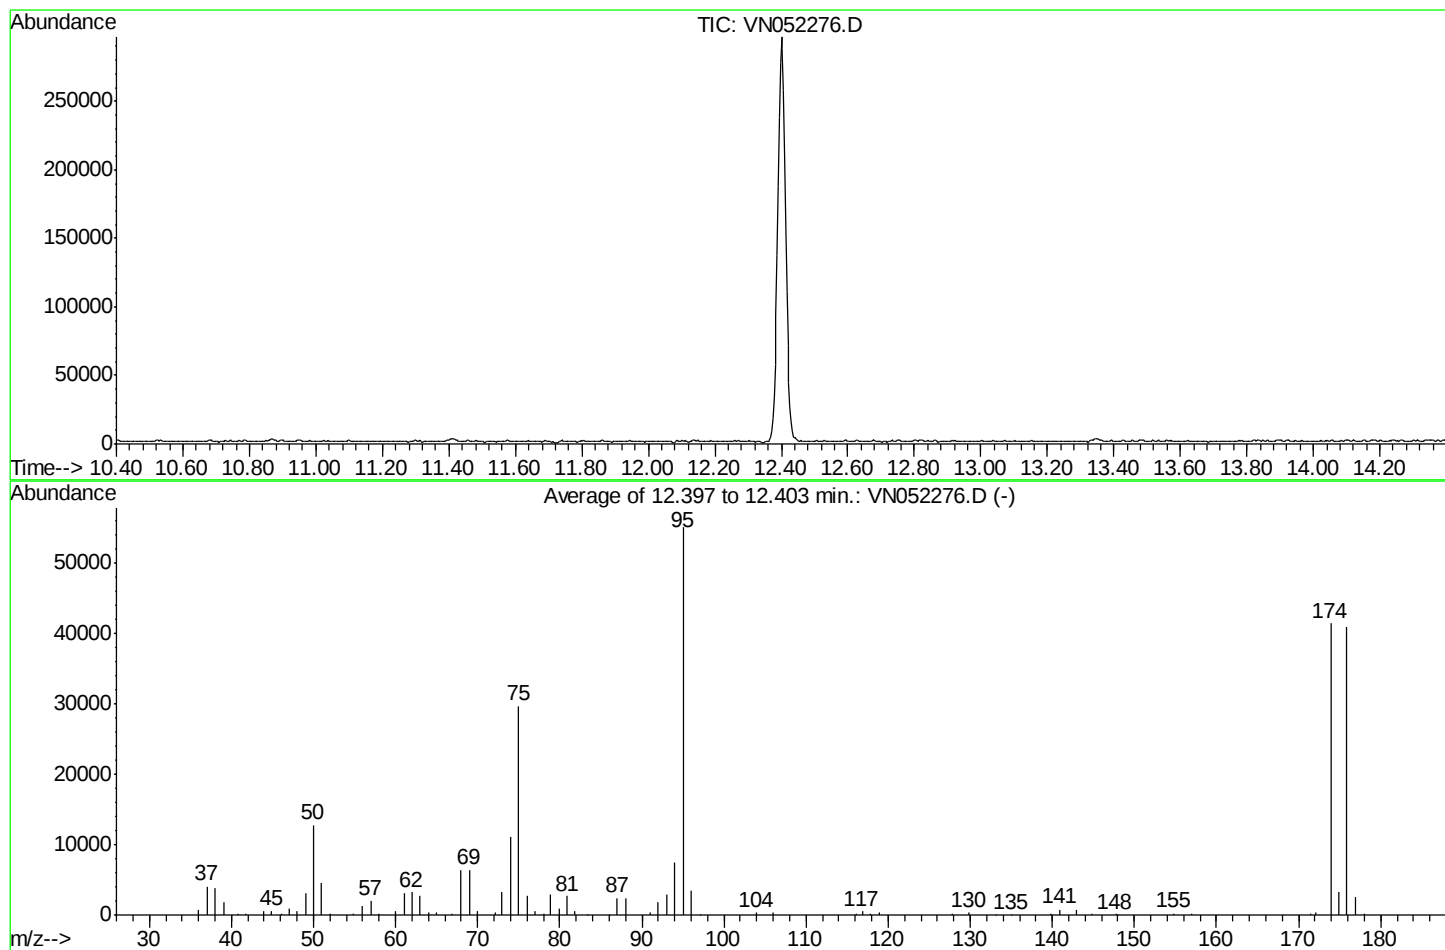

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	12760	PASS
75	95	30	60	53.9	29666	PASS
95	95	100	100	100.0	55077	PASS
96	95	5	9	6.3	3491	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.3	41458	PASS
175	174	5	9	7.9	3266	PASS
176	174	95	101	98.6	40885	PASS
177	176	5	9	6.4	2612	PASS