

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN111319\
 Data File : VN059215.D
 Acq On : 13 Nov 2019 17:27
 Operator : JC/SP
 Sample : K5814-08
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 30662

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.114	405	417	435	rVB4	12266	31255	1.59%	0.239%
2	3.799	610	630	643	rBV	15114	41986	2.14%	0.321%
3	4.043	687	706	734	rBV				

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN111319\
Data File : VN059215.D
Acq On : 13 Nov 2019 17:27
Operator : JC/SP
Sample : K5814-08
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
30662

Integration Parameters: RTEINT.P
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Title : SW846 8260


Sum of corrected areas: 13098504

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN111319\
Data File : VN059215.D
Acq On : 13 Nov 2019 17:27
Operator : JC/SP
Sample : K5814-08
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
30662

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

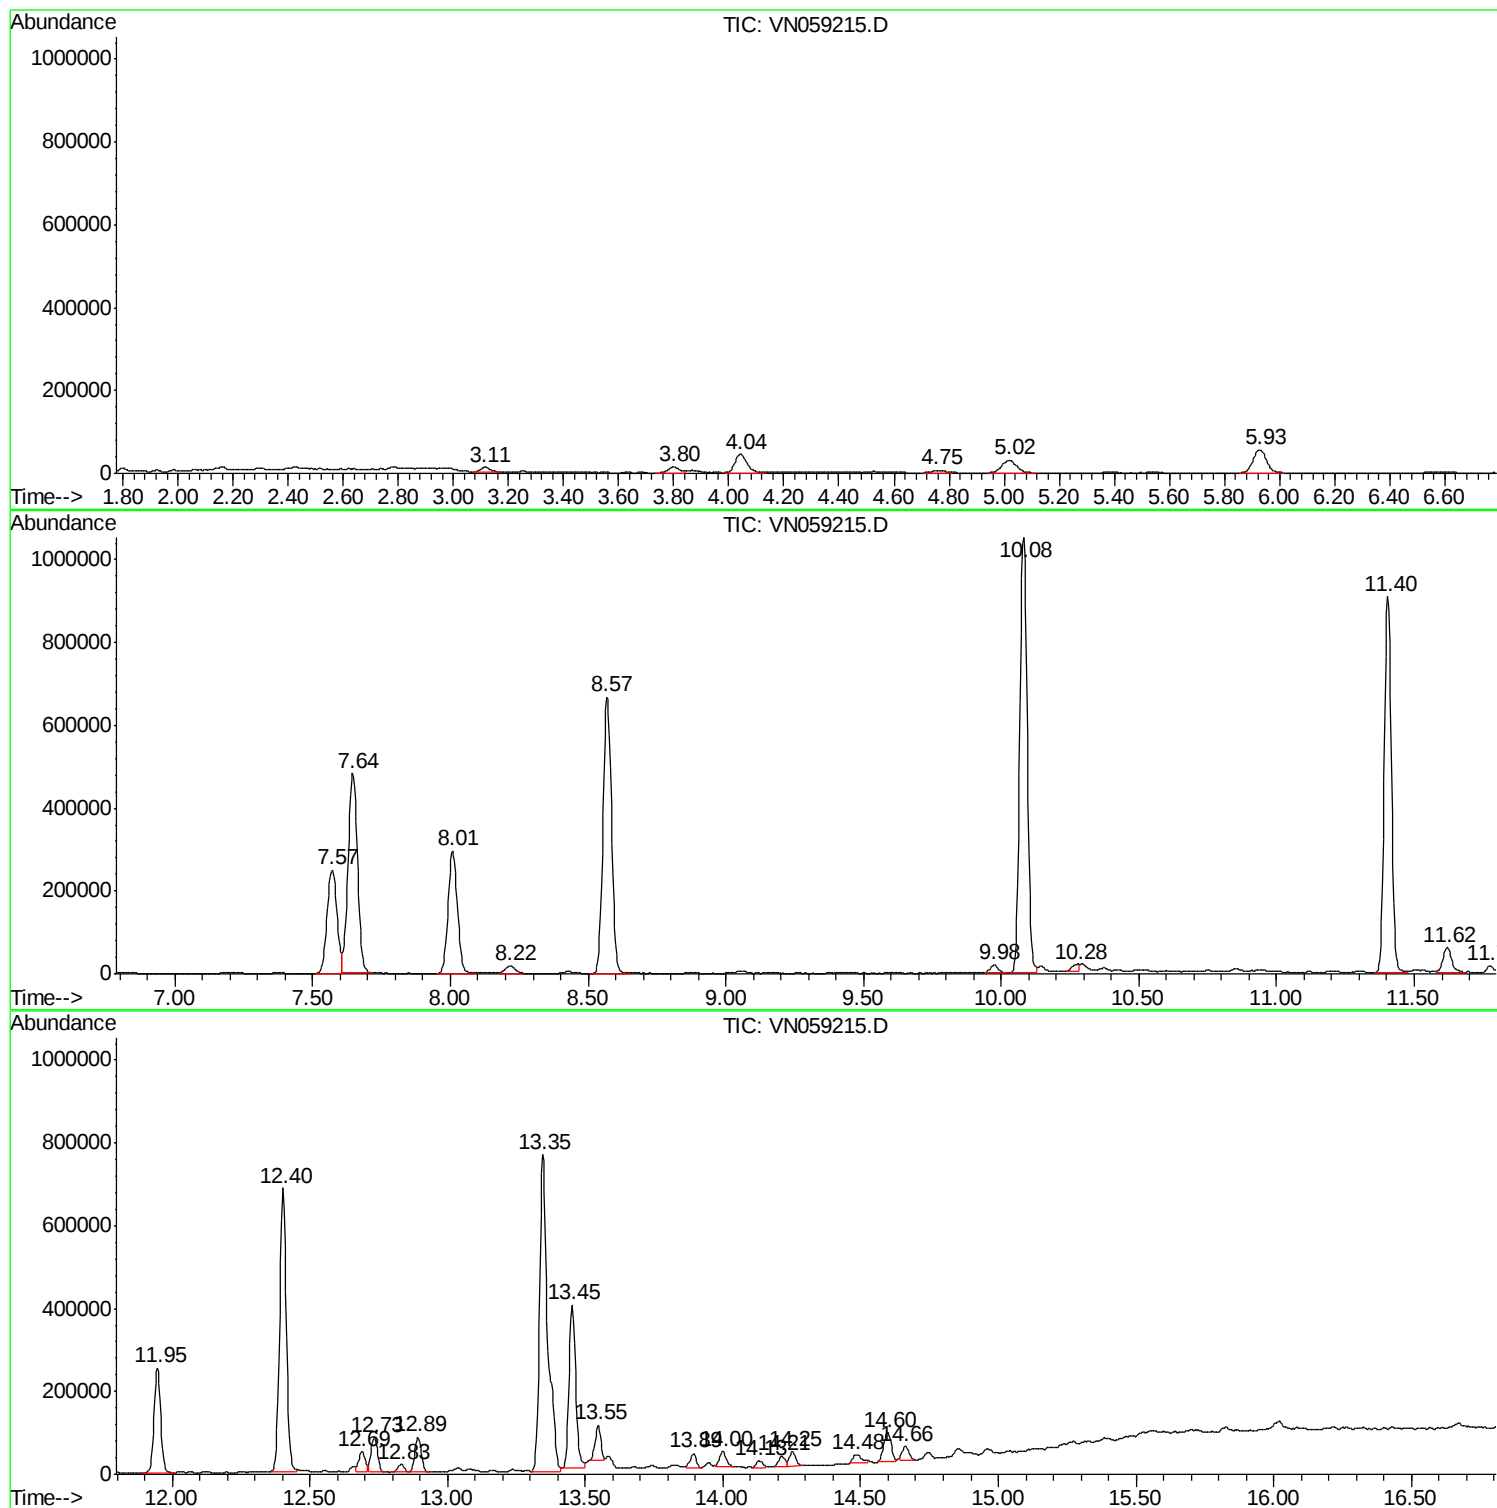

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN111319\
Data File : VN059215.D
Acq On : 13 Nov 2019 17:27
Operator : JC/SP
Sample : K5814-08
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampled :
30662

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.04	5.94 ug/l	136254	Pentafluorobenzene	7.64

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
2			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	43
3			Formic acid, 1-methylethyl ester	88	C4H8O2	000625-55-8	40
4			2-Pentanol	88	C5H12O	006032-29-7	9
5			Hydrazine, propyl-	74	C3H10N2	005039-61-2	9

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN111319\
Data File : VN059215.D
Acq On : 13 Nov 2019 17:27
Operator : JC/SP
Sample : K5814-08
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 12 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
30662

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 1-Hexanol, 2-ethyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.45	21.03 ug/l	666987	1,4-Dichlorobenzene-d4	13.35
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	1-Hexanol, 2-ethyl-	130 C8H18O	000104-76-7	74
2	2-Ethylhexyl hydrogen maleate	228 C12H20O4	002370-71-0	59
3	2-Ethyl-1-hexanol, pentafluoropr...	276 C11H17F5O2	1000365-51-1	47
4	2-Propyl-1-pentanol	130 C8H18O	058175-57-8	47
5	Heptane, 1,1'-oxybis-	214 C14H30O	000629-64-1	42

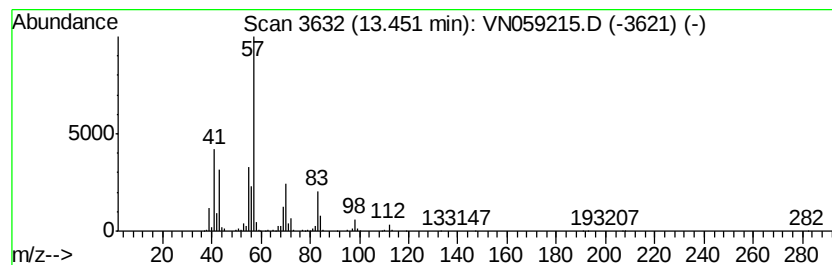

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN111319\
Data File : VN059215.D
Acq On : 13 Nov 2019 17:27
Operator : JC/SP
Sample : K5814-08
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
30662

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	4.04	5.9	ug/l	136254	1	7.64	1146820	50.0
1-Hexanol, 2-ethyl-	13.45	21.0	ug/l	666987	4	13.35	1585810	50.0