

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN111320\
 Data File : VN064644.D
 Acq On : 13 Nov 2020 20:46
 Operator : JC/MD
 Sample : L4719-08
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-3-D


Quant Time: Nov 17 02:00:15 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 04 12:09:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	216398	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	465061	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	516329	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	178722	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	221674	58.81	ug/l	0.00
Spiked Amount			Recovery	=	117.62%	
35) Dibromofluoromethane	7.55	113	161365	50.96	ug/l	0.00
Spiked Amount			Recovery	=	101.92%	
50) Toluene-d8	10.06	98	618815	50.56	ug/l	0.00
Spiked Amount			Recovery	=	101.12%	
62) 4-Bromofluorobenzene	12.38	95	232047	50.14	ug/l	0.00
Spiked Amount			Recovery	=	100.28%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.75	59	577	1.388	ug/l #	71
16) Acetone	3.78	43	13206	9.198	ug/l	99
18) Methyl Acetate	4.28	43	4124	1.461	ug/l #	78
20) Methylene Chloride	4.51	84	12508	4.391	ug/l	98
25) 2-Butanone	6.80	43	2966	1.621	ug/l #	79
29) Tetrahydrofuran	7.18	42	983	0.876	ug/l #	54
31) Cyclohexane	7.63	56	6381	1.393	ug/l #	26
36) 1,1-Dichloropropene	7.63	75	21582	4.393	ug/l #	48
37) Ethyl Acetate	6.88	43	202	0.802	ug/l #	71
38) Carbon Tetrachloride	7.62	117	25644	4.884	ug/l #	18
43) Isopropyl Acetate	8.13	43	83846	10.531	ug/l	99
45) 1,2-Dichloropropane	9.24	63	2008	0.521	ug/l #	45
48) Methyl methacrylate	9.14	41	5669	1.411	ug/l #	15
49) 1,4-Dioxane	9.22	88	31	0.586	ug/l #	21
51) 4-Methyl-2-Pentanone	9.95	43	7559	1.628	ug/l	98
54) cis-1,3-Dichloropropene	9.87	75	32537	5.264	ug/l #	72
56) Ethyl methacrylate	10.28	69	129	1.863	ug/l #	20
57) 1,3-Dichloropropane	10.74	76	6192	1.033	ug/l #	42
59) 2-Hexanone	10.74	43	101272	30.344	ug/l #	56
71) Bromoform	12.36	173	198	1.336	ug/l #	1
74) N-amyl acetate	12.00	43	3100	1.653	ug/l #	49
76) 1,2,3-Trichloropropane	12.38	75	129414	29.886	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.38	75	129414	83.445	ug/l #	8
95) Naphthalene	15.11	128	122	3.634	ug/l #	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

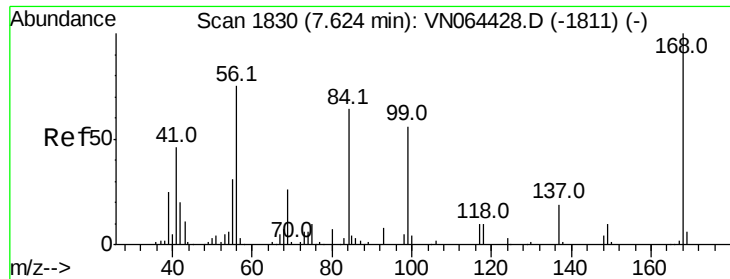

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampled :


TP-3-D

Tot Ion:168 Resp: 216398

Ion Ratio Lower Upper




168 100

99 71.4 53.4 80.2

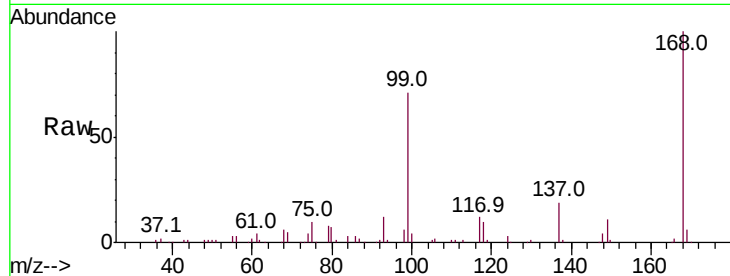

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

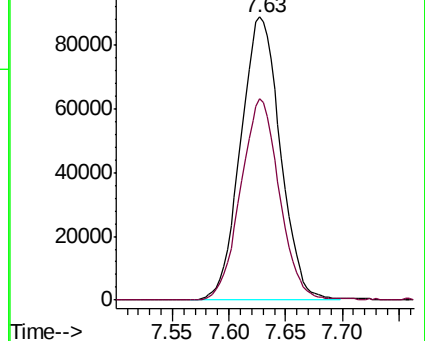

#11

Tert butyl alcohol

Concen: 1.388 ug/l

RT: 4.75 min Scan# 937

Delta R.T. 0.01 min

Lab File: VN064644.D


Acq: 13 Nov 2020 20:46

Tgt Ion: 59 Resp: 577

Ion Ratio Lower Upper



59 100


57 0.0 9.0 13.4#



Abundance Ion 59.00 (58.70 to 59.70): VN0

Ion 57.00 (56.70 to 57.70): VN0

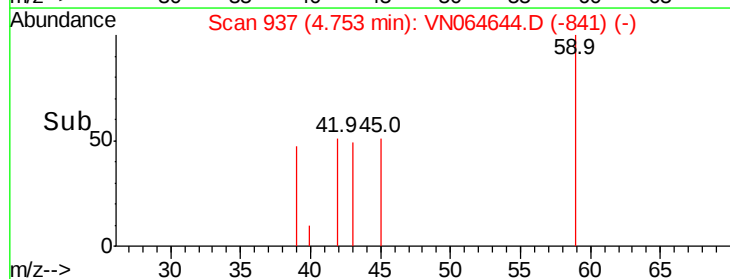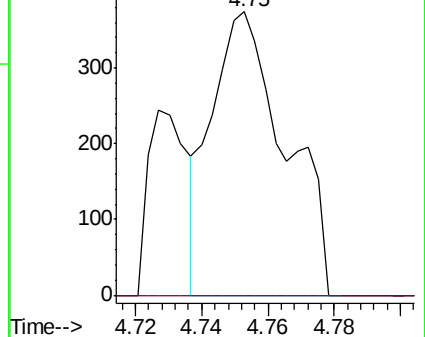

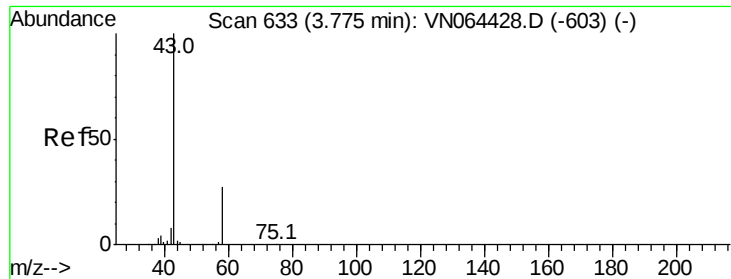

#16

Acetone

Concen: 9.198 ug/l

RT: 3.78 min Scan# 634

Delta R.T. 0.00 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampled :





TP-3-D

Tot Ion: 43 Resp: 13206

Ion Ratio Lower Upper

43 100

58 26.2 21.4 32.0

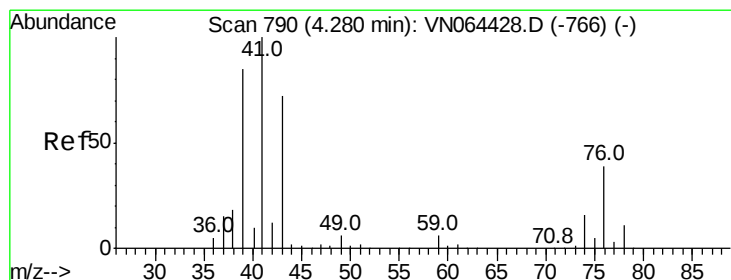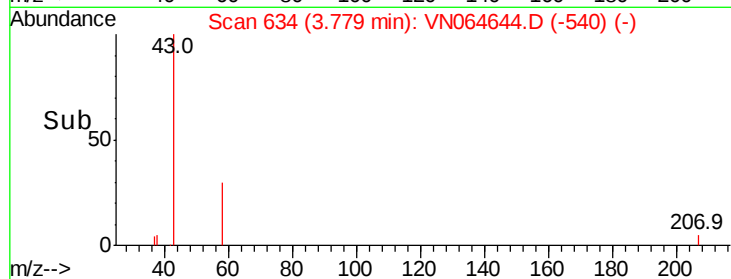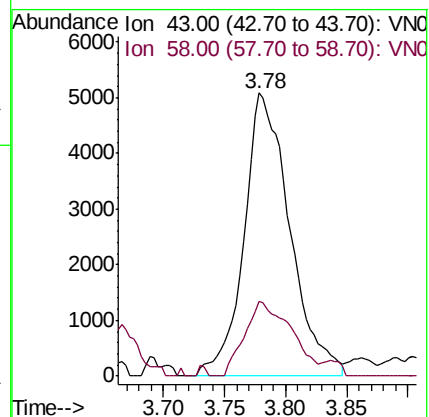

#18

Methyl Acetate

Concen: 1.461 ug/l

RT: 4.28 min Scan# 791

Delta R.T. 0.00 min

Lab File: VN064644.D




Acq: 13 Nov 2020 20:46


Tgt Ion: 43 Resp: 4124

Ion Ratio Lower Upper

43 100

74 10.8 17.0 25.4#

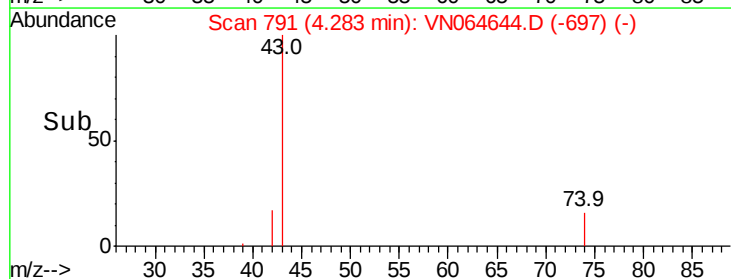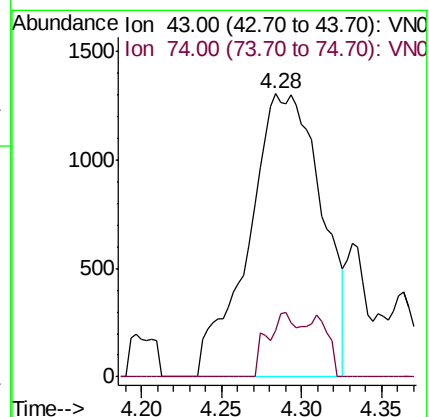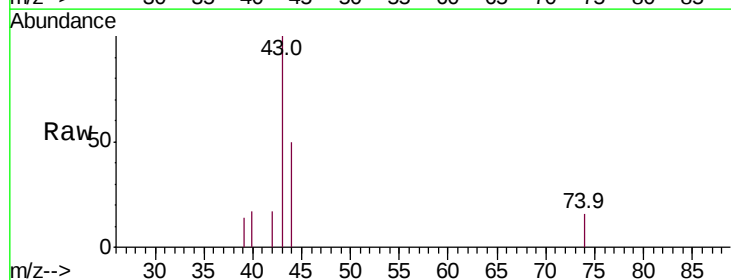

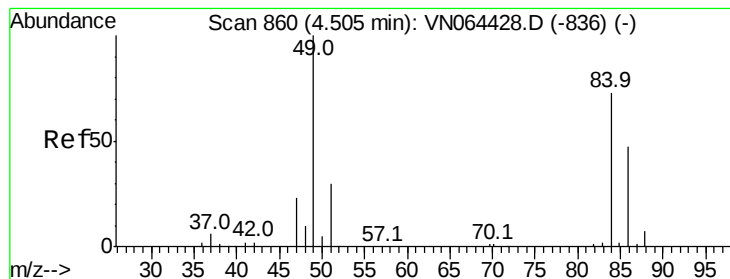

#20

Methvlene Chloride

Concen: 4.391 ug/l

RT: 4.51 min Scan# 860

Delta R.T. -0.00 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampled :

TP-3-D

Tot Ion: 84 Resp: 12508


Ion Ratio Lower Upper

84 100

49 138.3 110.1 165.1

51 47.9 33.6 50.4

86 63.5 52.1 78.1






Abundance Ion 83.90 (83.60 to 84.60): VN0

Ion 48.90 (48.60 to 49.60): VN0

Ion 50.90 (50.60 to 51.60): VN0

Ion 85.90 (85.60 to 86.60): VN0

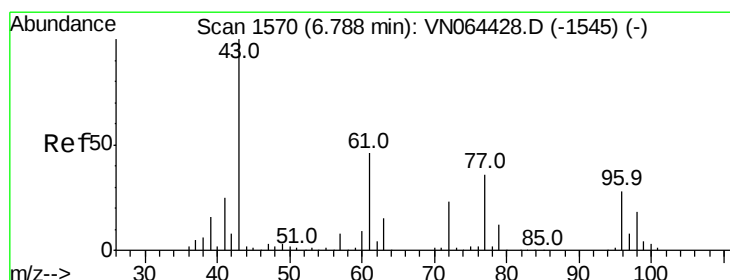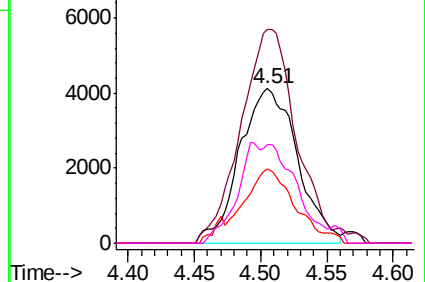

#25

2-Butanone

Concen: 1.621 ug/l

RT: 6.80 min Scan# 1573

Delta R.T. 0.01 min

Lab File: VN064644.D


Acq: 13 Nov 2020 20:46

Tgt Ion: 43 Resp: 2966

Ion Ratio Lower Upper



43 100


72 12.8 18.5 27.7#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 72.00 (71.70 to 72.70): VN0

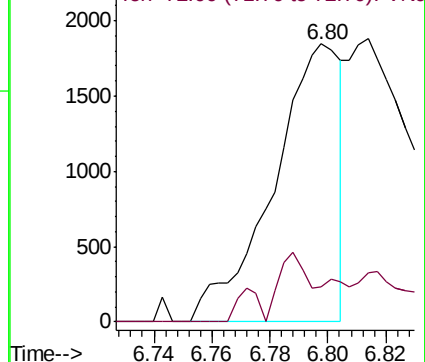



#29

Tetrahydrofuran

Concen: 0.876 ug/l

RT: 7.18 min Scan# 1691

Delta R.T. 0.01 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampleId :

TP-3-D


Tot Ion: 42 Resp: 983

Ion Ratio Lower Upper

42 100

72 10.4 31.7 47.5#




71 10.8 29.8 44.6#

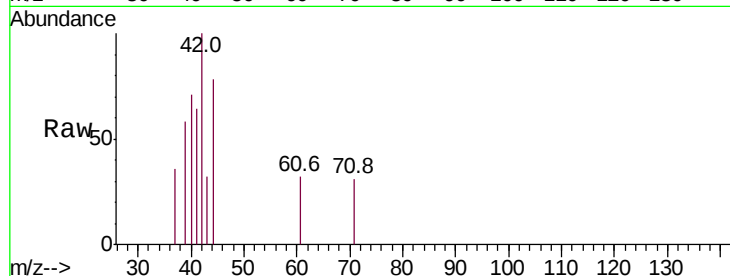

Abundance Ion 42.00 (41.70 to 42.70): VNC

Ion 72.00 (71.70 to 72.70): VNC

Ion 71.00 (70.70 to 71.70): VNC

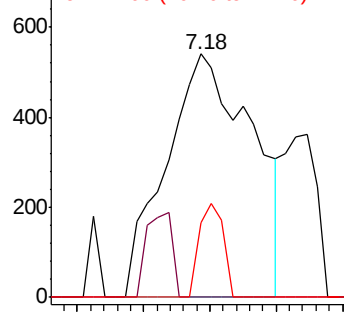

#31

Cyclohexane

Concen: 1.393 ug/l

RT: 7.63 min Scan# 1832

Delta R.T. 0.02 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46


Tgt Ion: 56 Resp: 6381

Ion Ratio Lower Upper

56 100

69 158.3 25.6 38.4#



84 89.6 63.0 94.6




Abundance Ion 56.00 (55.70 to 56.70): VNC

Ion 69.00 (68.70 to 69.70): VNC

Ion 84.00 (83.70 to 84.70): VNC




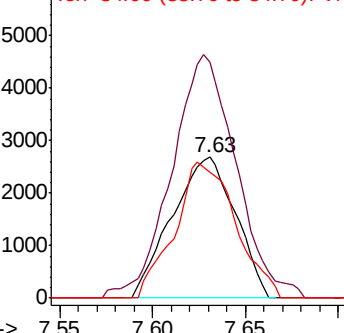


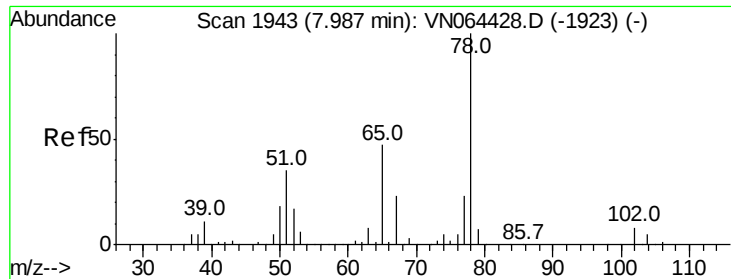

#33
 1,2-Dichloroethane-d4
 Concen: 58.810 ug/l
 RT: 7.99 min Scan# 1944
 Delta R.T. 0.00 min
 Lab File: VN064644.D
 Acq: 13 Nov 2020 20:46




Instrument :
 MSVOA_N
 ClientSampleId :
 TP-3-D


Tot Ion: 65 Resp: 221674
 Ion Ratio Lower Upper
 65 100
 67 50.3 0.0 101.6

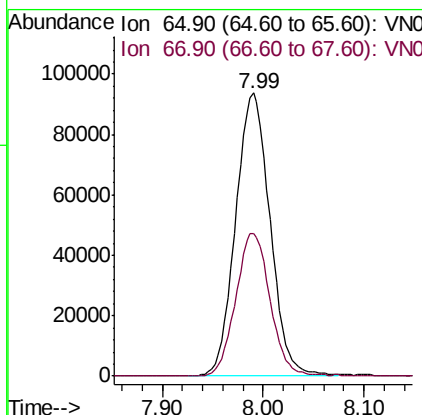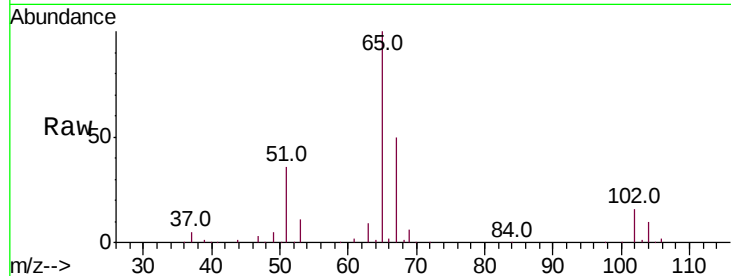

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. -0.00 min
 Lab File: VN064644.D
 Acq: 13 Nov 2020 20:46

Tgt Ion: 114 Resp: 465061
 Ion Ratio Lower Upper
 114 100
 63 23.0 0.0 45.6
 88 16.6 0.0 32.8


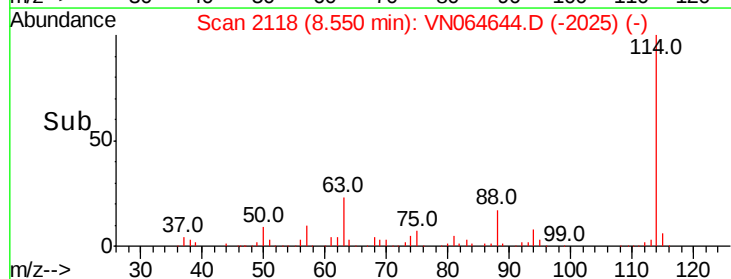
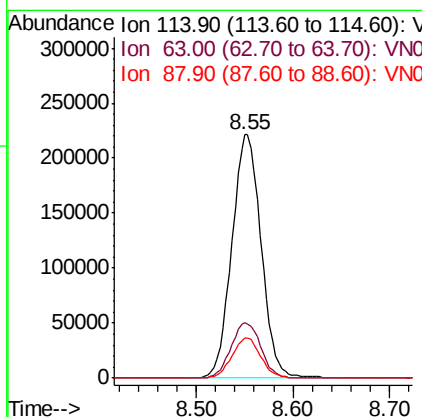





#35
Dibromofluoromethane
Concen: 50.961 ug/l
RT: 7.55 min Scan# 1808
Delta R.T. 0.01 min
Lab File: VN064644.D
Acq: 13 Nov 2020 20:46




Instrument :
MSVOA_N
ClientSampled :
TP-3-D


Tot Ion:113 Resp: 161365
Ion Ratio Lower Upper
113 100
111 103.7 81.1 121.7
192 16.2 12.8 19.2

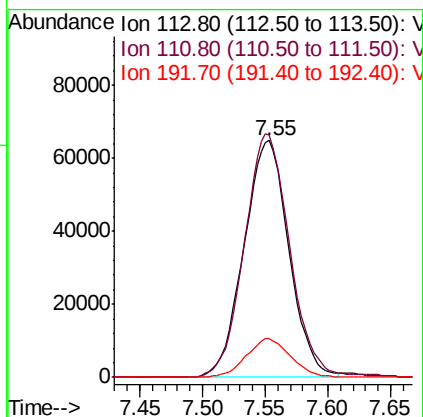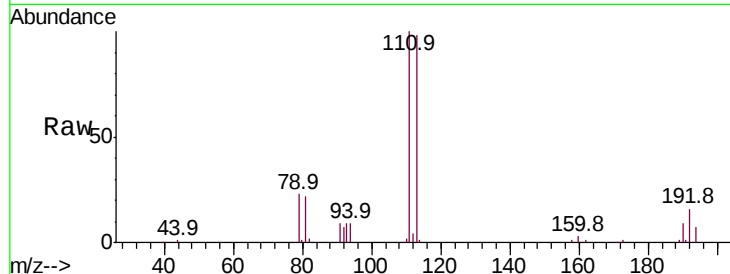

#36
1,1-Dichloropropene
Concen: 4.393 ug/l
RT: 7.63 min Scan# 1832
Delta R.T. -0.12 min
Lab File: VN064644.D
Acq: 13 Nov 2020 20:46

Tgt Ion: 75 Resp: 21582
Ion Ratio Lower Upper
75 100
110 5.3 16.0 48.0#
77 0.0 24.0 36.0#

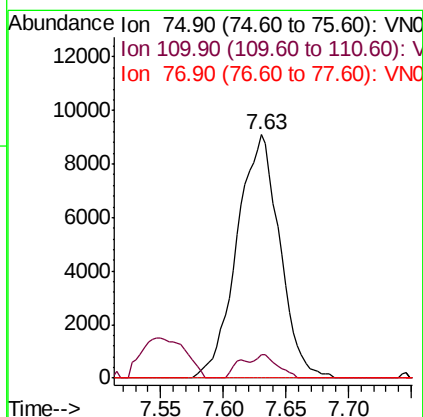



#37

Ethyl Acetate

Concen: 0.802 ug/l

RT: 6.88 min Scan# 1600

Delta R.T. 0.00 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampleId :

TP-3-D


Tot Ion: 43 Resp: 202

Ion Ratio Lower Upper

43 100

61 0.0 10.0 15.0#

70 0.0 7.1 10.7#



Abundance Ion 43.00 (42.70 to 43.70): VN064428.D (-1587) (-)

Ion 60.90 (60.60 to 61.60): VN064428.D (-1587) (-)

Ion 70.00 (69.70 to 70.70): VN064428.D (-1587) (-)

6.88



400

200

0

6.86 6.87 6.88 6.89

Time-->



#38

Carbon Tetrachloride

Concen: 4.884 ug/l

RT: 7.62 min Scan# 1830

Delta R.T. -0.11 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46


Tgt Ion: 117 Resp: 25644

Ion Ratio Lower Upper

117 100

119 6.3 75.5 113.3#

121 0.0 24.4 36.6#



Abundance Ion 116.80 (116.50 to 117.50): VN064428.D (-1845) (-)

Ion 118.80 (118.50 to 119.50): VN064428.D (-1845) (-)

Ion 120.80 (120.50 to 121.50): VN064428.D (-1845) (-)

7.62

15000


10000


5000

0

7.55 7.60 7.65 7.70

Time-->





#43

Isopropyl Acetate

Concen: 10.531 ug/l

RT: 8.13 min Scan# 1987

Delta R.T. 0.00 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampleId :

TP-3-D


Tot Ion: 43 Resp: 83846

Ion Ratio Lower Upper




43 100

61 17.2 14.0 21.0

87 12.3 9.1 13.7

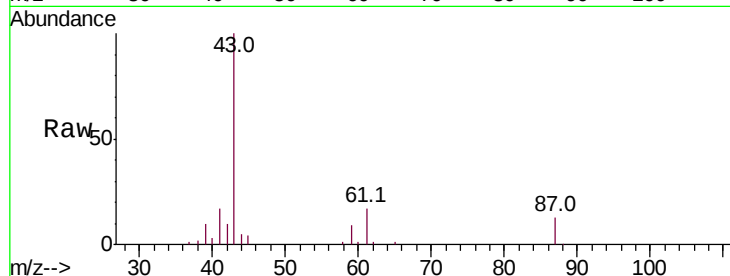

Abundance Ion 43.00 (42.70 to 43.70): VNO
Ion 61.00 (60.70 to 61.70): VNO
Ion 87.00 (86.70 to 87.70): VNO

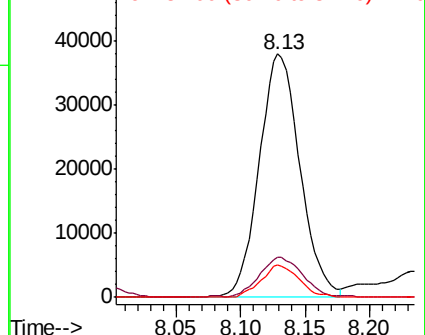

#45

1,2-Dichloropropane

Concen: 0.521 ug/l

RT: 9.24 min Scan# 2332

Delta R.T. 0.15 min

Lab File: VN064644.D


Acq: 13 Nov 2020 20:46

Tgt Ion: 63 Resp: 2008



Ion Ratio Lower Upper


63 100

65 0.0 23.6 35.4#



Abundance Ion 62.90 (62.60 to 63.60): VNO
Ion 64.90 (64.60 to 65.60): VNO

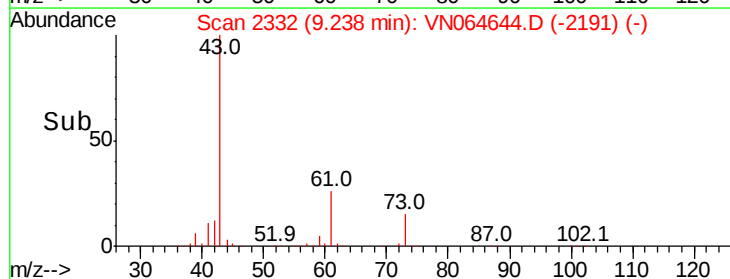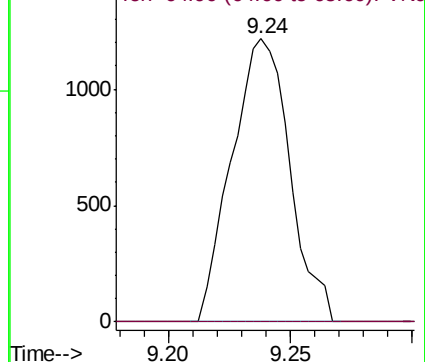


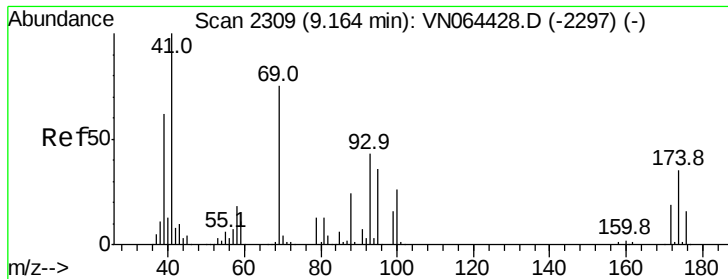




#48
Methvl methacrylate
Concen: 1.411 ug/l
RT: 9.14 min Scan# 2303
Delta R.T. -0.02 min
Lab File: VN064644.D
Acq: 13 Nov 2020 20:46

Instrument :
MSVOA_N
ClientSampled :
TP-3-D

Tot Ion: 41 Resp: 5669
Ion Ratio Lower Upper
41 100
69 0.0 60.4 90.6#
39 0.0 51.2 76.8#

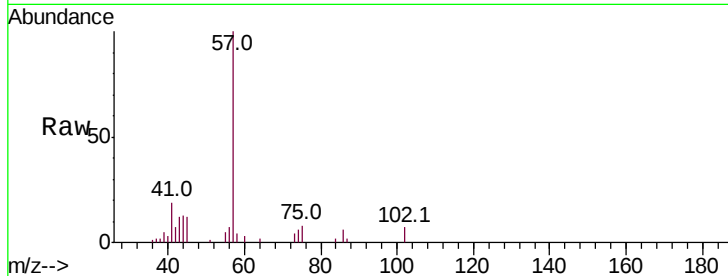


Abundance Ion 41.00 (40.70 to 41.70): VNC
Ion 69.00 (68.70 to 69.70): VNC
Ion 39.00 (38.70 to 39.70): VNC

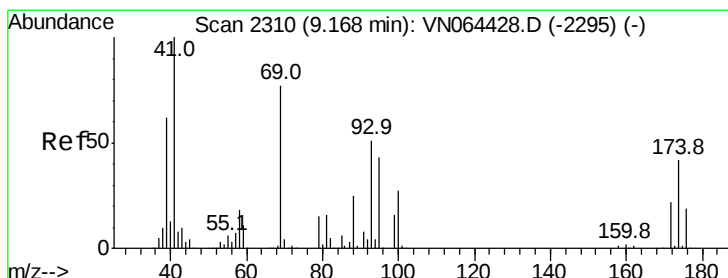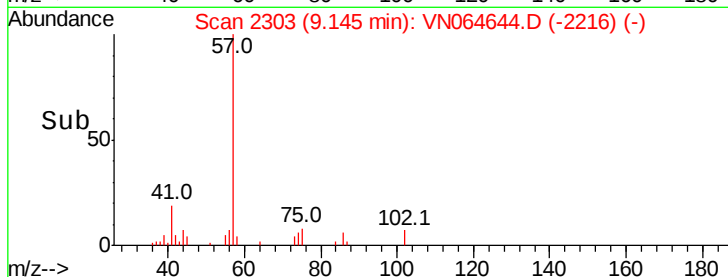
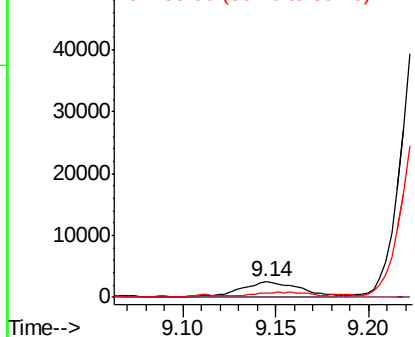



#49
1,4-Dioxane
Concen: 0.586 ug/l
RT: 9.22 min Scan# 2327
Delta R.T. 0.05 min
Lab File: VN064644.D
Acq: 13 Nov 2020 20:46

Tgt Ion: 88 Resp: 31
Ion Ratio Lower Upper
88 100
43 0.0 31.0 46.6#
58 0.0 58.4 87.6#

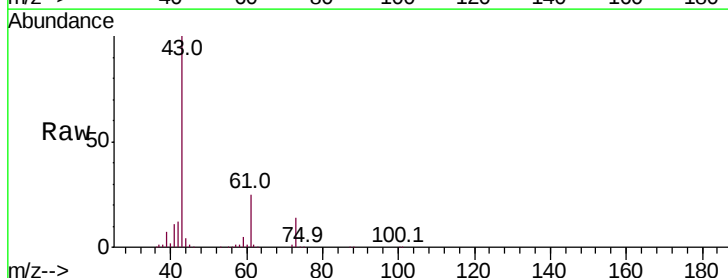

Abundance Ion 88.00 (87.70 to 88.70): VNC
Ion 43.00 (42.70 to 43.70): VNC
Ion 58.00 (57.70 to 58.70): VNC

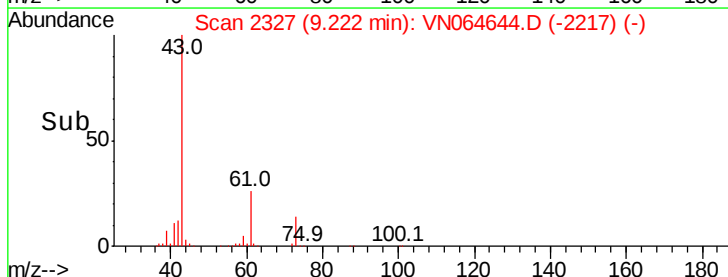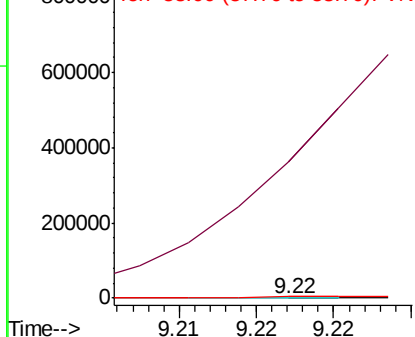

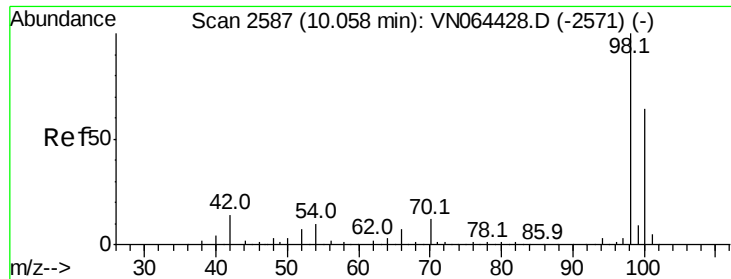

#50

Toluene-d8

Concen: 50.564 ug/l

RT: 10.06 min Scan# 2588

Delta R.T. 0.00 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampleId :


TP-3-D

Tot Ion: 98 Resp: 618815

Ion Ratio Lower Upper

98 100

100 63.2 50.7 76.1

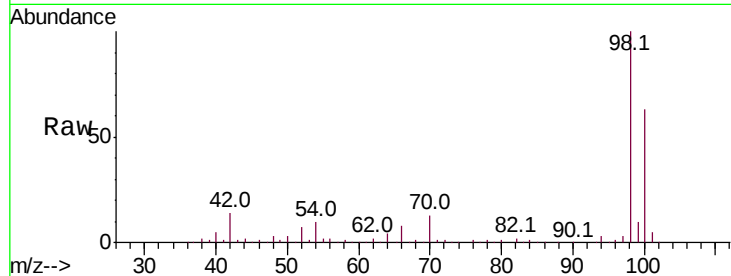

Abundance Ion 98.00 (97.70 to 98.70): VN064428.D (-2571) (-)

Ion 100.00 (99.70 to 100.70): VN064428.D (-2571) (-)

10.06



300000

200000

100000

0

Time-->

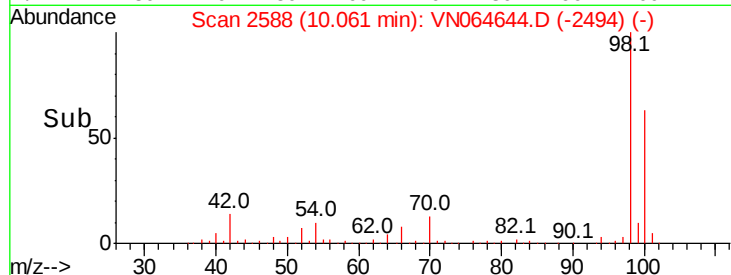

#51

4-Methyl-2-Pentanone

Concen: 1.628 ug/l

RT: 9.95 min Scan# 2554

Delta R.T. -0.00 min

Lab File: VN064644.D


Acq: 13 Nov 2020 20:46

Tgt Ion: 43 Resp: 7559

Ion Ratio Lower Upper

43 100

58 36.7 28.4 42.6



Abundance Ion 43.00 (42.70 to 43.70): VN064428.D (-2535) (-)

Ion 58.00 (57.70 to 58.70): VN064428.D (-2535) (-)

30000

25000

20000


15000


10000

5000

0

Time-->









#54
 cis-1,3-Dichloropropene
 Concen: 5.264 ug/l
 RT: 9.87 min Scan# 2530
 Delta R.T. 0.07 min
 Lab File: VN064644.D
 Acq: 13 Nov 2020 20:46




Instrument :
 MSVOA_N
 ClientSampleId :
 TP-3-D


Tot Ion: 75 Resp: 32537
 Ion Ratio Lower Upper
 75 100
 77 0.0 24.9 37.3#
 39 49.0 47.1 70.7

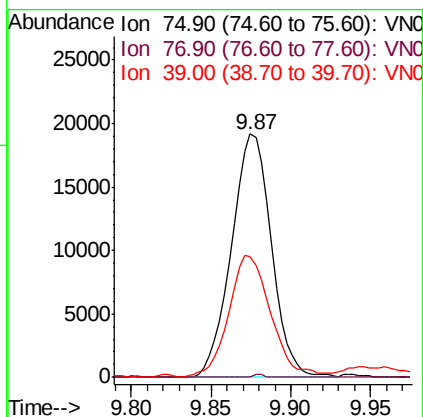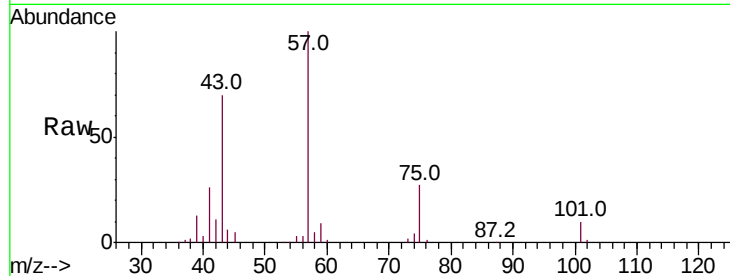

#56
 Ethyl methacrylate
 Concen: 1.863 ug/l
 RT: 10.28 min Scan# 2657
 Delta R.T. -0.11 min
 Lab File: VN064644.D
 Acq: 13 Nov 2020 20:46

Tgt Ion: 69 Resp: 129
 Ion Ratio Lower Upper
 69 100
 41 0.0 59.3 88.9#
 39 0.0 35.4 53.0#

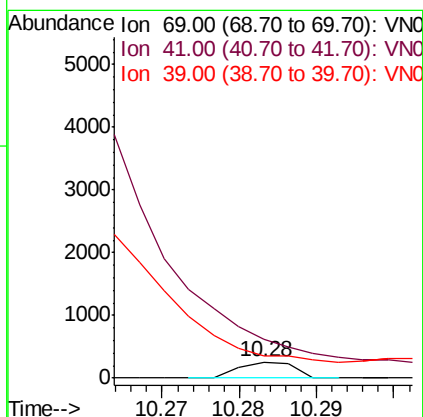



#57

1,3-Dichloropropane

Concen: 1.033 ug/l

RT: 10.74 min Scan# 2798

Delta R.T. 0.06 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampled :


TP-3-D

Tot Ion: 76 Resp: 6192

Ion Ratio Lower Upper




76 100

78 0.0 25.8 38.6#

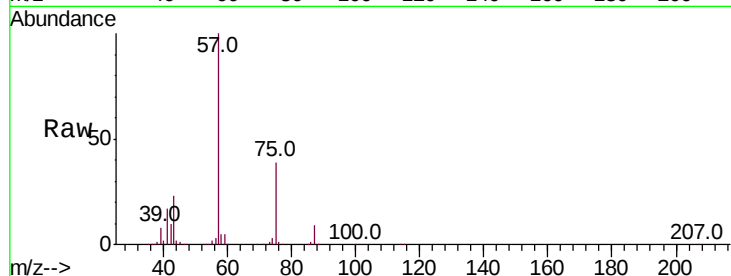

Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

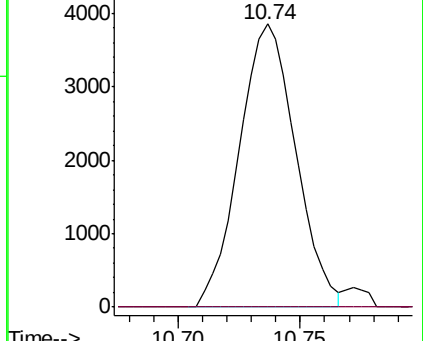

#59

2-Hexanone

Concen: 30.344 ug/l

RT: 10.74 min Scan# 2798

Delta R.T. 0.02 min

Lab File: VN064644.D


Acq: 13 Nov 2020 20:46

Tgt Ion: 43 Resp: 101272

Ion Ratio Lower Upper



43 100


58 19.6 24.7 74.1#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0




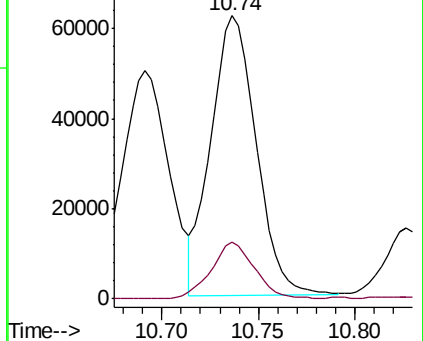


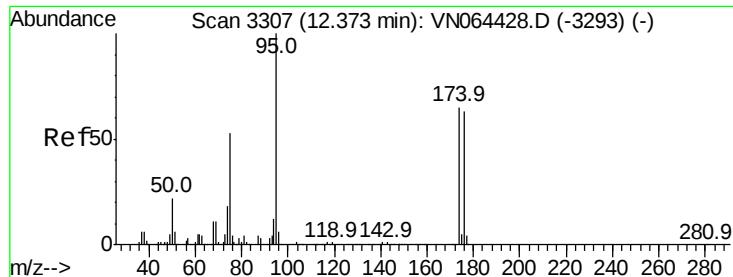

#62
4-Bromofluorobenzene
Concen: 50.136 ug/l
RT: 12.38 min Scan# 3308
Delta R.T. 0.00 min
Lab File: VN064644.D
Acq: 13 Nov 2020 20:46




Instrument :
MSVOA_N
ClientSampleId :
TP-3-D


Tot Ion: 95 Resp: 232047
Ion Ratio Lower Upper
95 100
174 70.0 0.0 132.6
176 67.5 0.0 129.2

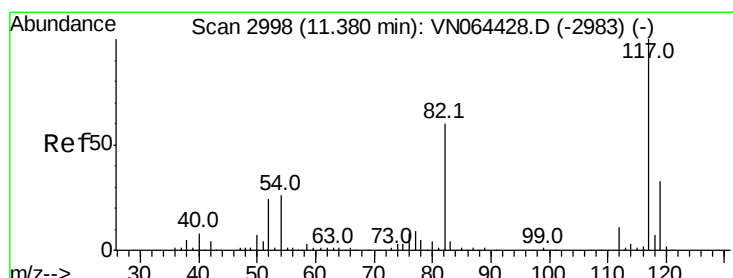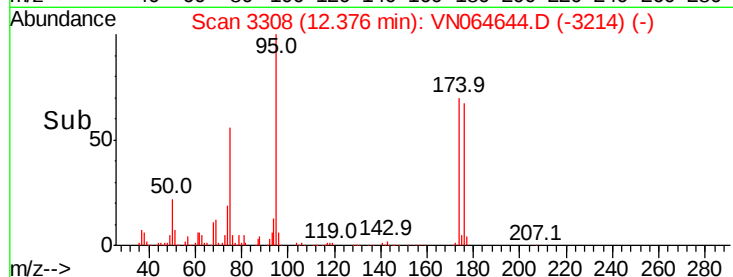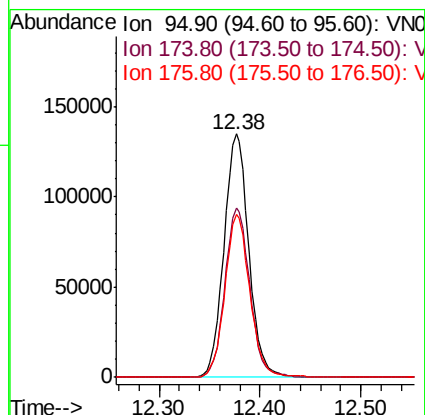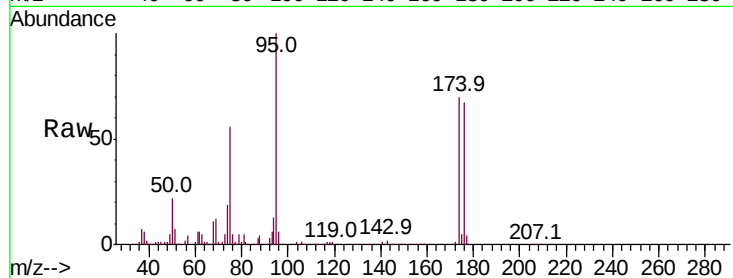

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.38 min Scan# 2998
Delta R.T. -0.00 min
Lab File: VN064644.D
Acq: 13 Nov 2020 20:46

Tgt Ion: 117 Resp: 516329
Ion Ratio Lower Upper
117 100
82 58.4 48.1 72.1
119 32.6 26.2 39.4

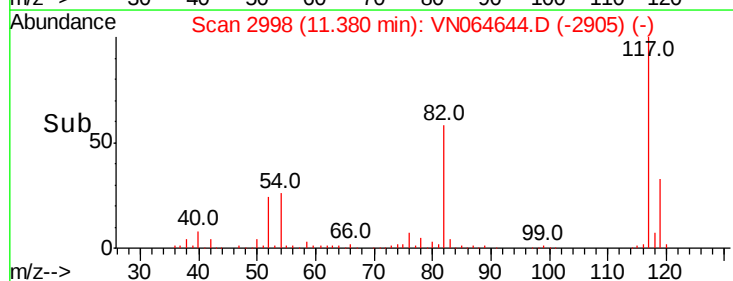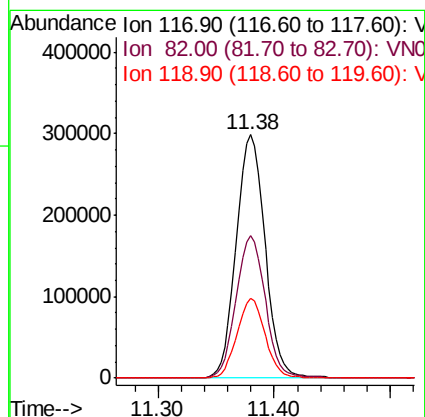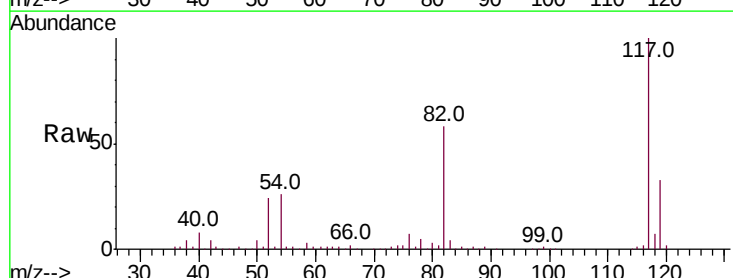



#71

Bromoform

Concen: 1.336 ug/l

RT: 12.36 min Scan# 3303

Delta R.T. 0.26 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampled :

TP-3-D


Tot Ion:173 Resp: 198

Ion Ratio Lower Upper

173 100

175 5394.9 23.7 71.1#




254 0.0 0.0 0.0



Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

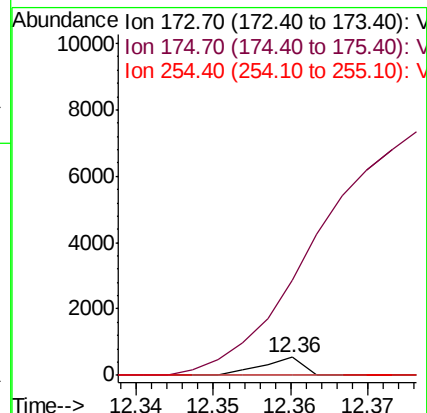

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3601

Delta R.T. 0.00 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46


Tgt Ion:152 Resp: 178722

Ion Ratio Lower Upper

152 100

115 65.7 32.0 96.0



150 158.7 0.0 353.8




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

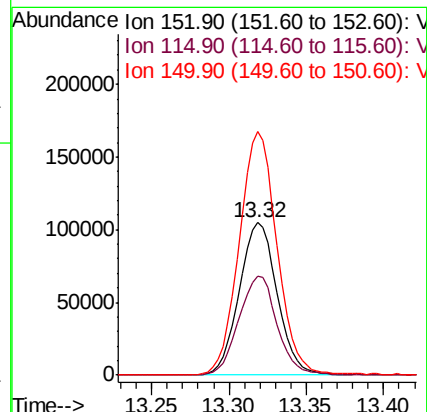

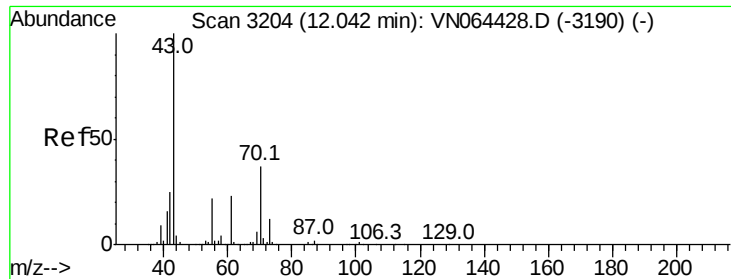

#74

N-amvl acetate

Concen: 1.653 ug/l

RT: 12.00 min Scan# 3192

Delta R.T. -0.04 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampleId :

TP-3-D

Tot Ion: 43 Resp: 3100



Ion Ratio Lower Upper

43 100

70 0.0 29.6 44.4#

55 5.1 18.4 27.6#

61 0.0 17.8 26.6#

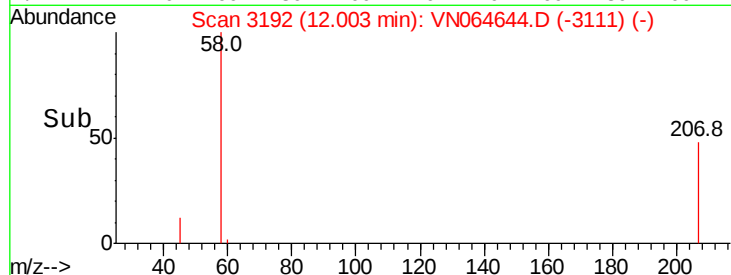
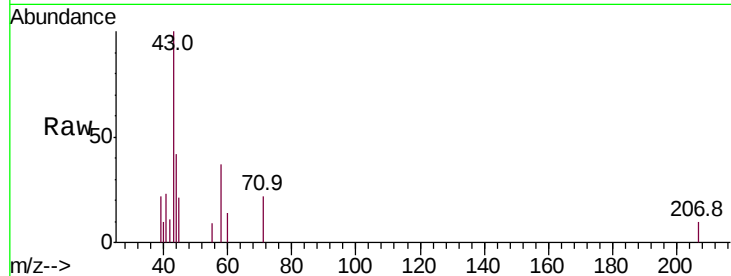


Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 70.00 (69.70 to 70.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

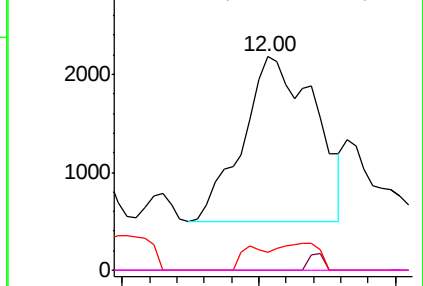

#76

1,2,3-Trichloropropane

Concen: 29.886 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. -0.15 min

Lab File: VN064644.D



Acq: 13 Nov 2020 20:46

Tgt Ion: 75 Resp: 129414

Ion Ratio Lower Upper


75 100


77 1.1 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

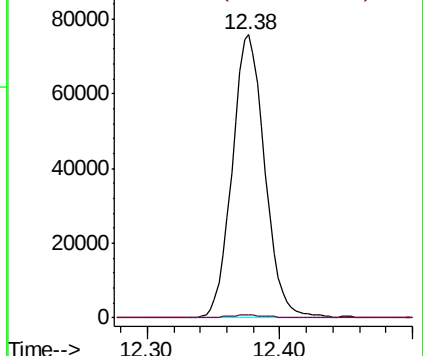

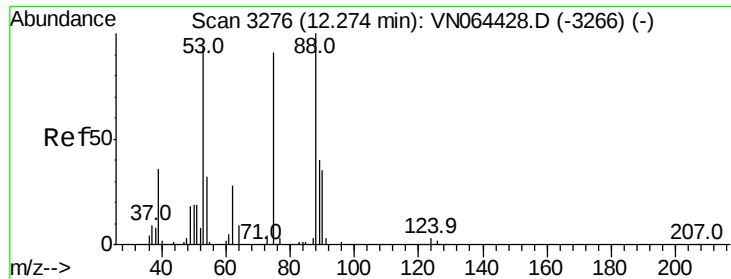

#81

trans-1,4-Dichloro-2-butene

Concen: 83.445 ug/l

RT: 12.38 min Scan# 3308

Delta R.T. 0.10 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46

Instrument :

MSVOA_N

ClientSampled :

TP-3-D


Tot Ion: 75 Resp: 129414

Ion Ratio Lower Upper

75 100

53 0.1 84.0 126.0#




89 0.0 36.3 54.5#

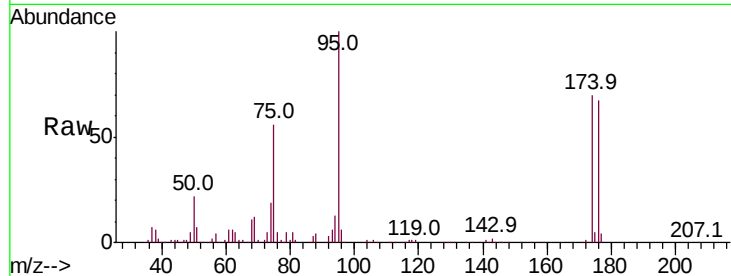

Abundance Ion 74.90 (74.60 to 75.60): VN064428.D (-3266) (-)

Ion 53.00 (52.70 to 53.70): VN064428.D (-3266) (-)

Ion 88.90 (88.60 to 89.60): VN064428.D (-3266) (-)

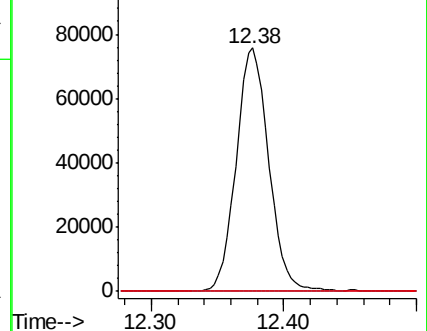

#95

Naphthalene

Concen: 3.634 ug/l

RT: 15.11 min Scan# 4159

Delta R.T. 0.01 min

Lab File: VN064644.D

Acq: 13 Nov 2020 20:46


Tgt Ion: 128 Resp: 122

Ion Ratio Lower Upper

128 100

127 0.0 10.5 15.7#

129 0.0 8.8 13.2#



Abundance Ion 128.00 (127.70 to 128.70): VN064428.D (-4139) (-)

Ion 127.00 (126.70 to 127.70): VN064428.D (-4139) (-)

Ion 129.00 (128.70 to 129.70): VN064428.D (-4139) (-)

