


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN111320\
Data File : VN064622.D
Acq On : 13 Nov 2020 10:35
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
Title : SW846 8260
Last Update : Wed Nov 04 12:09:03 2020

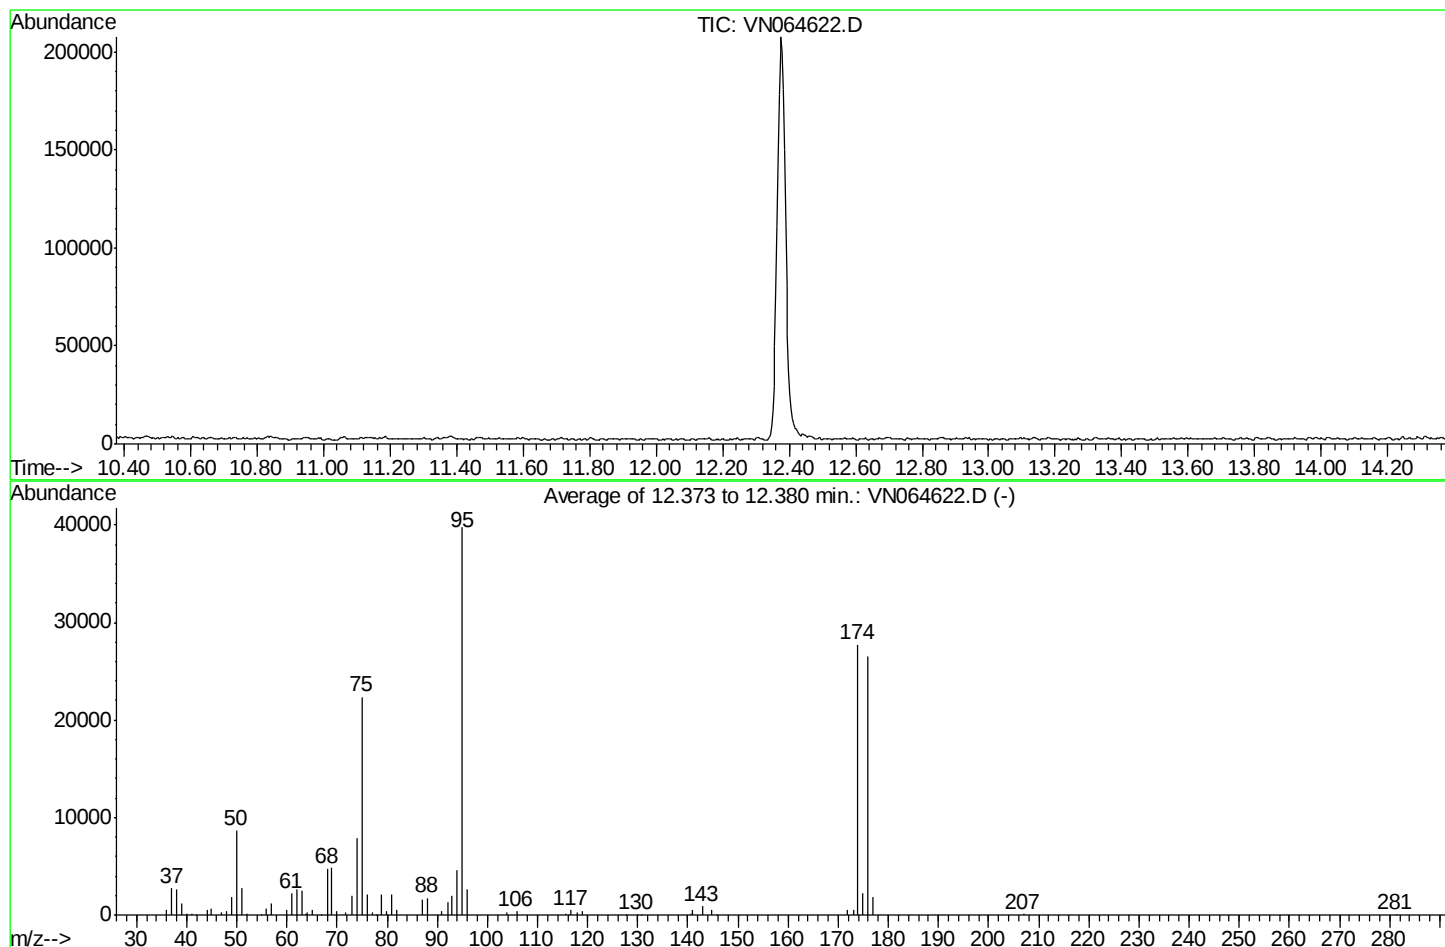

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	8614	PASS
75	95	30	60	56.2	22365	PASS
95	95	100	100	100.0	39762	PASS
96	95	5	9	6.7	2657	PASS
173	174	0.00	2	1.8	511	PASS
174	95	50	100	69.8	27741	PASS
175	174	5	9	7.9	2196	PASS
176	174	95	101	95.8	26576	PASS
177	176	5	9	6.7	1778	PASS