
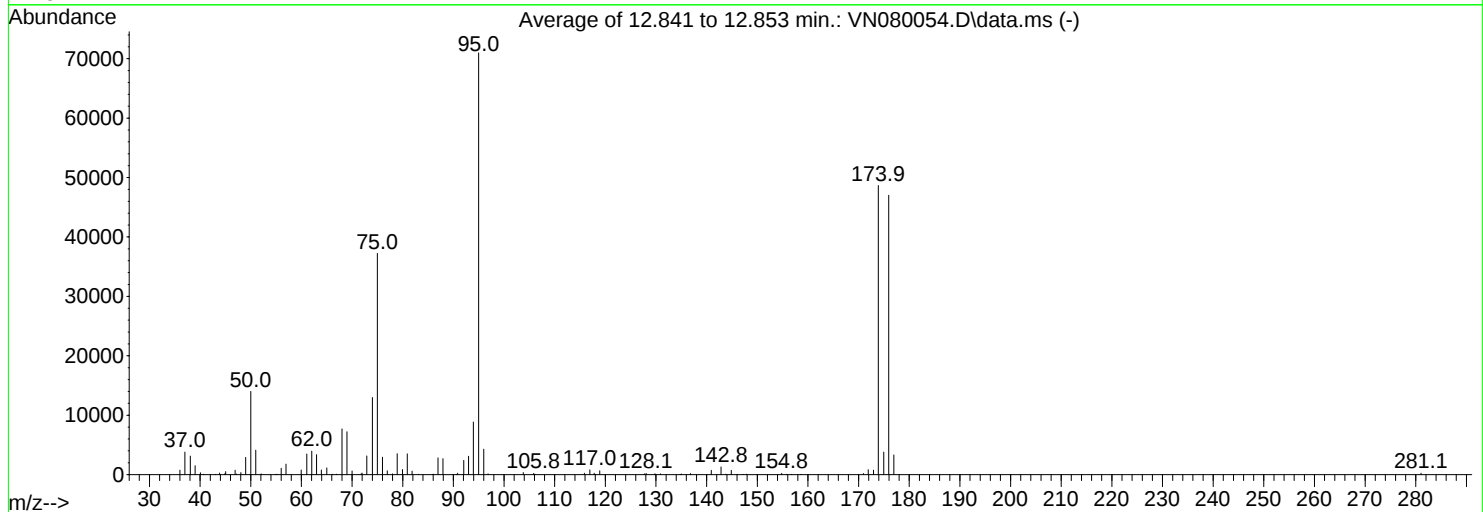


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111323\
Data File : VN080054.D
Acq On : 13 Nov 2023 08:29
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

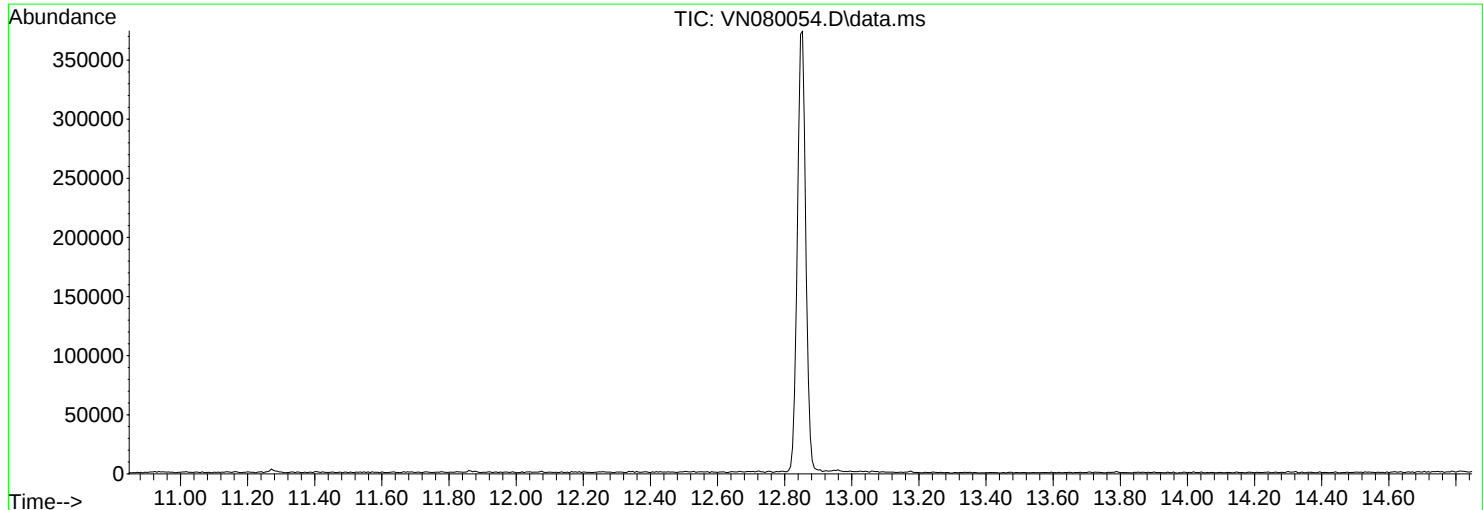

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	14002	PASS
75	95	30	60	52.5	37232	PASS
95	95	100	100	100.0	70984	PASS
96	95	5	9	6.0	4284	PASS
173	174	0.00	2	1.6	763	PASS
174	95	50	100	68.5	48659	PASS
175	174	5	9	7.8	3805	PASS
176	174	95	101	96.6	47013	PASS
177	176	5	9	7.1	3320	PASS

Average of 12.841 to 12.853 min.: VN080054.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	752	47.20	123	61.05	3475	71.95	271
37.00	3806	48.05	364	62.05	3970	72.90	314
38.05	3116	49.00	2923	63.00	3381	74.00	1298
39.00	1514	50.00	14002	63.95	783	75.00	3723
40.05	334	51.00	4133	65.00	1128	76.00	2941
40.70	55	52.05	147	66.20	54	76.95	642
43.00	62	54.90	67	66.90	81	78.00	141
43.85	273	55.20	78	68.00	7699	78.90	3537
44.90	161	56.00	1087	69.00	7204	79.95	870
45.05	501	56.95	1771	70.00	620	80.90	3508
46.90	750	59.95	788	71.80	146	81.85	587

Average of 12.841 to 12.853 min.: VN080054.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
83.10	63	96.00	4284	128.05	222	147.20	53
85.90	71	96.85	125	129.80	159	147.90	86
86.10	85	103.80	358	130.90	141	154.80	219
86.95	2828	105.85	223	134.80	63	155.80	57
87.95	2700	106.10	86	135.00	96	156.80	61
90.60	51	115.85	232	136.80	182	158.60	55
90.85	257	116.95	818	140.90	724	170.95	203
92.05	2388	117.80	235	142.85	1307	171.90	848
93.00	3096	118.10	61	143.80	74	172.95	763
93.95	8873	118.90	649	144.85	719	173.90	48659
95.00	70984	127.70	140	146.00	59	174.95	3805

Average of 12.841 to 12.853 min.: VN080054.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.95	47013						
176.95	3320						
281.05	246						

Instrument :

MSVOA_N

ClientSampleId :

BFB