
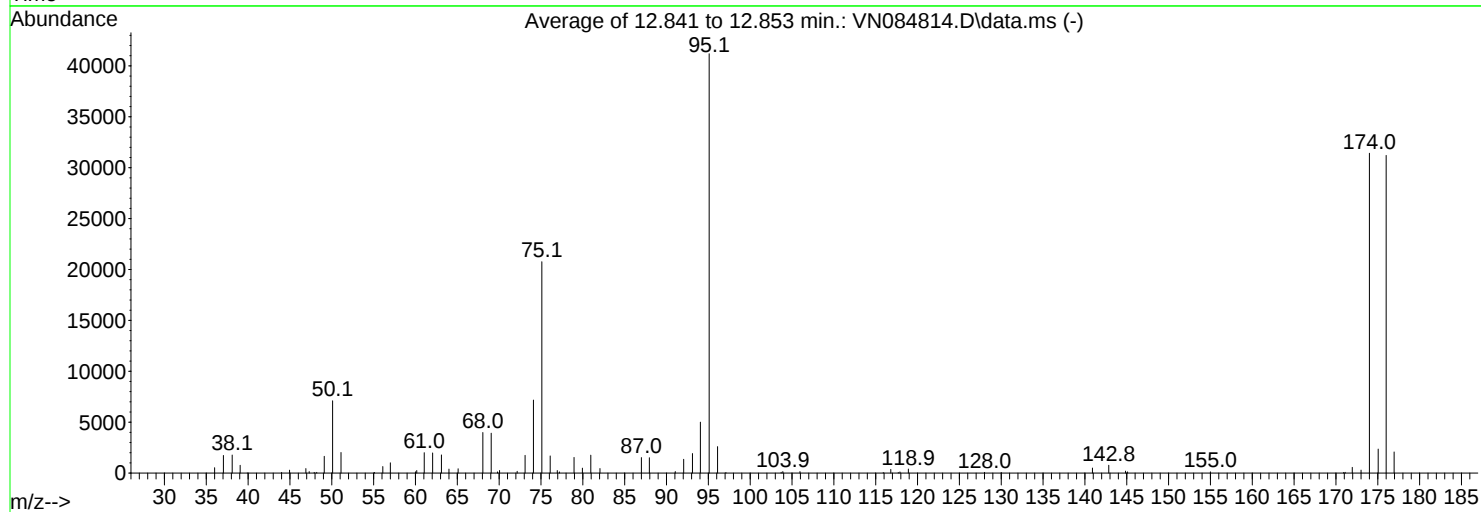


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111324\
Data File : VN084814.D
Acq On : 13 Nov 2024 08:53
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

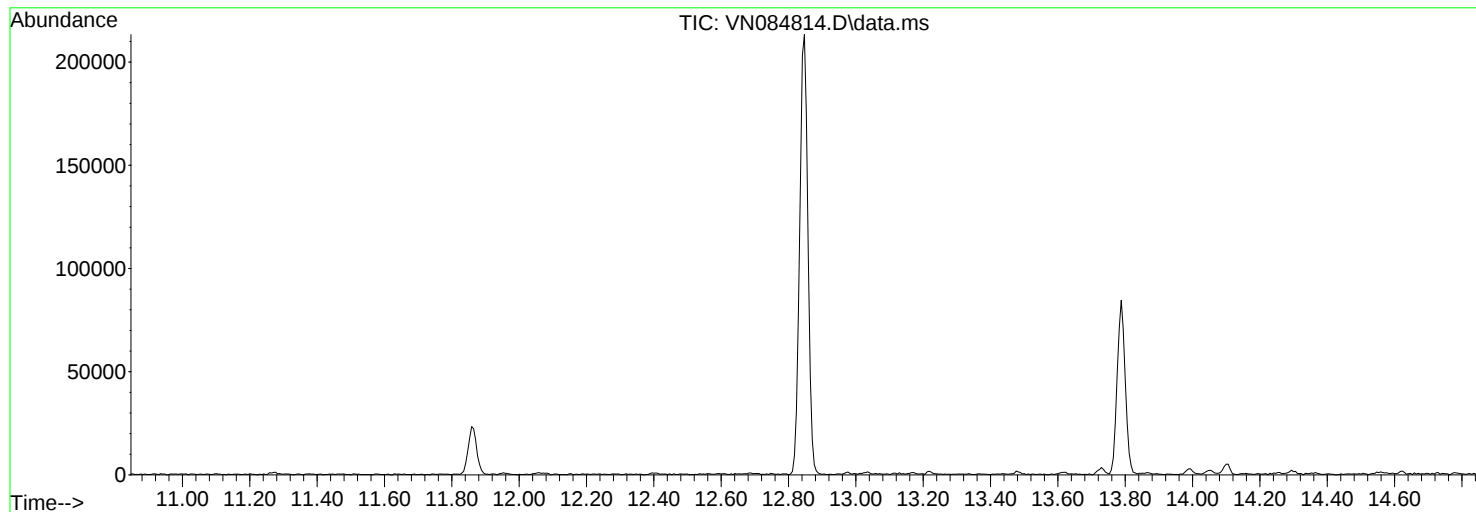

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	7103	PASS
75	95	30	60	50.4	20765	PASS
95	95	100	100	100.0	41195	PASS
96	95	5	9	6.3	2598	PASS
173	174	0.00	2	0.9	292	PASS
174	95	50	100	76.3	31419	PASS
175	174	5	9	7.5	2357	PASS
176	174	95	101	99.3	31208	PASS
177	176	5	9	6.6	2074	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	531	49.10	1649	64.00	393	76.95	248
37.05	1731	50.10	7103	65.10	427	77.20	115
38.10	1774	51.10	2022	68.05	3985	78.95	1539
39.05	763	55.10	61	69.05	3920	79.95	487
39.90	6	56.10	641	69.80	121	80.95	1758
44.00	58	57.00	1009	70.05	254	82.05	450
44.95	286	60.00	127	72.15	177	87.00	1523
46.90	445	60.15	250	73.10	1741	87.95	1510
47.30	144	61.05	2007	74.10	7173	91.05	153
47.90	65	62.05	1978	75.10	20765	92.05	1355
48.20	70	63.10	1784	76.10	1683	93.10	1921

Average of 12.841 to 12.853 min.: VN084814.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	5004	118.90	394	173.00	292		
95.10	41195	128.00	72	174.00	31419		
96.10	2598	130.00	53	175.05	2357		
97.10	55	140.90	496	176.00	31208		
103.70	80	142.85	768	176.95	2074		
103.90	150	144.85	194				
105.95	150	145.10	120				
115.90	53	155.00	125				
116.80	362	170.90	51				
117.70	55	171.10	74				
117.90	114	171.95	562				

Instrument :

MSVOA_N

ClientSampleId :

BFB