



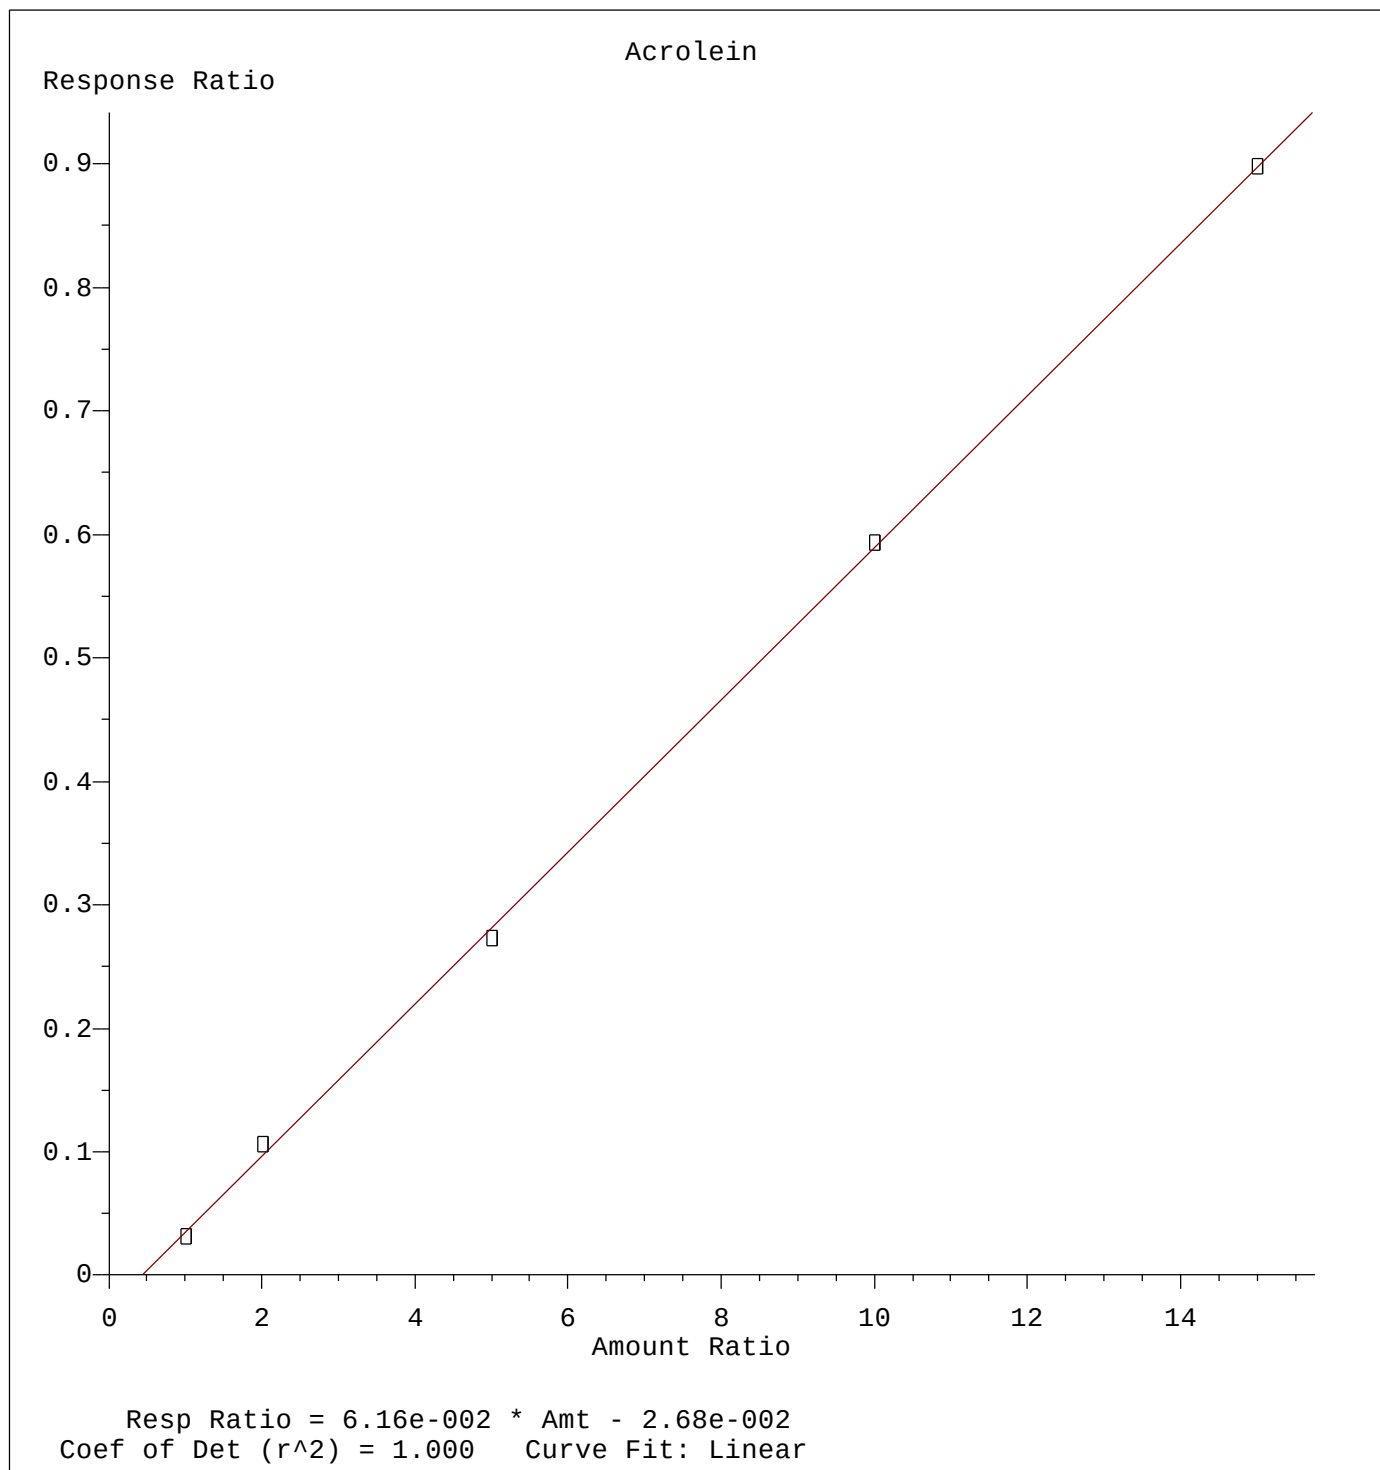


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Calibration Table Last Updated: Tue Nov 20 15:43:01 2018

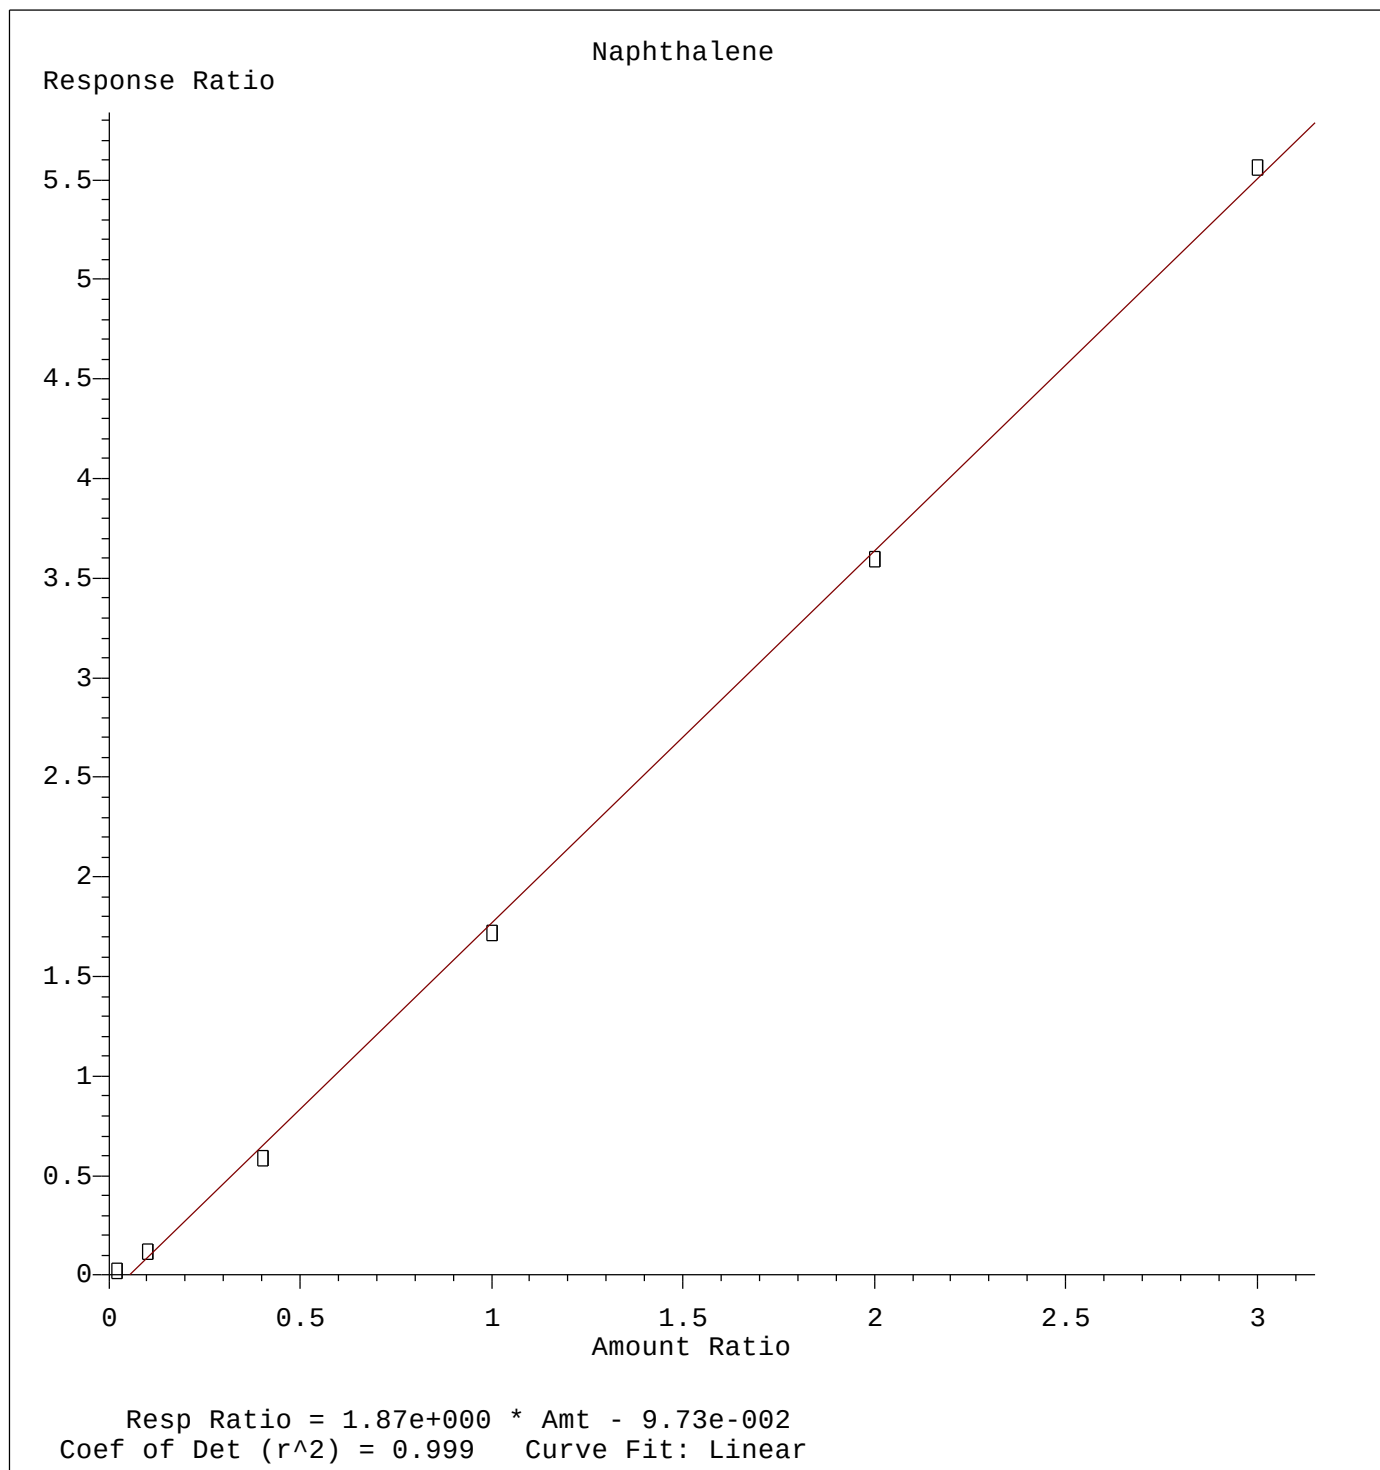

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Calibration Table Last Updated: Tue Nov 20 15:43:01 2018

1,2,4-Trichlorobenzene

Response Ratio

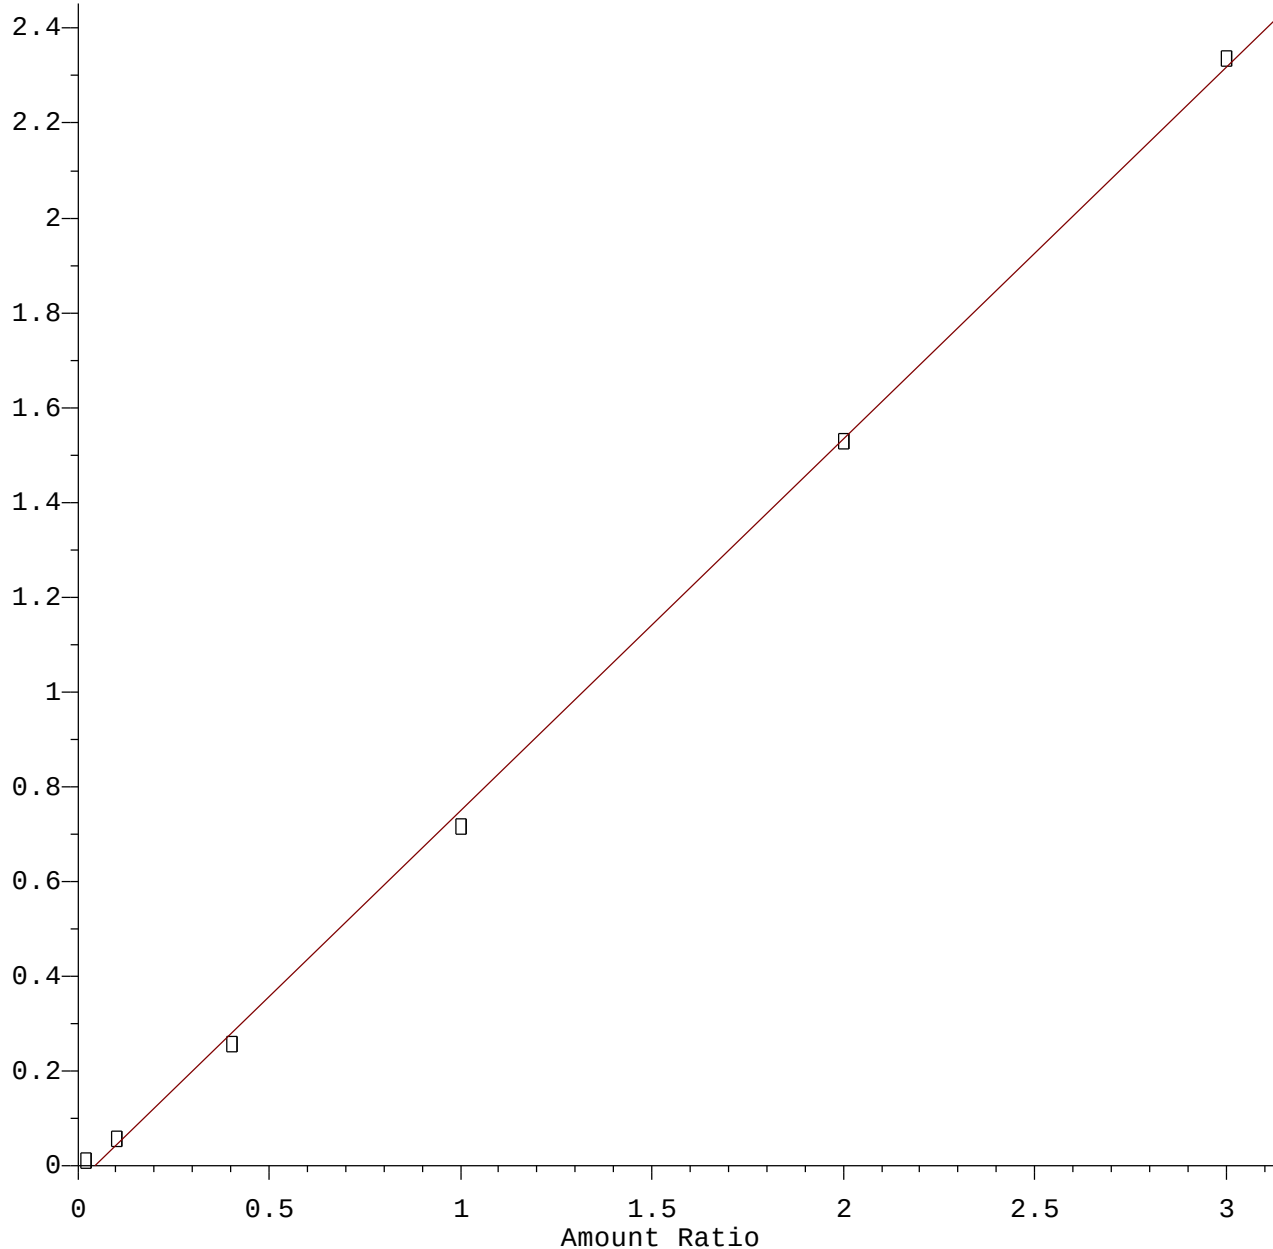


Resp Ratio = $7.84 \times 10^{-1} \times \text{Amt} - 3.54 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Calibration Table Last Updated: Tue Nov 20 15:43:01 2018


Methacrylonitrile

Response Ratio

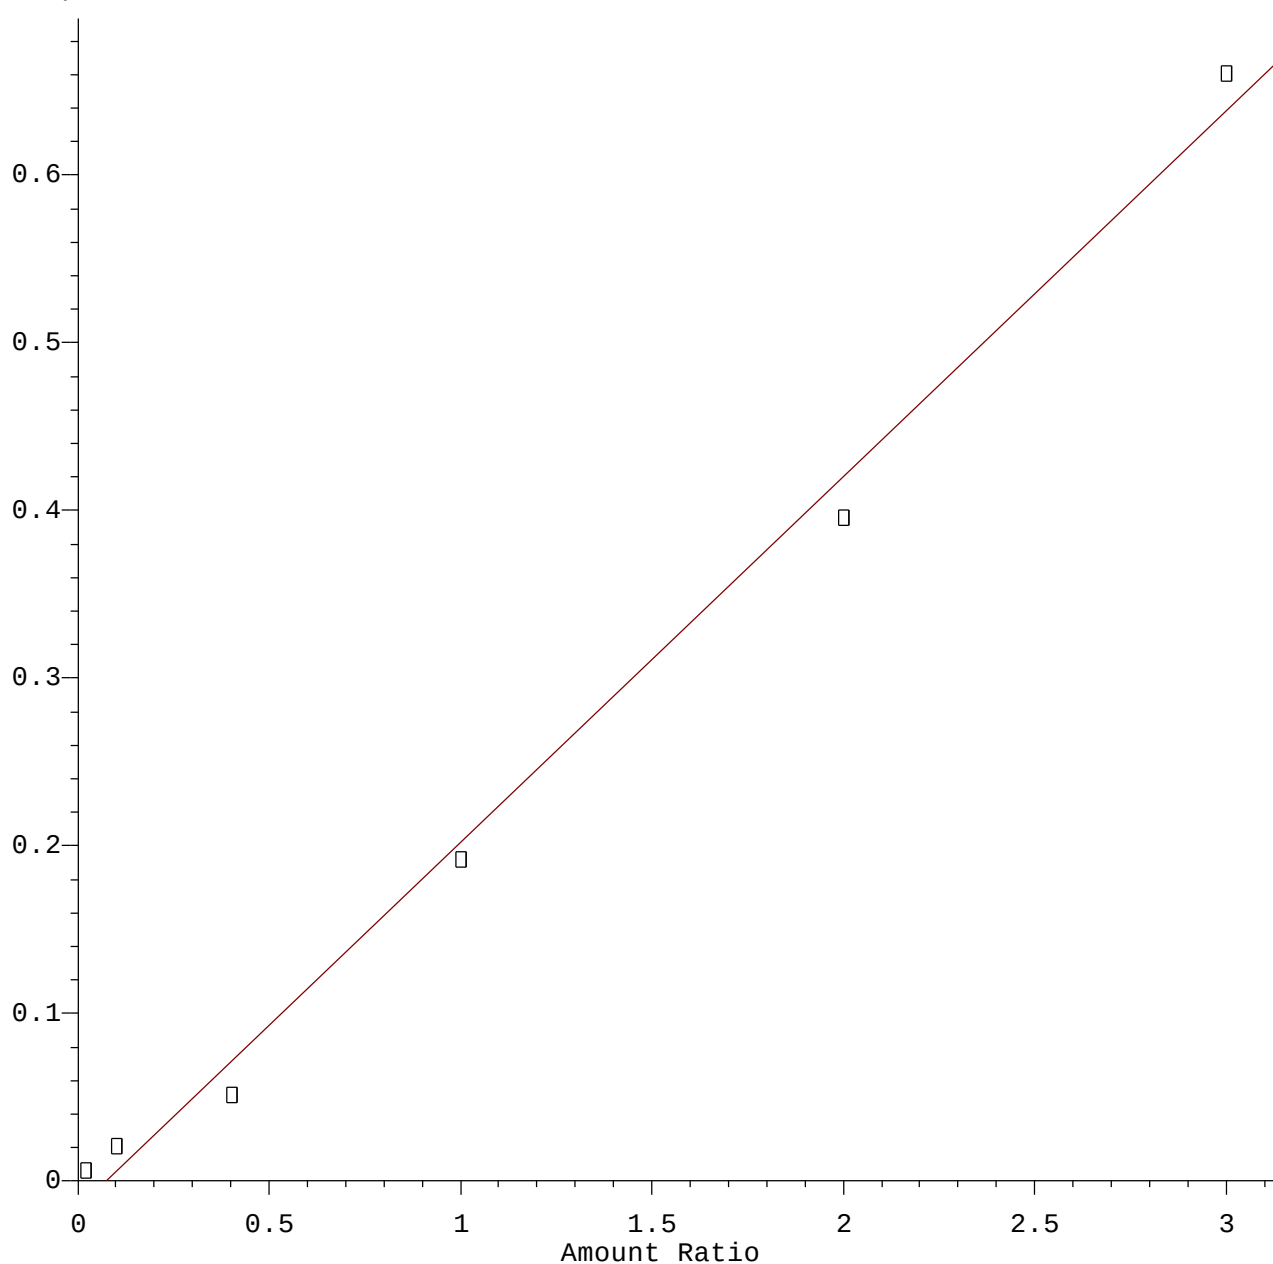

Resp Ratio = $2.18 \times 10^{-1} \times \text{Amt} - 1.61 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Calibration Table Last Updated: Tue Nov 20 15:43:01 2018

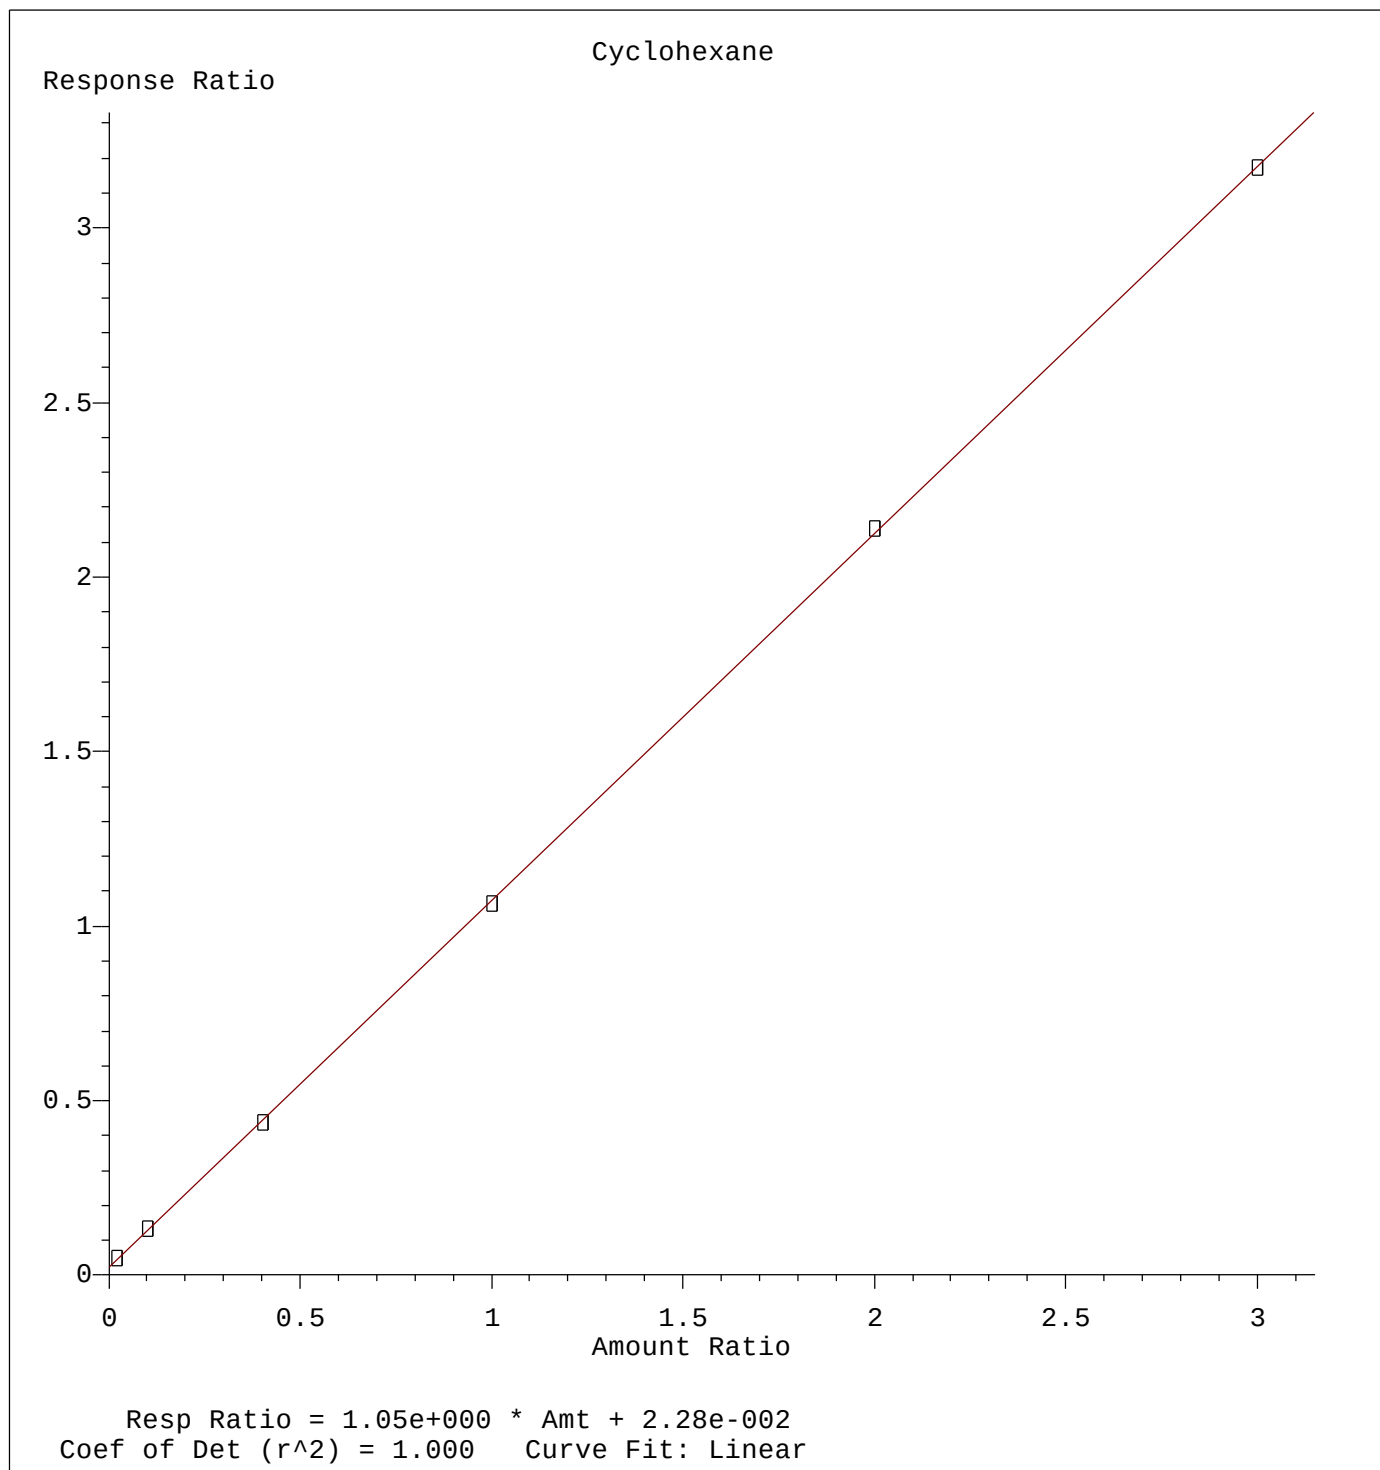

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Calibration Table Last Updated: Tue Nov 20 15:43:01 2018


Methylene Chloride

Response Ratio

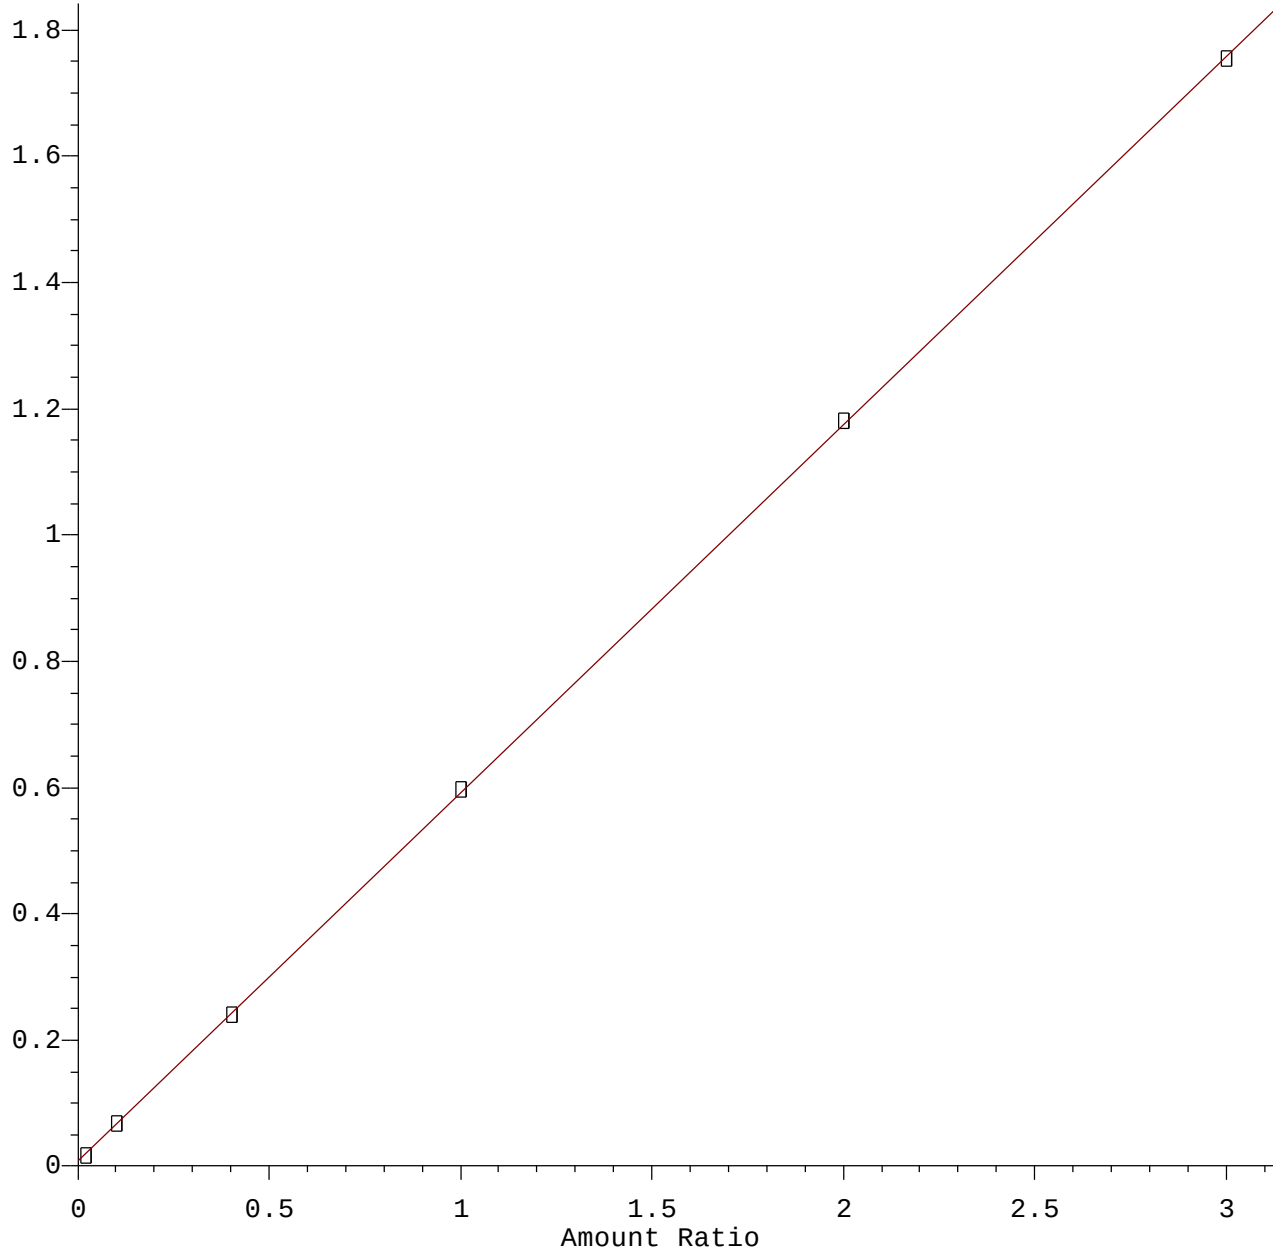

Resp Ratio = 5.83e-001 * Amt + 8.29e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Calibration Table Last Updated: Tue Nov 20 15:43:01 2018

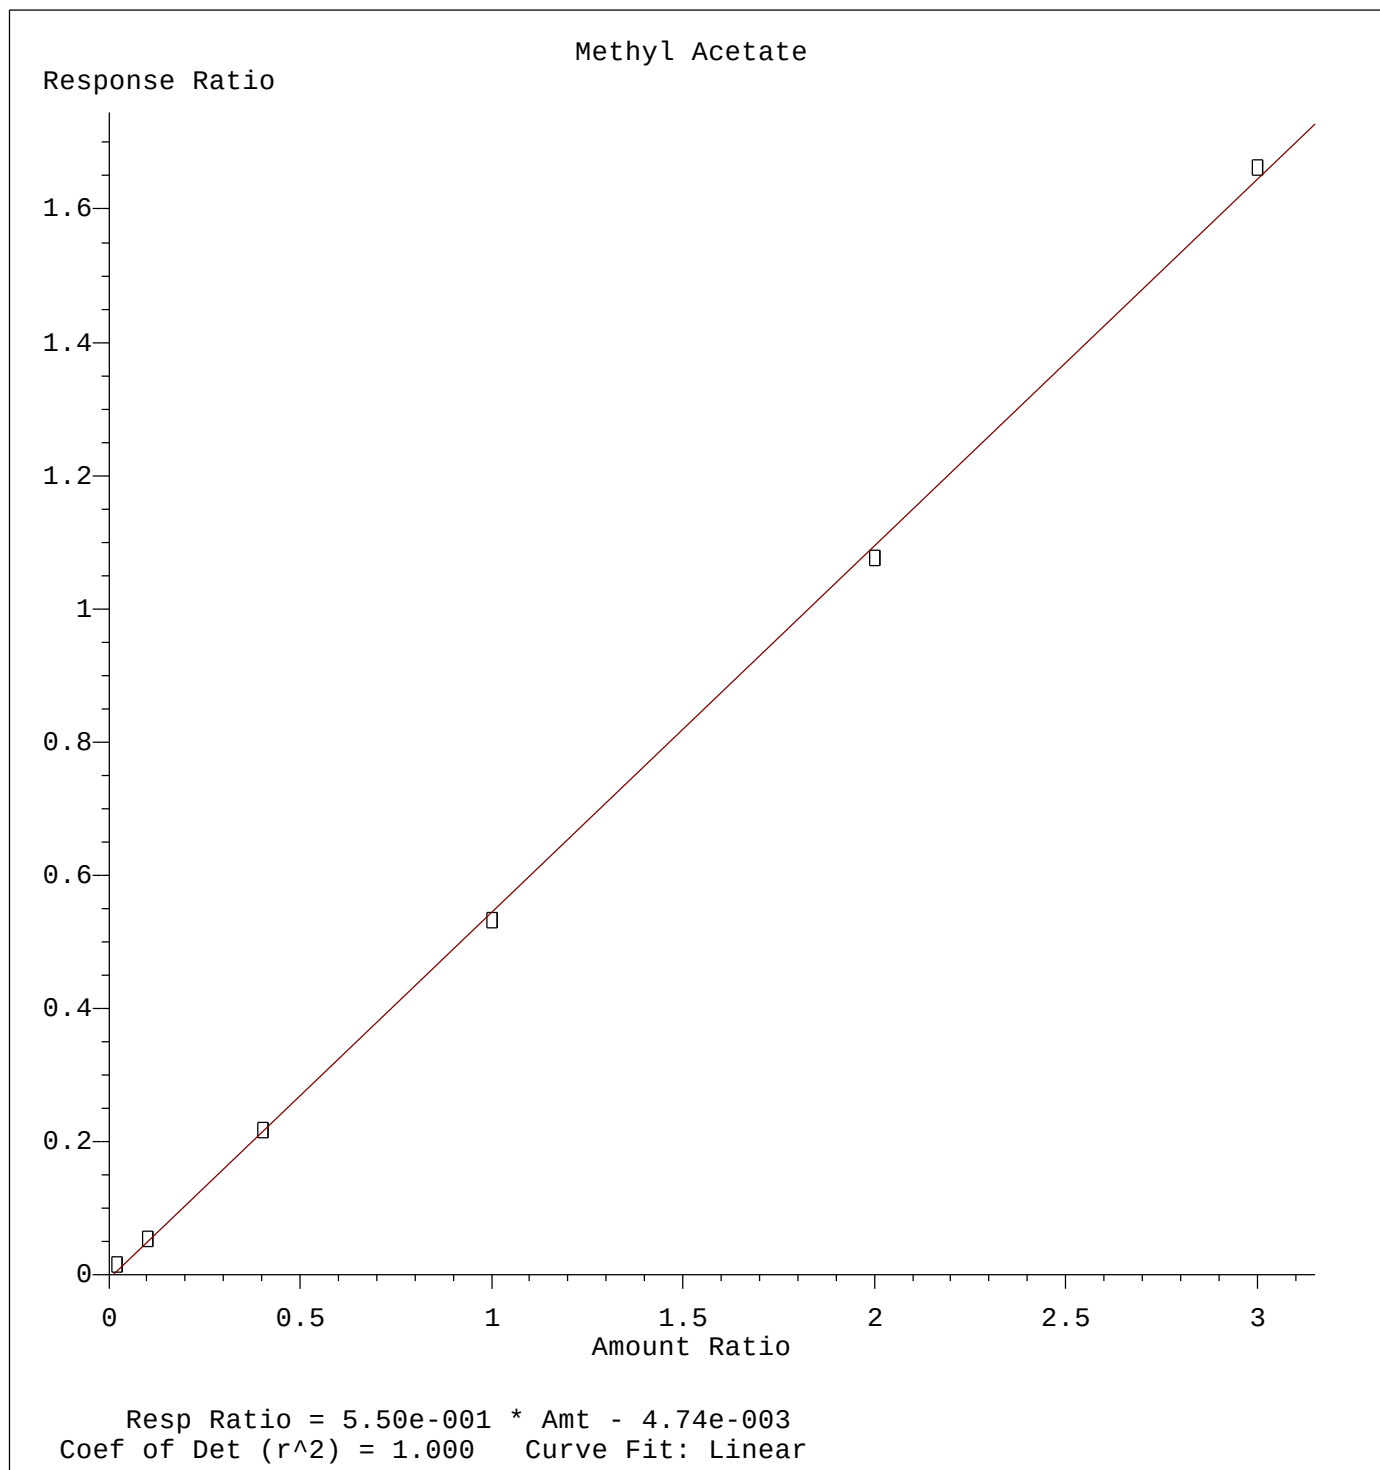

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Calibration Table Last Updated: Tue Nov 20 15:43:01 2018