


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN111418\
Data File : VN052303.D
Acq On : 14 Nov 2018 9:56
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Title : SW846 8260
Last Update : Thu Nov 15 03:02:37 2018

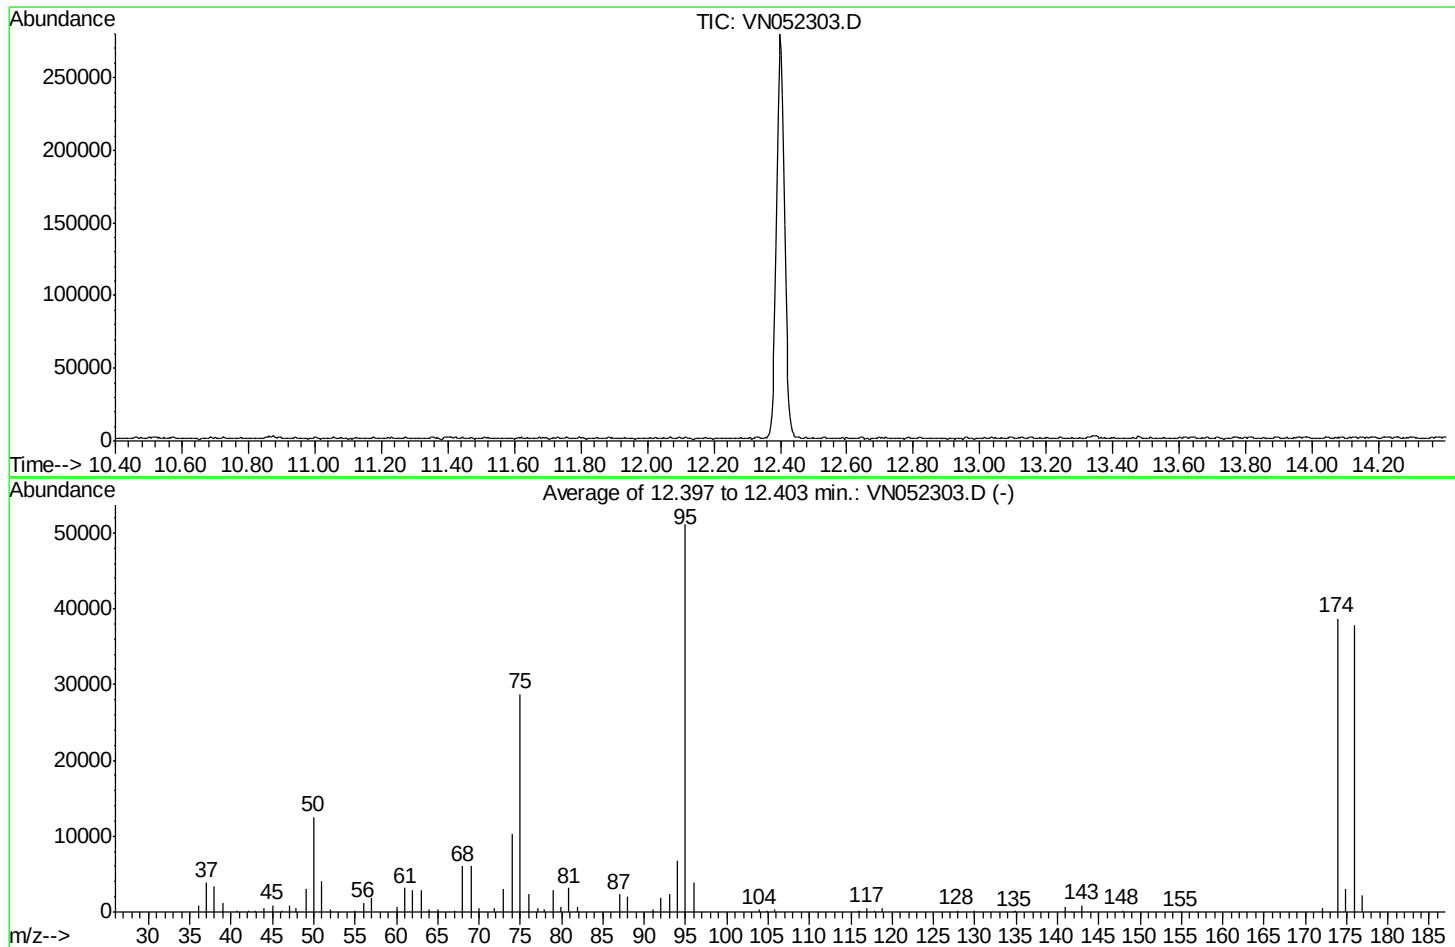

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.5	12536	PASS
75	95	30	60	56.2	28728	PASS
95	95	100	100	100.0	51130	PASS
96	95	5	9	7.5	3830	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.7	38706	PASS
175	174	5	9	7.7	2966	PASS
176	174	95	101	97.8	37845	PASS
177	176	5	9	6.0	2268	PASS