

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111422\
 Data File : VN075263.D
 Acq On : 14 Nov 2022 14:16
 Operator : JC\MD
 Sample : N5417-02
 Misc : 5.05g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 AUD-1732

Quant Time: Nov 15 03:51:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 09:48:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	198562	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	356075	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	302066	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	137719	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	130473	48.768	ug/l	-0.01
Spiked Amount	50.000	Range	74 - 125	Recovery	=	97.540%
35) Dibromofluoromethane	8.171	113	115680	55.340	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	110.680%
50) Toluene-d8	10.565	98	385992	47.595	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	95.180%
62) 4-Bromofluorobenzene	12.847	95	136109	47.776	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	95.560%
Target Compounds						
					Qvalue	
5) Bromomethane	2.901	94	514	Below Cal	#	49
6) Chloroethane	3.089	64	6238	2.223	ug/l #	56
11) Tert butyl alcohol	5.489	59	4626	7.415	ug/l #	72
16) Acetone	4.459	43	4486	3.960	ug/l #	86
18) Methyl Acetate	5.047	43	7074	1.912	ug/l	95
19) Methyl tert-butyl Ether	5.806	73	1691	0.216	ug/l #	56
20) Methylene Chloride	5.271	84	4678	1.852	ug/l #	68
23) Vinyl Acetate	6.724	43	2639	0.466	ug/l #	67
25) 2-Butanone	7.494	43	3900	2.189	ug/l	93
29) Tetrahydrofuran	7.853	42	266	0.231	ug/l #	26
31) Cyclohexane	8.218	56	4356	1.095	ug/l #	30
36) 1,1-Dichloropropene	8.224	75	15788	4.879	ug/l #	50
37) Ethyl Acetate	7.494	43	3900	1.099	ug/l #	66
38) Carbon Tetrachloride	8.218	117	21576	6.061	ug/l #	15
43) Isopropyl Acetate	8.794	43	5692	1.034	ug/l #	53
48) Methyl methacrylate	9.665	41	968	0.383	ug/l #	12
51) 4-Methyl-2-Pentanone	10.453	43	754	0.212	ug/l #	62
53) t-1,3-Dichloropropene	10.688	75	3009	0.801	ug/l #	62
59) 2-Hexanone	11.200	43	1609	0.597	ug/l	86
67) Ethyl Benzene	11.965	91	3020	0.260	ug/l	90
68) m/p-Xylenes	12.071	106	6960	1.495	ug/l	99
69) o-Xylene	12.400	106	2509	0.545	ug/l	94
71) Bromoform	12.847	173	973	0.543	ug/l #	1
74) N-amyl acetate	12.459	43	2154	0.527	ug/l #	41
75) 1,1,2,2-Tetrachloroethane	12.947	83	1536	Below Cal	#	30
76) 1,2,3-Trichloropropane	13.088	75	2673	0.914	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	71500	62.767	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.482	105	2414	0.257	ug/l	90
92) 1,2-Dibromo-3-Chloropr...	14.882	75	883	1.184	ug/l #	2
95) Naphthalene	15.635	128	3635	0.464	ug/l #	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111422\
Data File : VN075263.D
Acq On : 14 Nov 2022 14:16
Operator : JC\MD
Sample : N5417-02
Misc : 5.05g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Quant Time: Nov 15 03:51:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 09:48:49 2022
Response via : Initial Calibration

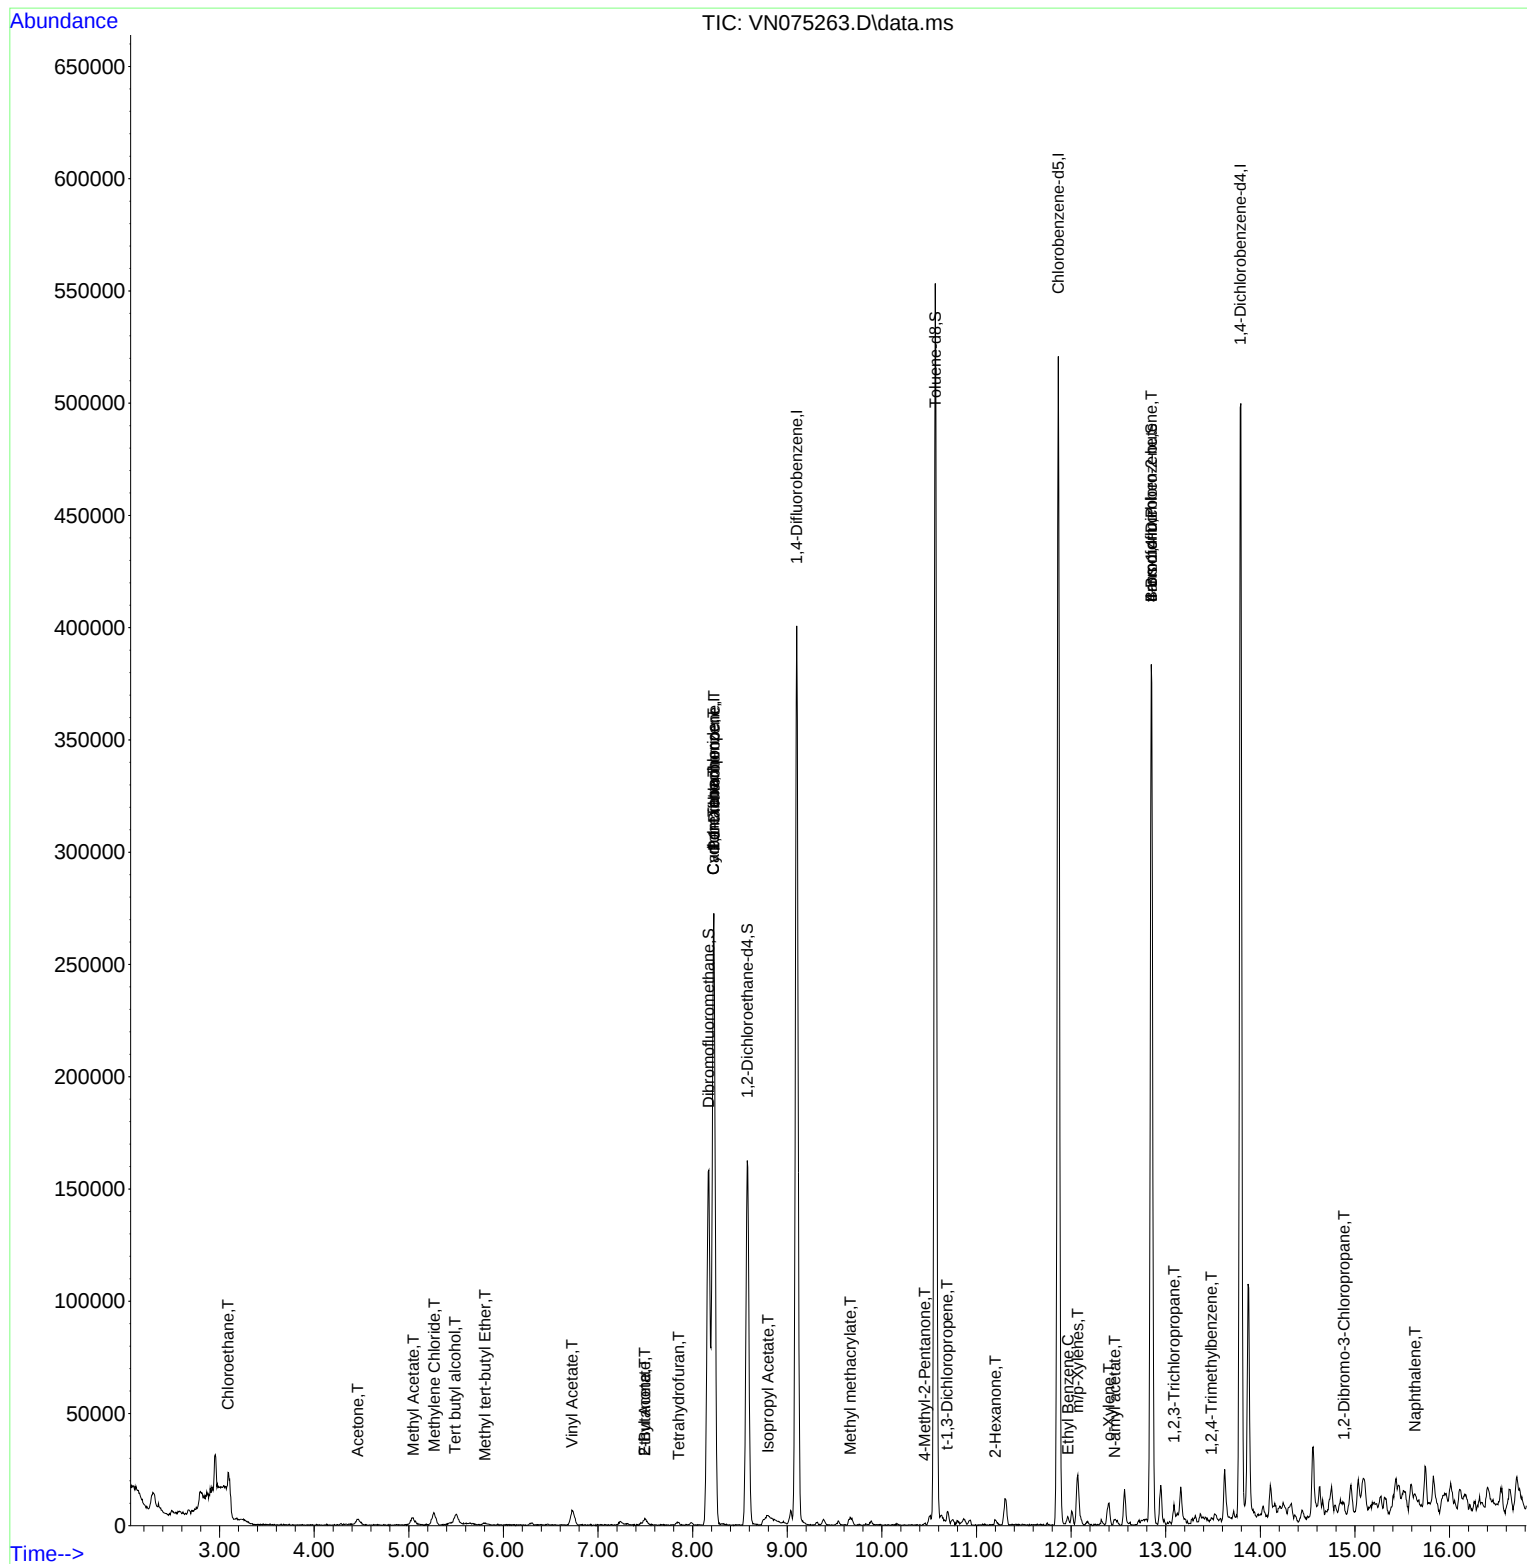



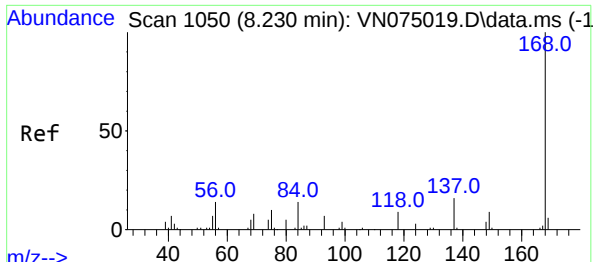


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 10
Delta R.T. -0.006 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Instrument :
MSVOA_N
ClientSampleId :
AUD-1732



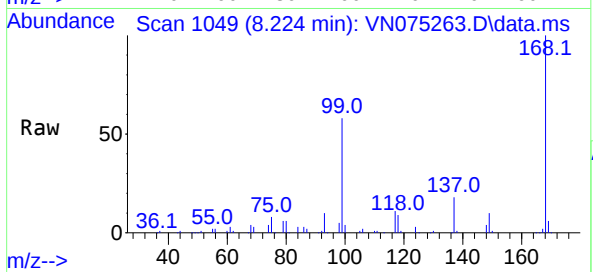



Tgt Ion:168 Resp: 198562
Ion Ratio Lower Upper
168 100
99 58.2 51.6 77.4

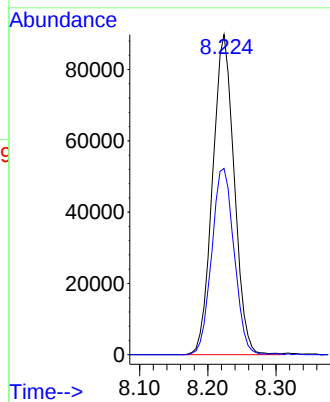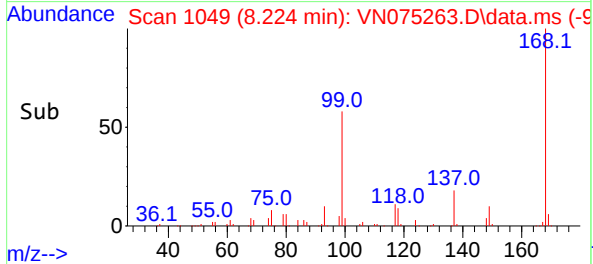

#5
Bromomethane
Concen: Below Cal
RT: 2.901 min Scan# 144
Delta R.T. -0.017 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 94 Resp: 514
Ion Ratio Lower Upper
94 100
96 137.7 71.8 107.6#


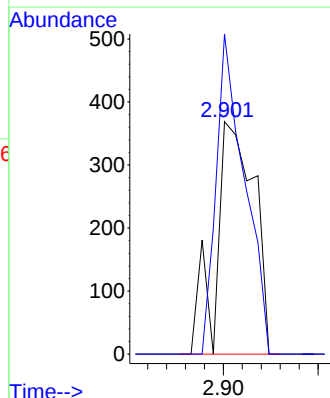
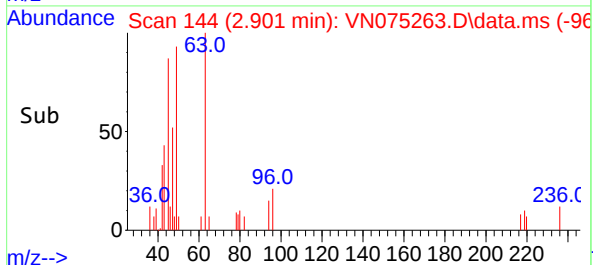
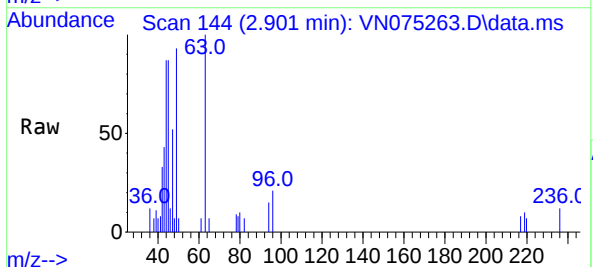


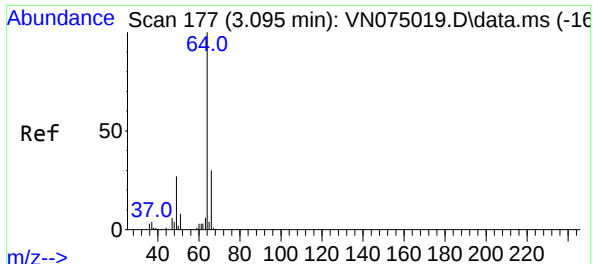

#6
Chloroethane
Concen: 2.223 ug/l
RT: 3.089 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion: 64 Resp: 6238
Ion Ratio Lower Upper
64 100
66 6.1 23.8 35.8#



#11
Tert butyl alcohol
Concen: 7.415 ug/l
RT: 5.489 min Scan# 584
Delta R.T. -0.053 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 59 Resp: 4626
Ion Ratio Lower Upper
59 100
57 0.0 8.5 12.7#


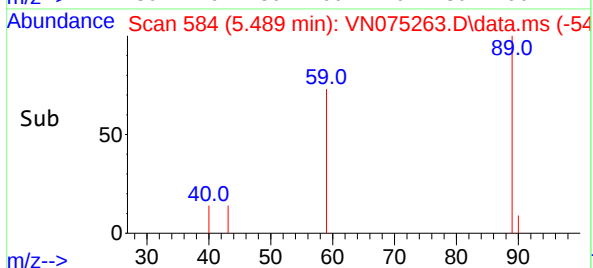

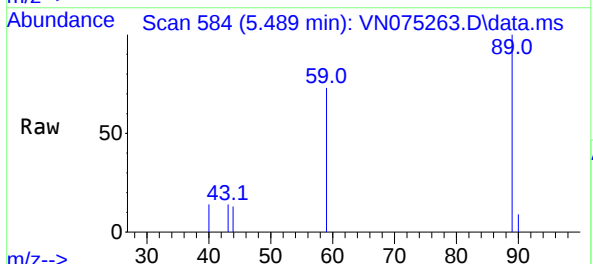




#16
Acetone
Concen: 3.960 ug/l
RT: 4.459 min Scan# 406
Delta R.T. 0.017 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion: 43 Resp: 4486
Ion Ratio Lower Upper
43 100
58 39.5 25.5 38.3#

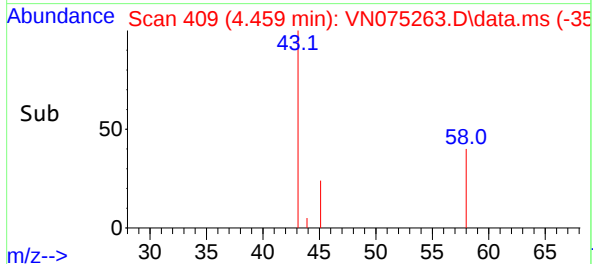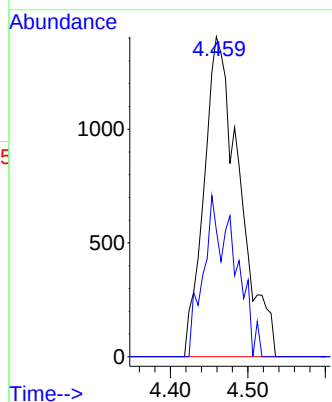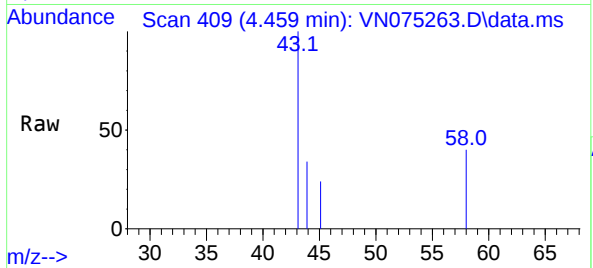

#18
Methyl Acetate
Concen: 1.912 ug/l
RT: 5.047 min Scan# 509
Delta R.T. 0.005 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 43 Resp: 7074
Ion Ratio Lower Upper
43 100
74 24.8 22.0 33.0


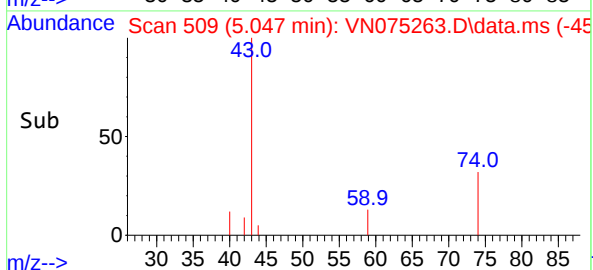






#19
Methyl tert-butyl Ether
Concen: 0.216 ug/l
RT: 5.806 min Scan# 61
Delta R.T. 0.000 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion: 73 Resp: 1691
Ion Ratio Lower Upper
73 100
57 0.0 16.3 24.5#

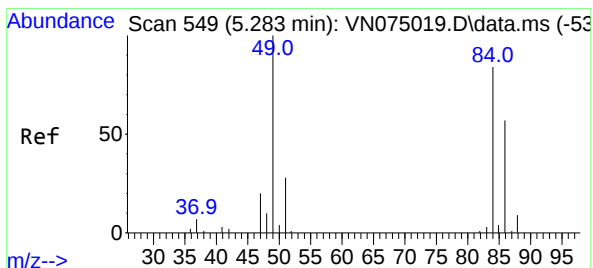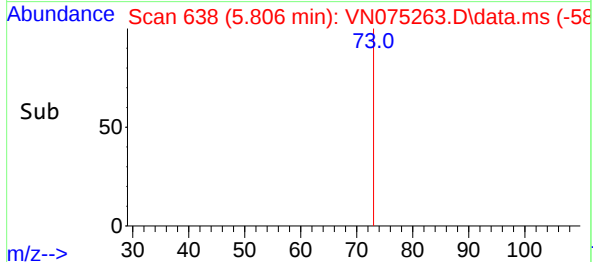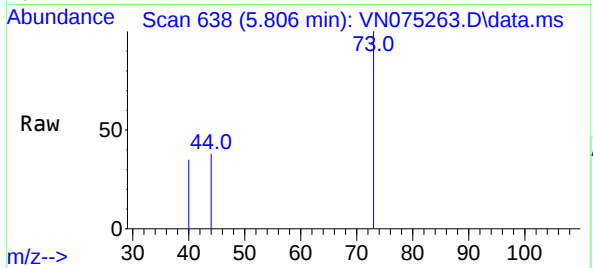

#20
Methylene Chloride
Concen: 1.852 ug/l
RT: 5.271 min Scan# 547
Delta R.T. -0.012 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 84 Resp: 4678
Ion Ratio Lower Upper
84 100
49 69.2 94.9 142.3#
51 21.7 26.8 40.2#
86 54.6 53.7 80.5


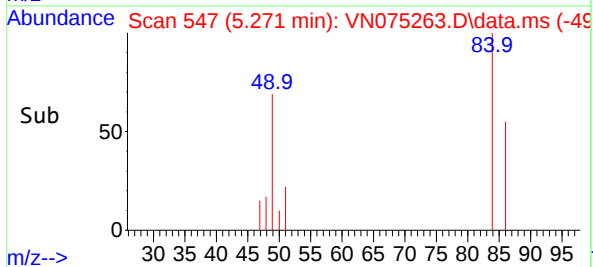

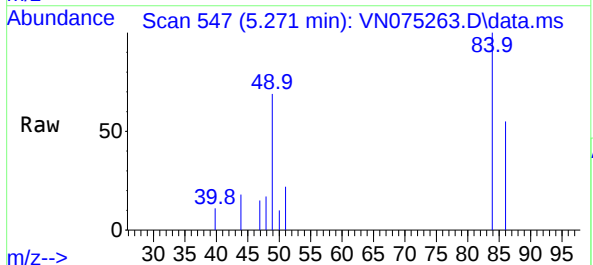




#23
 Vinyl Acetate
 Concen: 0.466 ug/l
 RT: 6.724 min Scan# 794
 Delta R.T. 0.112 min
 Lab File: VN075263.D
 Acq: 14 Nov 2022 14:16




Instrument :
 MSVOA_N
 ClientSampleId :
 AUD-1732


Tgt Ion: 43 Resp: 2639
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.7 16.1#

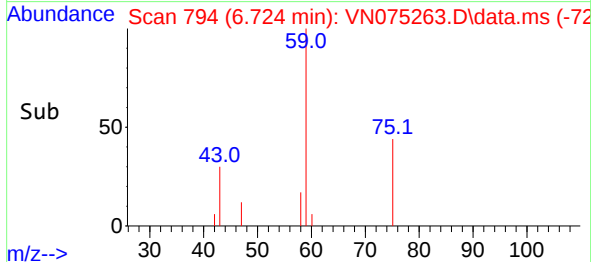

#25
 2-Butanone
 Concen: 2.189 ug/l
 RT: 7.494 min Scan# 925
 Delta R.T. 0.000 min
 Lab File: VN075263.D
 Acq: 14 Nov 2022 14:16

Tgt Ion: 43 Resp: 3900
 Ion Ratio Lower Upper
 43 100
 72 27.7 25.5 38.3

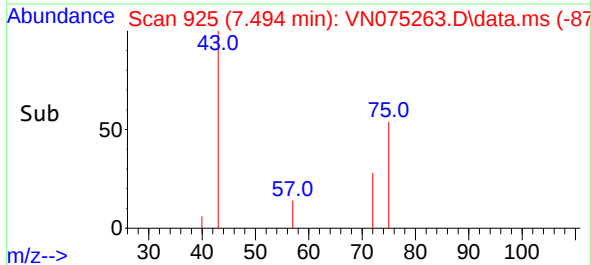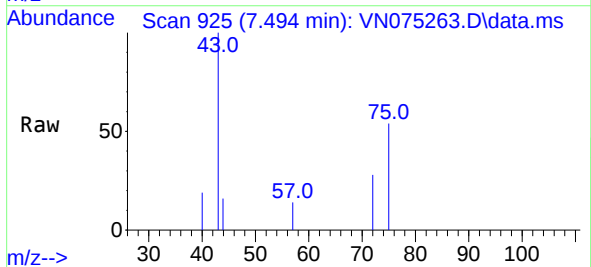



#29

Tetrahydrofuran

Concen: 0.231 ug/l

RT: 7.853 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN075263.D

Acq: 14 Nov 2022 14:16

Instrument :

MSVOA_N

ClientSampleId :

AUD-1732





Tgt Ion: 42 Resp: 266

Ion Ratio Lower Upper

42 100

72 0.0 43.0 64.6#

71 0.0 39.9 59.9#

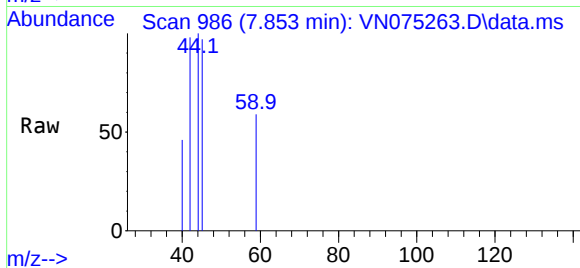

#31

Cyclohexane

Concen: 1.095 ug/l

RT: 8.218 min Scan# 1048

Delta R.T. -0.041 min

Lab File: VN075263.D

Acq: 14 Nov 2022 14:16




Tgt Ion: 56 Resp: 4356


Ion Ratio Lower Upper

56 100

69 151.2 25.2 37.8#

84 120.1 77.8 116.8#

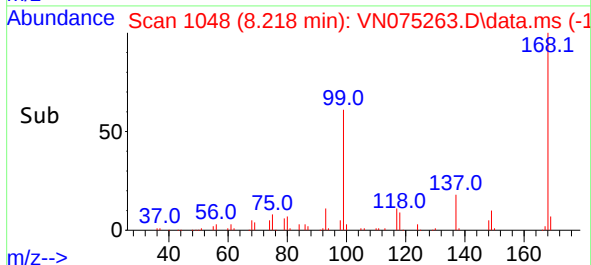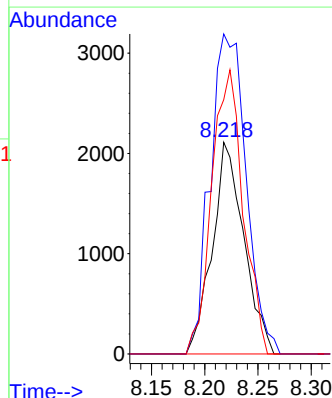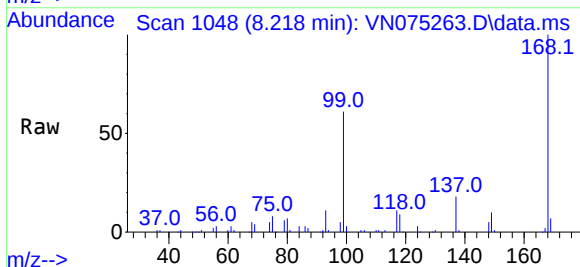



#33

1,2-Dichloroethane-d4

Concen: 48.768 ug/l

RT: 8.577 min Scan# 1111

Delta R.T. -0.011 min

Lab File: VN075263.D

Acq: 14 Nov 2022 14:16

Instrument :

MSVOA_N

ClientSampleId :





AUD-1732

Tgt Ion: 65 Resp: 130473

Ion Ratio Lower Upper

65 100

67 52.3 0.0 102.0

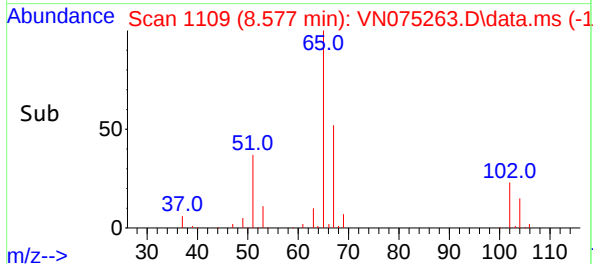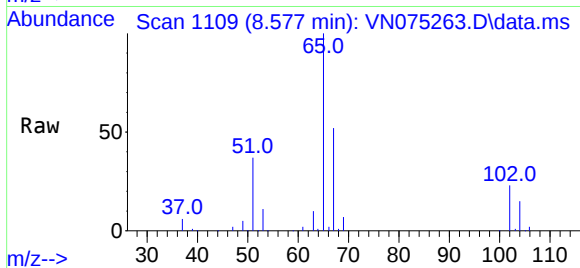

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1198

Delta R.T. -0.006 min

Lab File: VN075263.D

Acq: 14 Nov 2022 14:16




Tgt Ion: 114 Resp: 356075


Ion Ratio Lower Upper

114 100

63 18.5 0.0 39.6


88 14.7 0.0 29.0

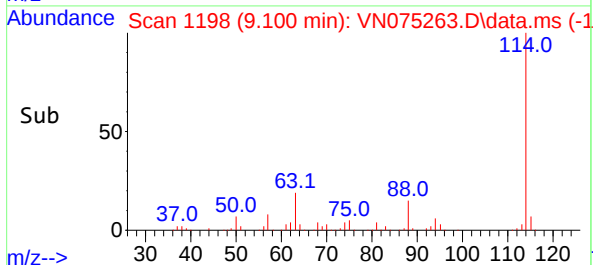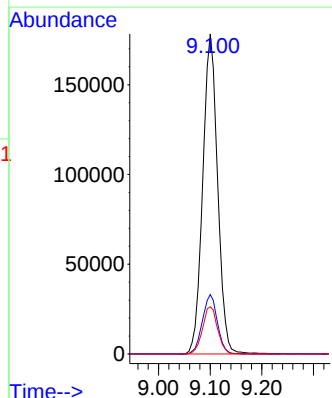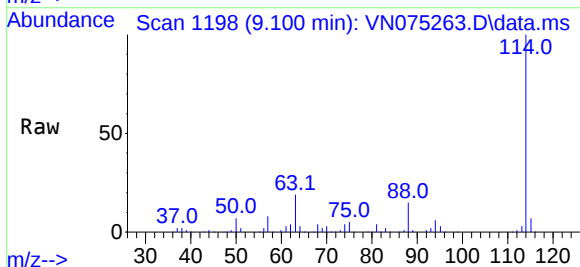



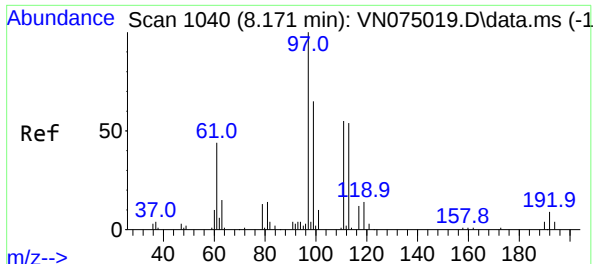


#35
Dibromofluoromethane
Concen: 55.340 ug/l
RT: 8.171 min Scan# 1040
Delta R.T. -0.000 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16


Instrument :
MSVOA_N
ClientSampleId :
AUD-1732

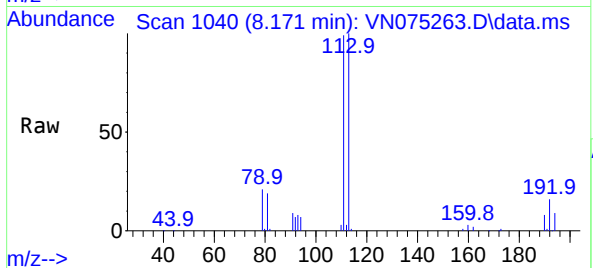



Tgt Ion:113 Resp: 115680
Ion Ratio Lower Upper
113 100
111 101.5 80.5 120.7
192 16.9 13.2 19.8

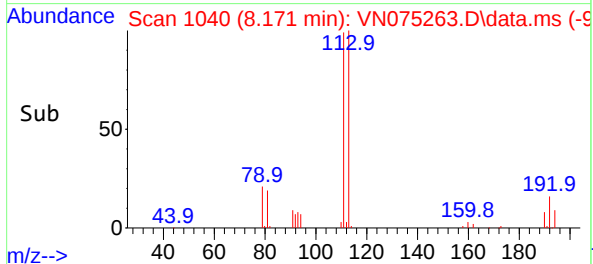


#36
1,1-Dichloropropene
Concen: 4.879 ug/l
RT: 8.224 min Scan# 1049
Delta R.T. -0.153 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

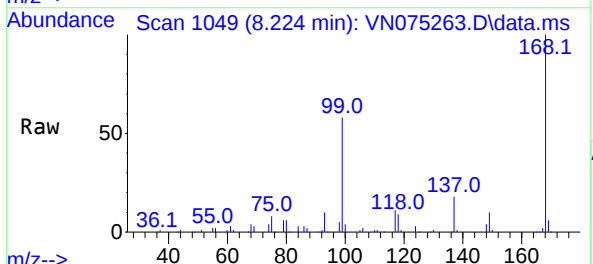

Tgt Ion: 75 Resp: 15788
Ion Ratio Lower Upper
75 100
110 9.1 17.8 53.3#
77 0.0 24.6 37.0#



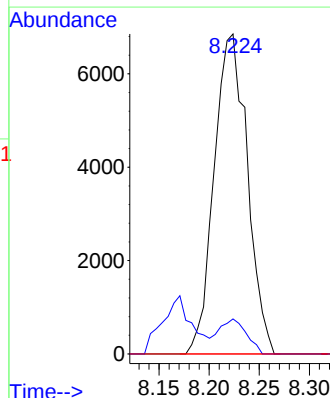
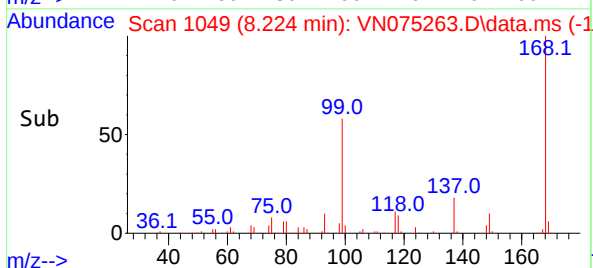




#37
Ethyl Acetate
Concen: 1.099 ug/l
RT: 7.494 min Scan# 91
Delta R.T. -0.077 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion: 43 Resp: 3900
Ion Ratio Lower Upper
43 100
61 0.0 12.2 18.4#
70 0.0 9.4 14.2#



#38
Carbon Tetrachloride
Concen: 6.061 ug/l
RT: 8.218 min Scan# 1048
Delta R.T. -0.153 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 117 Resp: 21576
Ion Ratio Lower Upper
117 100
119 4.4 76.7 115.1#
121 0.0 23.9 35.9#


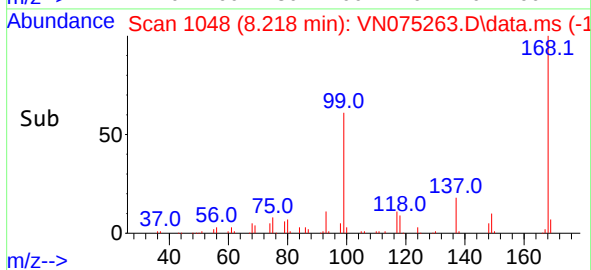






#43
Isopropyl Acetate
Concen: 1.034 ug/l
RT: 8.794 min Scan# 1129
Delta R.T. 0.100 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion: 43 Resp: 5692
Ion Ratio Lower Upper
43 100
61 0.0 22.4 33.6#
87 0.0 12.5 18.7#

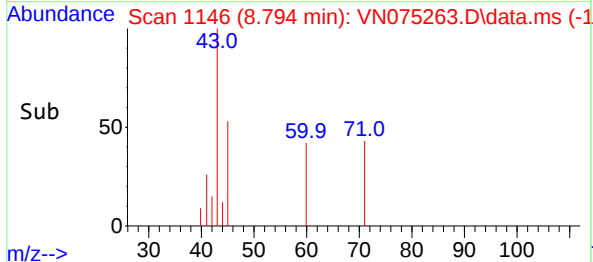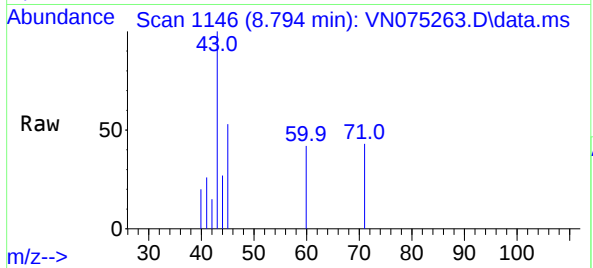

#48
Methyl methacrylate
Concen: 0.383 ug/l
RT: 9.665 min Scan# 1294
Delta R.T. -0.017 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 41 Resp: 968
Ion Ratio Lower Upper
41 100
69 0.0 80.2 120.2#
39 12.6 56.2 84.2#


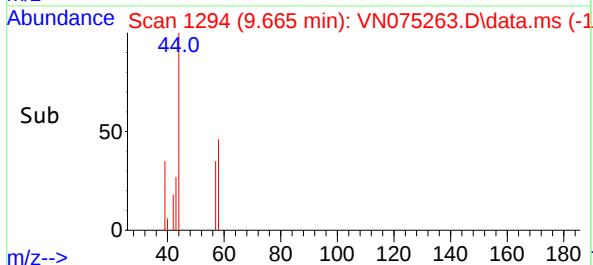
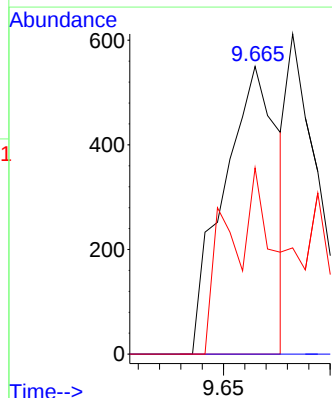
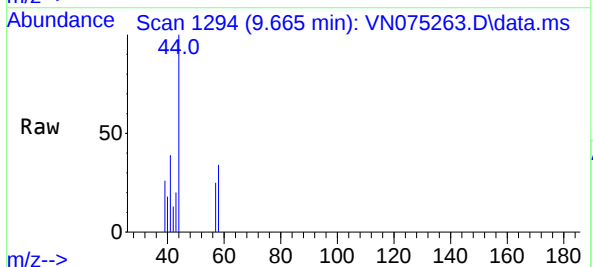




#50
Toluene-d8
Concen: 47.595 ug/l
RT: 10.565 min Scan# 1448
Delta R.T. -0.006 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion: 98 Resp: 385992
Ion Ratio Lower Upper
98 100
100 65.9 53.0 79.6



#51
4-Methyl-2-Pentanone
Concen: 0.212 ug/l
RT: 10.453 min Scan# 1428
Delta R.T. 0.006 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 43 Resp: 754
Ion Ratio Lower Upper
43 100
58 18.0 33.6 50.4#


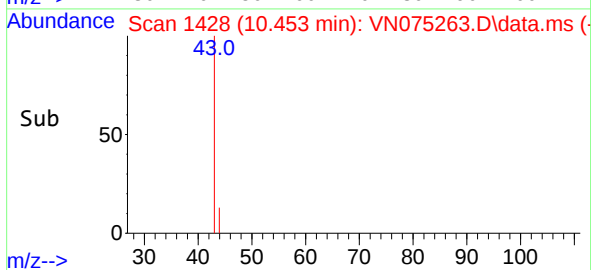






#53
t-1,3-Dichloropropene
Concen: 0.801 ug/l
RT: 10.688 min Scan# 1468
Delta R.T. -0.153 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion: 75 Resp: 3009
Ion Ratio Lower Upper
75 100
77 10.5 25.4 38.2#

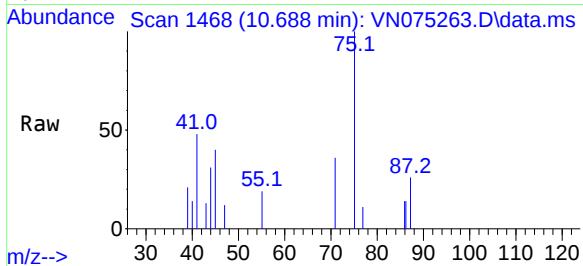

#59
2-Hexanone
Concen: 0.597 ug/l
RT: 11.200 min Scan# 1555
Delta R.T. 0.000 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 43 Resp: 1609
Ion Ratio Lower Upper
43 100
58 48.9 29.6 88.8


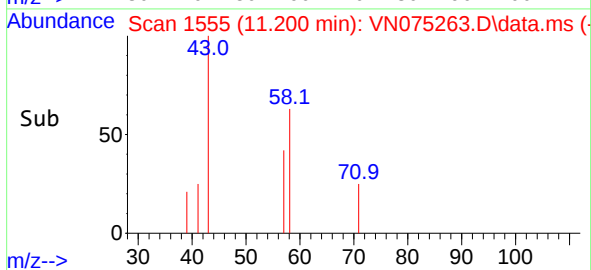

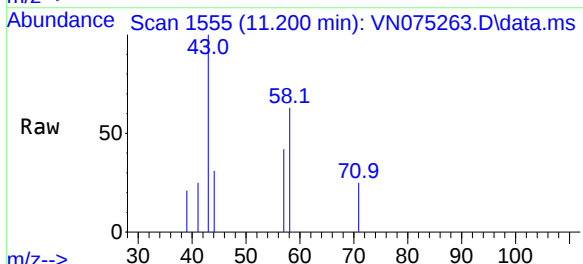




#62
4-Bromofluorobenzene
Concen: 47.776 ug/l
RT: 12.847 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion: 95 Resp: 136109
Ion Ratio Lower Upper
95 100
174 76.5 0.0 147.4
176 73.7 0.0 142.2



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1668
Delta R.T. -0.006 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 117 Resp: 302066
Ion Ratio Lower Upper
117 100
82 55.5 43.1 64.7
119 32.2 25.5 38.3





#67

Ethyl Benzene

Concen: 0.260 ug/l

RT: 11.965 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN075263.D

Acq: 14 Nov 2022 14:16

Instrument :

MSVOA_N

ClientSampleId :





AUD-1732

Tgt Ion: 91 Resp: 3020

Ion Ratio Lower Upper

91 100

106 36.5 24.9 37.3



#68

m/p-Xylenes

Concen: 1.495 ug/l

RT: 12.071 min Scan# 1703

Delta R.T. -0.005 min

Lab File: VN075263.D




Acq: 14 Nov 2022 14:16


Tgt Ion:106 Resp: 6960

Ion Ratio Lower Upper

106 100

91 197.2 156.0 234.0



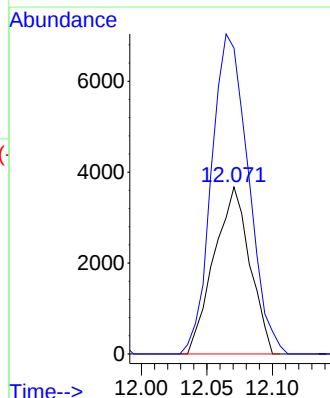





#69
o-Xylene
Concen: 0.545 ug/l
RT: 12.400 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion:106 Resp: 2509
Ion Ratio Lower Upper
106 100
91 219.8 105.2 315.5



#71
Bromoform
Concen: 0.543 ug/l
RT: 12.847 min Scan# 1835
Delta R.T. 0.265 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion:173 Resp: 973
Ion Ratio Lower Upper
173 100
175 684.0 24.6 74.0#
254 0.0 0.0 0.0


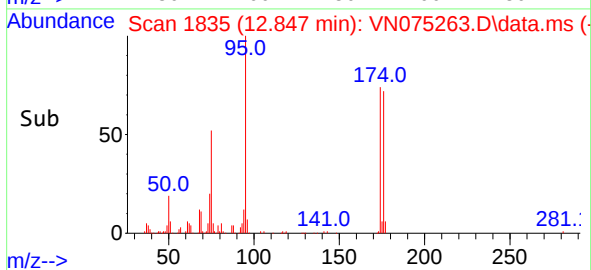






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 1995
Delta R.T. -0.006 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion:152 Resp: 137719
Ion Ratio Lower Upper
152 100
115 62.2 30.2 90.6
150 157.0 0.0 348.4

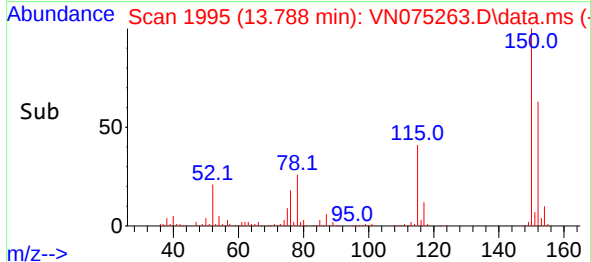

#74
N-ethyl acetate
Concen: 0.527 ug/l
RT: 12.459 min Scan# 1769
Delta R.T. -0.035 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 43 Resp: 2154
Ion Ratio Lower Upper
43 100
70 0.0 39.8 59.8#
55 4.4 19.9 29.9#
61 0.0 21.7 32.5#


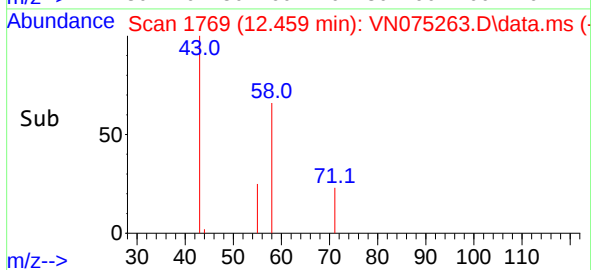






#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.947 min Scan# 1851
Delta R.T. 0.006 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion: 83 Resp: 1536
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.3#
85 3.5 31.6 94.7#

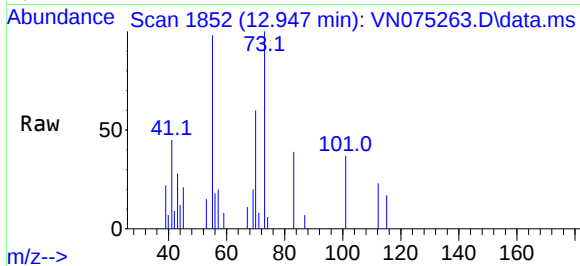

#76
1,2,3-Trichloropropane
Concen: 0.914 ug/l
RT: 13.088 min Scan# 1876
Delta R.T. 0.094 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 75 Resp: 2673
Ion Ratio Lower Upper
75 100
77 5.5 75.6 226.8#




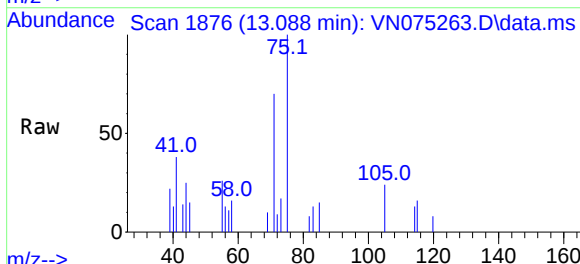




#81
trans-1,4-Dichloro-2-butene
Concen: 62.767 ug/l
RT: 12.847 min Scan# 1817
Delta R.T. 0.106 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16




Instrument :
MSVOA_N
ClientSampleId :
AUD-1732


Tgt Ion: 75 Resp: 71500
Ion Ratio Lower Upper
75 100
53 0.0 78.5 117.7#
89 0.1 37.7 56.5#

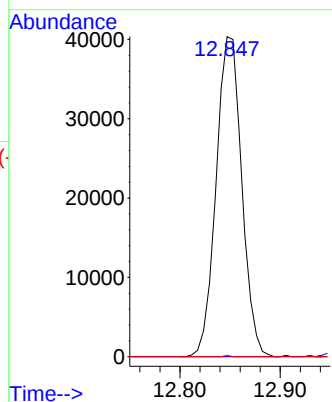

#84
1,2,4-Trimethylbenzene
Concen: 0.257 ug/l
RT: 13.482 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN075263.D
Acq: 14 Nov 2022 14:16

Tgt Ion: 105 Resp: 2414
Ion Ratio Lower Upper
105 100
120 39.0 22.7 68.1

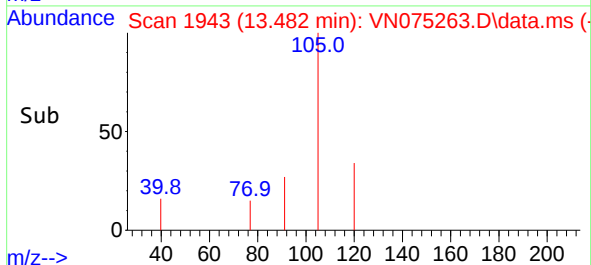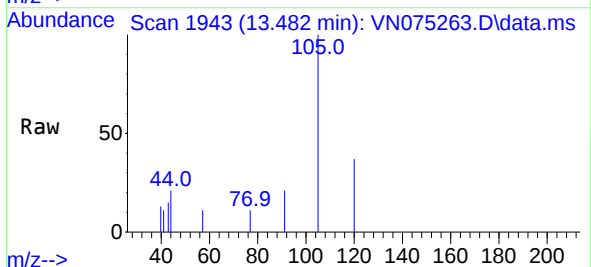



#92

1,2-Dibromo-3-Chloropropane

Concen: 1.184 ug/l

RT: 14.882 min Scan# 2153

Delta R.T. 0.165 min

Lab File: VN075263.D

Acq: 14 Nov 2022 14:16

Instrument :

MSVOA_N

ClientSampleId :

AUD-1732





Tgt Ion: 75 Resp: 883

Ion Ratio Lower Upper

75 100

155 0.0 42.1 126.3#

157 0.0 51.7 155.1#

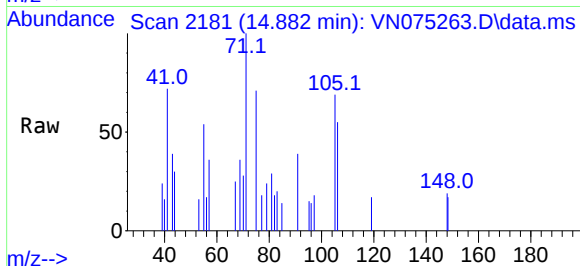

#95

Napthalene

Concen: 0.464 ug/l

RT: 15.635 min Scan# 2309

Delta R.T. -0.006 min

Lab File: VN075263.D

Acq: 14 Nov 2022 14:16

Tgt Ion: 128 Resp: 3635

Ion Ratio Lower Upper

128 100

127 7.8 10.4 15.6#

129 0.0 8.6 12.8#

