
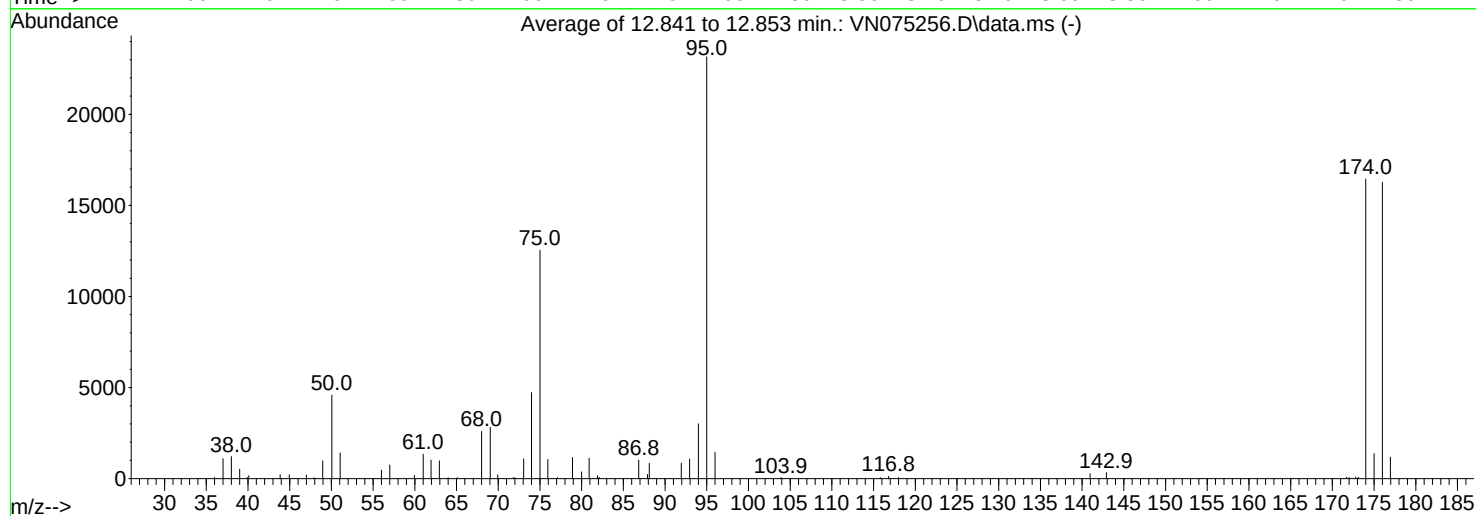


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111422\
 Data File : VN075256.D
 Acq On : 14 Nov 2022 10:00
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
 Title : SW846 8260
 Last Update : Thu Oct 27 09:48:49 2022

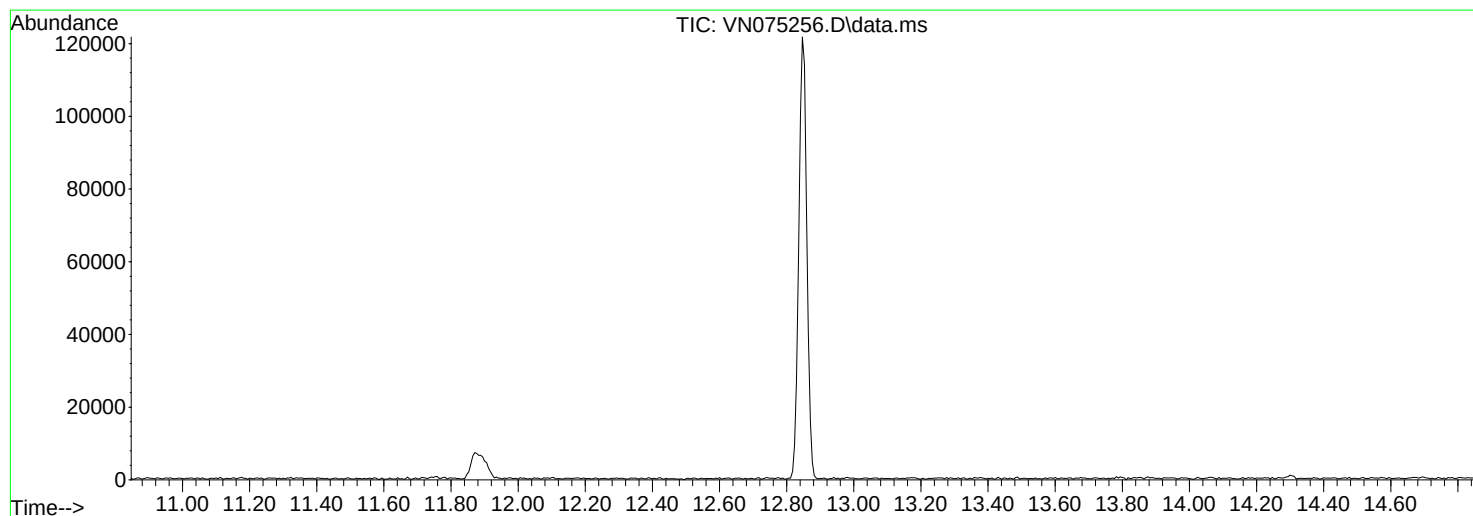

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	4584	PASS
75	95	30	60	54.2	12547	PASS
95	95	100	100	100.0	23155	PASS
96	95	5	9	6.3	1448	PASS
173	174	0.00	2	0.5	86	PASS
174	95	50	100	71.0	16441	PASS
175	174	5	9	8.4	1374	PASS
176	174	95	101	99.0	16269	PASS
177	176	5	9	7.3	1180	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	61	50.05	4584	69.05	2822	80.90	1114
37.00	1100	51.05	1416	69.95	209	81.90	15
38.00	1212	56.00	474	71.80	50	82.10	7
39.00	522	57.00	743	72.00	54	86.85	101
39.90	73	59.95	179	73.05	1093	87.90	229
40.10	164	61.00	1341	74.00	4729	88.10	841
43.85	224	61.95	1019	75.00	12547	91.95	856
44.95	215	62.95	978	75.95	1054	92.95	1077
47.00	202	64.00	54	77.10	59	94.00	3009
47.90	52	65.10	52	78.90	1159	95.00	23155
48.95	975	68.00	2593	80.00	373	96.00	1448

Average of 12.841 to 12.853 min.: VN075256.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.90	59	175.00	1374				
115.80	65	176.00	16269				
116.80	127	176.95	1180				
118.00	61						
140.95	273						
142.90	337						
171.70	67						
172.00	65						
172.80	86						
173.10	82						
174.00	16441						

Instrument :

MSVOA_N

ClientSampleId :

BFB