
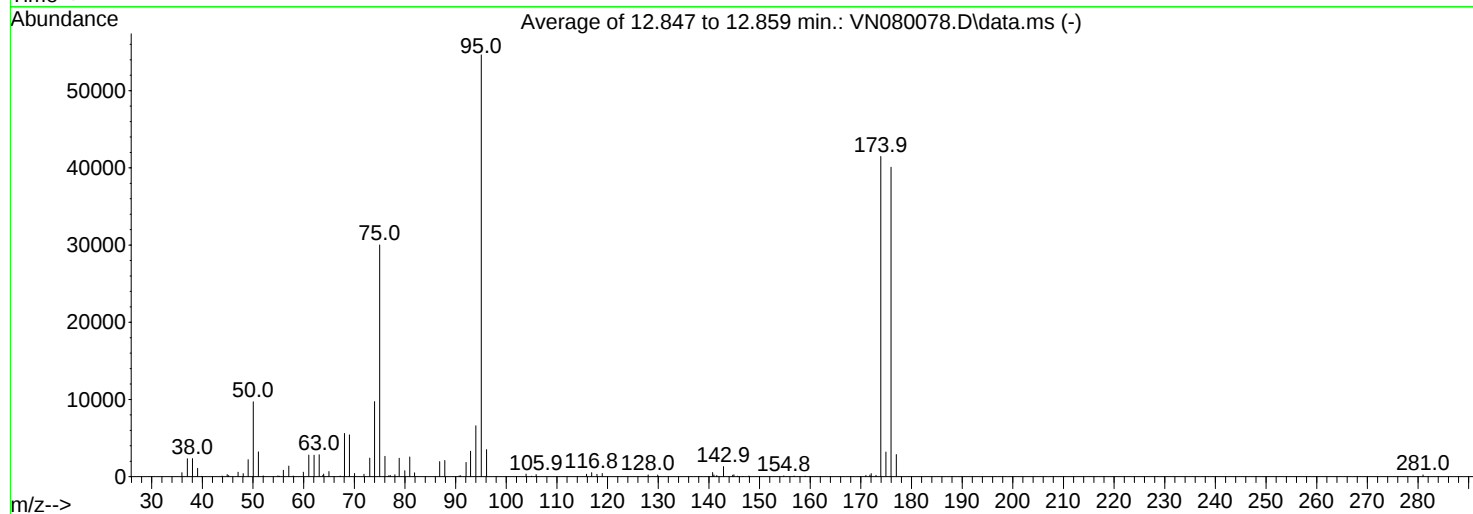


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111423\
Data File : VN080078.D
Acq On : 14 Nov 2023 10:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

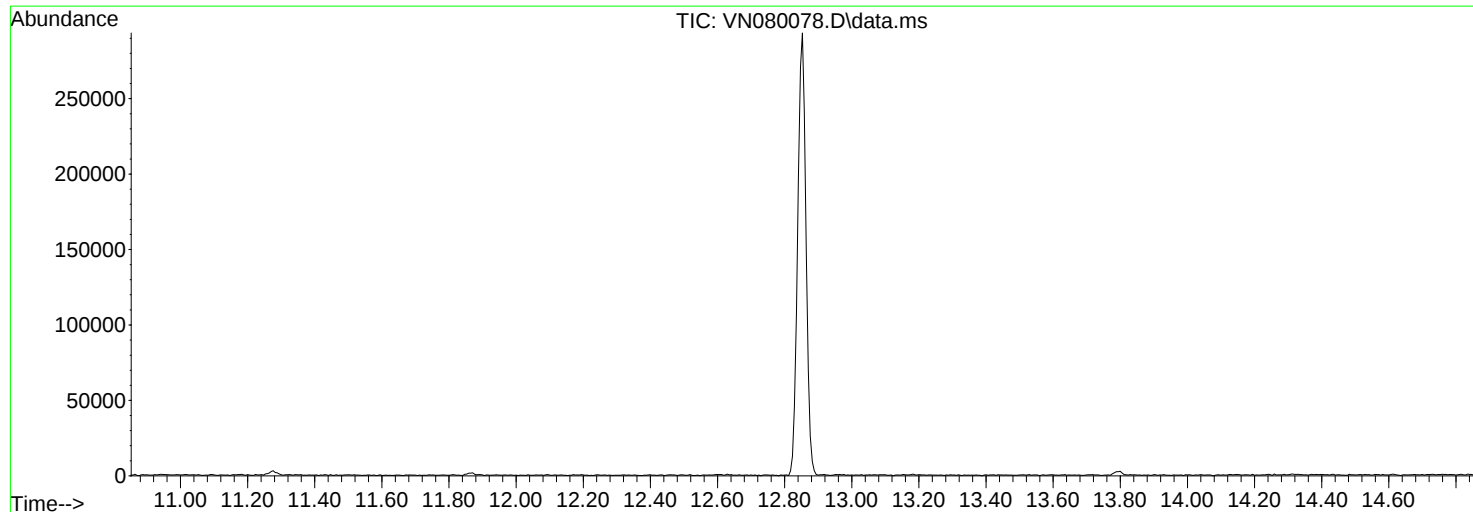

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	9705	PASS
75	95	30	60	54.9	30019	PASS
95	95	100	100	100.0	54640	PASS
96	95	5	9	6.4	3504	PASS
173	174	0.00	2	0.4	173	PASS
174	95	50	100	75.9	41472	PASS
175	174	5	9	7.7	3194	PASS
176	174	95	101	96.7	40096	PASS
177	176	5	9	7.1	2854	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	523	50.05	9705	63.05	2850	75.00	3001
37.05	2323	51.05	3207	63.80	168	76.05	262
38.05	2338	52.00	113	63.95	339	76.80	12
39.05	1084	54.90	111	65.00	667	77.10	16
39.85	53	55.20	60	67.20	82	78.00	243
43.90	91	56.00	836	68.05	5606	78.85	2389
44.90	263	57.05	1372	69.05	5414	79.95	766
45.20	154	57.90	78	70.05	425	80.95	2543
47.05	572	59.95	591	71.90	318	81.90	494
48.05	400	61.00	2792	73.05	2412	86.85	1955
49.05	2188	62.05	2786	74.00	9720	87.85	2085

Average of 12.847 to 12.859 min.: VN080078.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.70	100	116.85	518	145.70	73	174.95	3194
91.00	123	117.90	308	146.70	50	175.95	40096
92.05	1852	118.95	415	147.90	92	177.00	2854
92.95	3301	128.00	224	154.80	110	281.00	228
94.00	6589	129.90	204	156.80	86		
95.05	54640	140.75	541	159.00	62		
96.10	3504	141.00	237	171.00	177		
103.90	341	141.55	138	171.80	199		
105.00	66	142.90	1305	172.05	396		
105.90	279	144.70	189	173.00	173		
115.85	314	144.95	247	173.95	41472		

Instrument :

MSVOA_N

ClientSampleId :

BFB