
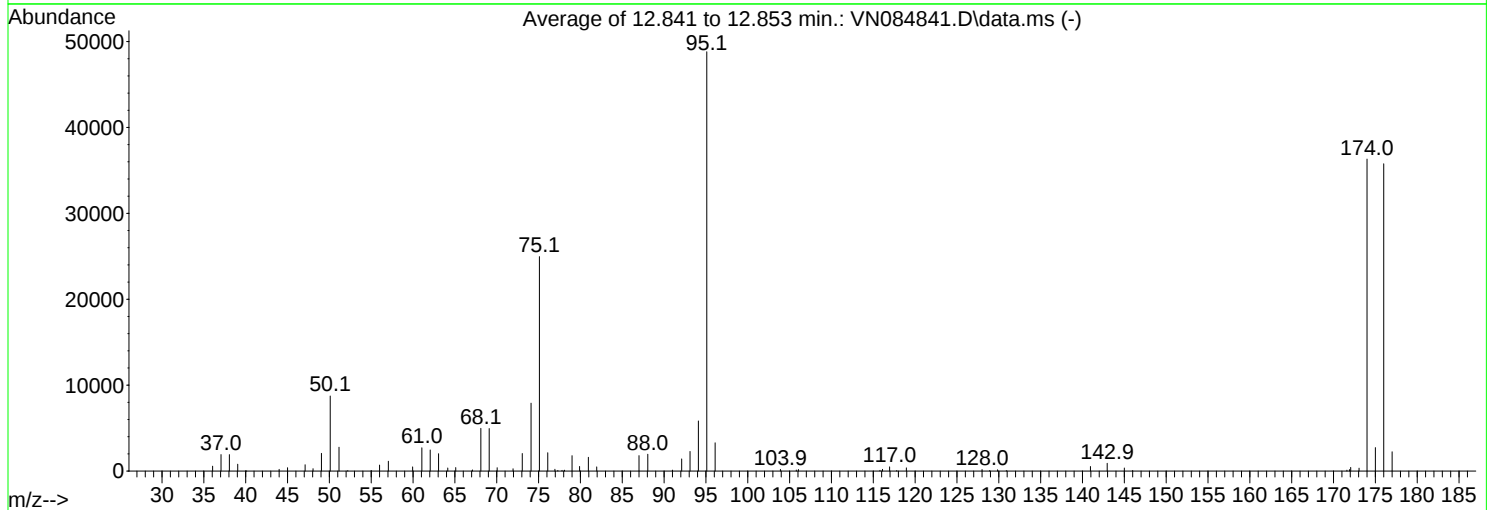


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111424\
Data File : VN084841.D
Acq On : 14 Nov 2024 08:53
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

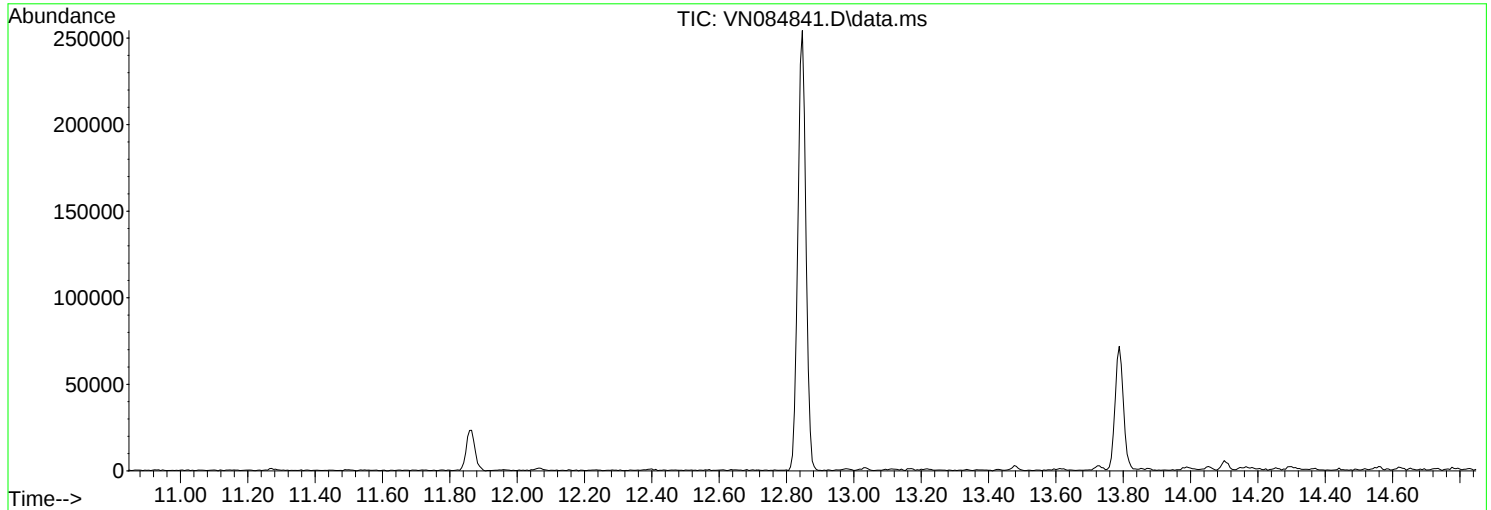

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	8743	PASS
75	95	30	60	51.1	24965	PASS
95	95	100	100	100.0	48816	PASS
96	95	5	9	6.7	3292	PASS
173	174	0.00	2	0.9	342	PASS
174	95	50	100	74.4	36320	PASS
175	174	5	9	7.5	2732	PASS
176	174	95	101	98.5	35773	PASS
177	176	5	9	6.3	2248	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	573	51.15	2779	67.10	137	77.80	83
37.05	1922	52.20	62	68.10	4973	78.10	109
38.05	1917	55.00	60	69.10	4952	79.00	179
39.05	801	56.00	699	70.05	391	79.90	537
40.00	0	57.05	1148	71.95	268	80.95	1605
44.00	200	59.95	489	73.05	2046	81.95	489
45.00	392	61.05	2708	74.10	7908	87.00	1799
47.10	736	62.05	2461	75.10	24965	88.05	1961
48.05	282	63.05	2024	76.10	2136	91.00	112
49.05	2064	64.15	360	76.95	213	92.10	1414
50.10	8743	65.10	407	77.30	73	93.10	2285

Average of 12.841 to 12.853 min.: VN084841.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.10	5835	128.00	178	173.05	342		
95.10	48816	128.90	54	174.00	36320		
96.10	3292	129.85	152	175.00	2732		
103.90	196	130.90	55	176.00	35773		
105.80	123	140.95	532	177.00	2248		
106.05	184	142.95	909				
115.80	88	145.00	360				
116.10	203	146.00	60				
116.95	492	171.60	106				
117.80	59	171.90	173				
118.95	373	172.05	427				

Instrument :

MSVOA_N

ClientSampleId :

BFB