

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN111518\
 Data File : VN052342.D
 Acq On : 15 Nov 2018 15:20
 Operator : MD\SY
 Sample : PB114828ZHE#06
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 14 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 PB114828ZHE#06

Quant Time: Nov 16 03:55:17 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 15 03:02:37 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	322713	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	549300	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	470972	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	163637	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	228928	50.23	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.46%	
35) Dibromofluoromethane	7.59	113	178532	50.39	ug/l	0.00
Spiked Amount 50.000			Recovery	=	100.78%	
50) Toluene-d8	10.09	98	695228	49.88	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.76%	
62) 4-Bromofluorobenzene	12.40	95	198723	43.34	ug/l	0.00
Spiked Amount 50.000			Recovery	=	86.68%	
Target Compounds						
16) Acetone	3.82	43	7165	5.71	ug/l	Qvalue 91
20) Methylene Chloride	4.56	84	13005	2.74	ug/l	94
43) Isopropyl Acetate	8.17	43	25781	3.34	ug/l #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN111518\
Data File : VN052342.D
Acq On : 15 Nov 2018 15:20
Operator : MD\SY
Sample : PB114828ZHE#06
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 14 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
PB114828ZHE#06

Quant Time: Nov 16 03:55:17 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 15 03:02:37 2018
Response via : Initial Calibration

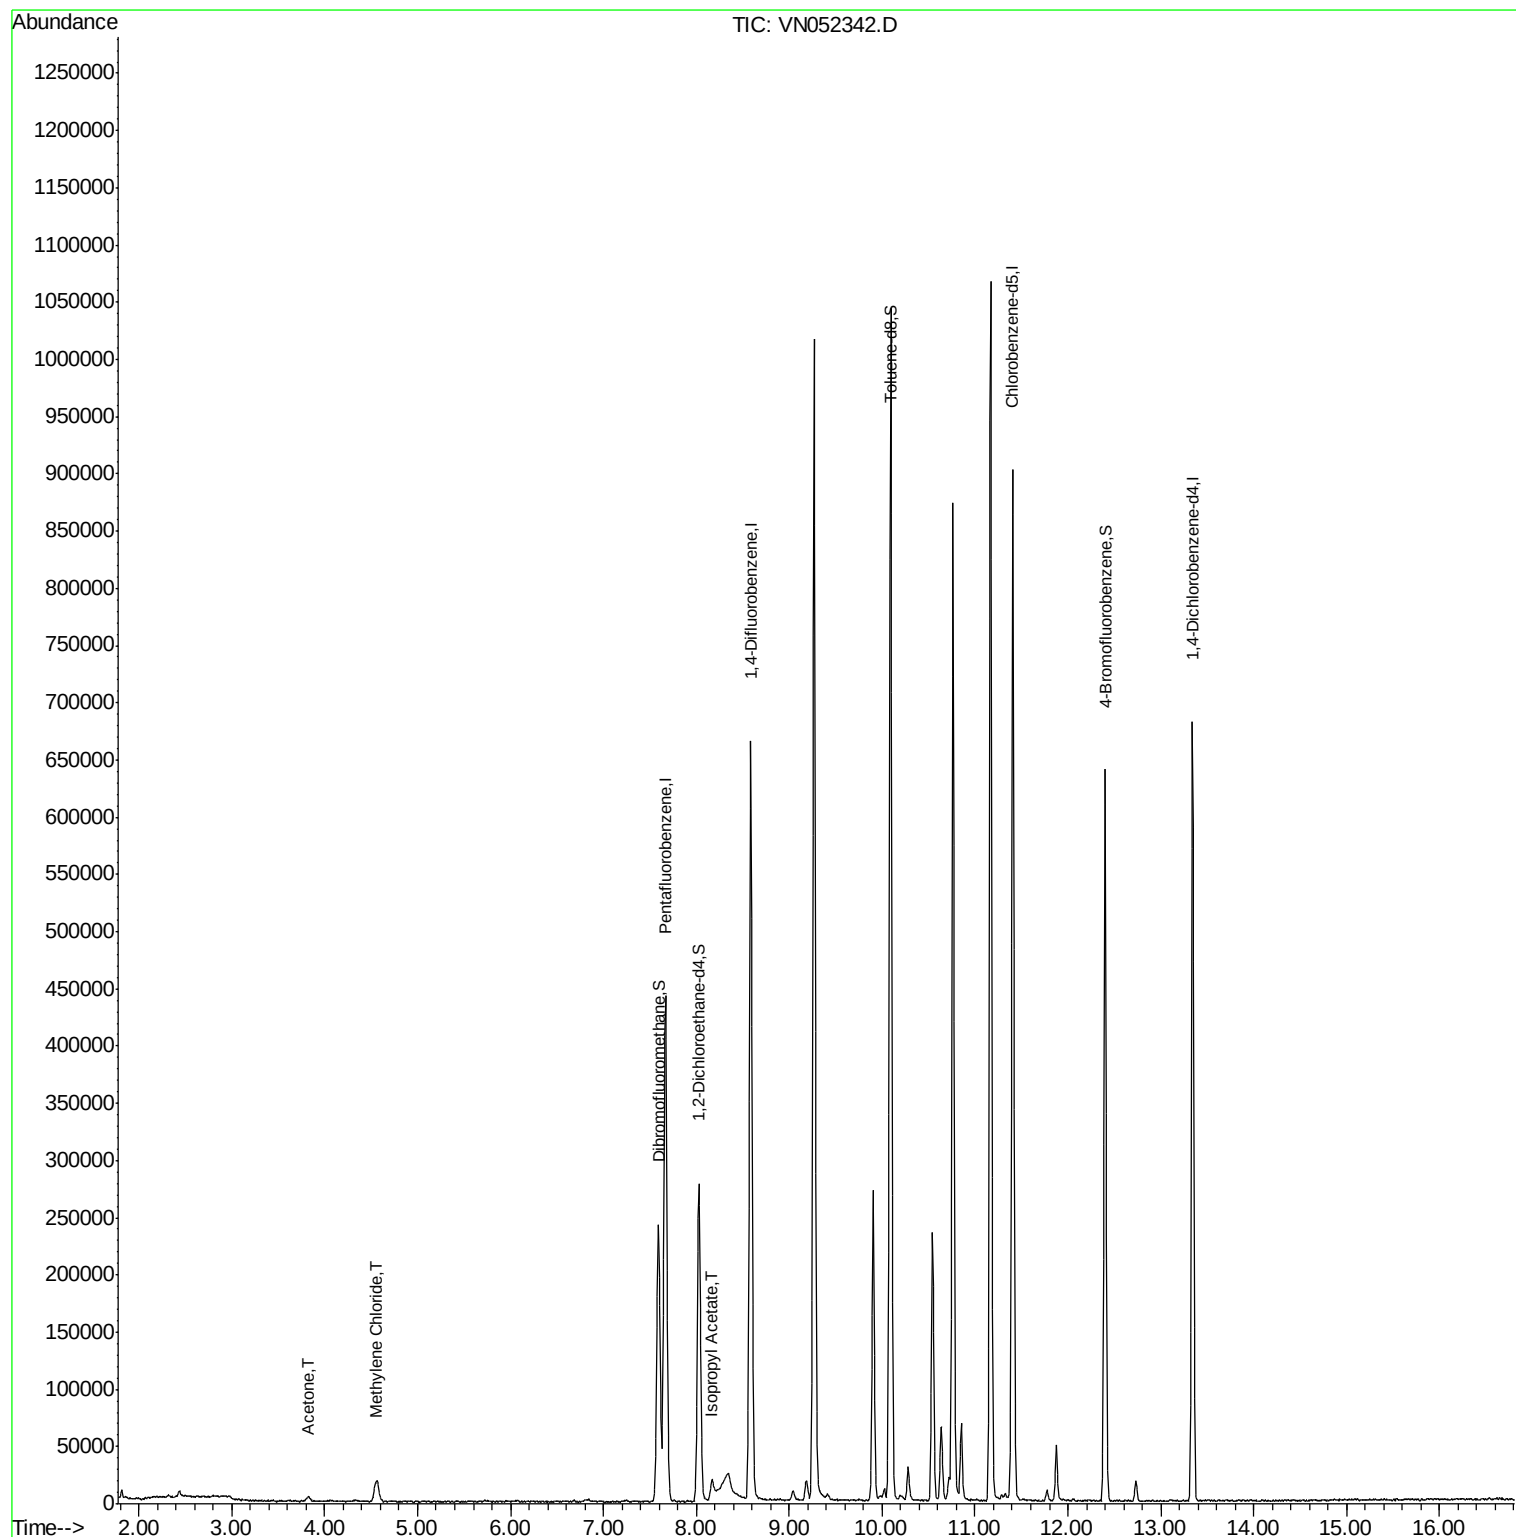

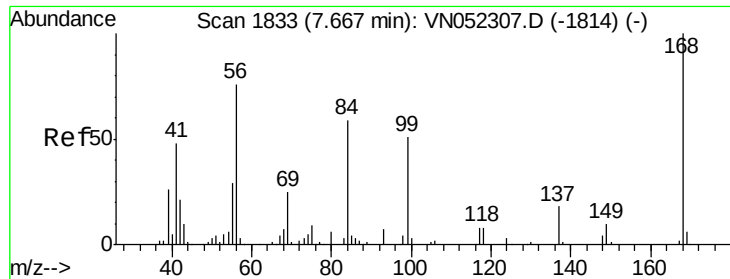

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.00 min

Lab File: VN052342.D

Acq: 15 Nov 2018 15:20

Instrument :

MSVOA_N

ClientSampleId :


PB114828ZHE#06

Tgt Ion:168 Resp: 322713

Ion Ratio Lower Upper

168 100

99 61.7 47.9 71.9

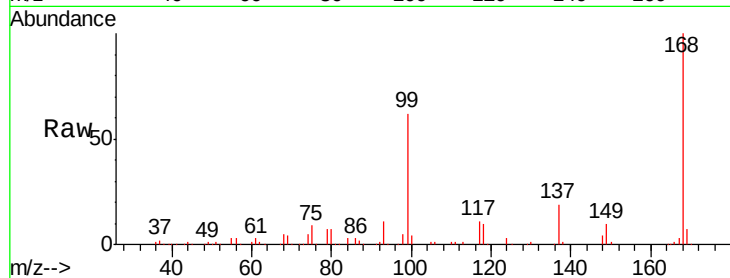

Abundance Ion 167.90 (167.60 to 168.60): VN052307.D (-1814) (-)

Ion 98.90 (98.60 to 99.60): VN052307.D (-1814) (-)

7.67



150000

100000

50000

0

Time-->

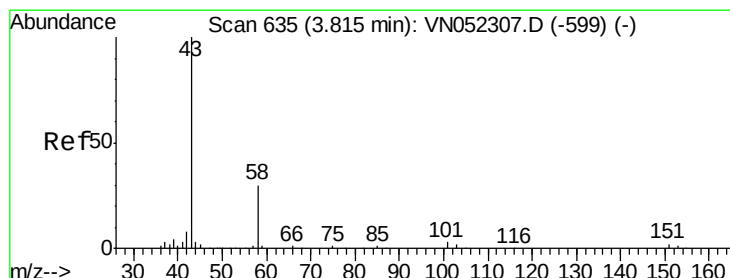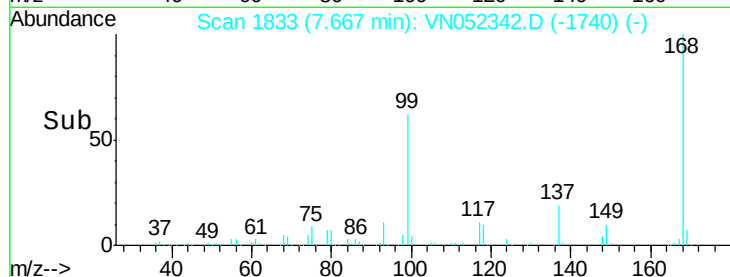

#16

Acetone

Concen: 5.71 ug/l

RT: 3.82 min Scan# 637

Delta R.T. 0.01 min

Lab File: VN052342.D


Acq: 15 Nov 2018 15:20

Tgt Ion: 43 Resp: 7165

Ion Ratio Lower Upper

43 100

58 25.5 24.2 36.4

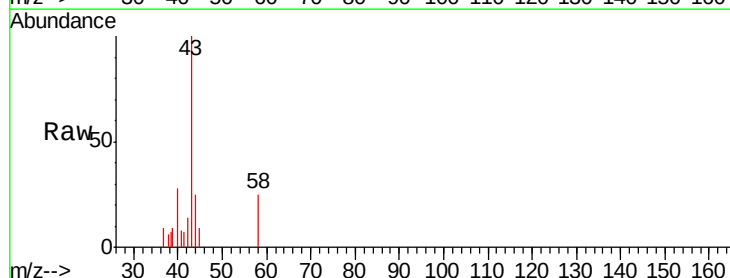

Abundance Ion 43.00 (42.70 to 43.70): VN052307.D (-599) (-)

Ion 58.00 (57.70 to 58.70): VN052307.D (-599) (-)

3.82

3000

2500

2000


1500


1000

500

0

Time-->

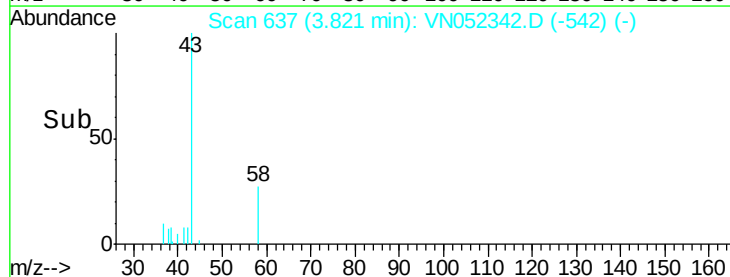


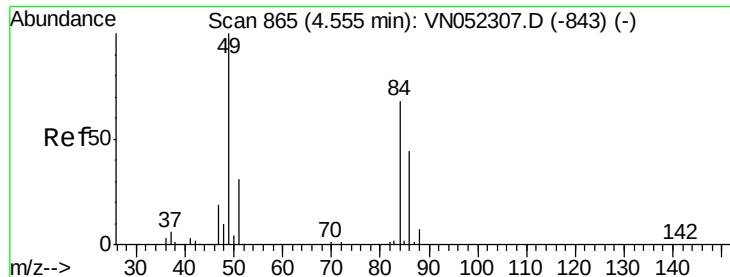




#20
Methylene Chloride
Concen: 2.74 ug/l
RT: 4.56 min Scan# 867
Delta R.T. 0.01 min
Lab File: VN052342.D
Acq: 15 Nov 2018 15:20

Instrument :
MSVOA_N
ClientSampleId :
PB114828ZHE#06

Tgt Ion: 84 Resp: 13005
Ion Ratio Lower Upper
84 100
49 155.5 118.2 177.2
51 45.7 36.1 54.1
86 56.2 51.6 77.4

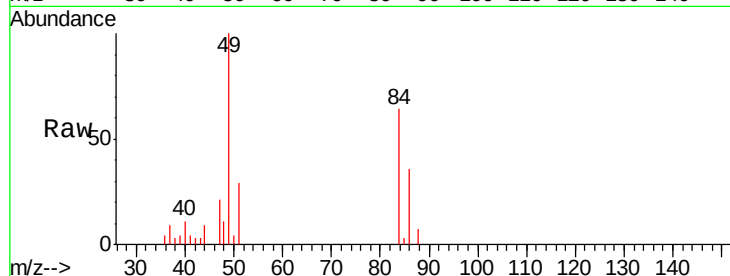


Abundance Ion 83.90 (83.60 to 84.60): VN0
Ion 48.90 (48.60 to 49.60): VN0
Ion 50.90 (50.60 to 51.60): VN0
Ion 85.90 (85.60 to 86.60): VN0

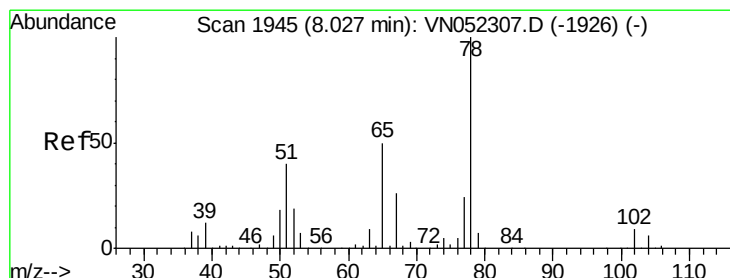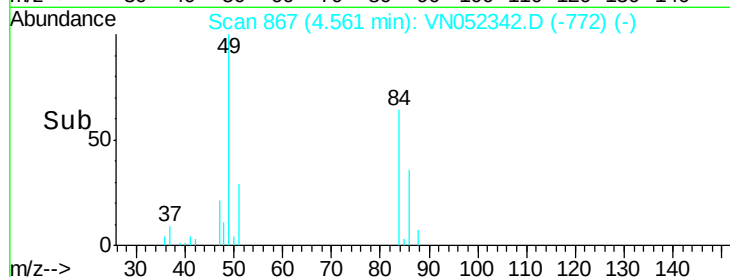
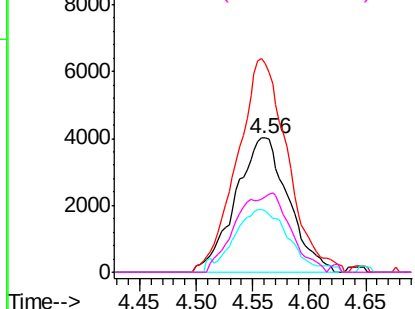



#33
1,2-Dichloroethane-d4
Concen: Below ug/l
RT: 8.03 min Scan# 1945
Delta R.T. -0.00 min
Lab File: VN052342.D
Acq: 15 Nov 2018 15:20

Tgt Ion: 65 Resp: 228928
Ion Ratio Lower Upper
65 100
67 51.9 0.0 105.2

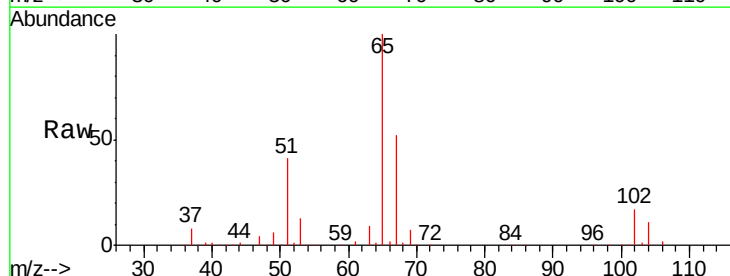

Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

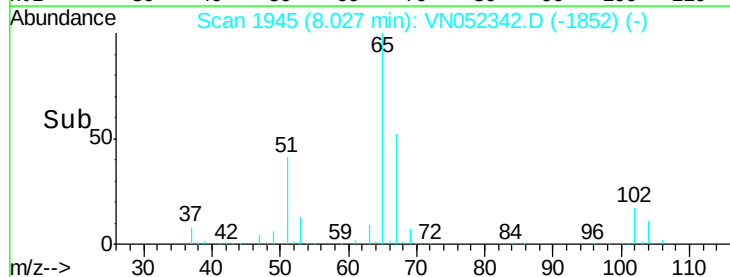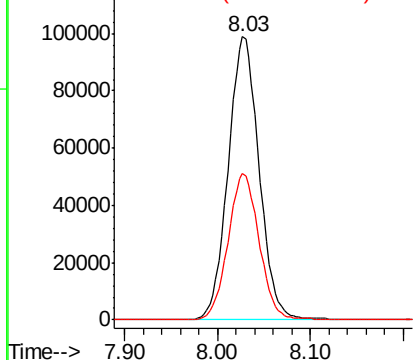


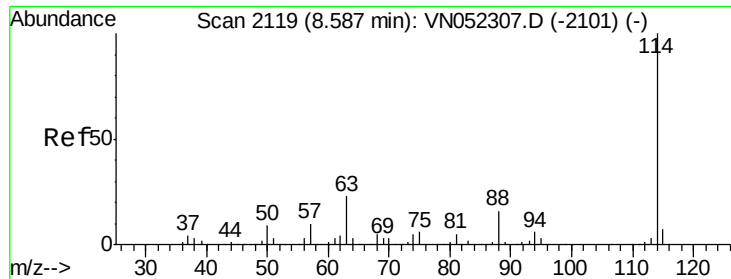




#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN052342.D
 Acq: 15 Nov 2018 15:20

Instrument :
 MSVOA_N
 ClientSampleId :
 PB114828ZHE#06

Tgt Ion:114 Resp: 549300
 Ion Ratio Lower Upper
 114 100
 63 22.2 0.0 45.4
 88 15.7 0.0 31.2

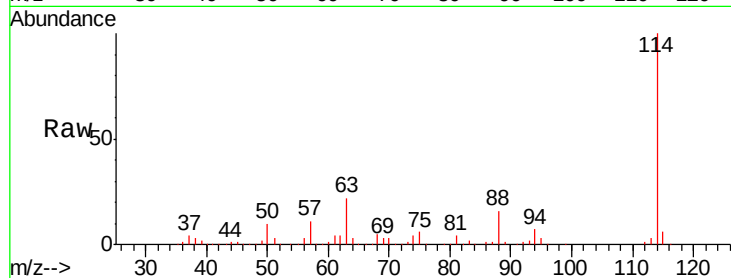


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

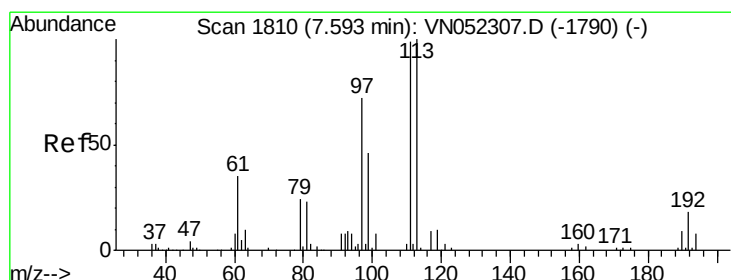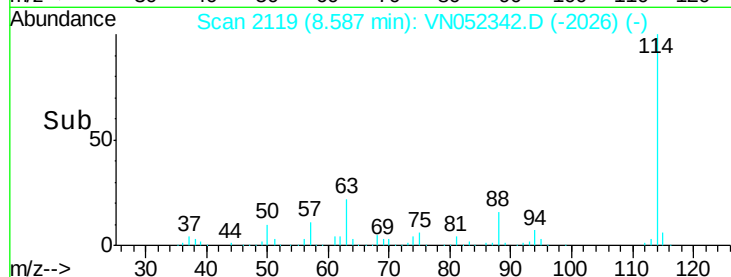
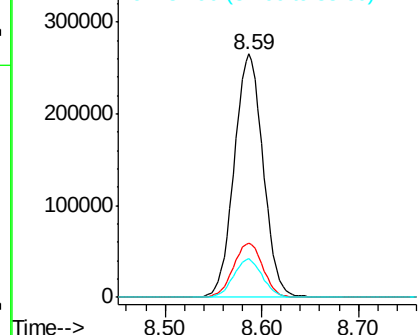



#35
 Dibromofluoromethane
 Concen: 50.00 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. -0.00 min
 Lab File: VN052342.D
 Acq: 15 Nov 2018 15:20

Tgt Ion:113 Resp: 178532
 Ion Ratio Lower Upper
 113 100
 111 102.6 81.0 121.6
 192 17.0 13.8 20.6

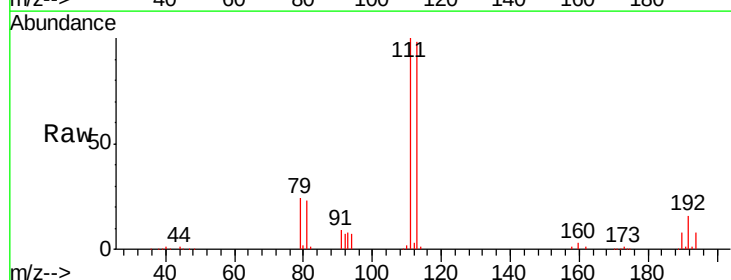

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

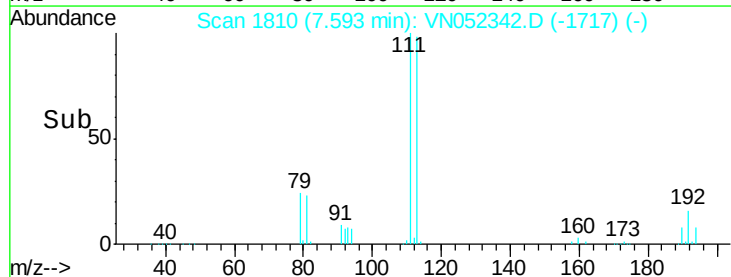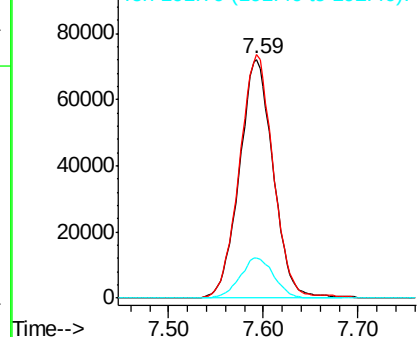

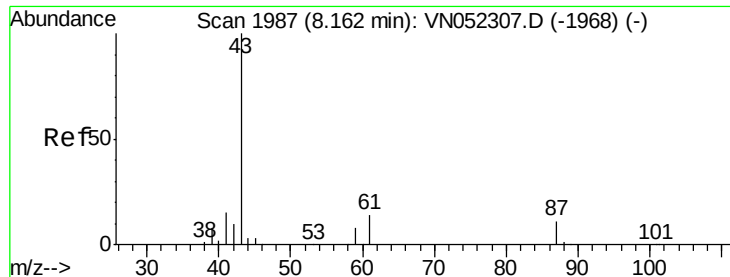

#43

Isopropyl Acetate

Concen: 3.34 ug/l

RT: 8.17 min Scan# 1989

Delta R.T. 0.01 min

Lab File: VN052342.D

Acq: 15 Nov 2018 15:20

Instrument :

MSVOA_N

ClientSampleId :

PB114828ZHE#06


Tgt Ion: 43 Resp: 25781

Ion Ratio Lower Upper

43 100

61 13.1 12.0 18.0




87 8.2 8.3 12.5#

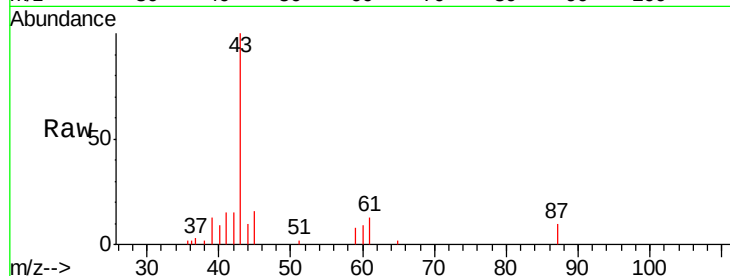

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 61.00 (60.70 to 61.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

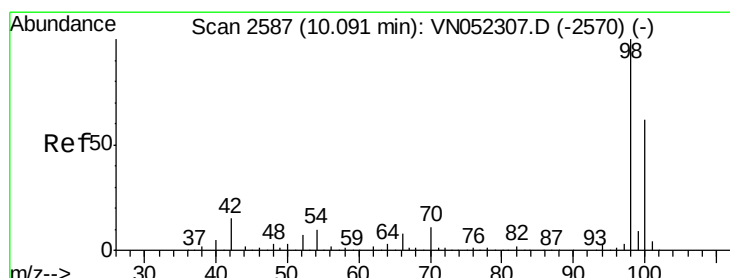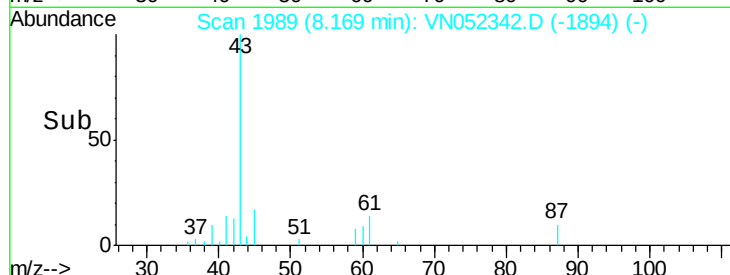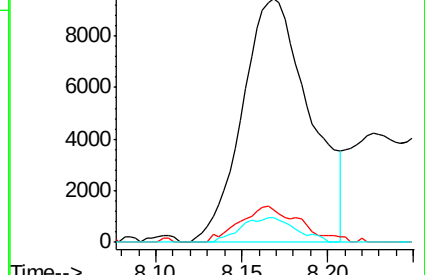

#50

Toluene-d8

Concen: N.D. ug/l

RT: 10.09 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN052342.D


Acq: 15 Nov 2018 15:20

Tgt Ion: 98 Resp: 695228

Ion Ratio Lower Upper



98 100


100 62.1 49.5 74.3

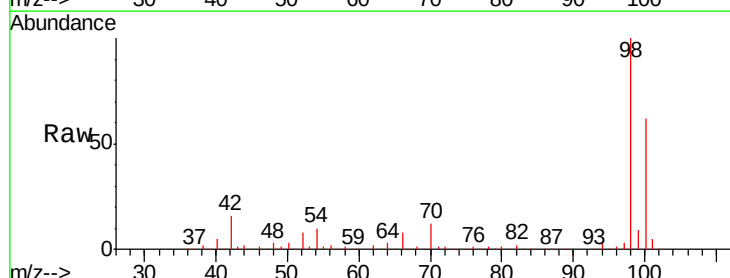

Abundance Ion 98.00 (97.70 to 98.70): VN0

Ion 100.00 (99.70 to 100.70): VN0

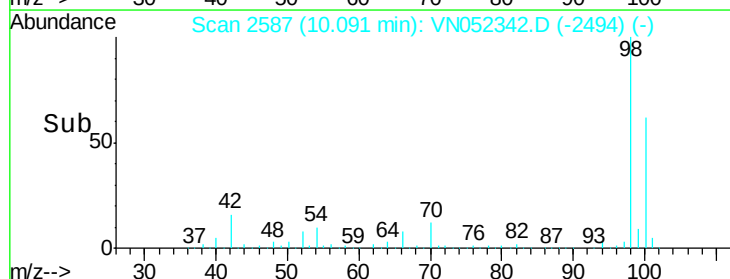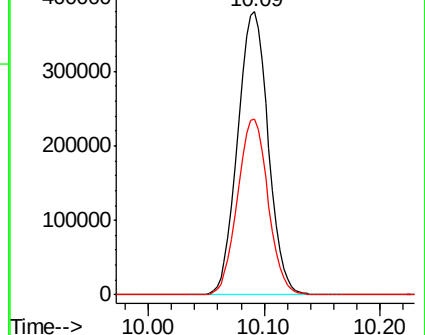

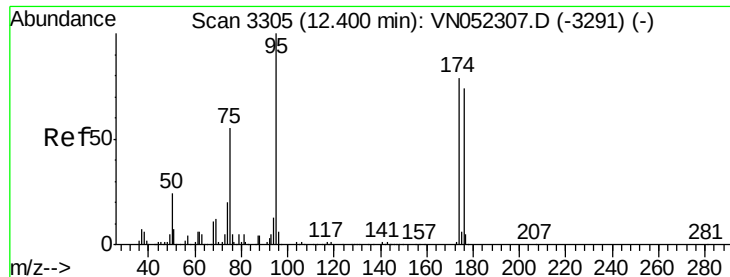

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN052342.D

Acq: 15 Nov 2018 15:20

Instrument :

MSVOA_N

ClientSampleId :

PB114828ZHE#06


Tgt Ion: 95 Resp: 198723

Ion Ratio Lower Upper

95 100

174 77.9 0.0 156.0




176 75.5 0.0 148.4

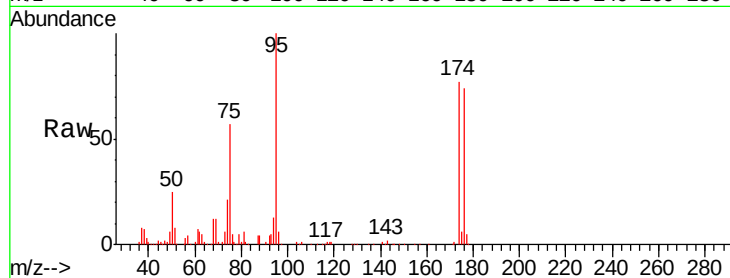

Abundance Ion 94.90 (94.60 to 95.60): VN0

Ion 173.80 (173.50 to 174.50): VN0

Ion 175.80 (175.50 to 176.50): VN0

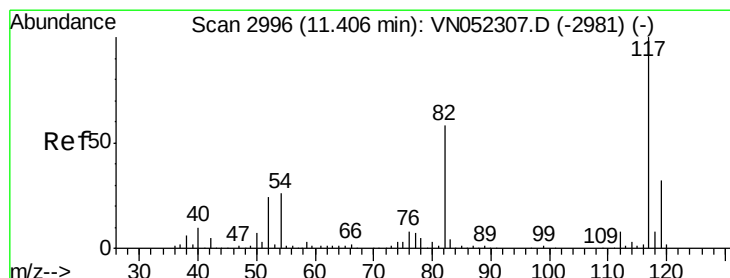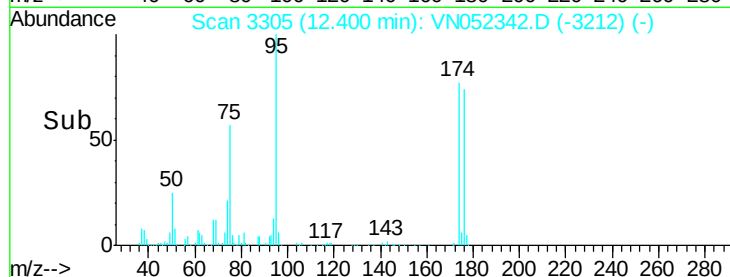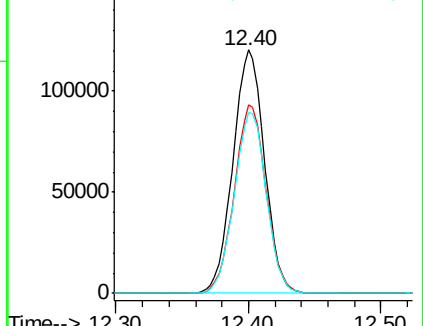

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. -0.00 min

Lab File: VN052342.D

Acq: 15 Nov 2018 15:20


Tgt Ion: 117 Resp: 470972

Ion Ratio Lower Upper

117 100

82 57.8 46.5 69.7



119 31.5 25.7 38.5

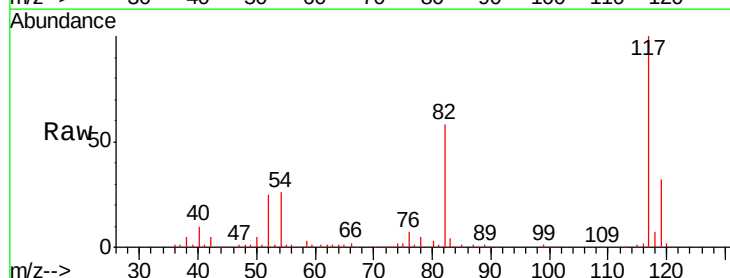


Abundance Ion 116.90 (116.60 to 117.60): VN0

Ion 82.00 (81.70 to 82.70): VN0

Ion 118.90 (118.60 to 119.60): VN0

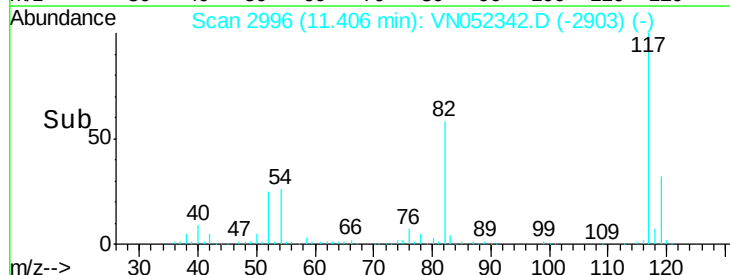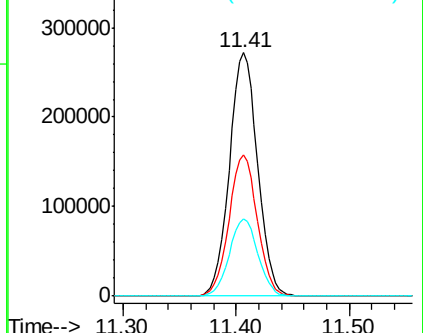

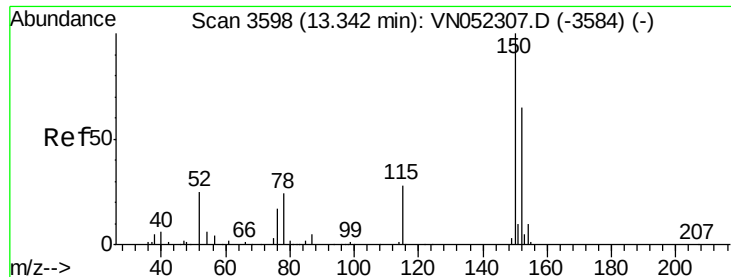

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. -0.00 min

Lab File: VN052342.D

Acq: 15 Nov 2018 15:20

Instrument :

MSVOA_N

ClientSampleId :

PB114828ZHE#06


Tgt Ion:152 Resp: 163637

Ion Ratio Lower Upper

152 100

115 60.7 30.3 91.0

150 159.9 0.0 348.2

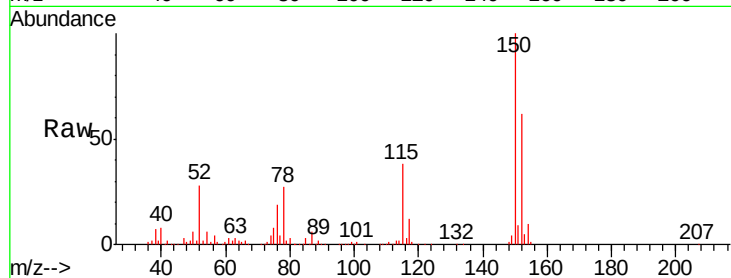

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

