

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111521\
 Data File : VN069501.D
 Acq On : 15 Nov 2021 19:31
 Operator : JC/MD
 Sample : M4693-04
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 16 00:55:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 09 18:18:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	1374110	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2437960	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2503992	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	973127	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	1007155	50.550	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 101.100%			
35) Dibromofluoromethane	8.021	113	703370	48.104	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 96.200%			
50) Toluene-d8	10.443	98	3154315	54.851	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 109.700%			
62) 4-Bromofluorobenzene	12.731	95	1139298	53.928	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 107.860%			
Target Compounds						Qvalue
11) Tert butyl alcohol	5.380	59	824	0.230	ug/l #	76
13) Acrolein	4.041	56	1459	Below Cal	#	46
16) Acetone	4.293	43	357063	33.216	ug/l	96
18) Methyl Acetate	4.870	43	39795	1.139	ug/l #	74
20) Methylene Chloride	5.103	84	42030	2.757	ug/l #	85
25) 2-Butanone	7.345	43	93256	6.407	ug/l	95
29) Tetrahydrofuran	7.699	42	20474	2.292	ug/l #	74
31) Cyclohexane	8.080	56	36598	1.345	ug/l #	38
36) 1,1-Dichloropropene	8.083	75	118461	5.775	ug/l #	49
37) Ethyl Acetate	7.345	43	93256	3.363	ug/l #	68
38) Carbon Tetrachloride	8.086	117	143334	7.237	ug/l #	16
41) Methacrylonitrile	7.694	41	11462	0.800	ug/l #	42
43) Isopropyl Acetate	8.566	43	147763	3.317	ug/l #	83
48) Methyl methacrylate	9.545	41	36397	1.737	ug/l #	8
49) 1,4-Dioxane	9.577	88	182	39.480	ug/l #	27
51) 4-Methyl-2-Pentanone	10.336	43	33036	1.149	ug/l	99
53) t-1,3-Dichloropropene	10.727	75	49	2.639	ug/l #	43
54) cis-1,3-Dichloropropene	10.245	75	183168	8.187	ug/l #	72
56) Ethyl methacrylate	10.875	69	1655	2.106	ug/l #	1
57) 1,3-Dichloropropane	11.089	76	99681	3.567	ug/l #	43
58) 2-Chloroethyl Vinyl ether	9.810	63	25	22.773	ug/l #	45
59) 2-Hexanone	11.092	43	1744897	77.539	ug/l #	48
60) Dibromochloromethane	11.492	129	1094	2.477	ug/l #	11
70) Styrene	12.296	104	1875	1.552	ug/l #	82
76) 1,2,3-Trichloropropane	12.734	75	640818	28.535	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.734	75	640818	80.894	ug/l #	5
90) Hexachloroethane	14.160	117	254	2.184	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.627	75	88	1.814	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.260	180	247	3.128	ug/l #	76
95) Naphthalene	15.507	128	151759	7.651	ug/l	98
96) 1,2,3-Trichlorobenzene	15.703	180	148	3.179	ug/l #	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111521\
Data File : VN069501.D
Acq On : 15 Nov 2021 19:31
Operator : JC/MD
Sample : M4693-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Nov 16 00:55:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 09 18:18:22 2021
Response via : Initial Calibration




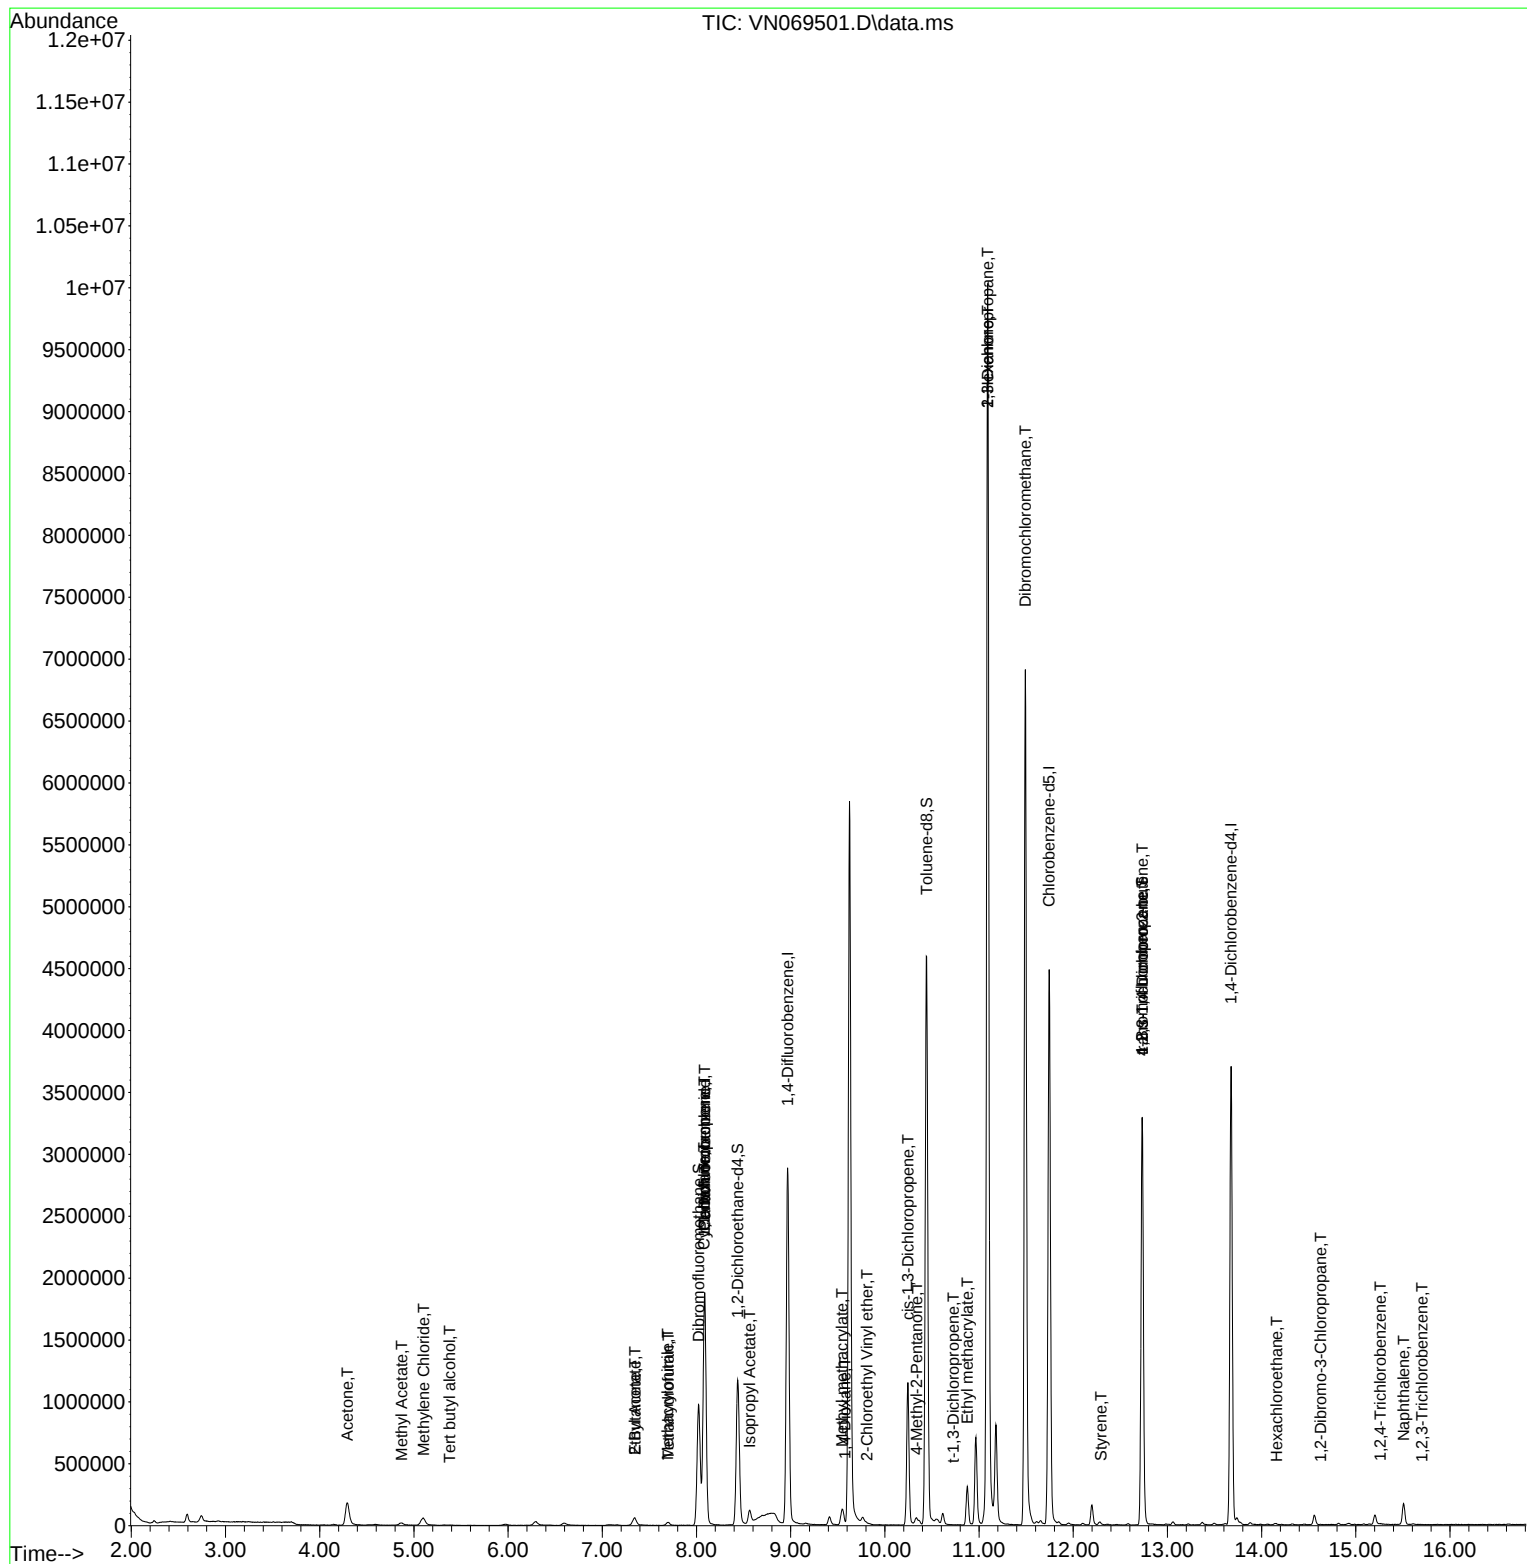




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 1374110
Ion Ratio Lower Upper
168 100
99 60.0 41.3 61.9

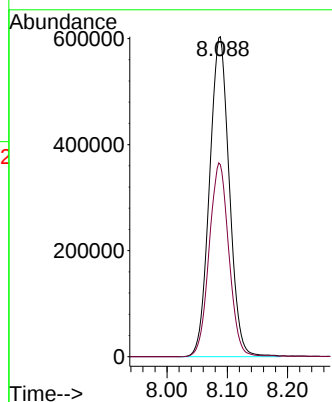

#11
Tert butyl alcohol
Concen: 0.230 ug/l
RT: 5.380 min Scan# 1264
Delta R.T. -0.005 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31


Tgt Ion: 59 Resp: 824
Ion Ratio Lower Upper
59 100
57 19.9 8.7 13.1#

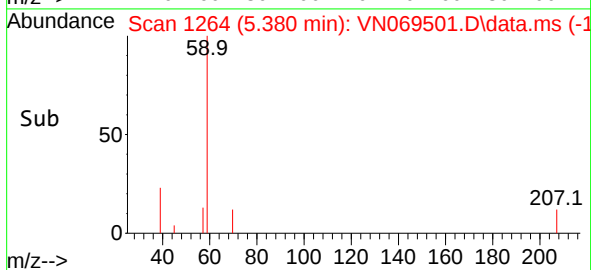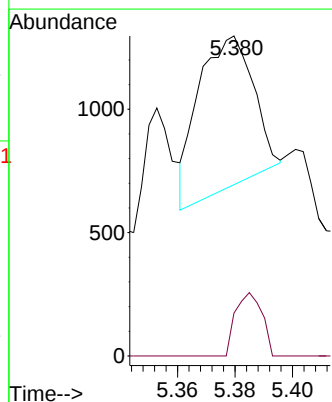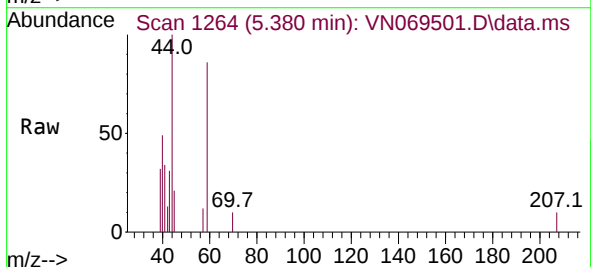






#13
Acrolein
Concen: Below Cal
RT: 4.041 min Scan# 765
Delta R.T. 0.000 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 1459
Ion Ratio Lower Upper
56 100
55 26.5 56.6 85.0#



#16
Acetone
Concen: 33.216 ug/l
RT: 4.293 min Scan# 859
Delta R.T. 0.005 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Tgt Ion: 43 Resp: 357063
Ion Ratio Lower Upper
43 100
58 26.7 23.1 34.7

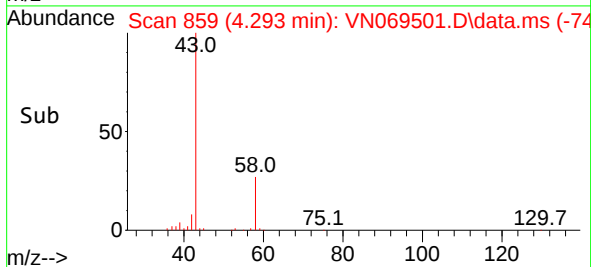

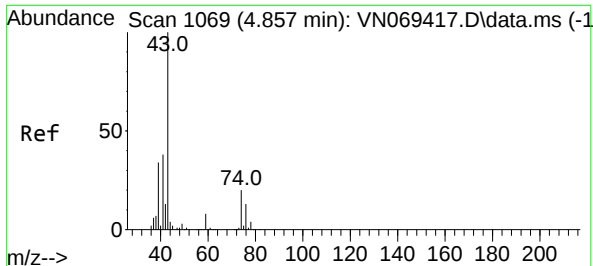

#18

Methyl Acetate

Concen: 1.139 ug/l

RT: 4.870 min Scan# 1106

Delta R.T. 0.013 min

Lab File: VN069501.D

Acq: 15 Nov 2021 19:31

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 39795

Ion Ratio Lower Upper

43 100

74 11.6 19.4 29.2#

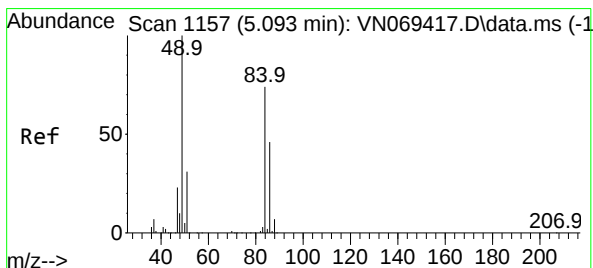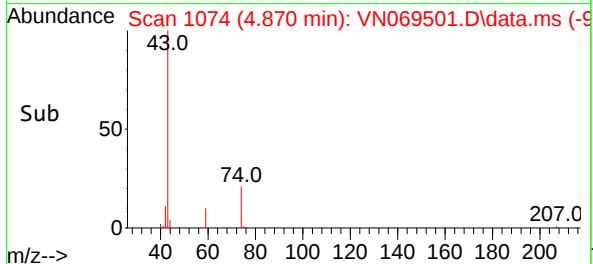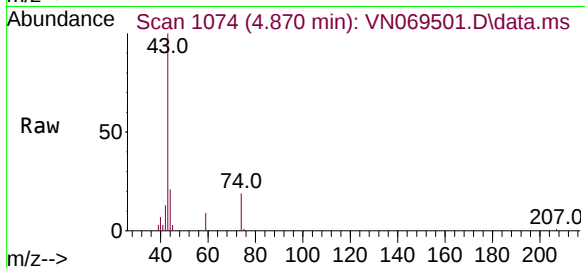

#20

Methylene Chloride

Concen: 2.757 ug/l

RT: 5.103 min Scan# 1161

Delta R.T. 0.010 min

Lab File: VN069501.D

Acq: 15 Nov 2021 19:31

Tgt Ion: 84 Resp: 42030




Ion Ratio Lower Upper


84 100

49 137.9 93.5 140.3

51 44.4 29.4 44.2#

86 58.8 53.0 79.4

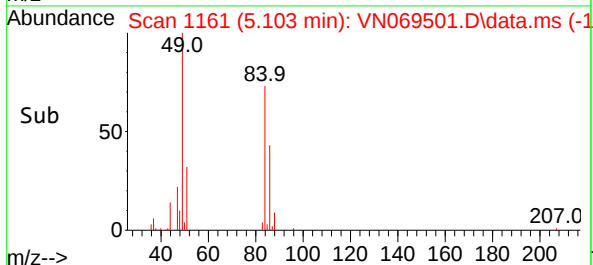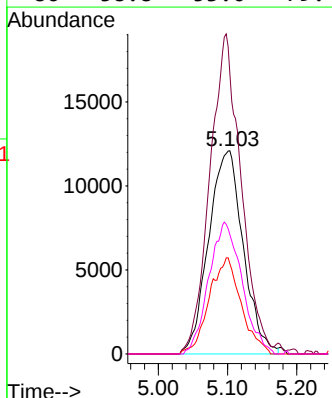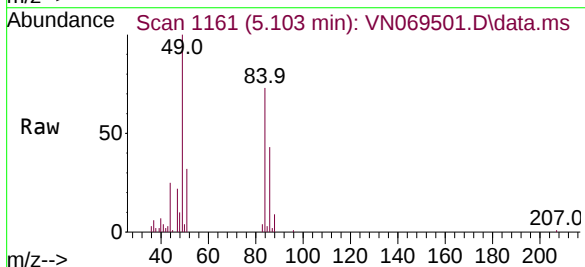

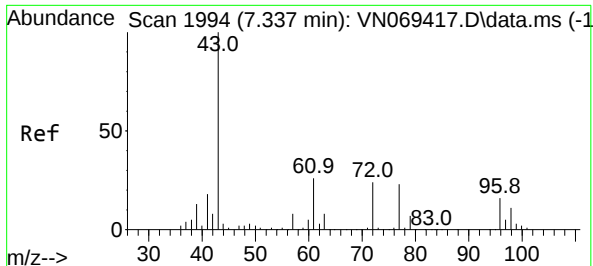

#25

2-Butanone

Concen: 6.407 ug/l

RT: 7.345 min Scan# 1994

Delta R.T. 0.008 min

Lab File: VN069501.D

Acq: 15 Nov 2021 19:31

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 93256

Ion Ratio Lower Upper

43 100

72 24.7 21.7 32.5

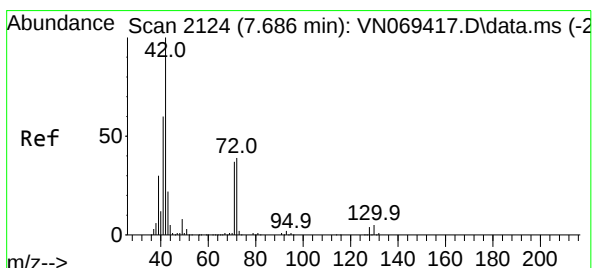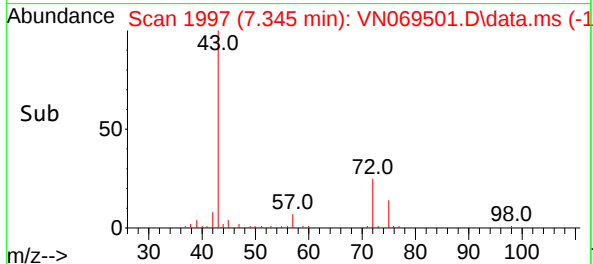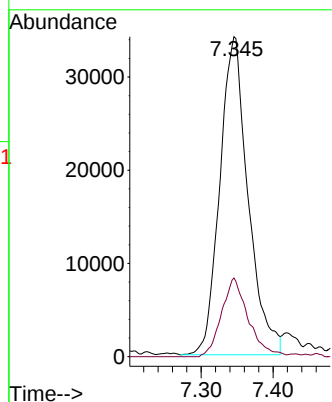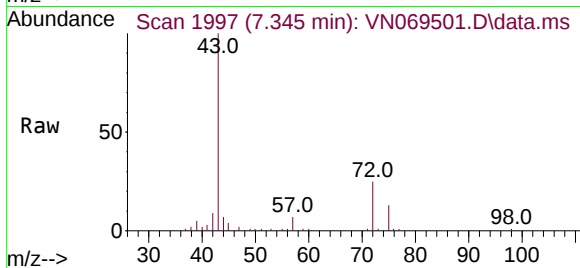

#29

Tetrahydrofuran

Concen: 2.292 ug/l

RT: 7.699 min Scan# 2129

Delta R.T. 0.013 min

Lab File: VN069501.D

Acq: 15 Nov 2021 19:31




Tgt Ion: 42 Resp: 20474


Ion Ratio Lower Upper

42 100

72 18.6 36.3 54.5#


71 37.0 34.7 52.1

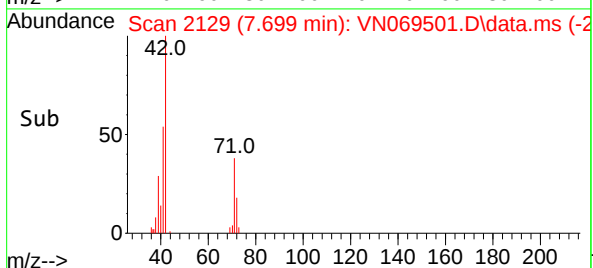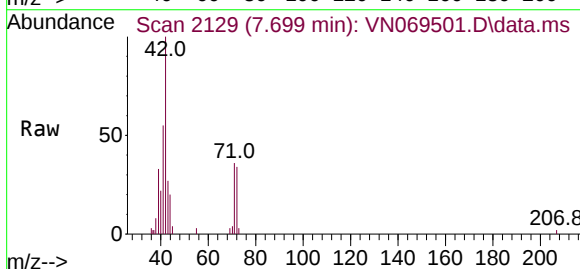






#31
Cyclohexane
Concen: 1.345 ug/l
RT: 8.080 min Scan# 21
Delta R.T. -0.014 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 36598
Ion Ratio Lower Upper
56 100
69 150.0 27.1 40.7#
84 100.9 73.4 110.0

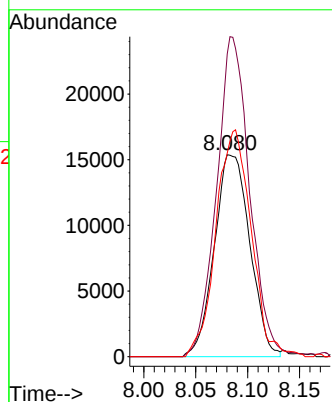

#33
1,2-Dichloroethane-d4
Concen: 50.550 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. -0.003 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31


Tgt Ion: 65 Resp: 1007155
Ion Ratio Lower Upper
65 100
67 51.0 0.0 103.0








#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. 0.000 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:114 Resp: 2437960
Ion Ratio Lower Upper
114 100
63 22.7 0.0 37.8
88 15.8 0.0 27.4

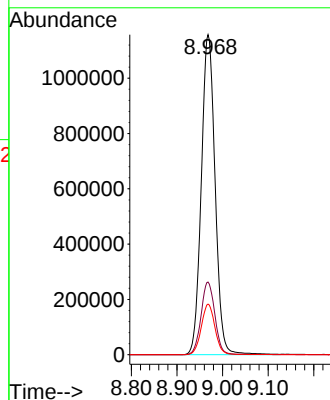

#35
Dibromofluoromethane
Concen: 48.104 ug/l
RT: 8.021 min Scan# 2249
Delta R.T. 0.000 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31


Tgt Ion:113 Resp: 703370
Ion Ratio Lower Upper
113 100
111 102.8 82.2 123.2
192 17.8 16.9 25.3

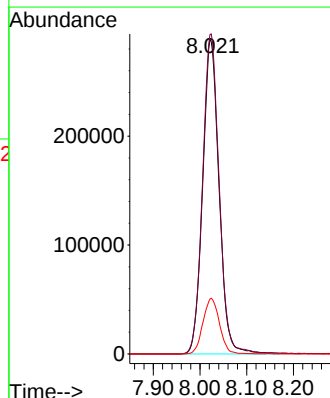






#36
1,1-Dichloropropene
Concen: 5.775 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.140 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Instrument :
MSVOA_N
ClientSampleId :



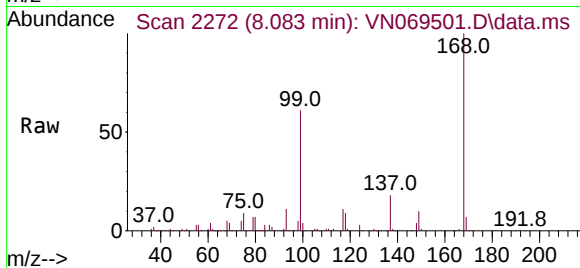



Tgt Ion: 75 Resp: 118461
Ion Ratio Lower Upper
75 100
110 9.1 18.4 55.2#
77 0.0 24.4 36.6#

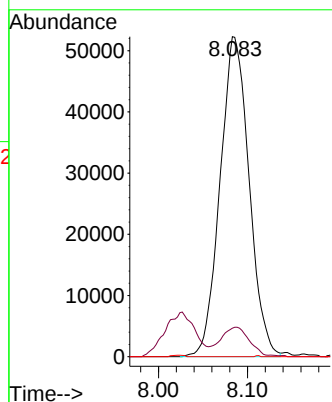

#37
Ethyl Acetate
Concen: 3.363 ug/l
RT: 7.345 min Scan# 1997
Delta R.T. -0.070 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31


Tgt Ion: 43 Resp: 93256
Ion Ratio Lower Upper
43 100
61 0.0 11.5 17.3#
70 0.0 7.9 11.9#

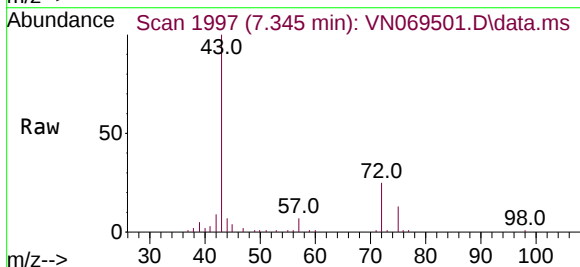






#38
Carbon Tetrachloride
Concen: 7.237 ug/l
RT: 8.086 min Scan# 2117
Delta R.T. -0.120 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 143334
Ion Ratio Lower Upper
117 100
119 5.3 76.1 114.1#
121 0.0 24.2 36.2#



#41
Methacrylonitrile
Concen: 0.800 ug/l
RT: 7.694 min Scan# 2127
Delta R.T. 0.056 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Tgt Ion: 41 Resp: 11462
Ion Ratio Lower Upper
41 100
39 56.0 48.1 72.1
67 0.0 68.3 102.5#
52 0.0 29.6 44.4#


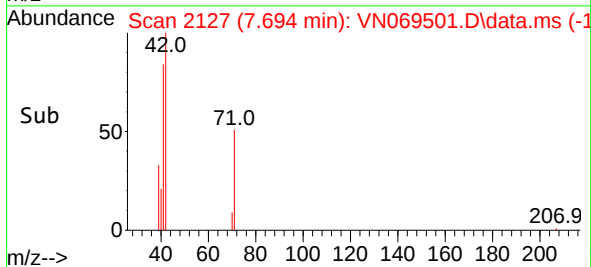






#43
Isopropyl Acetate
Concen: 3.317 ug/l
RT: 8.566 min Scan# 2451
Delta R.T. 0.003 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 147763
Ion Ratio Lower Upper
43 100
61 14.6 20.4 30.6#
87 10.1 11.2 16.8#

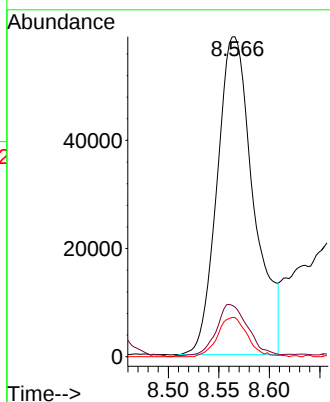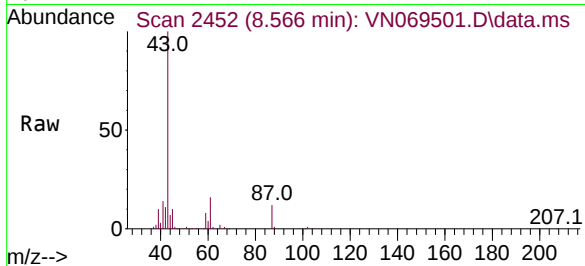

#48
Methyl methacrylate
Concen: 1.737 ug/l
RT: 9.545 min Scan# 2817
Delta R.T. -0.016 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Tgt Ion: 41 Resp: 36397
Ion Ratio Lower Upper
41 100
69 0.2 72.4 108.6#
39 0.0 58.4 87.6#

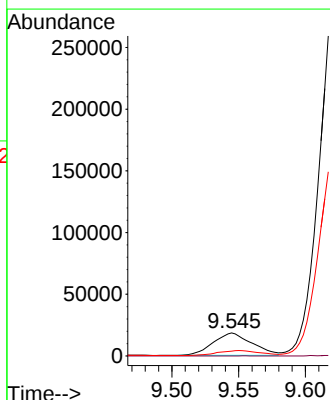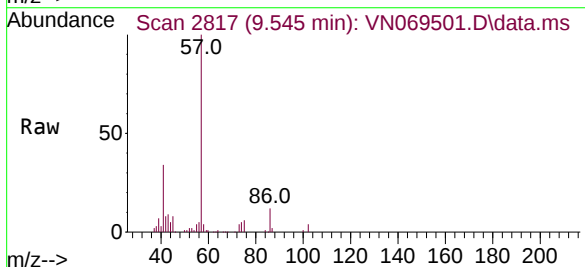



#49

1,4-Dioxane

Concen: 39.480 ug/l

RT: 9.577 min Scan# 21

Delta R.T. 0.005 min

Lab File: VN069501.D

Acq: 15 Nov 2021 19:31

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 88 Resp: 182

Ion Ratio Lower Upper

88 100

43 0.0 23.4 35.2#

58 0.0 50.6 75.8#

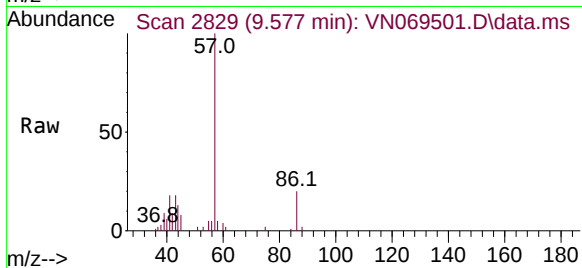

#50

Toluene-d8

Concen: 54.851 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. 0.002 min

Lab File: VN069501.D




Acq: 15 Nov 2021 19:31


Tgt Ion: 98 Resp: 3154315

Ion Ratio Lower Upper

98 100

100 63.9 50.4 75.6

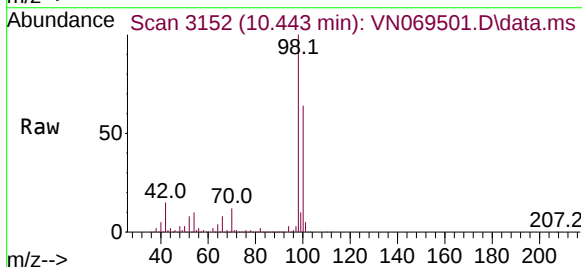

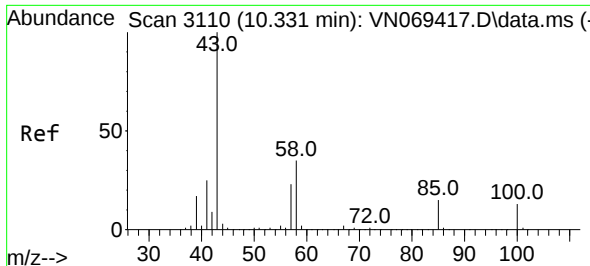

#51

4-Methyl-2-Pentanone

Concen: 1.149 ug/l

RT: 10.336 min Scan# 3110

Delta R.T. 0.005 min

Lab File: VN069501.D

Acq: 15 Nov 2021 19:31

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion: 43 Resp: 33036

Ion Ratio Lower Upper

43 100

58 37.6 30.4 45.6

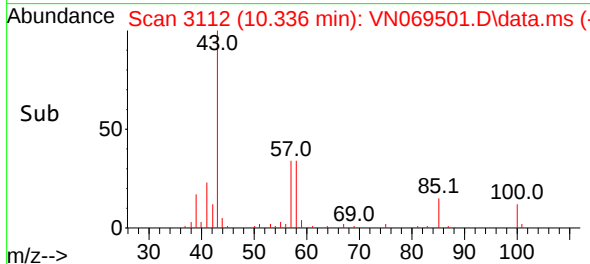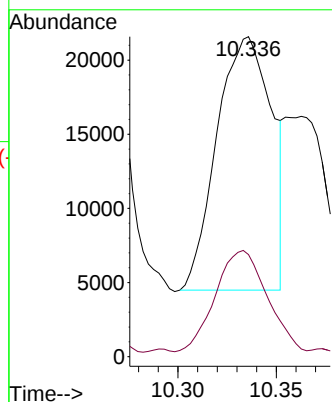

#53

t-1,3-Dichloropropene

Concen: 2.639 ug/l

RT: 10.727 min Scan# 3258

Delta R.T. 0.008 min

Lab File: VN069501.D




Acq: 15 Nov 2021 19:31


Tgt Ion: 75 Resp: 49

Ion Ratio Lower Upper

75 100

77 0.0 25.6 38.4#


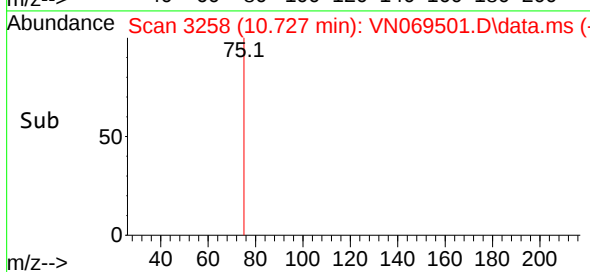
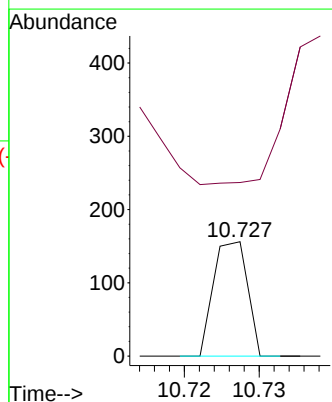
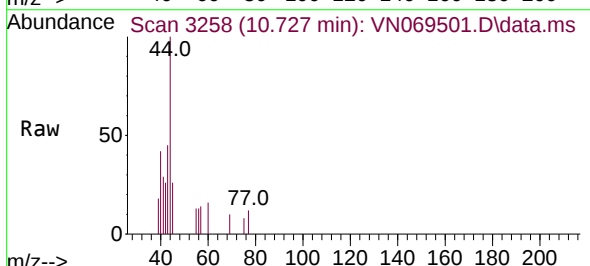




#54
cis-1,3-Dichloropropene
Concen: 8.187 ug/l
RT: 10.245 min Scan# 3057
Delta R.T. 0.057 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 183168
Ion Ratio Lower Upper
75 100
77 0.5 26.4 39.6#
39 46.4 42.5 63.7

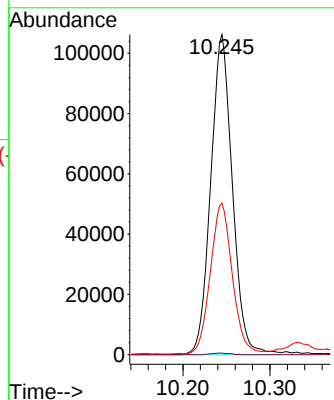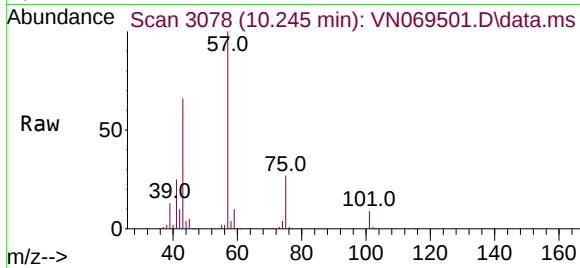

#56
Ethyl methacrylate
Concen: 2.106 ug/l
RT: 10.875 min Scan# 3313
Delta R.T. 0.113 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Tgt Ion: 69 Resp: 1655
Ion Ratio Lower Upper
69 100
41 4106.2 51.4 77.0#
39 1901.7 34.6 52.0#


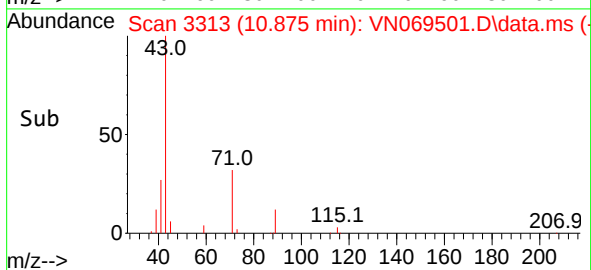
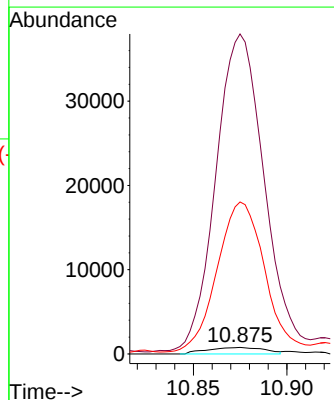
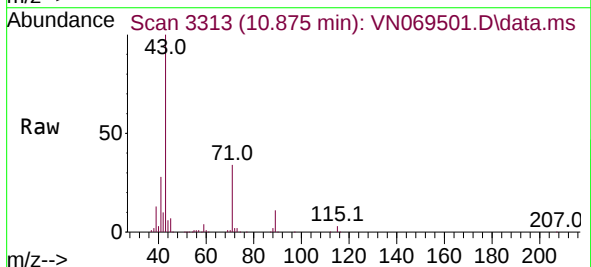


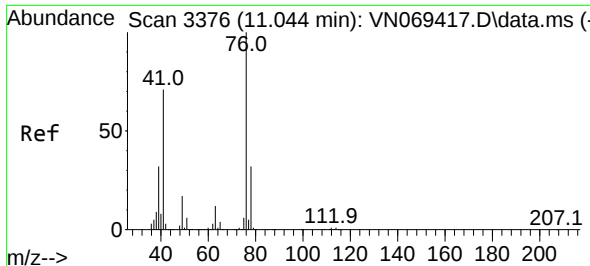

#57
1,3-Dichloropropane
Concen: 3.567 ug/l
RT: 11.089 min Scan# 311
Delta R.T. 0.045 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 76 Resp: 99681
Ion Ratio Lower Upper
76 100
78 0.4 25.7 38.5#

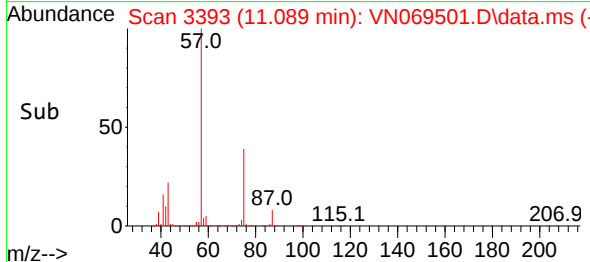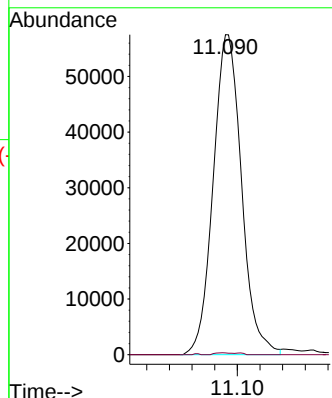

#58
2-Chloroethyl Vinyl ether
Concen: 22.773 ug/l
RT: 9.810 min Scan# 2916
Delta R.T. -0.231 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Tgt Ion: 63 Resp: 25
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#


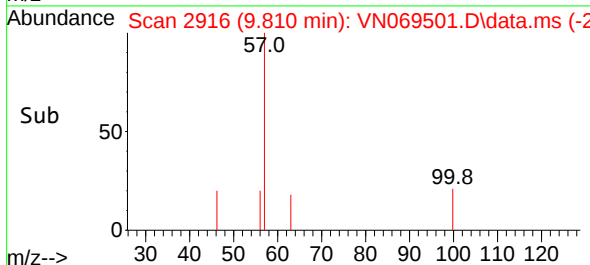
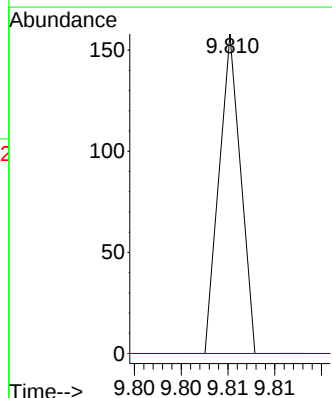
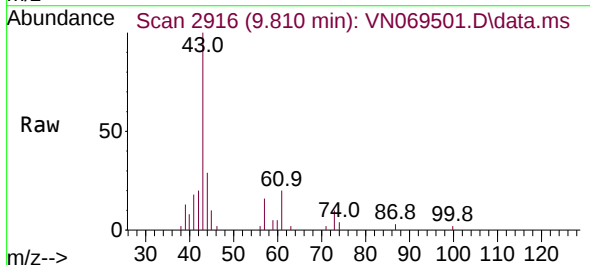




#59
2-Hexanone
Concen: 77.539 ug/l
RT: 11.092 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 1744897
Ion Ratio Lower Upper
43 100
58 16.8 26.9 80.7#

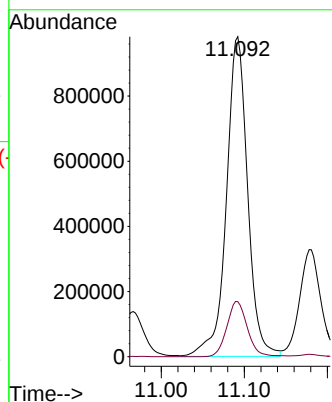

#60
Dibromochloromethane
Concen: 2.477 ug/l
RT: 11.492 min Scan# 3543
Delta R.T. 0.252 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Tgt Ion:129 Resp: 1094
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#




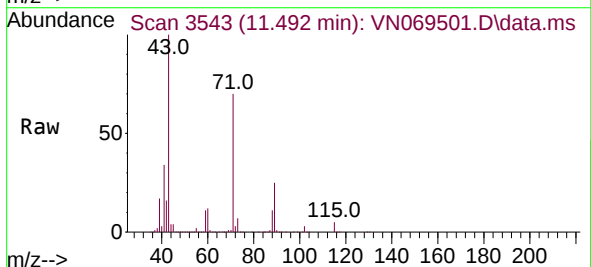


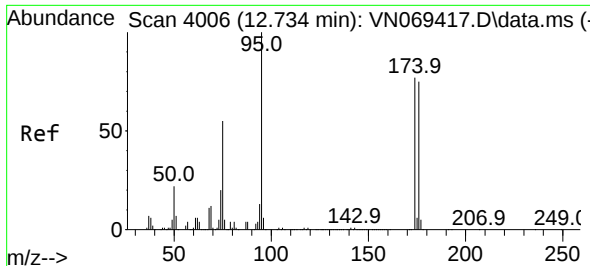

#62
4-Bromofluorobenzene
Concen: 53.928 ug/l
RT: 12.731 min Scan# 4006
Delta R.T. -0.003 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 1139298
Ion Ratio Lower Upper
95 100
174 76.0 0.0 187.2
176 72.9 0.0 181.4

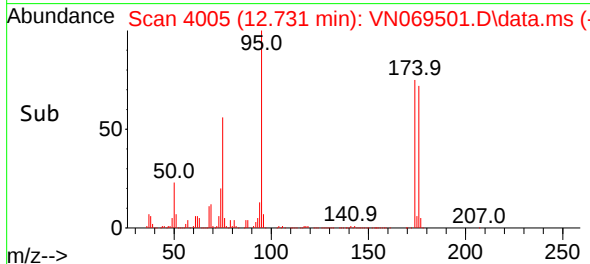

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3637
Delta R.T. -0.003 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Tgt Ion: 117 Resp: 2503992
Ion Ratio Lower Upper
117 100
82 58.4 42.4 63.6
119 32.5 25.4 38.2


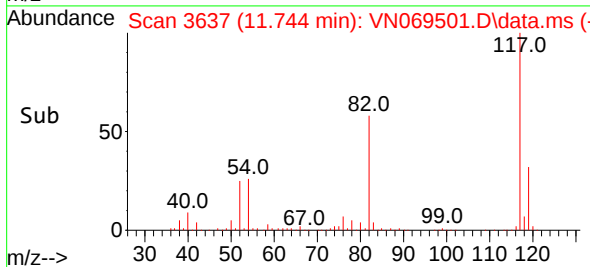

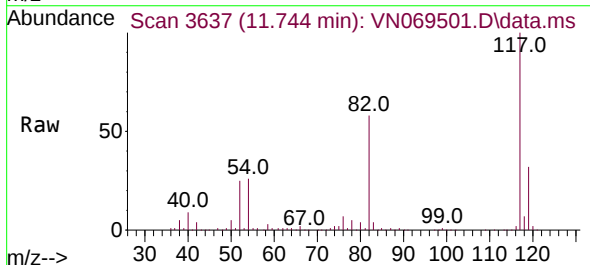


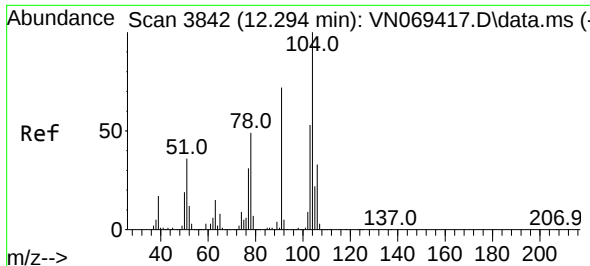

#70
Styrene
Concen: 1.552 ug/l
RT: 12.296 min Scan# 3842
Delta R.T. 0.002 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:104 Resp: 1875
Ion Ratio Lower Upper
104 100
78 43.6 38.7 58.1
103 76.5 45.0 67.6#

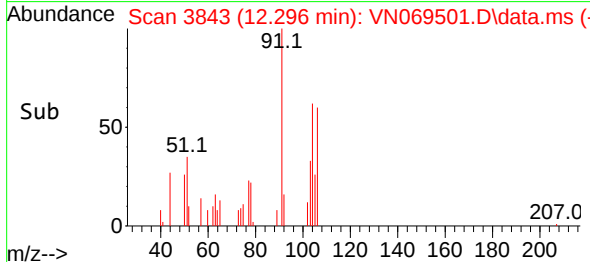

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.000 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Tgt Ion:152 Resp: 973127
Ion Ratio Lower Upper
152 100
115 61.0 27.5 82.5
150 158.0 0.0 344.4


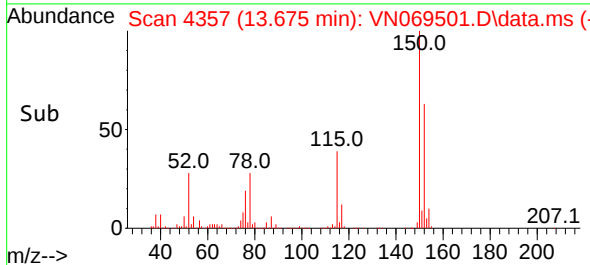

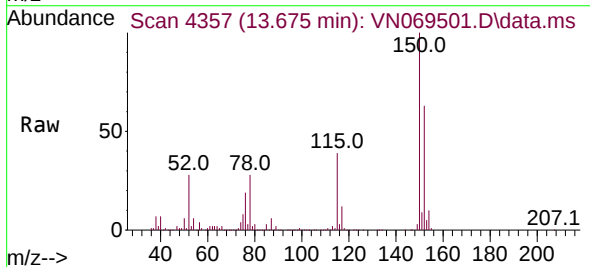


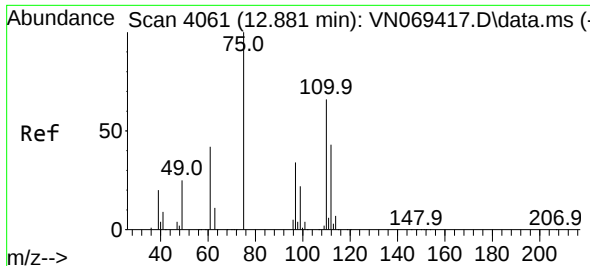

#76
1,2,3-Trichloropropane
Concen: 28.535 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.147 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 640818
Ion Ratio Lower Upper
75 100
77 1.0 82.6 247.8#

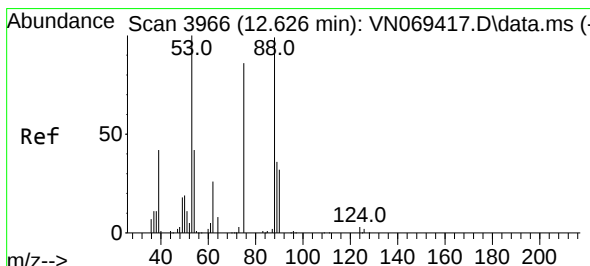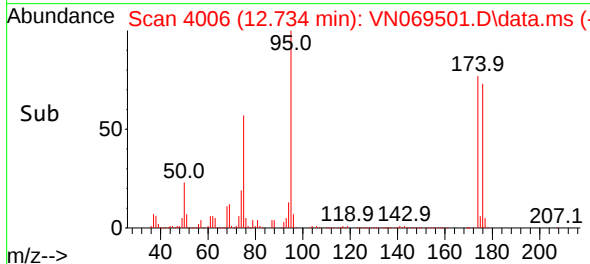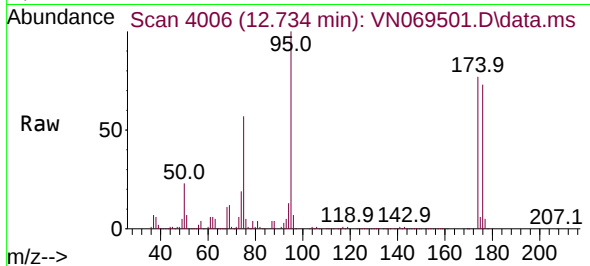

#81
trans-1,4-Dichloro-2-butene
Concen: 80.894 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.108 min
Lab File: VN069501.D
Acq: 15 Nov 2021 19:31

Tgt Ion: 75 Resp: 640818
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

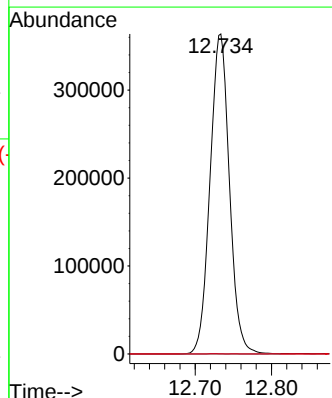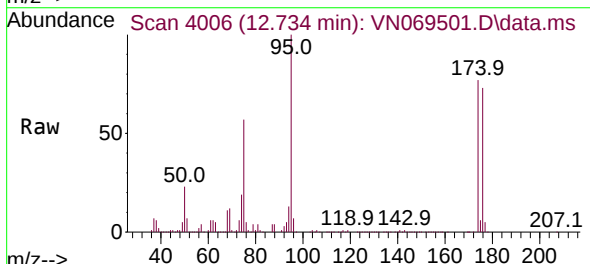



#90

Hexachloroethane

Concen: 2.184 ug/l

RT: 14.160 min Scan# 41

Delta R.T. -0.051 min

Lab File: VN069501.D

Acq: 15 Nov 2021 19:31

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:117 Resp: 254

Ion Ratio Lower Upper

117 100

201 0.0 43.9 131.6#

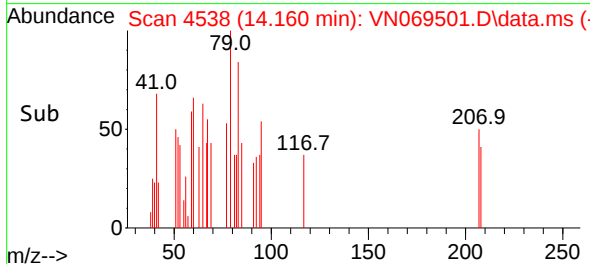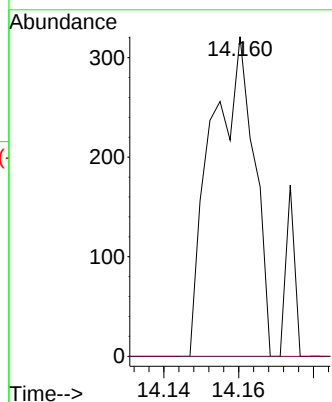

#92

1,2-Dibromo-3-Chloropropane

Concen: 1.814 ug/l

RT: 14.627 min Scan# 4712

Delta R.T. 0.021 min

Lab File: VN069501.D

Acq: 15 Nov 2021 19:31




Tgt Ion: 75 Resp: 88


Ion Ratio Lower Upper

75 100

155 0.0 46.9 140.7#

157 0.0 60.6 181.7#


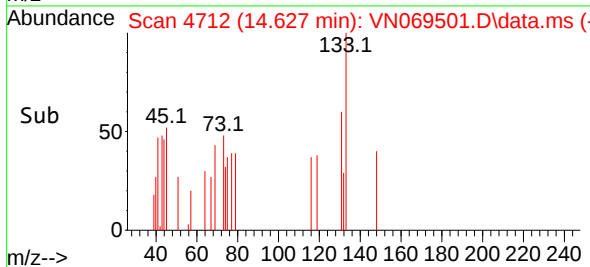

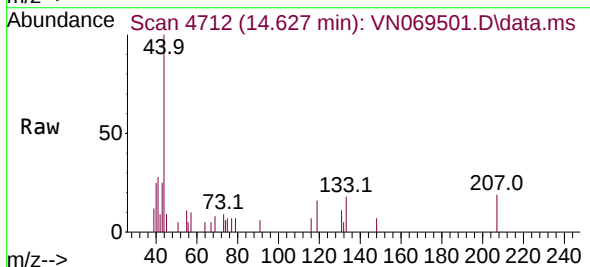




#93
 1,2,4-Trichlorobenzene
 Concen: 3.128 ug/l
 RT: 15.260 min Scan# 4950
 Delta R.T. -0.005 min
 Lab File: VN069501.D
 Acq: 15 Nov 2021 19:31




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:180 Resp: 247
 Ion Ratio Lower Upper
 180 100
 182 76.1 48.3 144.9
 145 10.1 14.5 43.5#

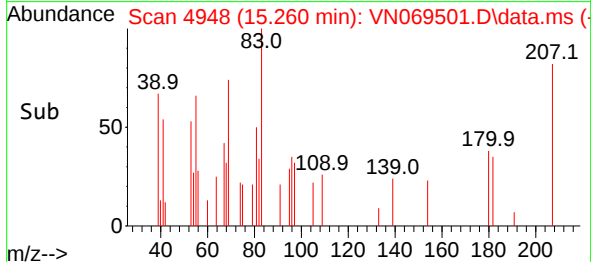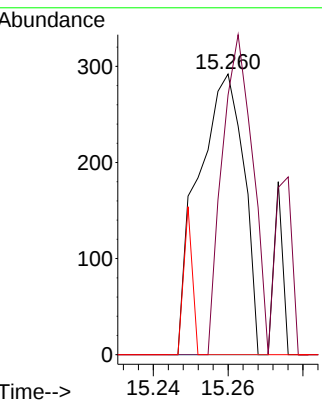

#95
 Naphthalene
 Concen: 7.651 ug/l
 RT: 15.507 min Scan# 5040
 Delta R.T. -0.000 min
 Lab File: VN069501.D
 Acq: 15 Nov 2021 19:31


Tgt Ion:128 Resp: 151759
 Ion Ratio Lower Upper
 128 100
 127 14.1 10.5 15.7
 129 10.8 8.7 13.1

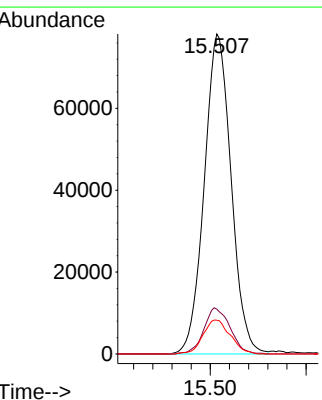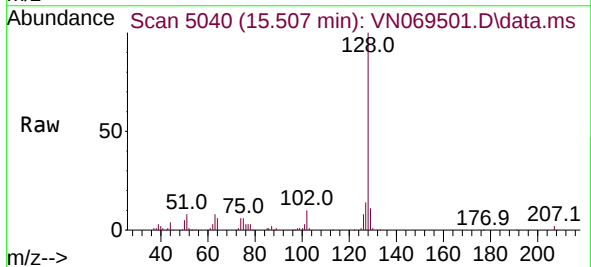



#96
 1,2,3-Trichlorobenzene
 Concen: 3.179 ug/l
 RT: 15.703 min Scan# 5113
 Delta R.T. 0.003 min
 Lab File: VN069501.D
 Acq: 15 Nov 2021 19:31

Instrument :
 MSVOA_N
 ClientSampleId :

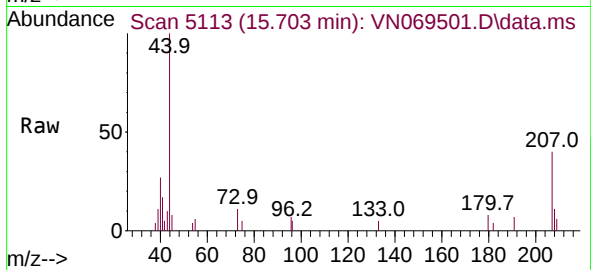

Tgt Ion:180 Resp: 148
 Ion Ratio Lower Upper
 180 100
 182 53.4 47.4 142.2
 145 72.3 15.0 45.1#

