
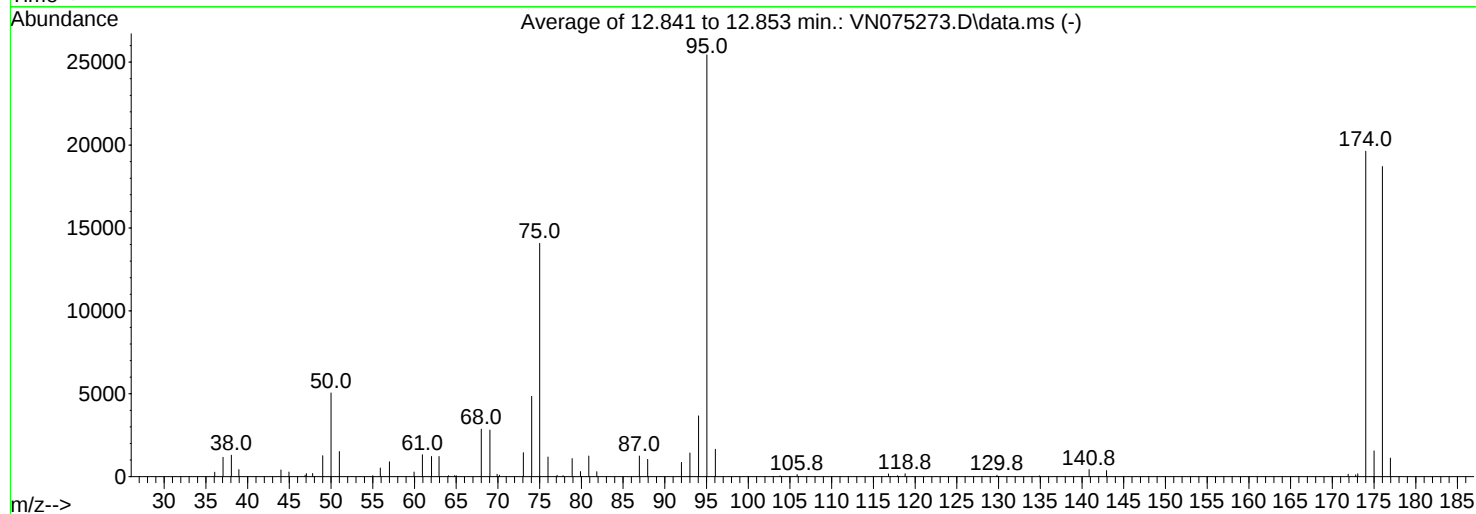


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111522\
Data File : VN075273.D
Acq On : 15 Nov 2022 10:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

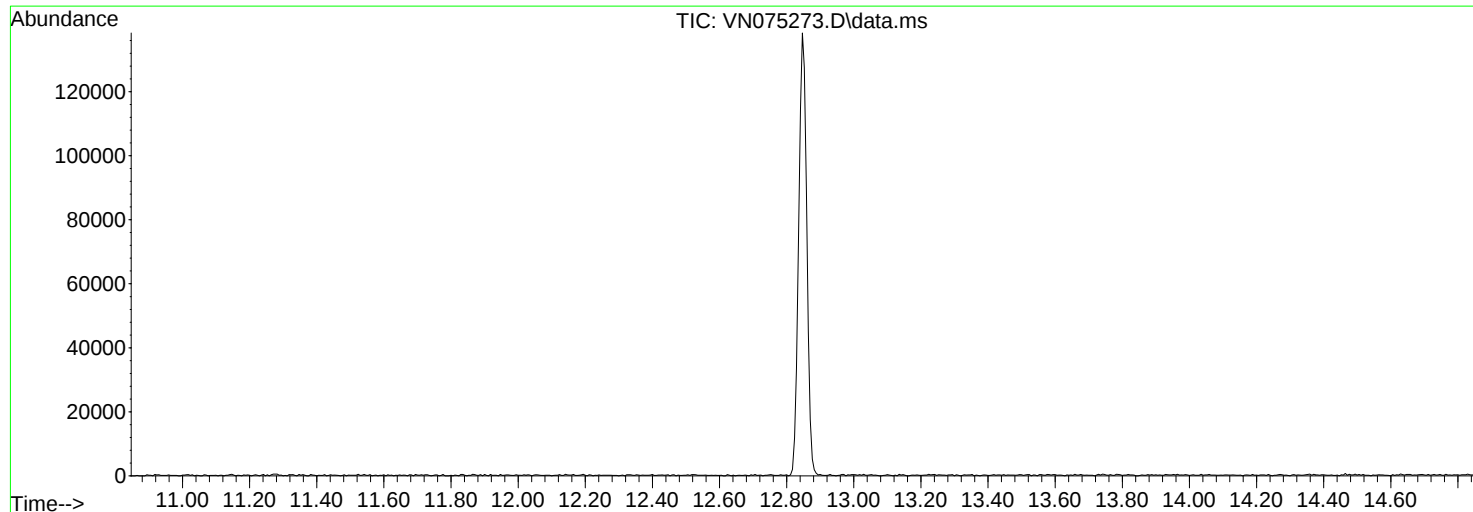

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	5046	PASS
75	95	30	60	55.3	14075	PASS
95	95	100	100	100.0	25440	PASS
96	95	5	9	6.5	1648	PASS
173	174	0.00	2	0.9	172	PASS
174	95	50	100	77.2	19627	PASS
175	174	5	9	7.9	1551	PASS
176	174	95	101	95.3	18701	PASS
177	176	5	9	6.0	1116	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	273	51.00	1512	68.00	2862	79.90	30
37.05	1164	55.00	58	69.05	2807	80.90	125
38.05	1298	55.90	517	69.90	144	81.85	30
38.95	425	57.00	893	70.20	90	86.95	125
44.00	407	59.95	277	73.05	1449	87.95	1047
44.95	279	60.95	1327	74.05	4840	92.00	858
46.90	83	62.05	1217	75.00	14075	93.00	1432
47.05	180	62.95	1215	76.00	1188	94.05	3671
47.80	190	64.10	59	77.10	75	95.05	25440
49.00	1265	64.80	58	77.80	55	96.05	1648
50.00	5046	65.00	62	78.90	1087	103.80	51

Average of 12.841 to 12.853 min.: VN075273.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.85	127	174.00	19627				
116.80	169	175.00	1551				
117.90	60	176.00	18701				
118.80	175	176.95	1116				
129.80	88						
134.90	52						
140.85	421						
142.95	366						
171.90	148						
172.80	109						
173.05	172						

Instrument :

MSVOA_N

ClientSampleId :

BFB