
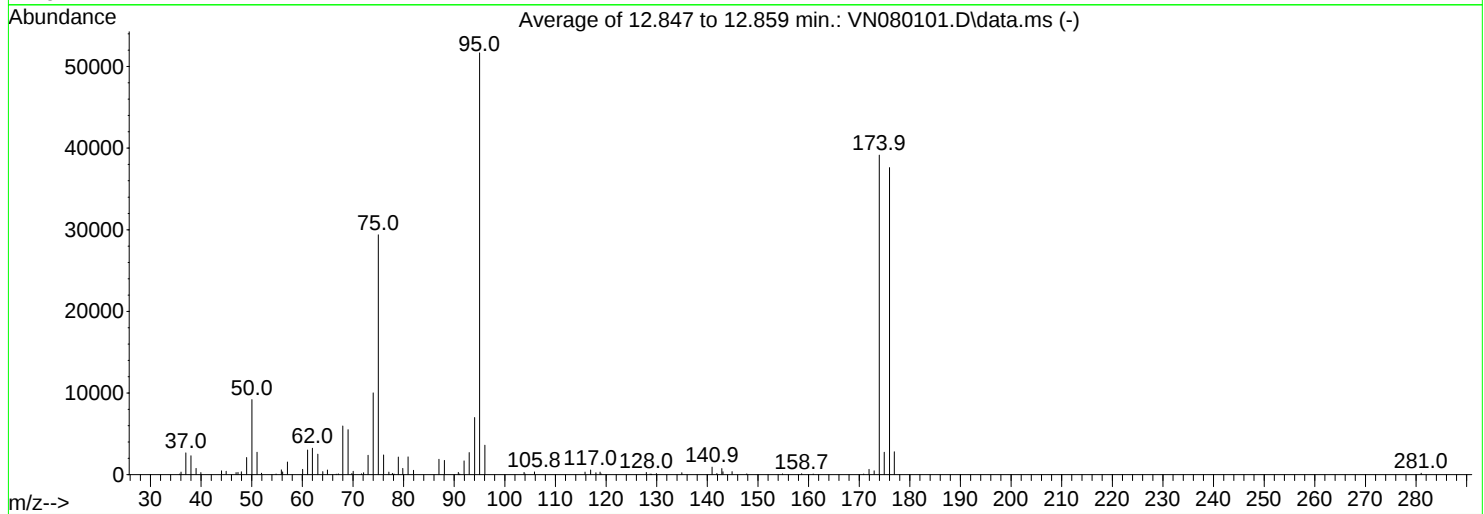


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111523\
Data File : VN080101.D
Acq On : 15 Nov 2023 10:25
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110123W.M
Title : SW846 8260
Last Update : Thu Nov 02 05:49:08 2023

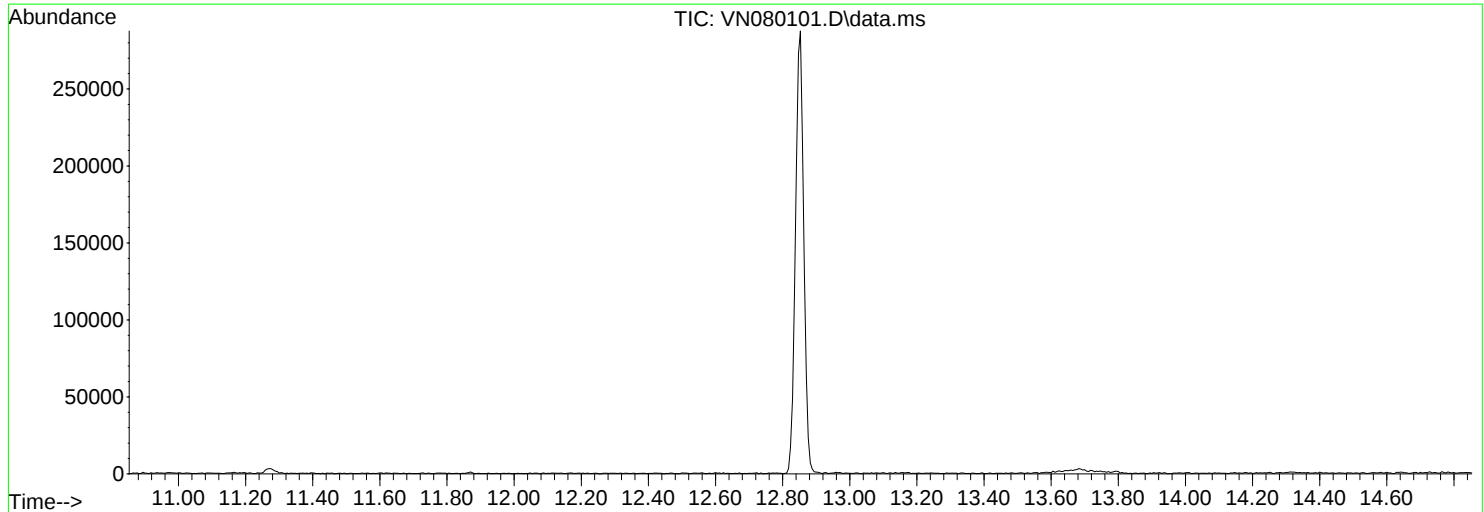

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	9200	PASS
75	95	30	60	56.9	29381	PASS
95	95	100	100	100.0	51675	PASS
96	95	5	9	7.0	3613	PASS
173	174	0.00	2	1.2	476	PASS
174	95	50	100	75.7	39141	PASS
175	174	5	9	7.0	2736	PASS
176	174	95	101	96.1	37611	PASS
177	176	5	9	7.5	2803	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	72	49.00	2097	63.05	2502	73.00	2361
36.05	306	50.05	9200	64.05	375	74.00	1002
37.00	2664	51.05	2750	64.95	574	75.00	2938
38.00	2314	51.95	177	66.70	61	76.05	240
39.00	775	54.80	89	67.10	102	77.10	307
39.95	247	55.85	587	68.00	5951	77.80	153
44.05	466	56.10	341	69.05	5509	78.10	71
44.95	411	57.05	1545	69.80	140	78.95	2149
46.90	261	60.05	644	70.05	413	79.85	765
47.30	268	61.05	3028	71.70	98	80.90	2170
47.95	345	62.00	3239	72.10	230	81.95	522

Average of 12.847 to 12.859 min.: VN080101.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.00	1884	105.85	334	140.95	914	172.95	476
88.05	1742	115.85	306	141.90	141	173.95	39141
90.80	273	116.95	566	142.85	748	174.95	2736
91.10	77	118.00	242	143.10	347	176.00	37611
91.95	1697	118.80	310	144.90	379	176.95	2803
92.95	2701	119.00	108	147.80	103	281.00	177
94.05	7004	127.95	273	154.85	104		
95.00	51675	128.70	72	158.65	116		
96.05	3613	129.00	57	160.90	76		
103.80	266	129.95	142	170.90	75		
104.00	76	134.95	228	171.95	651		

Instrument :

MSVOA_N

ClientSampleId :

BFB