

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111524\
 Data File : VN084875.D
 Acq On : 15 Nov 2024 17:36
 Operator : JC\MD
 Sample : P4853-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 002-35TH-AVE(NOV)

Quant Time: Nov 15 22:27:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N103124W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Fri Nov 01 02:38:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Bromochloromethane	7.806	128	23575	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.100	114	122982	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.865	117	114966	30.000	ug/l	0.00
System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.577	65	58387	30.806	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	102.700%
60) 4-Bromofluorobenzene	12.847	95	52268	26.404	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	88.000%
63) Toluene-d8	10.565	98	153284	28.164	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	93.867%
Target Compounds						
					Qvalue	
3) Chloromethane	2.389	50	589	0.357	ug/l #	43
5) Bromomethane	2.895	94	222	0.285	ug/l	82
6) Chloroethane	2.953	64	4350	4.322	ug/l #	47
12) Methyl Acetate	5.030	43	18868	8.810	ug/l	96
15) Acetone	4.424	58	111564	619.747	ug/l	91
16) Carbon Disulfide	4.706	76	1883	0.466	ug/l #	89
18) Methylene Chloride	5.259	84	686	0.426	ug/l #	25
23) tert-Butyl Alcohol	5.518	59	121	0.495	ug/l #	100
25) Chloroform	7.959	83	3990	1.382	ug/l	92
30) 2-Butanone	7.482	43	38351	44.883	ug/l	100
35) Methacrylonitrile	7.782	41	1821	1.798	ug/l #	39
36) 1,2-Dichloroethane	9.094	62	4224	2.075	ug/l #	74
45) 1,4-Dioxane	9.341	88	190	7.828	ug/l #	31
48) t-1,3-Dichloropropene	10.629	75	9699	4.444	ug/l #	1
49) cis-1,3-Dichloropropene	10.629	75	9699	4.146	ug/l #	1
50) 1,1,2-Trichloroethane	10.882	97	362	0.262	ug/l #	13
55) 2-Chloroethyl vinyl ether	10.629	63	94256	90.181	ug/l #	1
56) Bromoform	12.847	173	433	0.399	ug/l #	1
58) 4-Methyl-2-Pentanone	10.441	43	14219	7.840	ug/l	97
59) 2-Hexanone	11.194	43	442	0.333	ug/l #	33
62) Toluene	10.629	91	1364653	208.406	ug/l	98
66) Ethyl Benzene	11.959	91	1924	0.280	ug/l	96
67) m/p-Xylenes	12.070	106	2075	0.788	ug/l	100
68) o-Xylene	12.400	106	759	0.299	ug/l	74
70) Isopropylbenzene	13.094	105	1847	0.293	ug/l	88
72) 1,2,3-Trichloropropane	12.847	75	26302	15.053	ug/l	1
77) t-1,4-Dichloro-2-butene	12.847	75	26302	36.702	ug/l #	7
79) tert-butylbenzene	13.729	119	19225	4.310	ug/l	64
80) 1,2,4-Trimethylbenzene	13.482	105	4816	0.885	ug/l	79
82) p-Isopropyltoluene	13.729	119	19225	3.722	ug/l	93
86) Hexachloroethane	14.435	117	217	0.205	ug/l #	15
91) Naphthalene	15.635	128	3007	0.652	ug/l #	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111524\
Data File : VN084875.D
Acq On : 15 Nov 2024 17:36
Operator : JC\MD
Sample : P4853-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)

Quant Time: Nov 15 22:27:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N103124W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Fri Nov 01 02:38:04 2024
Response via : Initial Calibration




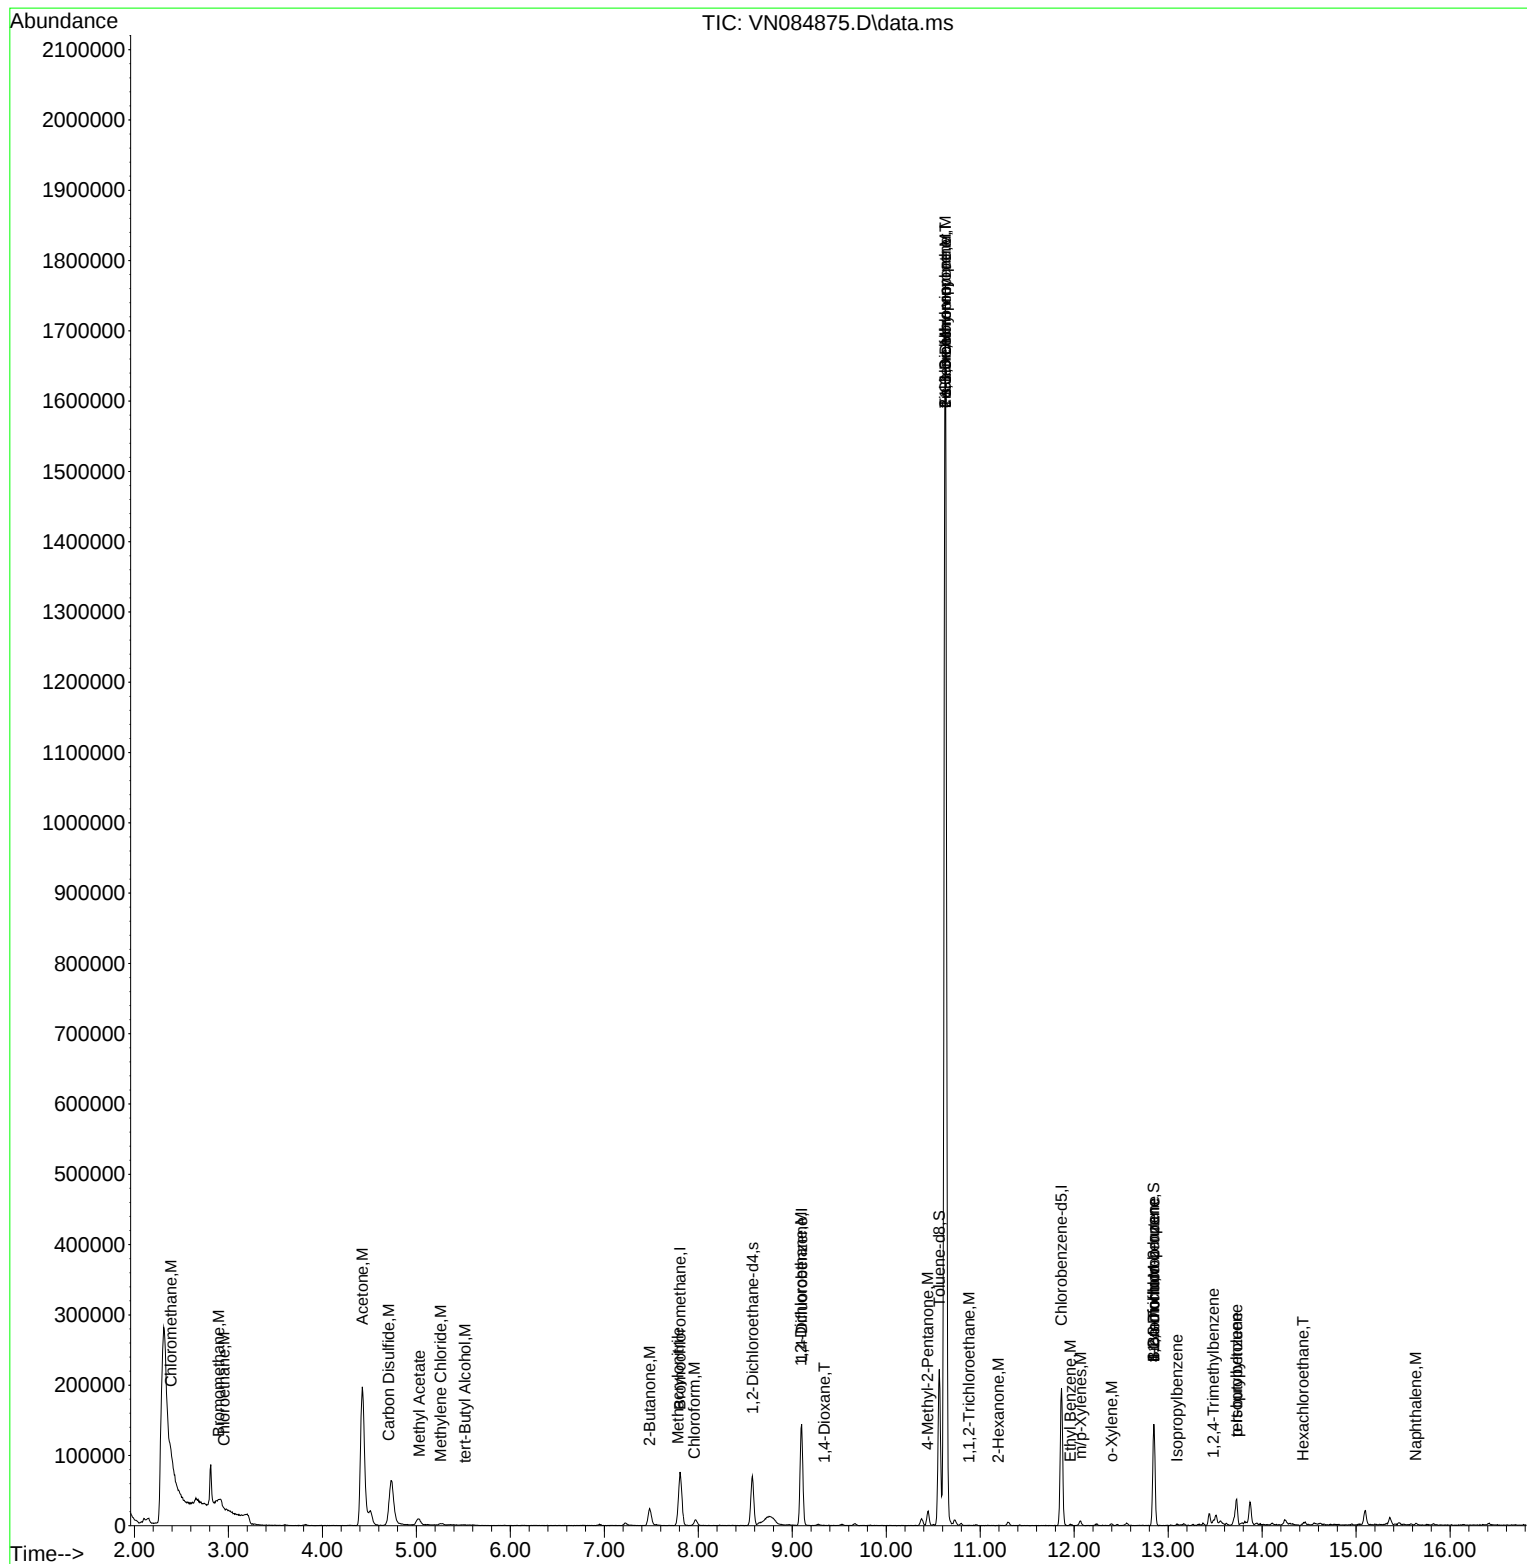




#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.806 min Scan# 91
Delta R.T. 0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion:128 Resp: 23575
Ion Ratio Lower Upper
128 100
49 159.4 0.0 427.0
130 129.7 0.0 322.2

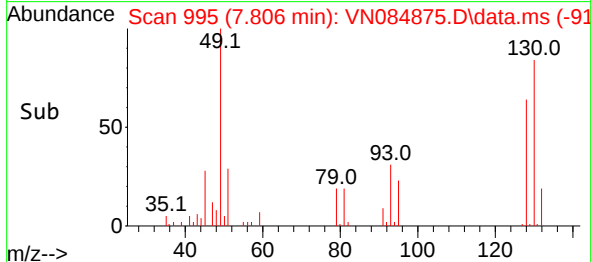

#3
Chloromethane
Concen: 0.357 ug/l
RT: 2.389 min Scan# 74
Delta R.T. 0.029 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 50 Resp: 589
Ion Ratio Lower Upper
50 100
52 0.0 25.5 38.3#




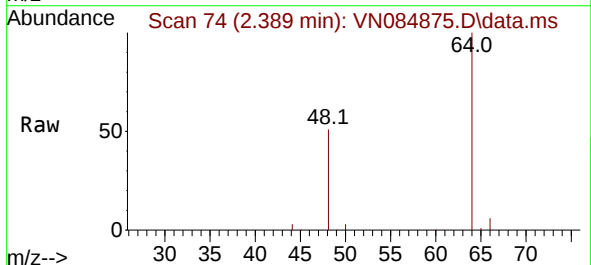




#5
Bromomethane
Concen: 0.285 ug/l
RT: 2.895 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion: 94 Resp: 222
Ion Ratio Lower Upper
94 100
96 73.5 72.7 109.1

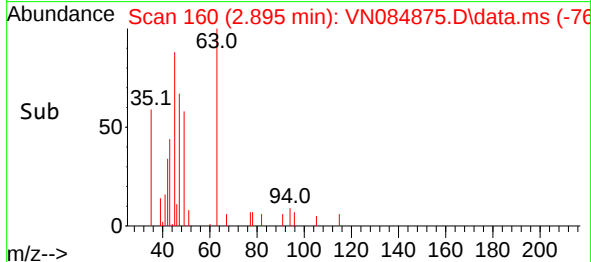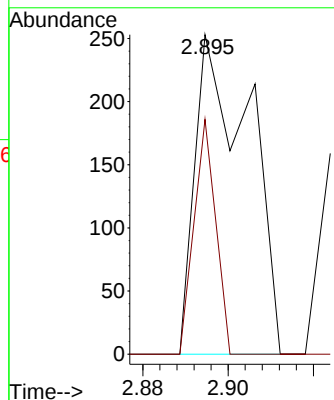

#6
Chloroethane
Concen: 4.322 ug/l
RT: 2.953 min Scan# 170
Delta R.T. -0.106 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 64 Resp: 4350
Ion Ratio Lower Upper
64 100
66 0.0 22.1 33.1#


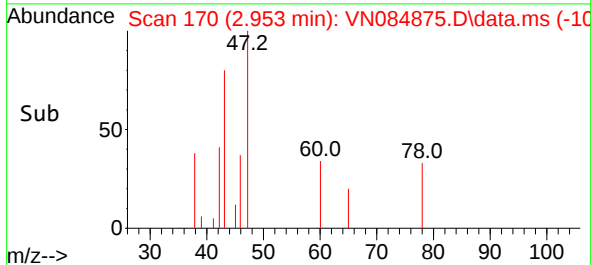
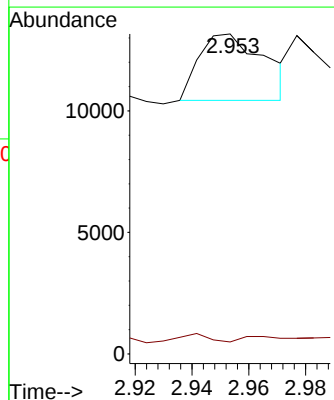





#12
Methyl Acetate
Concen: 8.810 ug/l
RT: 5.030 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion: 43 Resp: 18868
Ion Ratio Lower Upper
43 100
74 25.6 19.0 28.4

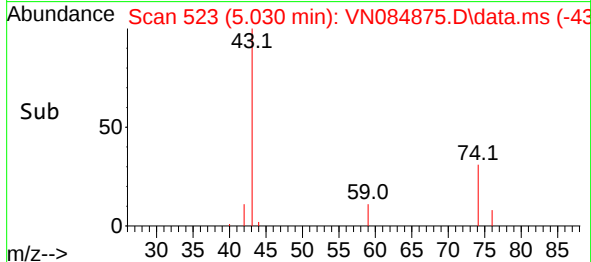

#15
Acetone
Concen: 619.747 ug/l
RT: 4.424 min Scan# 420
Delta R.T. -0.006 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 58 Resp: 111564
Ion Ratio Lower Upper
58 100
43 307.7 233.0 349.6

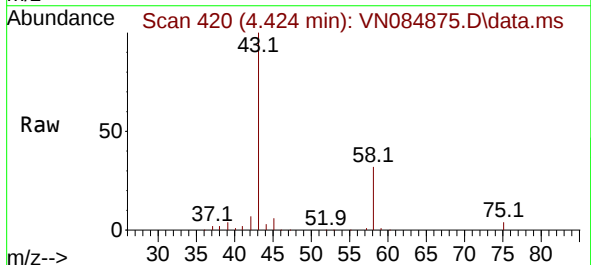



#16

Carbon Disulfide

Concen: 0.466 ug/l

RT: 4.706 min Scan# 4

Delta R.T. 0.012 min

Lab File: VN084875.D

Acq: 15 Nov 2024 17:36

Instrument :

MSVOA_N

ClientSampleId :





002-35TH-AVE(NOV)

Tgt Ion: 76 Resp: 1883

Ion Ratio Lower Upper

76 100

78 4.3 6.6 9.8#

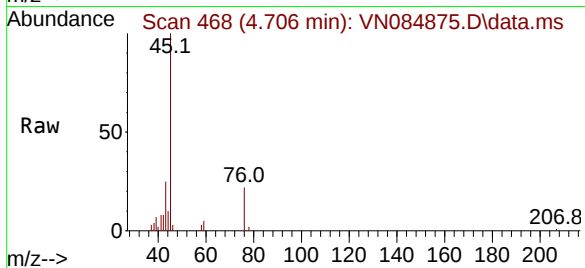

#18

Methylene Chloride

Concen: 0.426 ug/l

RT: 5.259 min Scan# 562

Delta R.T. -0.006 min

Lab File: VN084875.D

Acq: 15 Nov 2024 17:36

Tgt Ion: 84 Resp: 686




Ion Ratio Lower Upper


84 100

49 19.5 93.0 139.6#

51 21.3 28.9 43.3#

86 2.4 50.6 76.0#




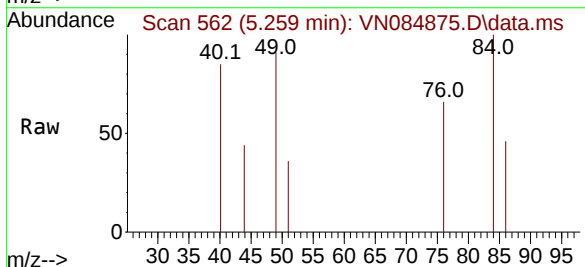




#23
tert-Butyl Alcohol
Concen: 0.495 ug/l
RT: 5.518 min Scan# 606
Delta R.T. -0.024 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion: 59 Resp: 121
Ion Ratio Lower Upper
59 100
52 0.0 0.0 0.0

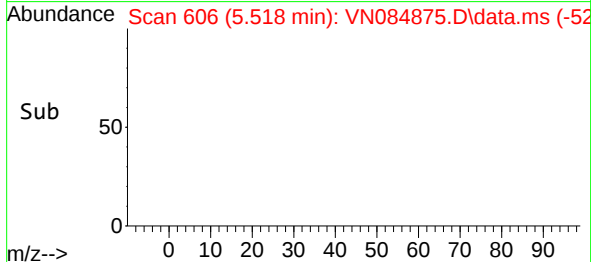

#25
Chloroform
Concen: 1.382 ug/l
RT: 7.959 min Scan# 1021
Delta R.T. -0.006 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 83 Resp: 3990
Ion Ratio Lower Upper
83 100
85 60.4 53.4 80.2




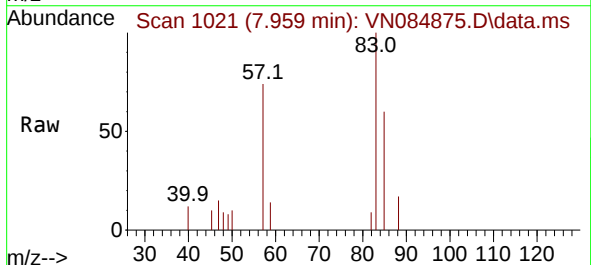


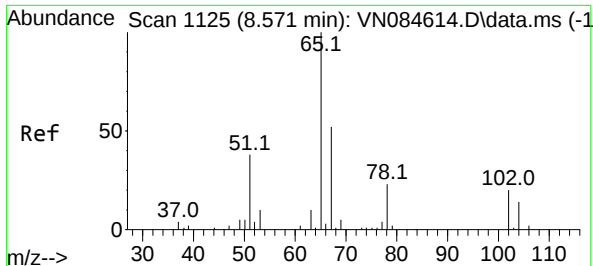

#27
1,2-Dichloroethane-d4
Concen: 30.806 ug/l
RT: 8.577 min Scan# 1125
Delta R.T. 0.006 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion: 65 Resp: 58387
Ion Ratio Lower Upper
65 100
67 51.3 40.7 61.1

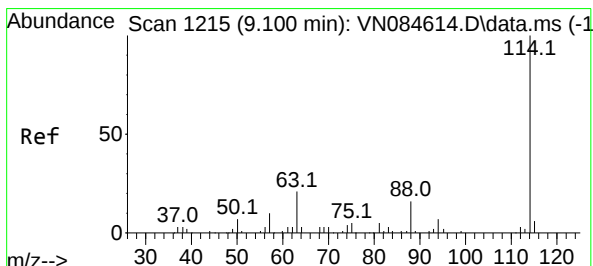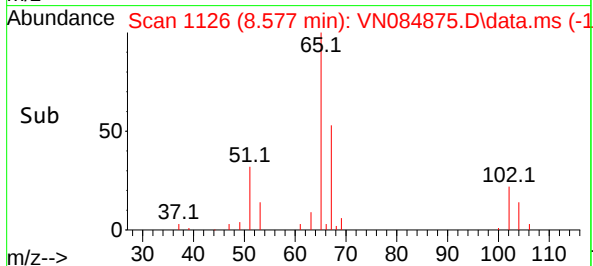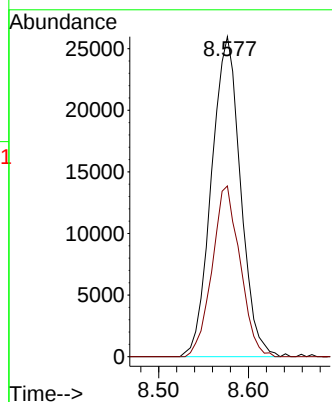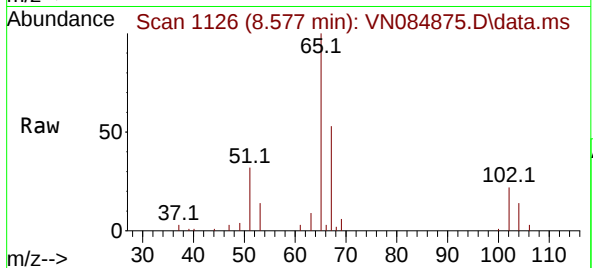

#28
1,4-Difluorobenzene
Concen: 30.000 ug/l
RT: 9.100 min Scan# 1215
Delta R.T. -0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 114 Resp: 122982
Ion Ratio Lower Upper
114 100
63 21.0 16.8 25.2
88 17.0 12.9 19.3


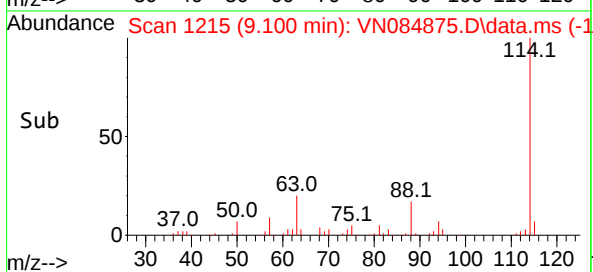
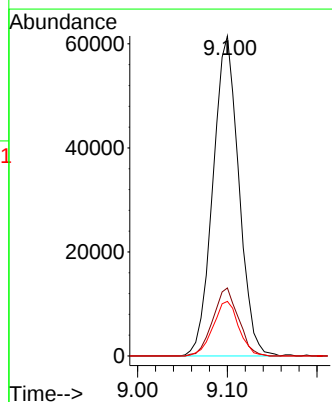
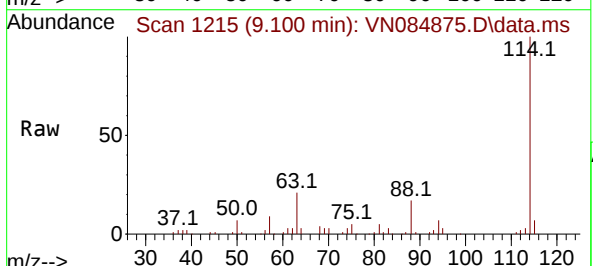




#30
2-Butanone
Concen: 44.883 ug/l
RT: 7.482 min Scan# 940
Delta R.T. -0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion: 43 Resp: 38351
Ion Ratio Lower Upper
43 100
57 7.9 6.2 9.4
72 27.0 21.5 32.3

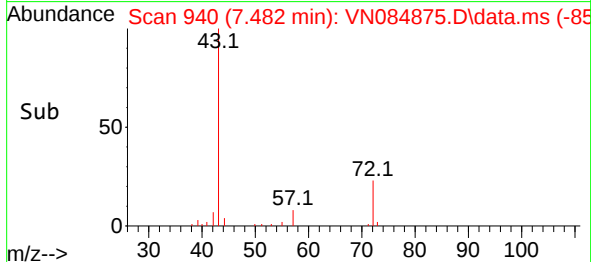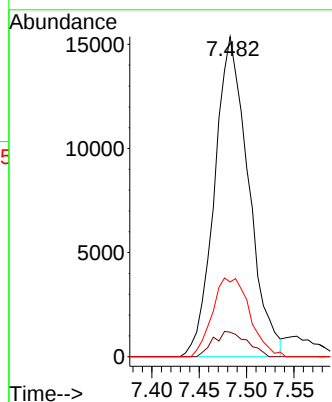

#35
Methacrylonitrile
Concen: 1.798 ug/l
RT: 7.782 min Scan# 991
Delta R.T. 0.006 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 41 Resp: 1821
Ion Ratio Lower Upper
41 100
39 32.8 28.2 84.6
67 0.0 35.6 106.8#
52 0.0 14.4 43.4#

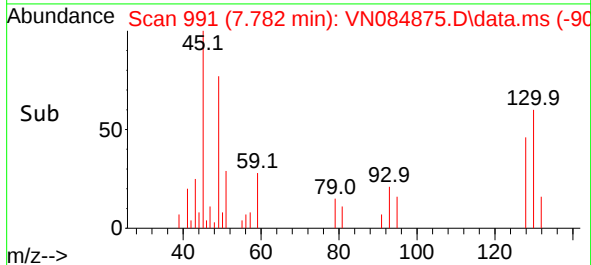

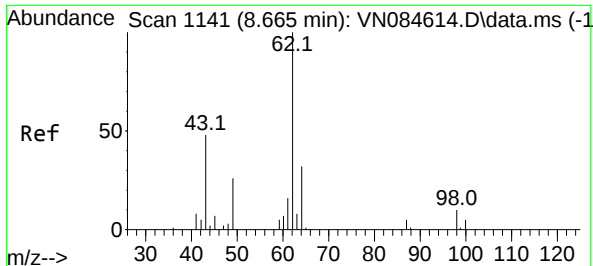

#36

1,2-Dichloroethane

Concen: 2.075 ug/l

RT: 9.094 min Scan# 1141

Delta R.T. 0.429 min

Lab File: VN084875.D

Acq: 15 Nov 2024 17:36

Instrument :

MSVOA_N

ClientSampleId :





002-35TH-AVE(NOV)

Tgt Ion: 62 Resp: 4224

Ion Ratio Lower Upper

62 100

98 0.0 7.8 11.6#

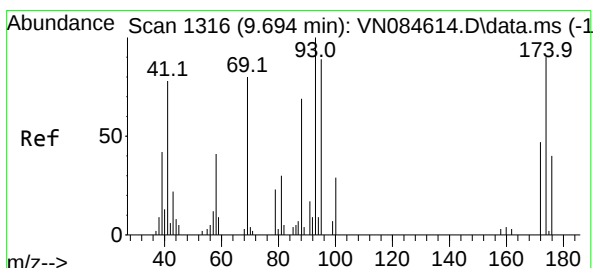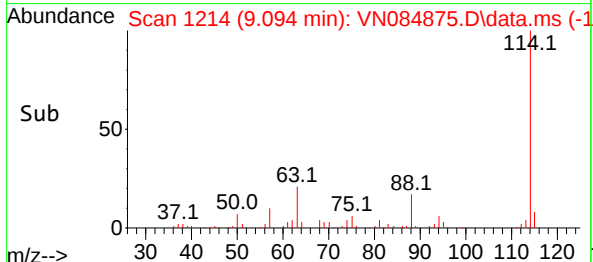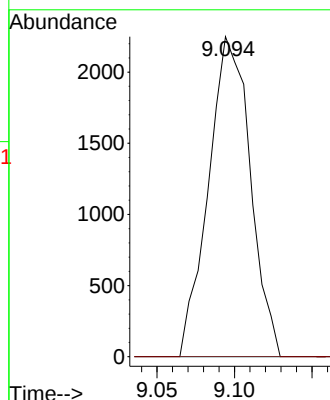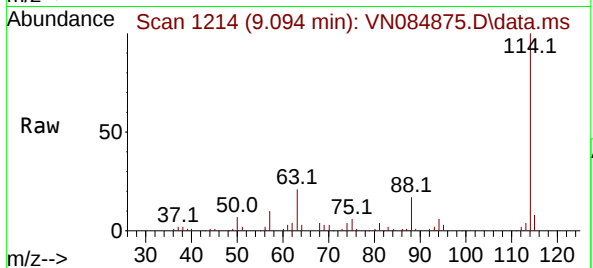

#45

1,4-Dioxane

Concen: 7.828 ug/l

RT: 9.341 min Scan# 1256

Delta R.T. -0.353 min

Lab File: VN084875.D

Acq: 15 Nov 2024 17:36




Tgt Ion: 88 Resp: 190


Ion Ratio Lower Upper

88 100

43 42.1 20.8 31.2#

58 0.0 53.4 80.2#


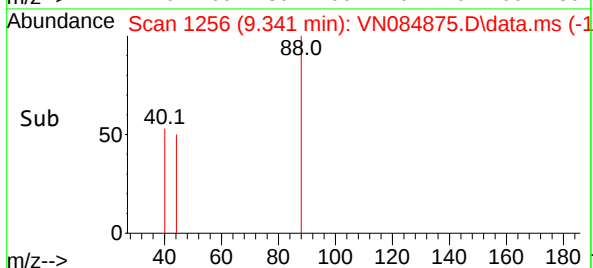
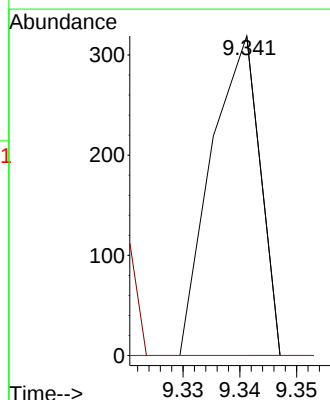
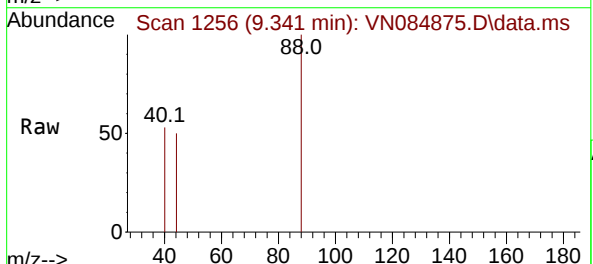


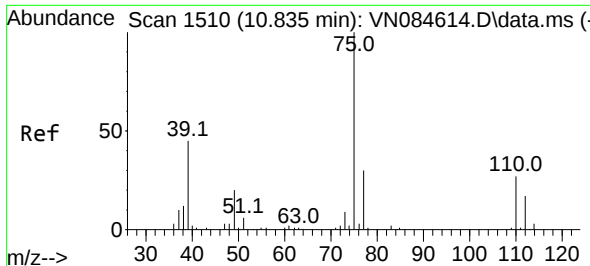

#48
t-1,3-Dichloropropene
Concen: 4.444 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. -0.206 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion: 75 Resp: 9699
Ion Ratio Lower Upper
75 100
77 170.4 24.4 36.6#

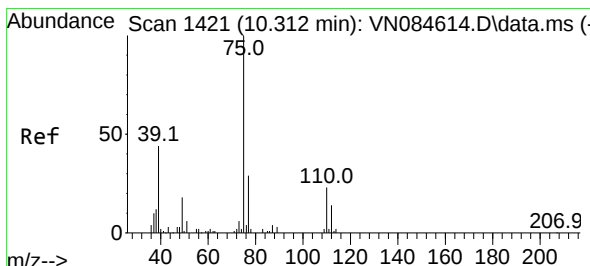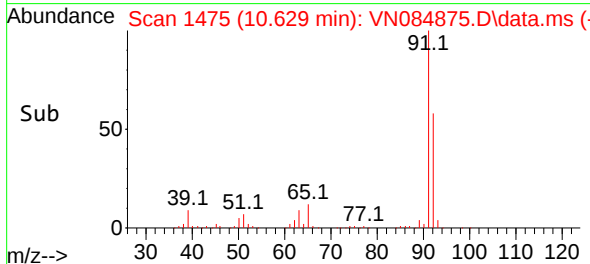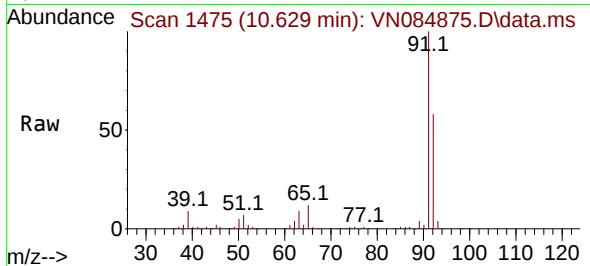

#49
cis-1,3-Dichloropropene
Concen: 4.146 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. 0.317 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 75 Resp: 9699
Ion Ratio Lower Upper
75 100
77 170.4 23.4 35.2#
39 1150.5 35.4 53.2#


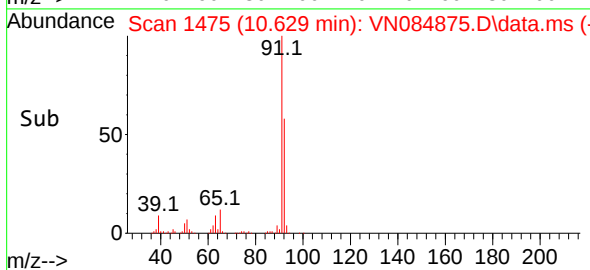

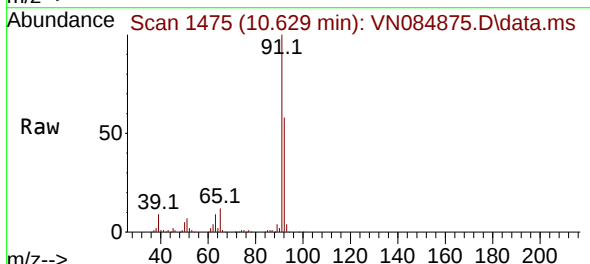




#50
1,1,2-Trichloroethane
Concen: 0.262 ug/l
RT: 10.882 min Scan# 1475
Delta R.T. -0.135 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion: 97	Resp:	362
Ion	Ratio	Lower Upper
97	100	
83	0.0	69.8 104.8#
85	0.0	48.6 73.0#
99	0.0	52.9 79.3#

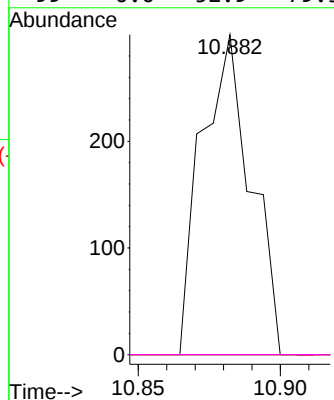

#55
2-Chloroethyl vinyl ether
Concen: 90.181 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. 0.470 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 63	Resp:	94256
Ion	Ratio	Lower Upper
63	100	
65	133.6	25.5 38.3#
106	0.0	22.3 33.5#


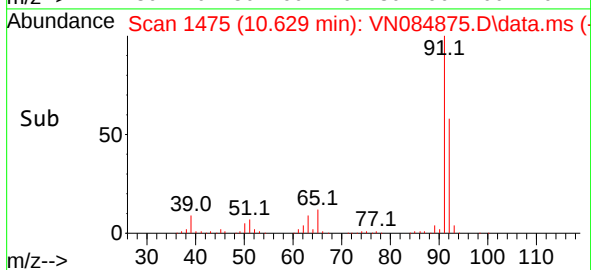
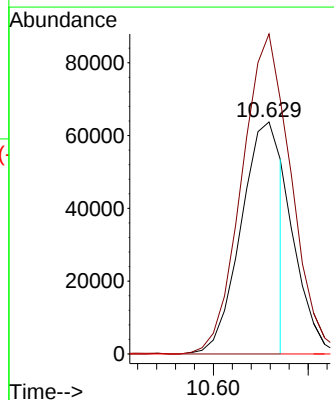





#56
Bromoform
Concen: 0.399 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.270 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion:173 Resp: 433
Ion Ratio Lower Upper
173 100
175 679.4 39.4 59.2#
254 0.0 6.4 9.6#

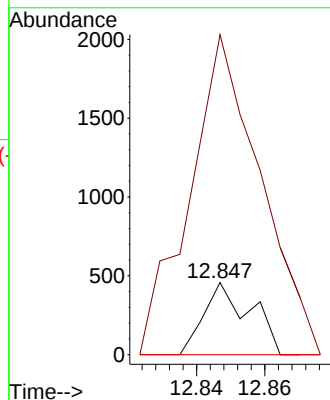

#57
Chlorobenzene-d5
Concen: 30.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion:117 Resp: 114966
Ion Ratio Lower Upper
117 100
82 57.5 45.5 68.3
119 32.1 25.3 37.9

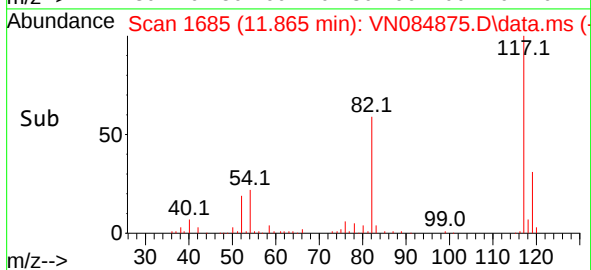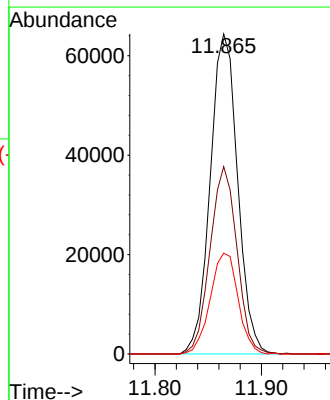



#58

4-Methyl-2-Pentanone

Concen: 7.840 ug/l

RT: 10.441 min Scan# 1444

Delta R.T. -0.006 min

Lab File: VN084875.D

Acq: 15 Nov 2024 17:36

Instrument :

MSVOA_N

ClientSampleId :

002-35TH-AVE(NOV)





Tgt Ion: 43 Resp: 14219

Ion Ratio Lower Upper

43 100

58 36.9 31.2 46.8

85 16.9 14.9 22.3

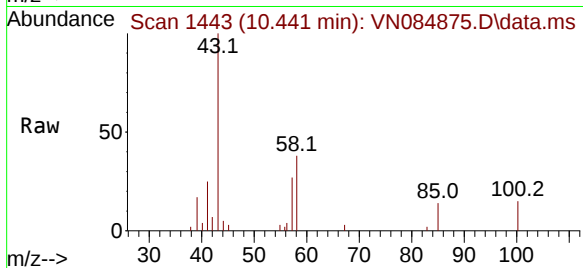

#59

2-Hexanone

Concen: 0.333 ug/l

RT: 11.194 min Scan# 1571

Delta R.T. -0.000 min

Lab File: VN084875.D

Acq: 15 Nov 2024 17:36




Tgt Ion: 43 Resp: 442


Ion Ratio Lower Upper

43 100

58 0.0 43.8 65.6#

57 0.0 15.0 22.6#




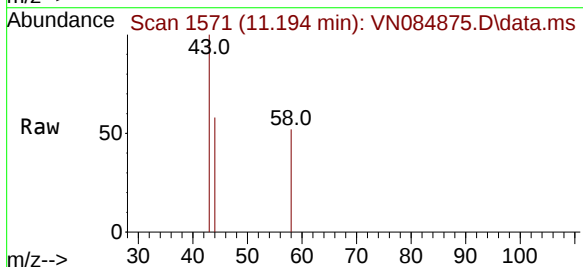




#60
4-Bromofluorobenzene
Concen: 26.404 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion: 95 Resp: 52268
Ion Ratio Lower Upper
95 100
174 75.2 59.6 89.4
176 73.4 58.6 88.0

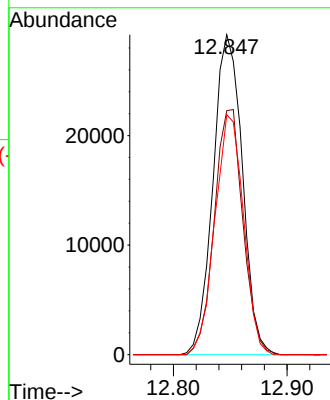

#62
Toluene
Concen: 208.406 ug/l
RT: 10.629 min Scan# 1475
Delta R.T. -0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 91 Resp: 1364653
Ion Ratio Lower Upper
91 100
92 58.0 47.5 71.3



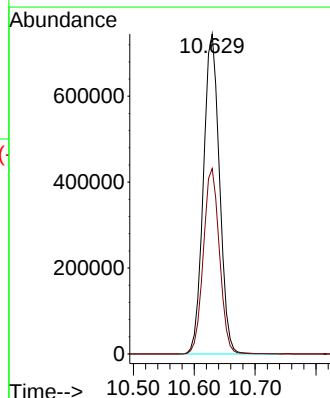



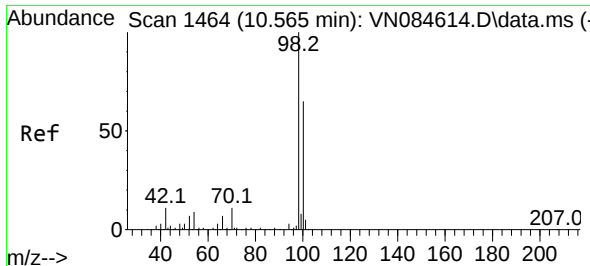

#63
Toluene-d8
Concen: 28.164 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion: 98 Resp: 153284
Ion Ratio Lower Upper
98 100
100 64.8 52.2 78.2

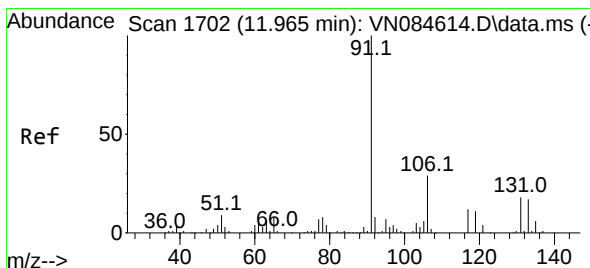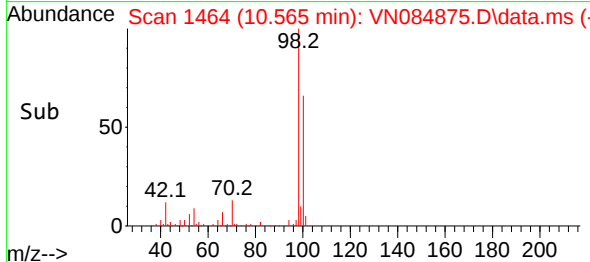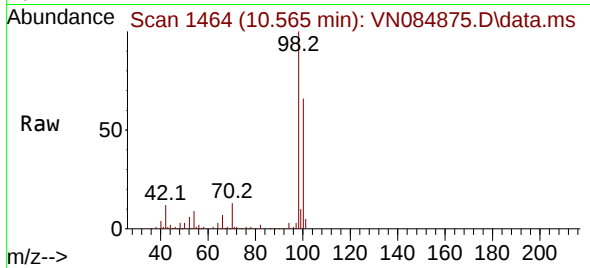

#66
Ethyl Benzene
Concen: 0.280 ug/l
RT: 11.959 min Scan# 1701
Delta R.T. -0.006 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 91 Resp: 1924
Ion Ratio Lower Upper
91 100
106 26.7 22.9 34.3


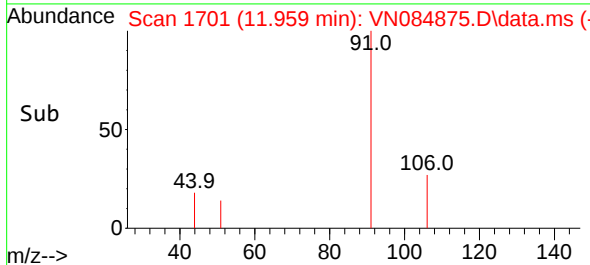

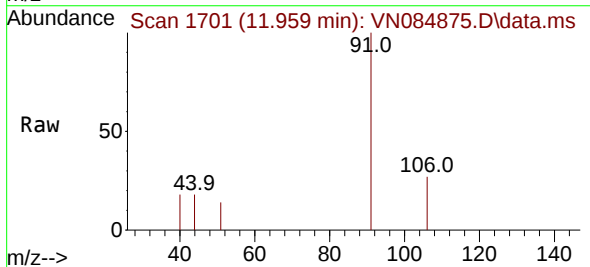




#67
m/p-Xylenes
Concen: 0.788 ug/l
RT: 12.070 min Scan# 1720
Delta R.T. -0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion:106 Resp: 2075
Ion Ratio Lower Upper
106 100
91 210.4 168.1 252.1



#68
o-Xylene
Concen: 0.299 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. -0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion:106 Resp: 759
Ion Ratio Lower Upper
106 100
91 256.3 107.7 322.9


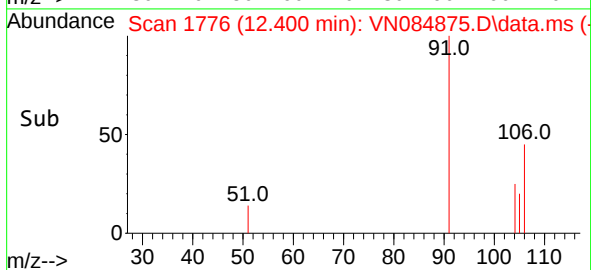






#70
Isopropylbenzene
Concen: 0.293 ug/l
RT: 13.094 min Scan# 1847
Delta R.T. 0.400 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion:105 Resp: 1847
Ion Ratio Lower Upper
105 100
120 32.9 18.7 34.7

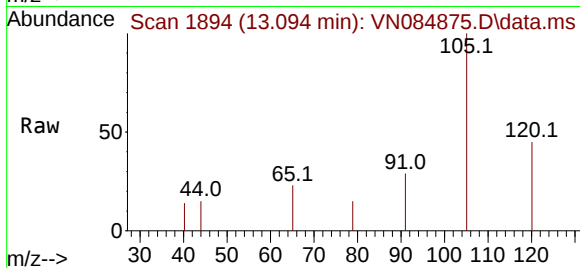

#72
1,2,3-Trichloropropane
Concen: 15.053 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.147 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 75 Resp: 26302
Ion Ratio Lower Upper
75 100
77 1.0 0.0 358.4




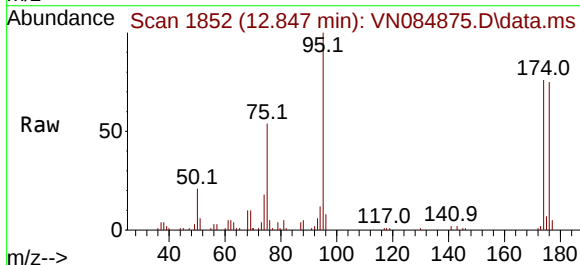




#77
t-1,4-Dichloro-2-butene
Concen: 36.702 ug/l
RT: 12.847 min Scan# 11
Delta R.T. 0.112 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion: 75 Resp: 26302
Ion Ratio Lower Upper
75 100
53 0.0 52.4 157.2#
89 0.0 26.0 78.0#

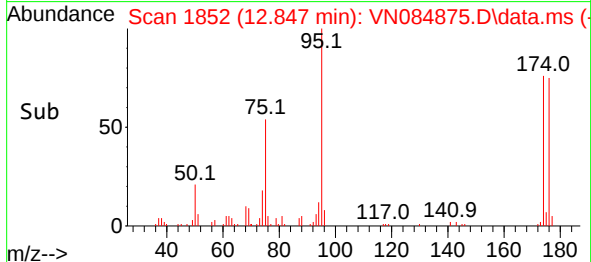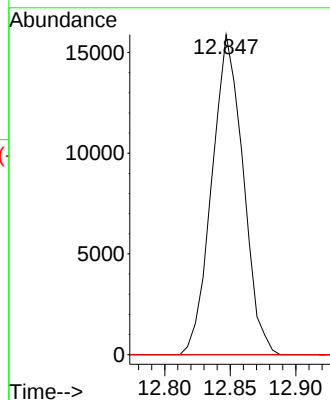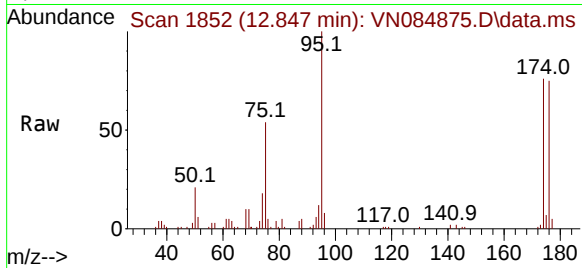

#79
tert-butylbenzene
Concen: 4.310 ug/l
RT: 13.729 min Scan# 2002
Delta R.T. 0.294 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 119 Resp: 19225
Ion Ratio Lower Upper
119 100
91 32.0 0.0 143.2
134 26.5 0.0 49.4


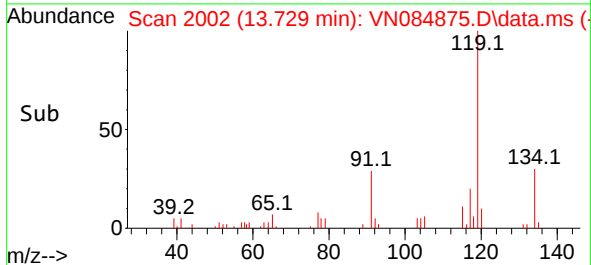
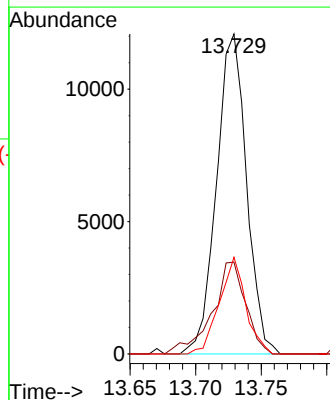
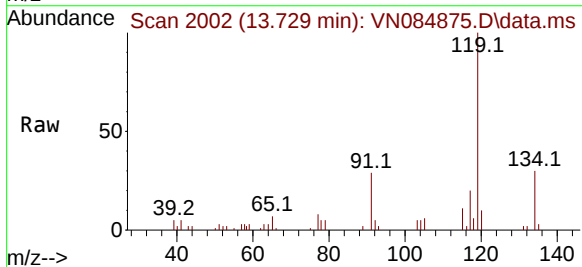




#80
1,2,4-Trimethylbenzene
Concen: 0.885 ug/l
RT: 13.482 min Scan# 1960
Delta R.T. -0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36




Instrument :
MSVOA_N
ClientSampleId :
002-35TH-AVE(NOV)


Tgt Ion:105 Resp: 4816
Ion Ratio Lower Upper
105 100
120 31.5 0.0 90.4



#82
p-Isopropyltoluene
Concen: 3.722 ug/l
RT: 13.729 min Scan# 2002
Delta R.T. -0.000 min
Lab File: VN084875.D
Acq: 15 Nov 2024 17:36

Tgt Ion:119 Resp: 19225
Ion Ratio Lower Upper
119 100
134 26.5 0.0 51.4
91 32.0 0.0 50.4

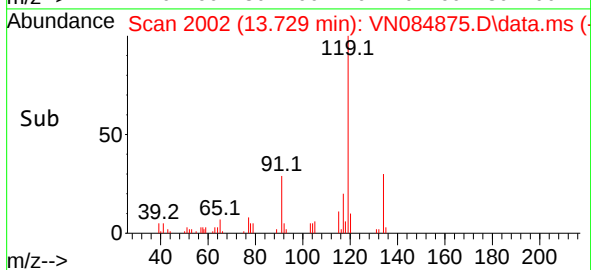



#86

Hexachloroethane

Concen: 0.205 ug/l

RT: 14.435 min Scan# 2104

Delta R.T. 0.106 min

Lab File: VN084875.D

Acq: 15 Nov 2024 17:36

Instrument :

MSVOA_N

ClientSampleId :





002-35TH-AVE(NOV)

Tgt Ion:117 Resp: 217

Ion Ratio Lower Upper

117 100

201 0.0 34.4 103.3#

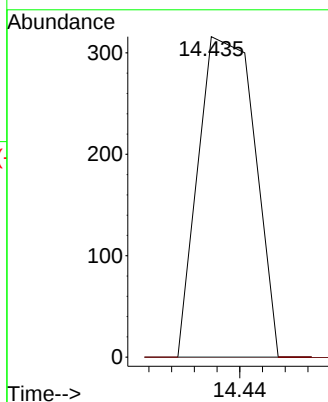

#91

Naphthalene

Concen: 0.652 ug/l

RT: 15.635 min Scan# 2326

Delta R.T. -0.006 min

Lab File: VN084875.D

Acq: 15 Nov 2024 17:36

Tgt Ion:128 Resp: 3007

Ion Ratio Lower Upper

128 100

127 7.9 10.3 15.5#

129 7.7 8.6 12.8#

