


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN111618\
Data File : VN052350.D
Acq On : 16 Nov 2018 7:41
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 28

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
Title : SW846 8260
Last Update : Thu Nov 15 03:02:37 2018

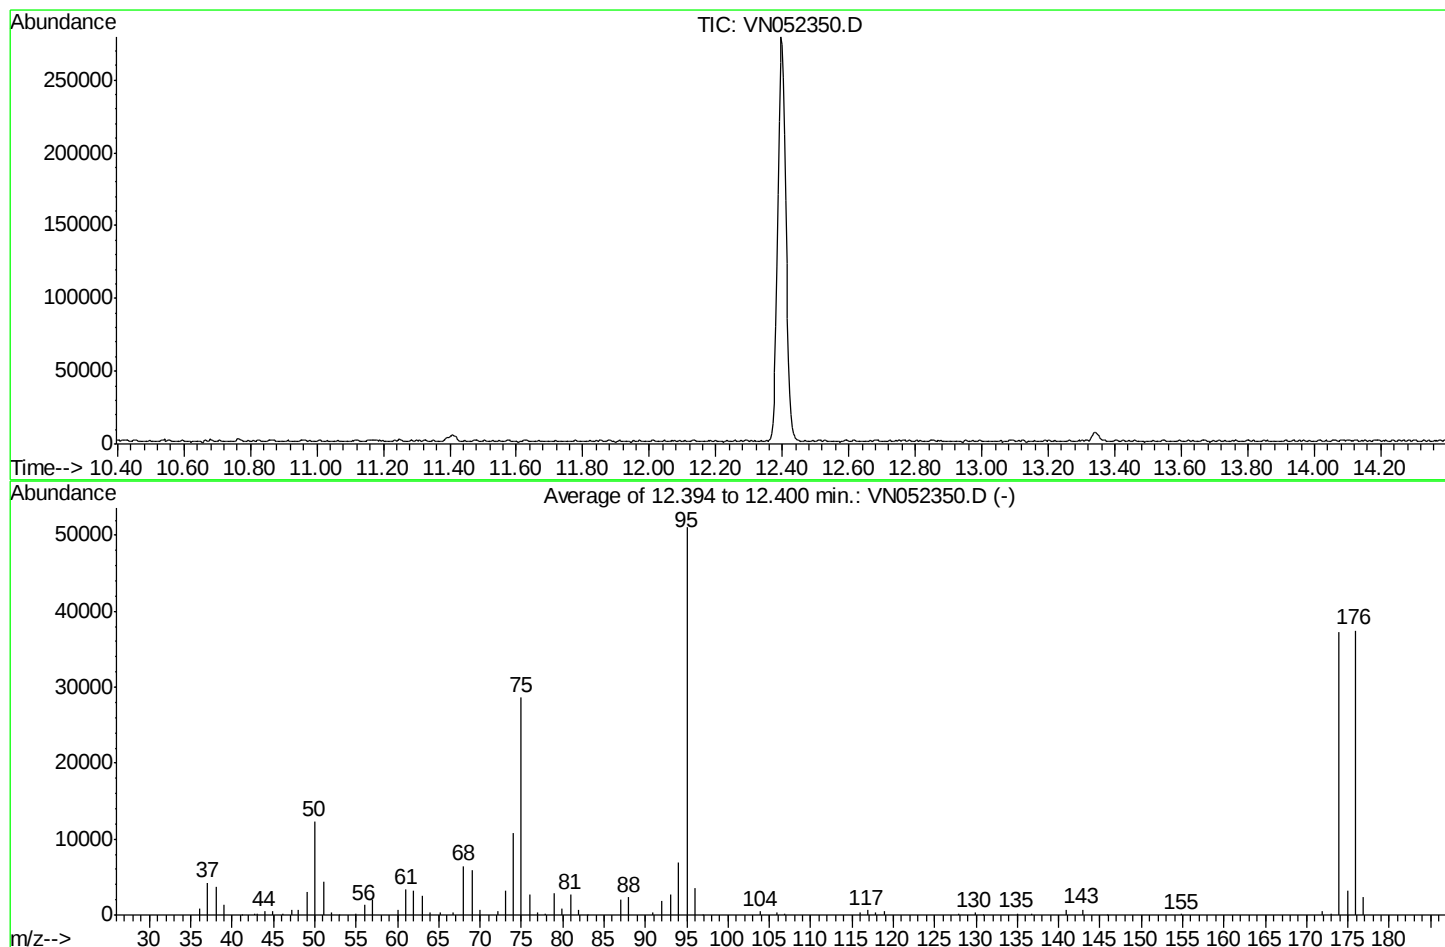

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	12259	PASS
75	95	30	60	56.0	28592	PASS
95	95	100	100	100.0	51048	PASS
96	95	5	9	6.9	3508	PASS
173	174	0.00	2	0.6	225	PASS
174	95	50	100	73.0	37261	PASS
175	174	5	9	8.7	3225	PASS
176	174	95	101	100.5	37450	PASS
177	176	5	9	6.5	2446	PASS