


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN111620\
 Data File : VN064648.D
 Acq On : 16 Nov 2020 8:11
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110420W.M
 Title : SW846 8260
 Last Update : Wed Nov 04 12:09:03 2020

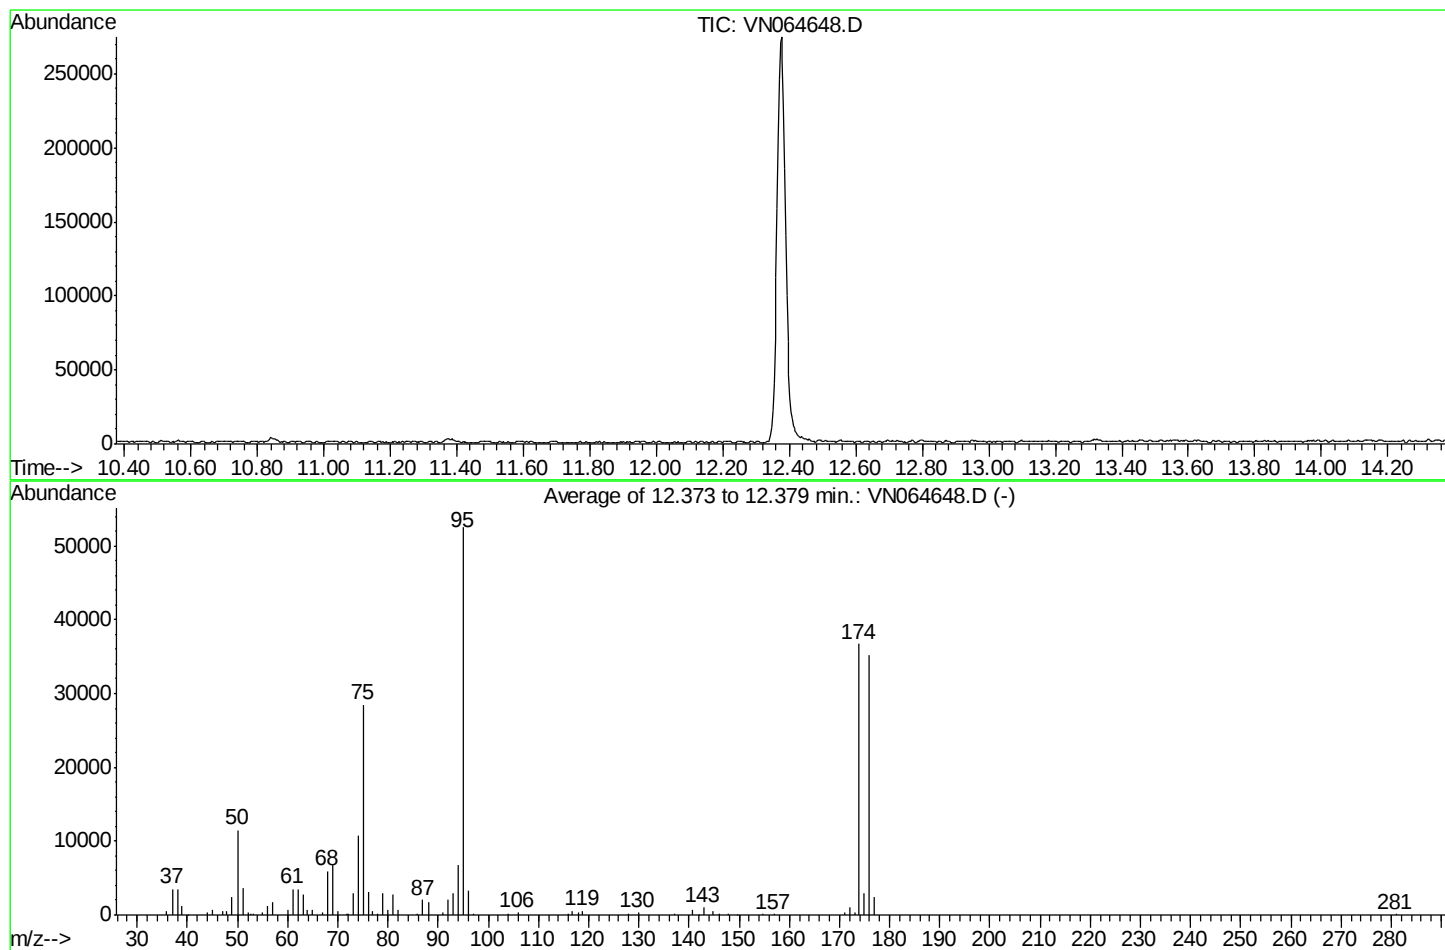

AutoFind: Scans 3307, 3308, 3309; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	11515	PASS
75	95	30	60	54.2	28448	PASS
95	95	100	100	100.0	52501	PASS
96	95	5	9	6.3	3282	PASS
173	174	0.00	2	0.9	314	PASS
174	95	50	100	69.9	36677	PASS
175	174	5	9	7.8	2874	PASS
176	174	95	101	96.0	35202	PASS
177	176	5	9	6.8	2389	PASS