

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111621\
 Data File : VN069505.D
 Acq On : 16 Nov 2021 12:31
 Operator : JC/MD
 Sample : VN1116MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 16 16:17:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 09 18:18:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	1376064	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2395814	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.744	117	2343124	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	878372	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	995293	49.884	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	99.760%		
35) Dibromofluoromethane	8.024	113	701876	48.846	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	97.700%		
50) Toluene-d8	10.440	98	3012708	53.310	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	106.620%		
62) 4-Bromofluorobenzene	12.731	95	1052951	50.718	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	101.440%		
Target Compounds					Qvalue	
13) Acrolein	4.057	56	286	Below Cal	#	1
15) Acrylonitrile	5.565	53	2220	0.241	ug/l #	39
16) Acetone	4.288	43	5087	0.473	ug/l	96
25) 2-Butanone	7.348	43	4024	0.276	ug/l	93
29) Tetrahydrofuran	7.702	42	2048	0.229	ug/l #	51
31) Cyclohexane	8.083	56	36466	1.338	ug/l #	31
36) 1,1-Dichloropropene	8.086	75	118773	5.892	ug/l #	49
38) Carbon Tetrachloride	8.086	117	144204	7.409	ug/l #	16
49) 1,4-Dioxane	9.569	88	472	40.170	ug/l #	8
53) t-1,3-Dichloropropene	10.719	75	410	2.653	ug/l #	81
54) cis-1,3-Dichloropropene	10.194	75	431	1.748	ug/l #	15
56) Ethyl methacrylate	10.765	69	2104	2.121	ug/l #	43
58) 2-Chloroethyl Vinyl ether	10.046	63	50	22.776	ug/l #	45
59) 2-Hexanone	11.089	43	23132	8.881	ug/l	83
60) Dibromochloromethane	11.237	129	143	2.425	ug/l #	11
61) 1,2-Dibromoethane	11.347	107	311	1.089	ug/l	100
70) Styrene	12.294	104	3879	1.591	ug/l #	83
71) Bromoform	12.457	173	332	3.451	ug/l #	29
74) N-amyl acetate	12.393	43	13676	0.461	ug/l #	89
76) 1,2,3-Trichloropropane	12.731	75	583330	28.777	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	583330	81.532	ug/l #	5
87) 1,3-Dichlorobenzene	13.616	146	6352	0.229	ug/l	97
88) 1,4-Dichlorobenzene	13.616	146	6352	0.233	ug/l	98
89) n-Butylbenzene	13.940	91	14774	0.322	ug/l	91
90) Hexachloroethane	14.203	117	214	2.182	ug/l #	6
91) 1,2-Dichlorobenzene	13.989	146	7052	0.267	ug/l	97
92) 1,2-Dibromo-3-Chloropr...	14.605	75	1273	2.077	ug/l	65
93) 1,2,4-Trichlorobenzene	15.263	180	11554	3.897	ug/l	97
95) Naphthalene	15.509	128	51802	5.661	ug/l	98
96) 1,2,3-Trichlorobenzene	15.700	180	13852	4.151	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111621\
Data File : VN069505.D
Acq On : 16 Nov 2021 12:31
Operator : JC/MD
Sample : VN1116MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Nov 16 16:17:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 09 18:18:22 2021
Response via : Initial Calibration




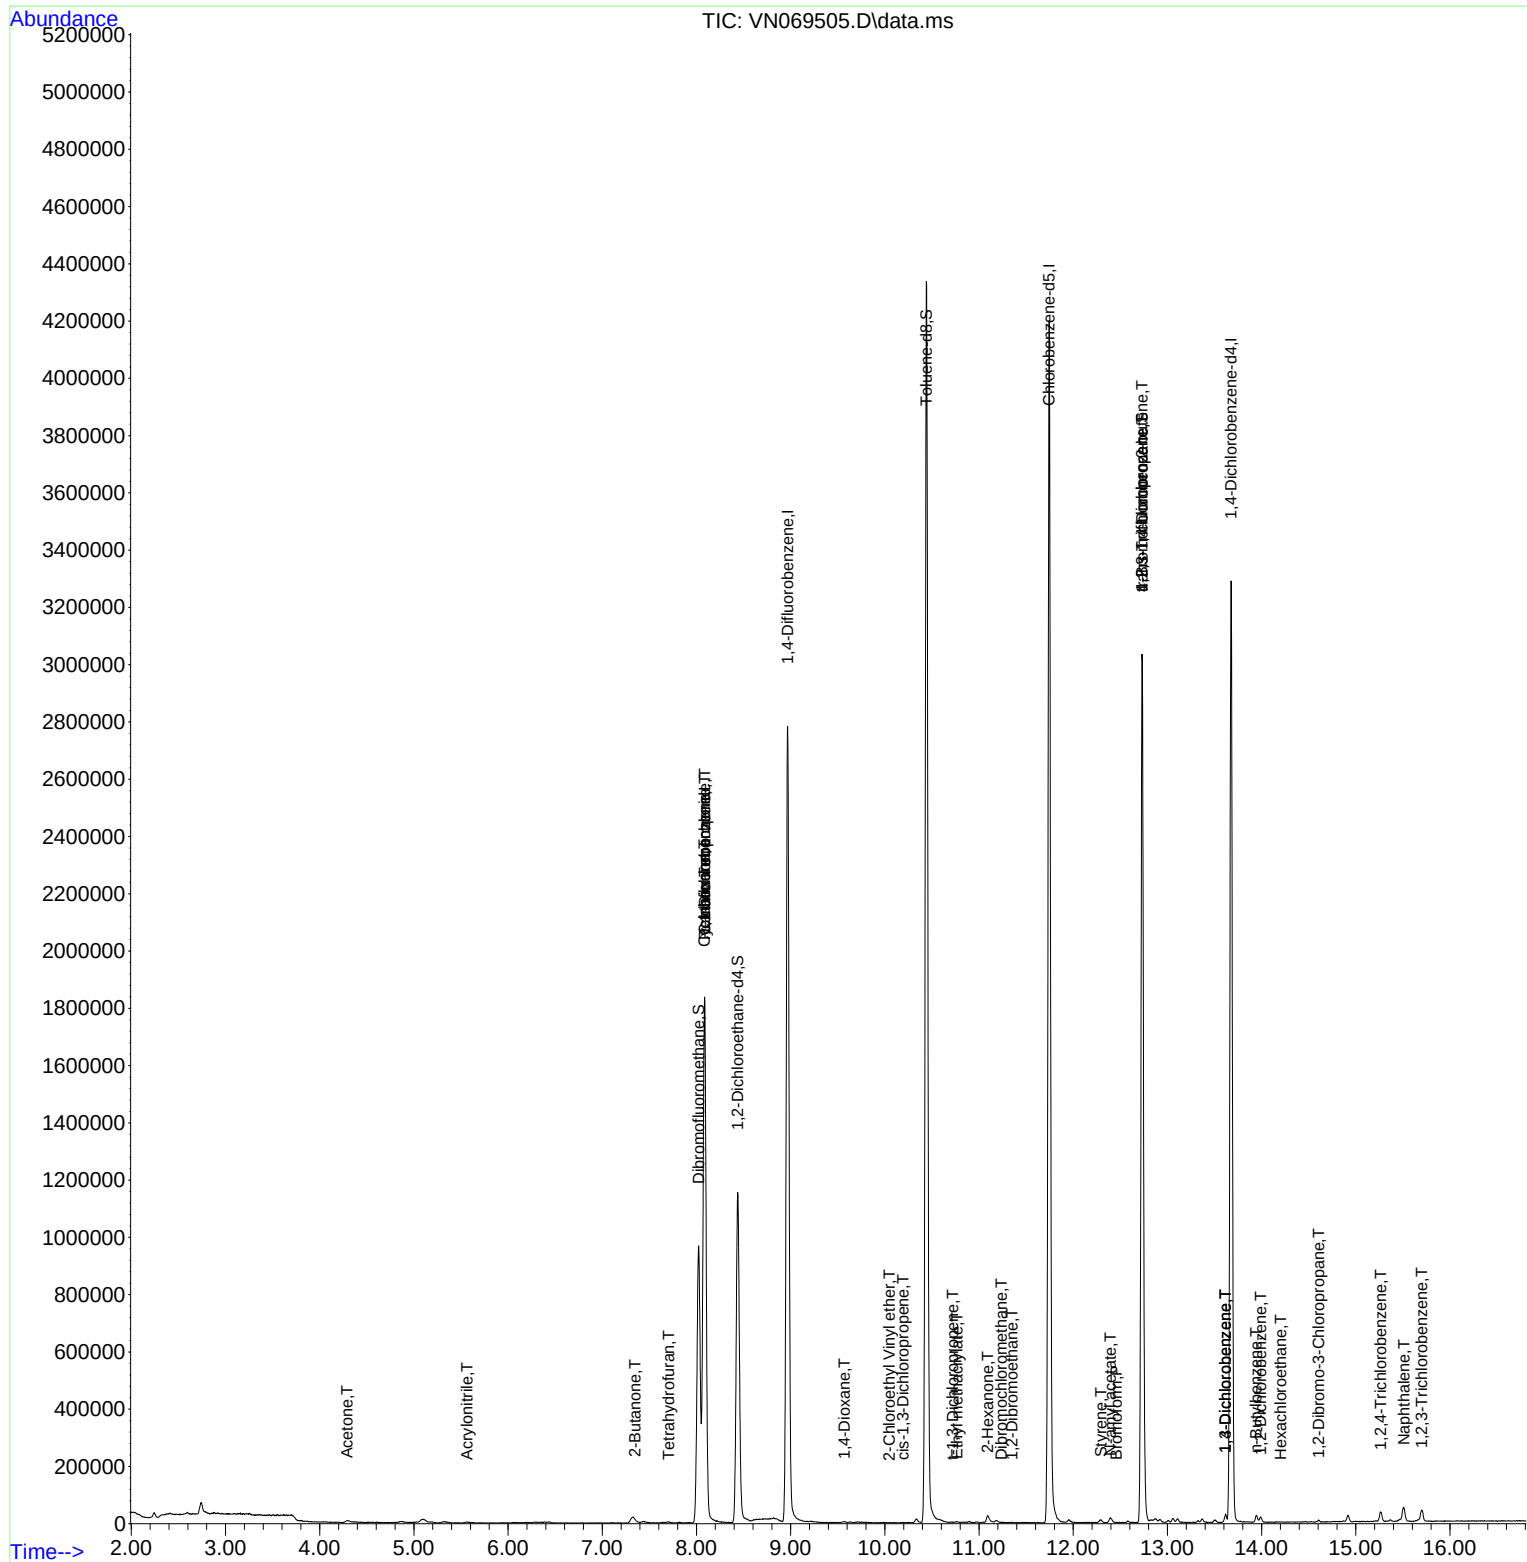




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 1376064
Ion Ratio Lower Upper
168 100
99 58.7 41.3 61.9

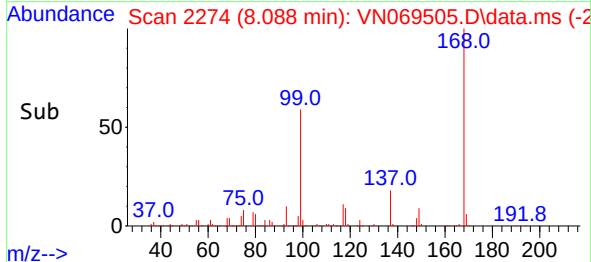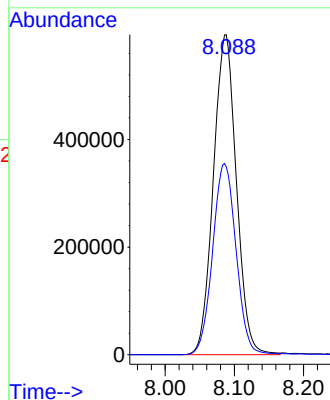

#13
Acrolein
Concen: Below Cal
RT: 4.057 min Scan# 771
Delta R.T. 0.016 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Tgt Ion: 56 Resp: 286
Ion Ratio Lower Upper
56 100
55 297.6 56.6 85.0#


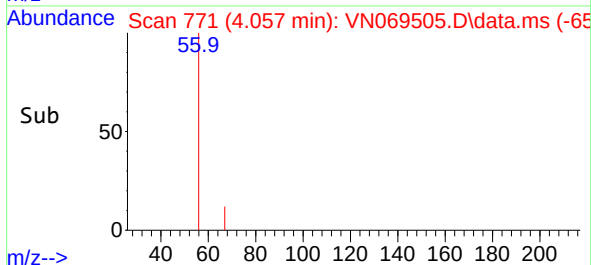
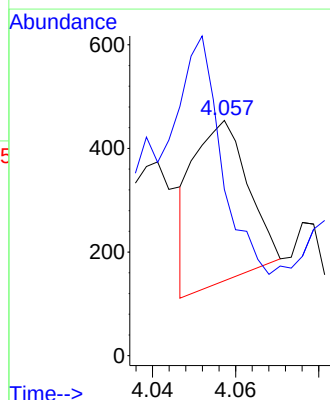
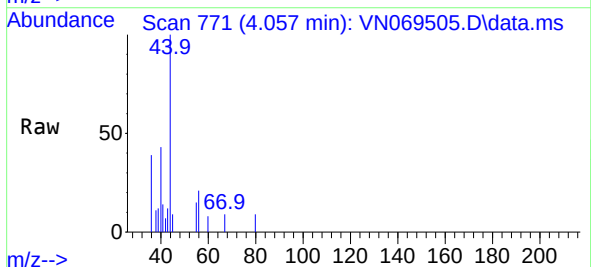


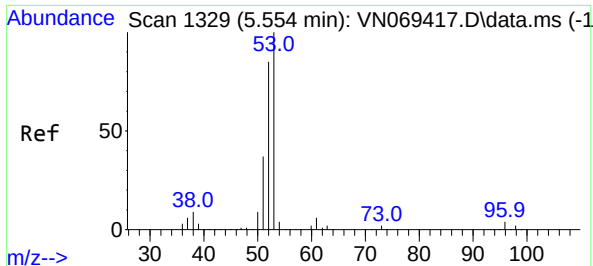

#15
Acrylonitrile
Concen: 0.241 ug/l
RT: 5.565 min Scan# 11
Delta R.T. 0.011 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 53 Resp: 2220
Ion Ratio Lower Upper
53 100
52 28.0 66.2 99.2#
51 0.0 29.6 44.4#

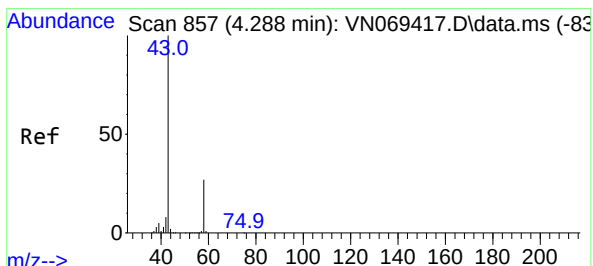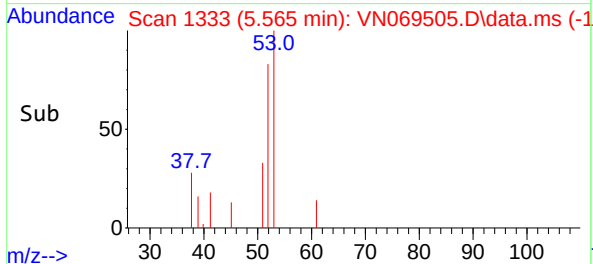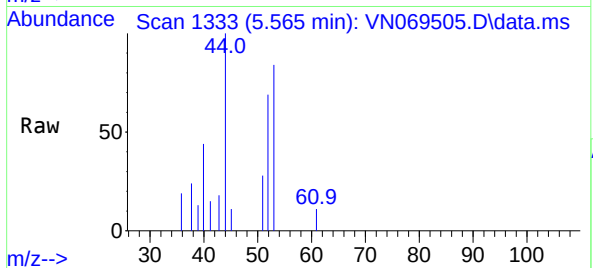

#16
Acetone
Concen: 0.473 ug/l
RT: 4.288 min Scan# 857
Delta R.T. -0.000 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Tgt Ion: 43 Resp: 5087
Ion Ratio Lower Upper
43 100
58 26.7 23.1 34.7


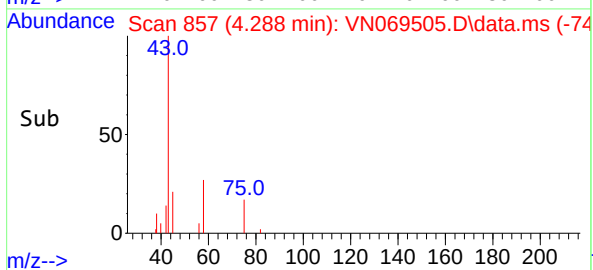

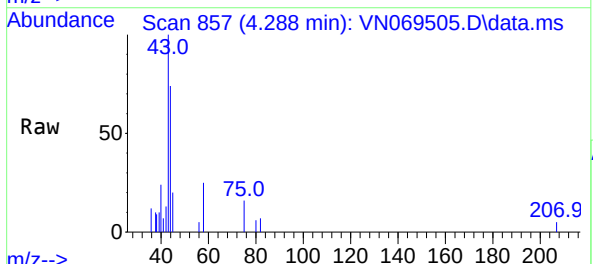


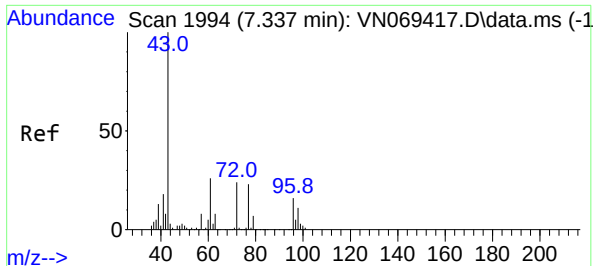

#25
2-Butanone
Concen: 0.276 ug/l
RT: 7.348 min Scan# 1994
Delta R.T. 0.011 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 4024
Ion Ratio Lower Upper
43 100
72 31.0 21.7 32.5

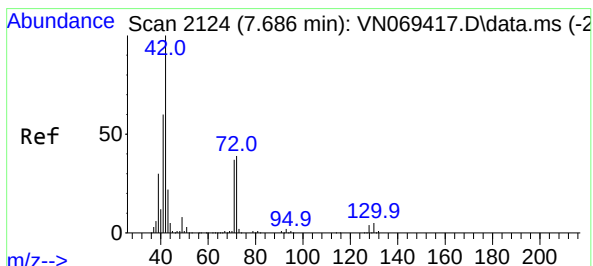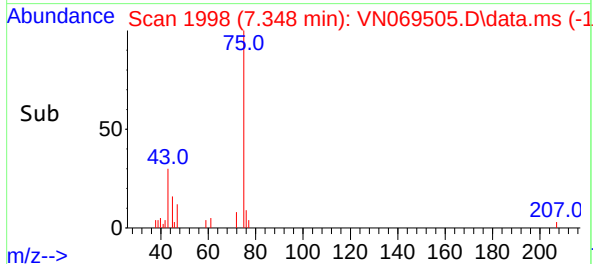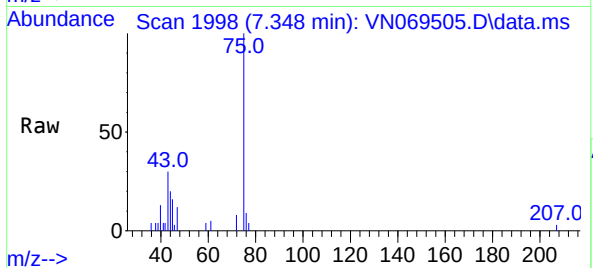

#29
Tetrahydrofuran
Concen: 0.229 ug/l
RT: 7.702 min Scan# 2130
Delta R.T. 0.016 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31


Tgt Ion: 42 Resp: 2048
Ion Ratio Lower Upper
42 100
72 13.3 36.3 54.5#
71 11.8 34.7 52.1#

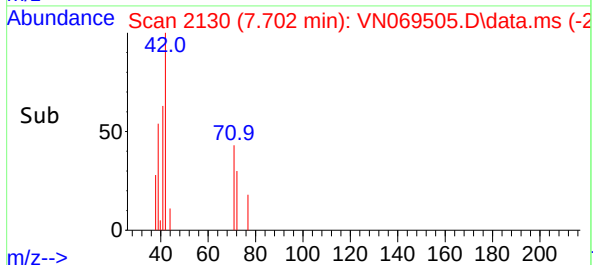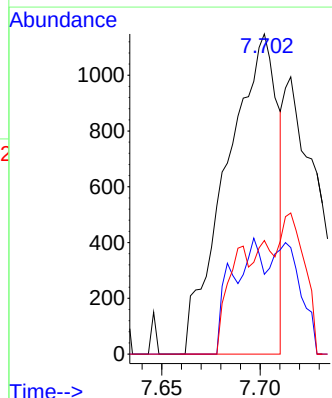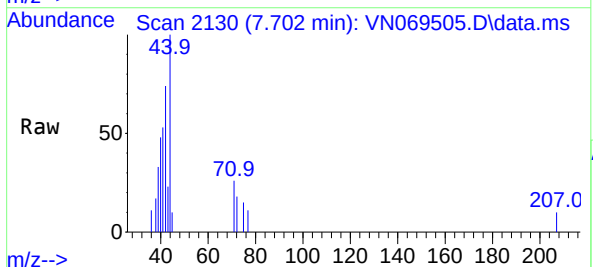



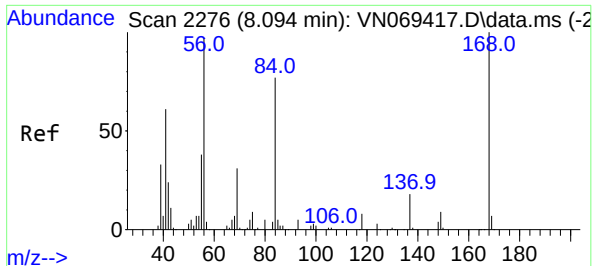


#31
Cyclohexane
Concen: 1.338 ug/l
RT: 8.083 min Scan# 21
Delta R.T. -0.011 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Instrument :
MSVOA_N
ClientSampleId :



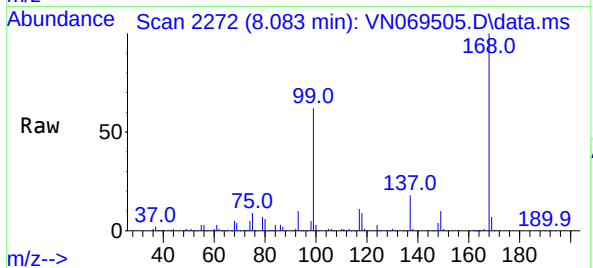



Tgt Ion: 56 Resp: 36466
Ion Ratio Lower Upper
56 100
69 141.2 27.1 40.7#
84 115.3 73.4 110.0#

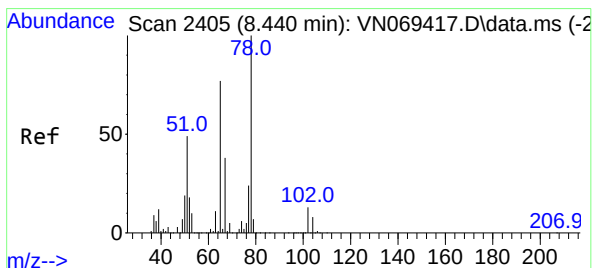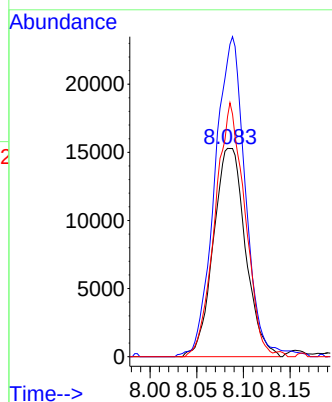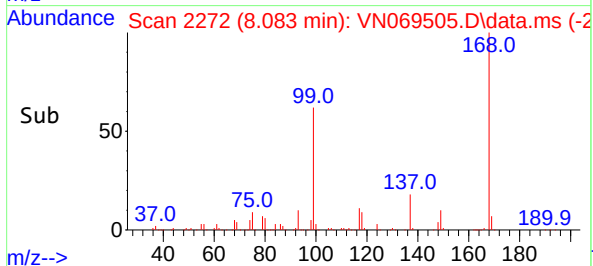

#33
1,2-Dichloroethane-d4
Concen: 49.884 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. -0.003 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31


Tgt Ion: 65 Resp: 995293
Ion Ratio Lower Upper
65 100
67 50.9 0.0 103.0

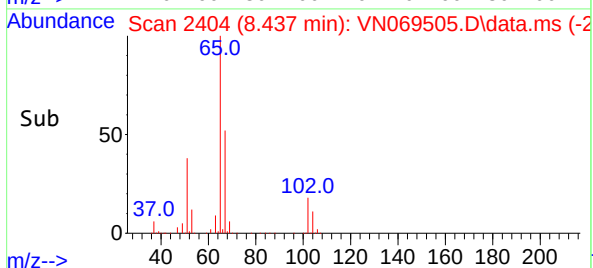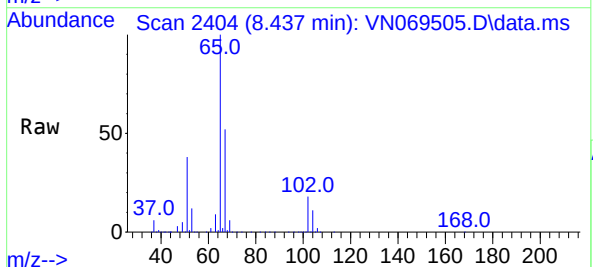






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:114 Resp: 2395814
Ion Ratio Lower Upper
114 100
63 22.6 0.0 37.8
88 15.7 0.0 27.4

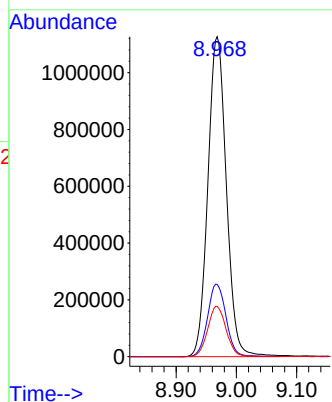

#35
Dibromofluoromethane
Concen: 48.846 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Tgt Ion:113 Resp: 701876
Ion Ratio Lower Upper
113 100
111 103.3 82.2 123.2
192 18.5 16.9 25.3

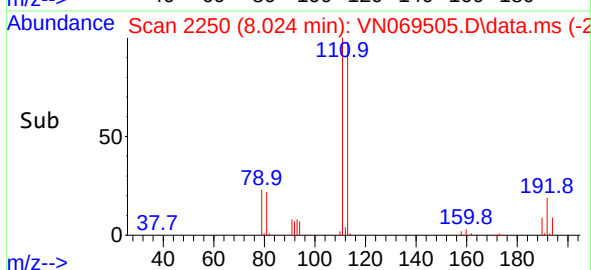

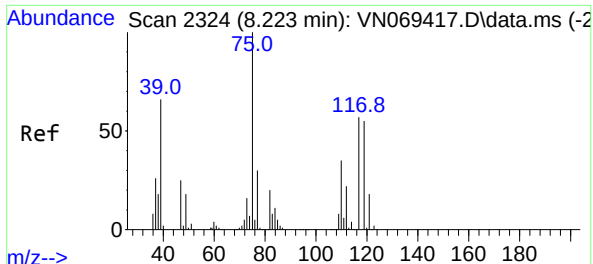

#36

1,1-Dichloropropene

Concen: 5.892 ug/l

RT: 8.086 min Scan# 21

Delta R.T. -0.137 min

Lab File: VN069505.D

Acq: 16 Nov 2021 12:31

Instrument :

MSVOA_N

ClientSampleId :





Tgt Ion: 75 Resp: 118773

Ion Ratio Lower Upper

75 100

110 8.5 18.4 55.2#

77 0.0 24.4 36.6#

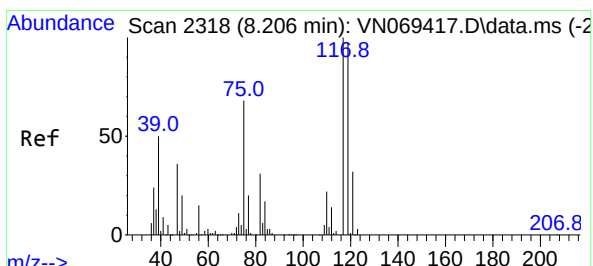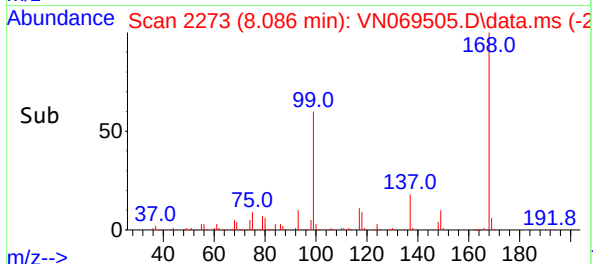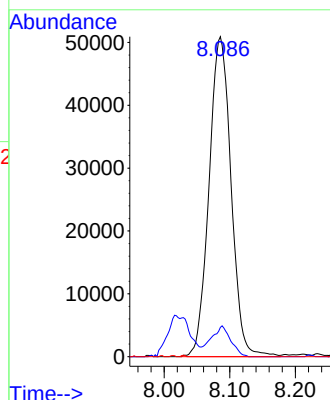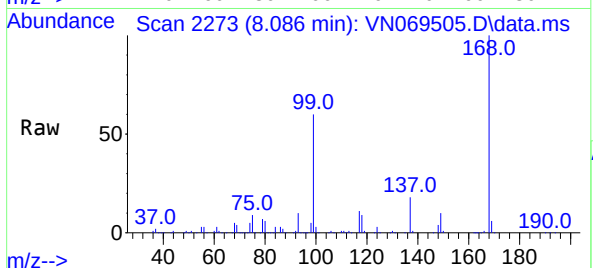

#38

Carbon Tetrachloride

Concen: 7.409 ug/l

RT: 8.086 min Scan# 2273

Delta R.T. -0.120 min

Lab File: VN069505.D

Acq: 16 Nov 2021 12:31




Tgt Ion: 117 Resp: 144204


Ion Ratio Lower Upper

117 100

119 4.8 76.1 114.1#

121 0.0 24.2 36.2#


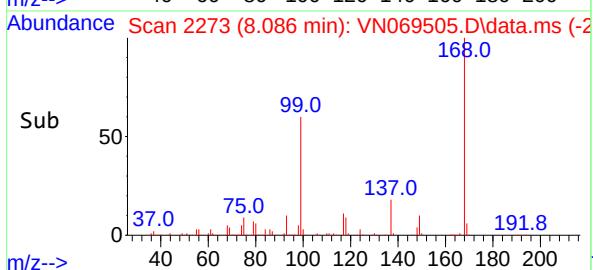
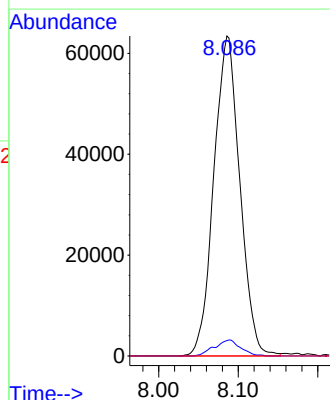
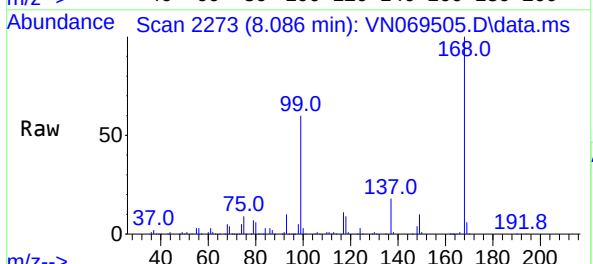




#49
1,4-Dioxane
Concen: 40.170 ug/l
RT: 9.569 min Scan# 21
Delta R.T. -0.003 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 88 Resp: 472
Ion Ratio Lower Upper
88 100
43 28.4 23.4 35.2
58 166.7 50.6 75.8#

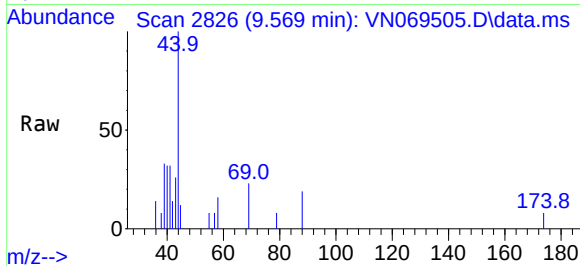

#50
Toluene-d8
Concen: 53.310 ug/l
RT: 10.440 min Scan# 3151
Delta R.T. -0.001 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Tgt Ion: 98 Resp: 3012708
Ion Ratio Lower Upper
98 100
100 63.8 50.4 75.6



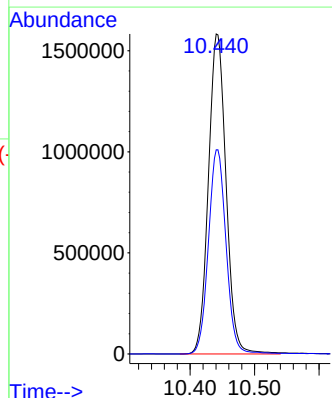
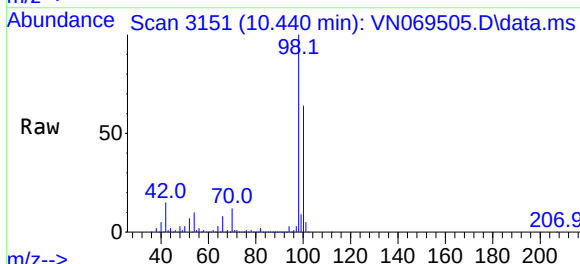




#53
t-1,3-Dichloropropene
Concen: 2.653 ug/l
RT: 10.719 min Scan# 31
Delta R.T. 0.000 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 410
Ion Ratio Lower Upper
75 100
77 42.7 25.6 38.4#

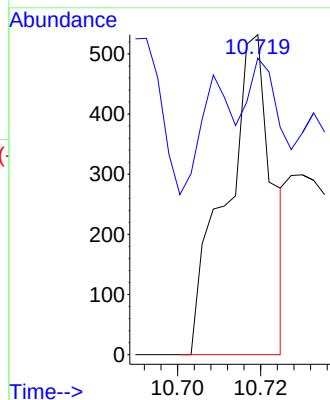

#54
cis-1,3-Dichloropropene
Concen: 1.748 ug/l
RT: 10.194 min Scan# 3059
Delta R.T. 0.006 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Tgt Ion: 75 Resp: 431
Ion Ratio Lower Upper
75 100
77 0.0 26.4 39.6#
39 125.7 42.5 63.7#


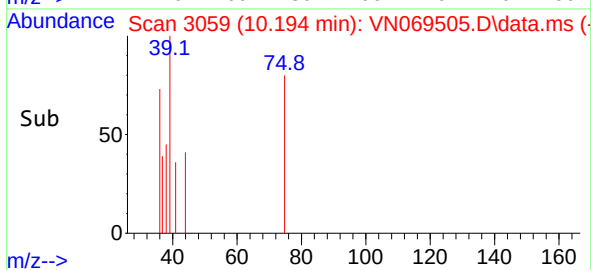
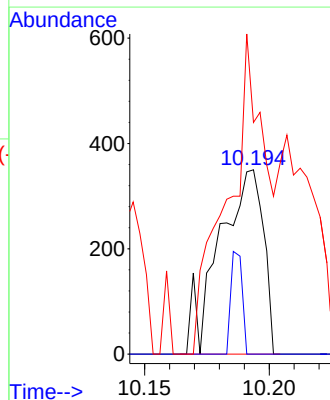





#56
Ethyl methacrylate
Concen: 2.121 ug/l
RT: 10.765 min Scan# 310
Delta R.T. 0.003 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 69 Resp: 2104
Ion Ratio Lower Upper
69 100
41 125.0 51.4 77.0#
39 25.7 34.6 52.0#



#58
2-Chloroethyl Vinyl ether
Concen: 22.776 ug/l
RT: 10.046 min Scan# 3004
Delta R.T. 0.005 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Tgt Ion: 63 Resp: 50
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#


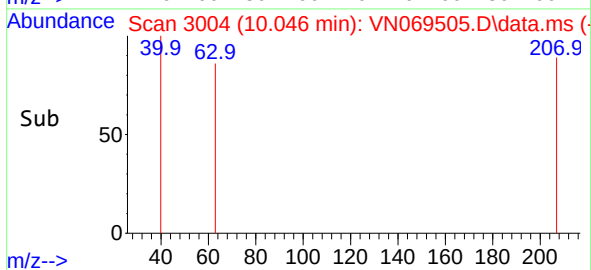






#59
2-Hexanone
Concen: 8.881 ug/l
RT: 11.089 min Scan# 31
Delta R.T. 0.002 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 23132
Ion Ratio Lower Upper
43 100
58 41.8 26.9 80.7

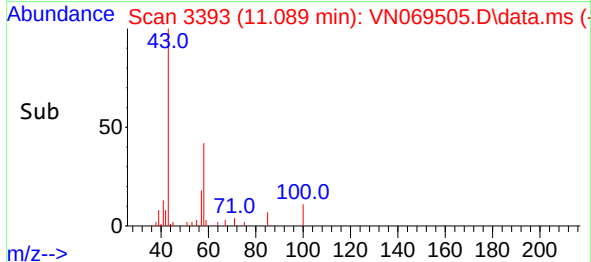

#60
Dibromochloromethane
Concen: 2.425 ug/l
RT: 11.237 min Scan# 3448
Delta R.T. -0.003 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31


Tgt Ion: 129 Resp: 143
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#

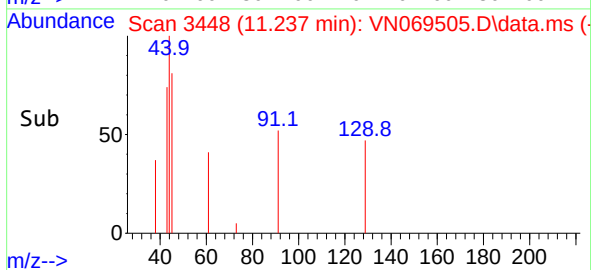






#61
1,2-Dibromoethane
Concen: 1.089 ug/l
RT: 11.347 min Scan# 3489
Delta R.T. -0.000 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Instrument :
MSVOA_N
ClientSampleId :



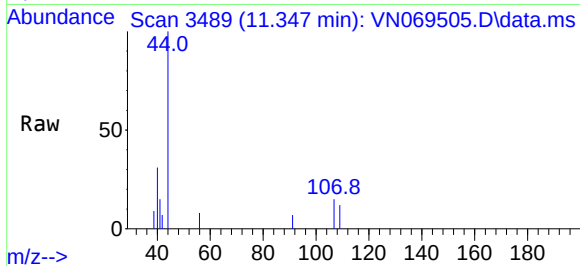



Tgt Ion:107 Resp: 311
Ion Ratio Lower Upper
107 100
109 94.5 75.7 113.5



#62
4-Bromofluorobenzene
Concen: 50.718 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.003 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31


Tgt Ion: 95 Resp: 1052951
Ion Ratio Lower Upper
95 100
174 76.4 0.0 187.2
176 74.1 0.0 181.4

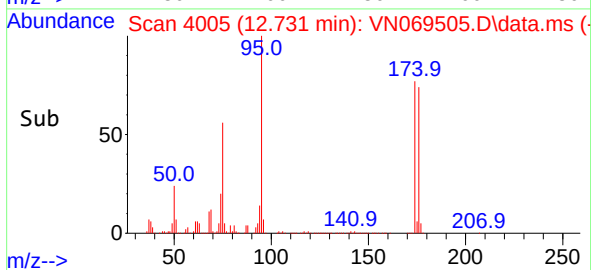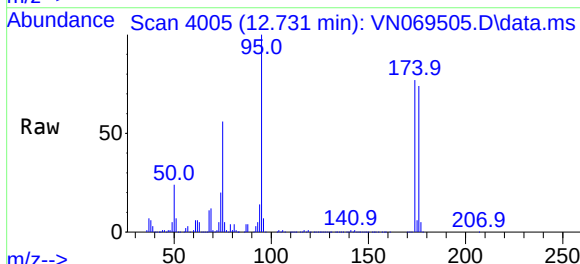






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.744 min Scan# 3638
Delta R.T. -0.003 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:117 Resp: 2343124




Ion	Ratio	Lower	Upper
117	100		
82	58.0	42.4	63.6
119	31.9	25.4	38.2

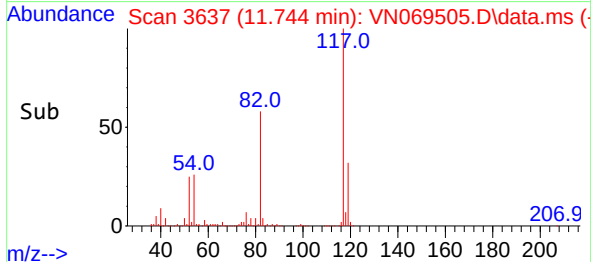


#70
Styrene
Concen: 1.591 ug/l
RT: 12.294 min Scan# 3842
Delta R.T. -0.000 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Tgt Ion:104 Resp: 3879

Ion	Ratio	Lower	Upper
104	100		
78	32.3	38.7	58.1#
103	48.6	45.0	67.6


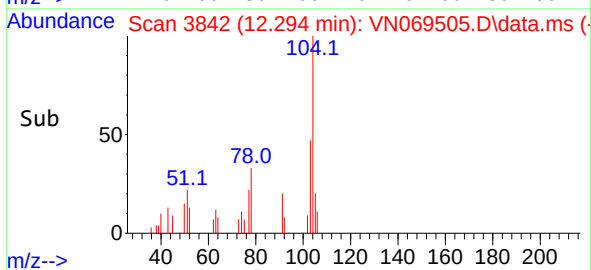






#71
Bromoform
Concen: 3.451 ug/l
RT: 12.457 min Scan# 3903
Delta R.T. -0.003 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 332
Ion Ratio Lower Upper
173 100
175 0.0 24.2 72.6#
254 0.0 0.0 0.0

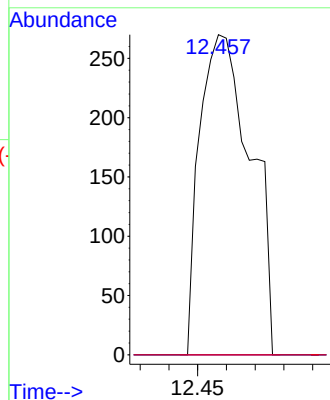

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.000 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31


Tgt Ion:152 Resp: 878372
Ion Ratio Lower Upper
152 100
115 60.5 27.5 82.5
150 157.3 0.0 344.4

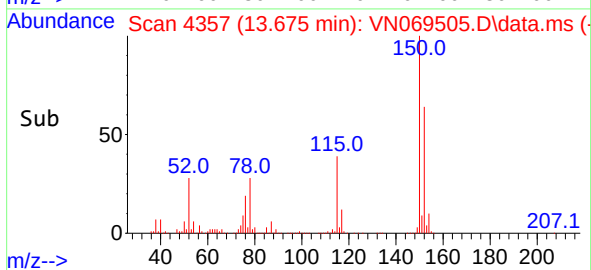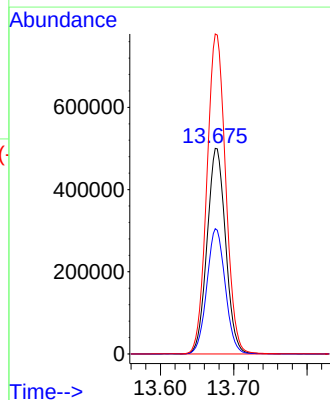






#74
N-amy1 acetate
Concen: 0.461 ug/l
RT: 12.393 min Scan# 31
Delta R.T. 0.005 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 43 Resp: 13676
Ion Ratio Lower Upper
43 100
70 28.9 33.4 50.0#
55 23.8 19.3 28.9
61 21.0 18.5 27.7



#76
1,2,3-Trichloropropane
Concen: 28.777 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.150 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31


Tgt Ion: 75 Resp: 583330
Ion Ratio Lower Upper
75 100
77 0.9 82.6 247.8#

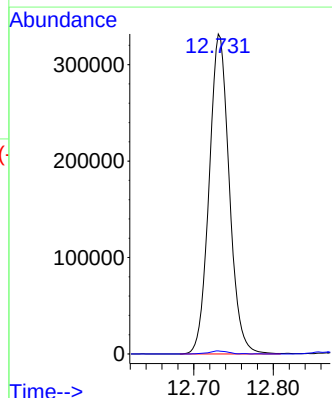






#81
trans-1,4-Dichloro-2-butene
Concen: 81.532 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 75 Resp: 583330
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

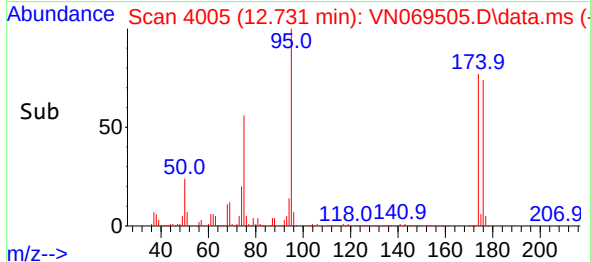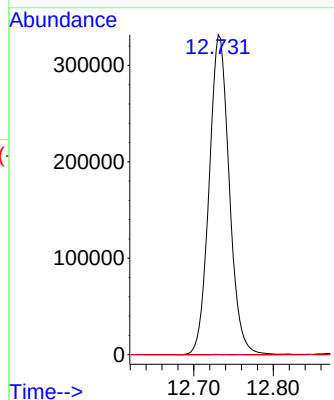

#87
1,3-Dichlorobenzene
Concen: 0.229 ug/l
RT: 13.616 min Scan# 4335
Delta R.T. -0.000 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31


Tgt Ion:146 Resp: 6352
Ion Ratio Lower Upper
146 100
111 34.2 18.6 55.6
148 64.7 31.6 95.0

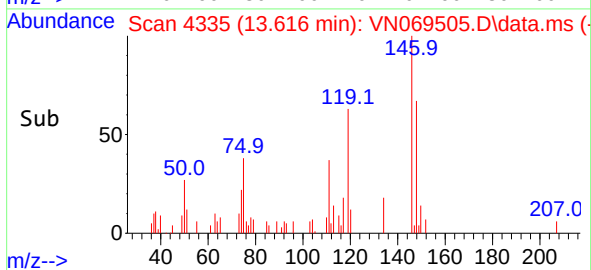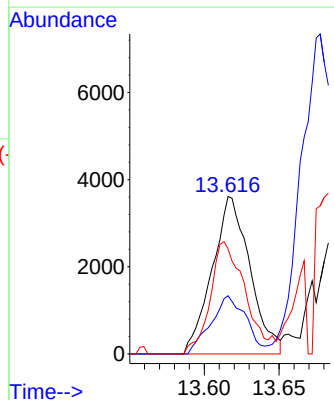






#88
1,4-Dichlorobenzene
Concen: 0.233 ug/l
RT: 13.616 min Scan# 41
Delta R.T. -0.080 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:146 Resp: 6352
Ion Ratio Lower Upper
146 100
111 34.2 18.3 54.8
148 64.7 31.8 95.4

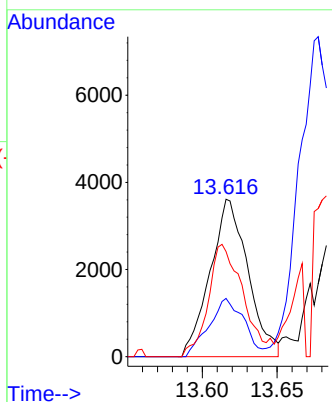


#89
n-Butylbenzene
Concen: 0.322 ug/l
RT: 13.940 min Scan# 4456
Delta R.T. -0.003 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31



Tgt Ion: 91 Resp: 14774
Ion Ratio Lower Upper
91 100
92 45.1 25.4 76.0
134 21.7 13.6 40.8









#90
Hexachloroethane
Concen: 2.182 ug/l
RT: 14.203 min Scan# 4554
Delta R.T. -0.008 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 214
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#



#91
1,2-Dichlorobenzene
Concen: 0.267 ug/l
RT: 13.989 min Scan# 4474
Delta R.T. -0.000 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

Tgt Ion:146 Resp: 7052
Ion Ratio Lower Upper
146 100
111 43.4 19.1 57.3
148 64.6 32.1 96.3


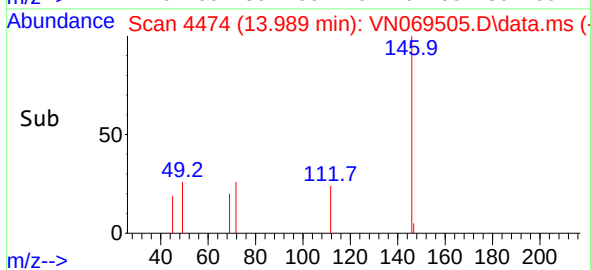




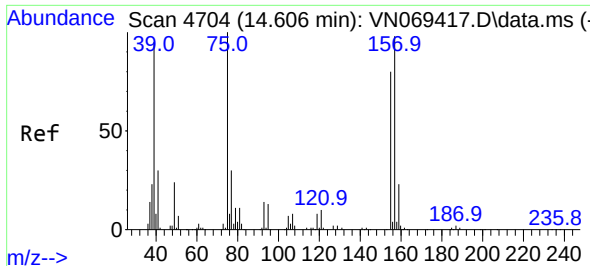

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 2.077 ug/l
 RT: 14.605 min Scan# 41
 Delta R.T. -0.001 min
 Lab File: VN069505.D
 Acq: 16 Nov 2021 12:31




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 1273
 Ion Ratio Lower Upper
 75 100
 155 52.9 46.9 140.7
 157 87.7 60.6 181.7

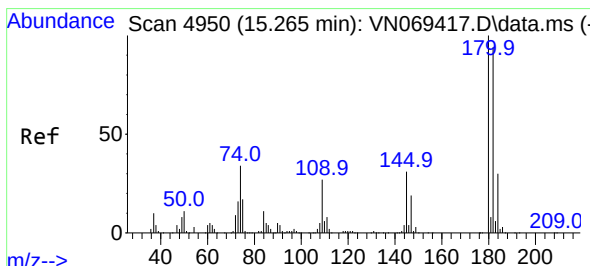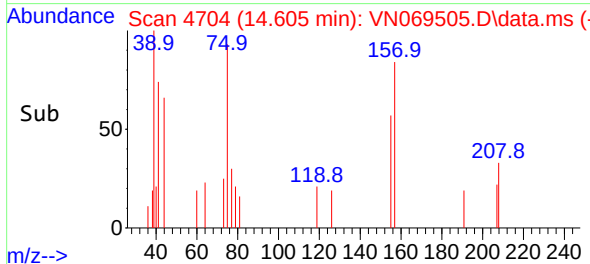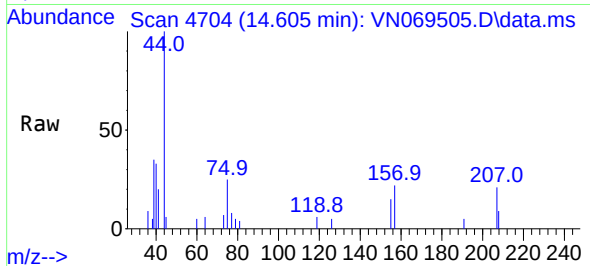

#93
 1,2,4-Trichlorobenzene
 Concen: 3.897 ug/l
 RT: 15.263 min Scan# 4949
 Delta R.T. -0.002 min
 Lab File: VN069505.D
 Acq: 16 Nov 2021 12:31


Tgt Ion:180 Resp: 11554
 Ion Ratio Lower Upper
 180 100
 182 95.2 48.3 144.9
 145 32.3 14.5 43.5

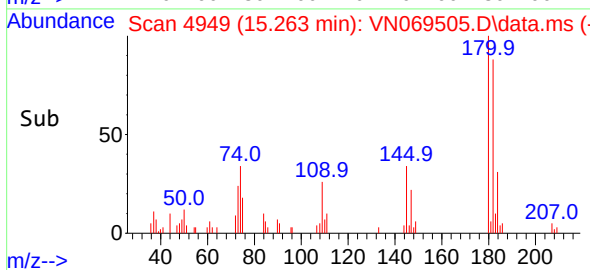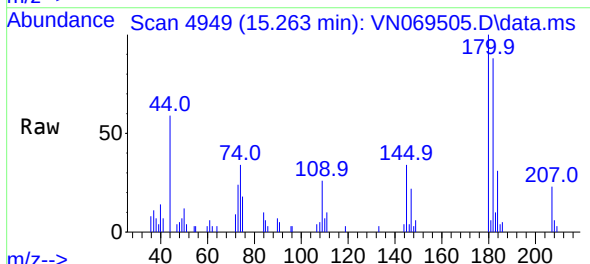






#95
Naphthalene
Concen: 5.661 ug/l
RT: 15.509 min Scan# 5040
Delta R.T. 0.002 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31


Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:128 Resp: 51802
Ion Ratio Lower Upper
128 100
127 12.6 10.5 15.7
129 10.2 8.7 13.1

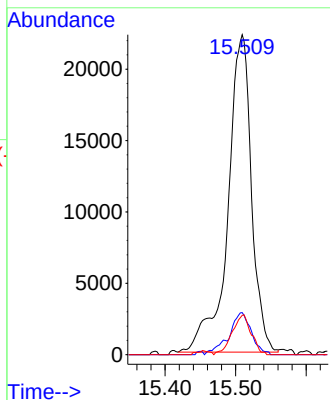

#96
1,2,3-Trichlorobenzene
Concen: 4.151 ug/l
RT: 15.700 min Scan# 5112
Delta R.T. -0.000 min
Lab File: VN069505.D
Acq: 16 Nov 2021 12:31

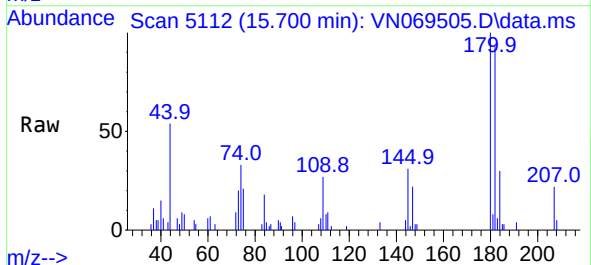

Tgt Ion:180 Resp: 13852
Ion Ratio Lower Upper
180 100
182 95.3 47.4 142.2
145 30.1 15.0 45.1

