

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111621\
 Data File : VN069518.D
 Acq On : 16 Nov 2021 19:23
 Operator : JC/MD
 Sample : M4714-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 17 01:00:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 09 18:18:22 2021
 Response via : Initial Calibration

Compound	R.T.	QI on	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.086	168	1419177	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2477114	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	2447865	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	919963	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	1034546	50.28	ug/l	0.00
Spike Amount	50.000	Range 61 - 141	Recovery	=	100.56%	
35) Dibromofluoromethane	8.024	113	718634	48.37	ug/l	0.00
Spike Amount	50.000	Range 69 - 133	Recovery	=	96.74%	
50) Toluene-d8	10.443	98	3144165	53.81	ug/l	0.00
Spike Amount	50.000	Range 65 - 126	Recovery	=	107.62%	
62) 4-Bromofluorobenzene	12.734	95	1112879	51.85	ug/l	0.00
Spike Amount	50.000	Range 58 - 135	Recovery	=	103.70%	
Target Compounds						
3) Chloromethane	2.306	50	3568	0.20	ug/l	95
13) Acrolein	4.044	56	821	Below	Cal #	67
16) Acetone	4.296	43	28320	2.55	ug/l	98
25) 2-Butanone	7.348	43	20790	1.38	ug/l	92
27) cis-1,2-Dichloroethene	7.327	96	17366	1.09	ug/l	100
30) Chloroform	7.823	83	17541	0.61	ug/l	94
31) Cyclohexane	8.088	56	36545	1.30	ug/l #	39
36) 1,1-Dichloropropene	8.086	75	121478	5.83	ug/l #	49
37) Ethyl Acetate	7.348	43	20790	0.74	ug/l #	1
38) Carbon Tetrachloride	8.086	117	146737	7.29	ug/l #	17
44) Trichloroethene	9.217	130	11164	0.73	ug/l	90
49) 1,4-Dioxane	9.585	88	63	39.20	ug/l #	27
53) t-1,3-Dichloropropene	10.719	75	75	2.64	ug/l #	43
54) cis-1,3-Dichloropropene	10.432	75	328	1.74	ug/l #	1
56) Ethyl methacrylate	10.762	69	172	2.06	ug/l #	1
58) 2-Chloroethyl Vinyl ether	9.821	63	57	22.78	ug/l #	45
59) 2-Hexanone	11.076	43	711	7.97	ug/l	95
60) Dibromochloromethane	10.977	129	29234	3.99	ug/l #	11
64) Tetrachloroethene	10.977	164	29400	1.99	ug/l	94
70) Styrene	12.291	104	268	1.53	ug/l #	58
71) Bromoform	12.712	173	661	3.47	ug/l #	29
76) 1,2,3-Trichloropropane	12.731	75	633832	29.85	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.731	75	633832	84.37	ug/l #	5
90) Hexachloroethane	13.981	117	27	2.16	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.606	75	100	1.82	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.257	180	510	3.15	ug/l #	58
95) Naphthalene	15.507	128	4189	4.54	ug/l #	88
96) 1,2,3-Trichlorobenzene	15.705	180	909	3.23	ug/l #	61

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111621\
 Data File : VN069518.D
 Acq On : 16 Nov 2021 19:23
 Operator : JC/MD
 Sample : M4714-03
 Mi sc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 17 01:00:19 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 09 18:18:22 2021
 Response via : Initial Calibration

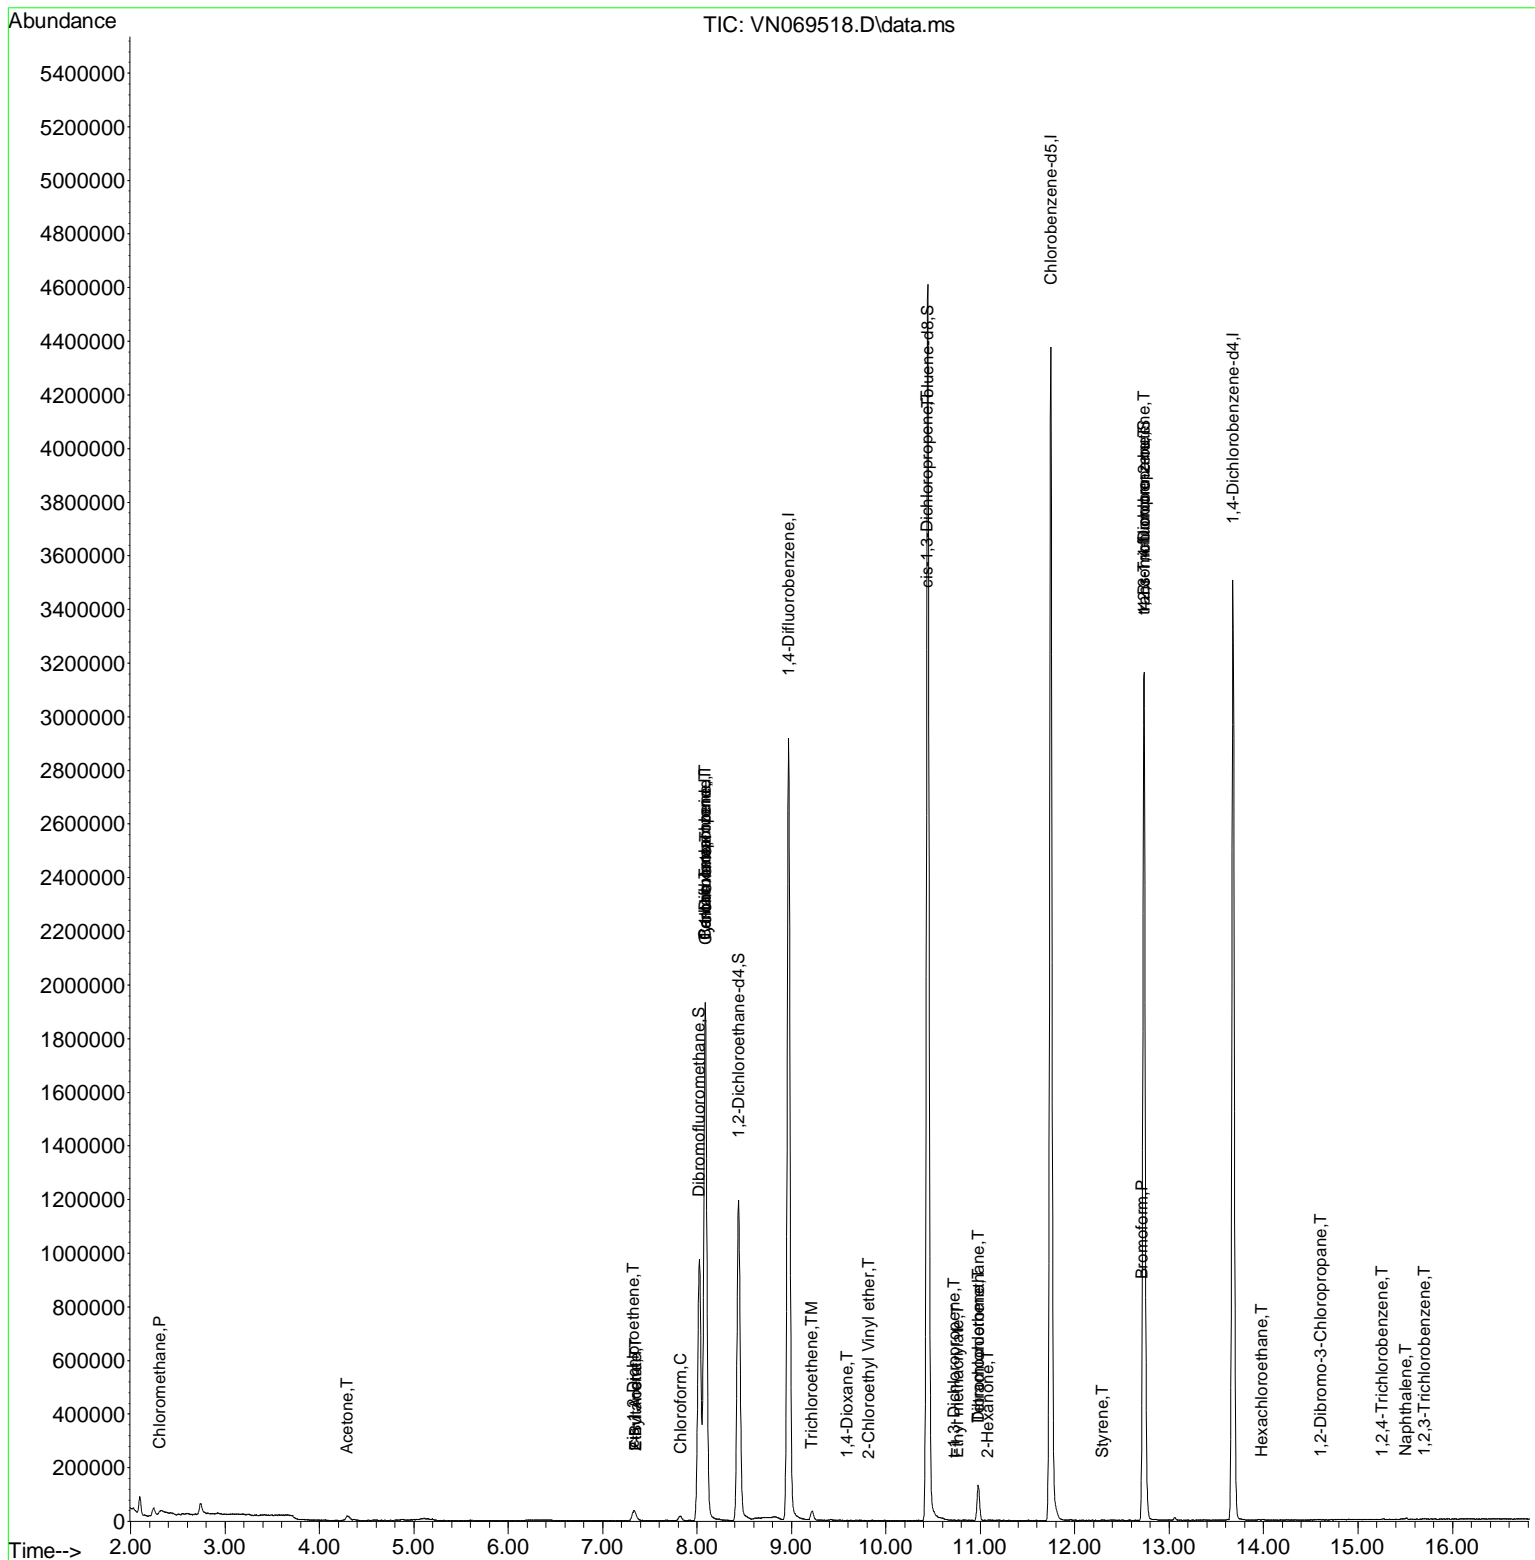


Abundance Scan 2273 (8.086 min): VN069417.D\data.ms (-2249) (-)



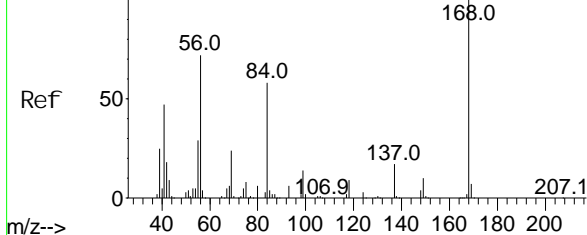


Pentafluorobenzene
Concen: 50.00 ug/l
RT: 8.086 min Scan# 118
Delta R.T. -0.000 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23


Instrument : MSVOA_N
ClientSampleId :

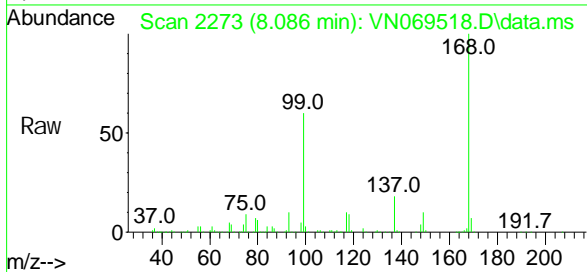



Tgt Ion: 168 Resp: 1419177
Ion Ratio Lower Upper
168 100
99 60.3 41.3 61.9

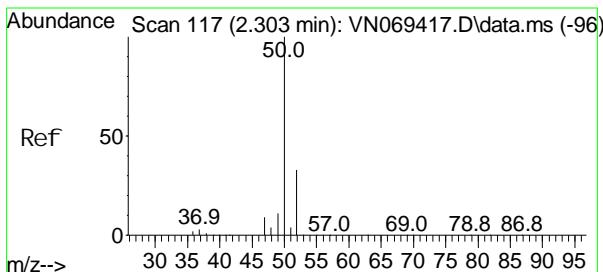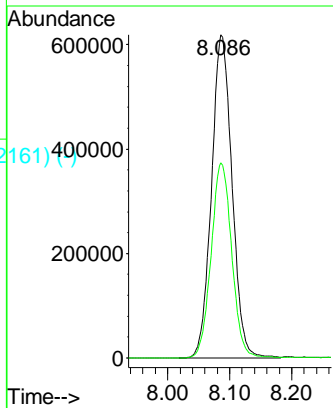


Chloromethane
Concen: 0.20 ug/l
RT: 2.306 min Scan# 118
Delta R.T. 0.003 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23



Tgt Ion: 50 Resp: 3568
Ion Ratio Lower Upper
50 100
52 29.0 25.4 38.0



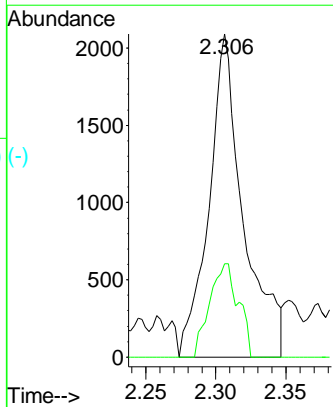
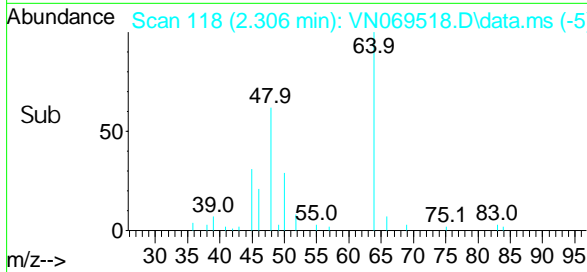


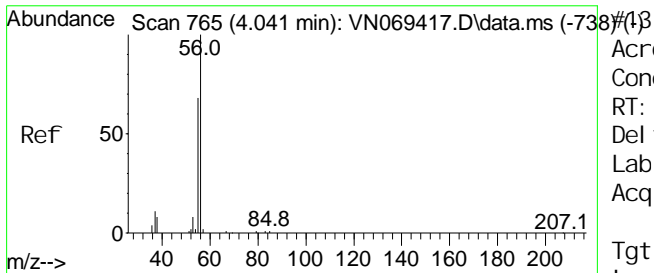

Acrol ei n
 Concen: Below Cal
 RT: 4.044 mi n Scan#
 Del ta R. T. 0.003 mi n
 Lab Fi le: VN069518. D
 Acq: 16 Nov 2021 19: 23




Instrument :
 MSVOA_N
 ClientSampleId :

Tgt Ion: 56 Resp: 821
 Ion Ratio Lower Upper
 56 100
 55 43.5 56.6 85.0#

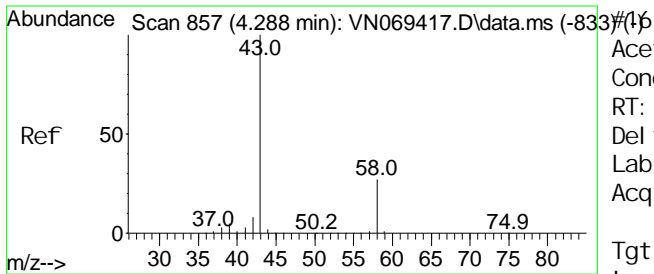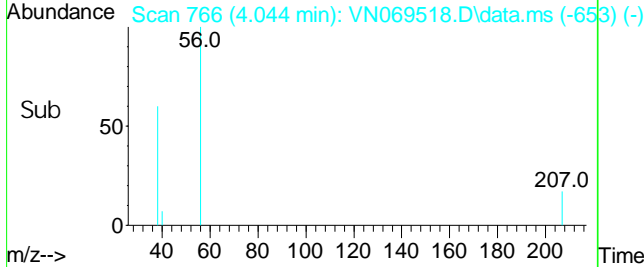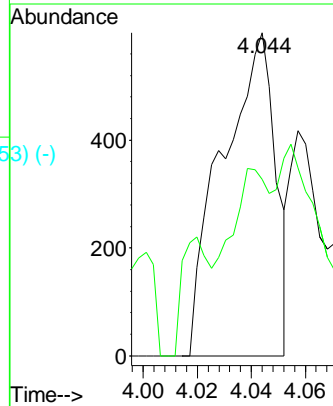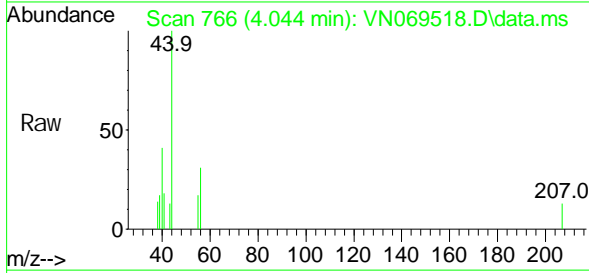


Acetone
 Concen: 2.55 ug/l
 RT: 4.296 mi n Scan# 860
 Del ta R. T. 0.008 mi n
 Lab Fi le: VN069518. D
 Acq: 16 Nov 2021 19: 23

Tgt Ion: 43 Resp: 28320
 Ion Ratio Lower Upper
 43 100
 58 27.8 23.1 34.7

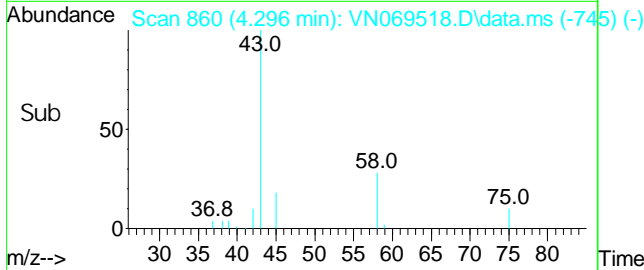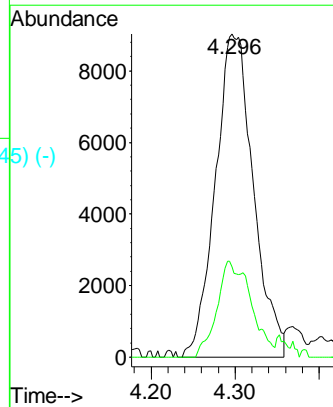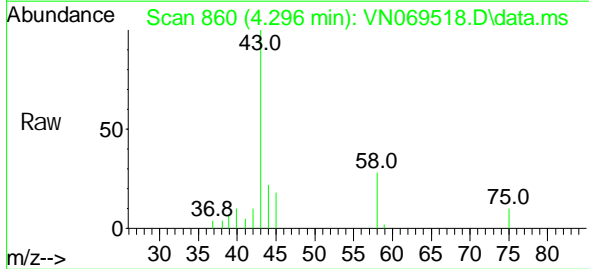



Abundance Scan 1994 (7.337 min): VN069417.D\data.ms (-1962) (-)

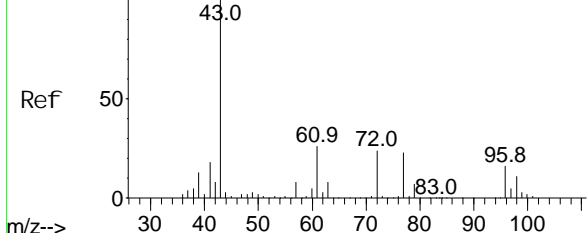


2-Butanone
Concen: 1.38 ug/l
RT: 7.348 min Scan#
Delta R.T. 0.011 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23

Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 20790
Ion Ratio Lower Upper
43 100
72 23.1 21.7 32.5

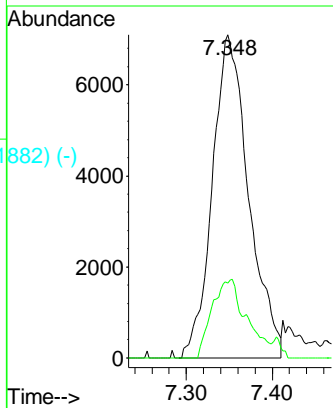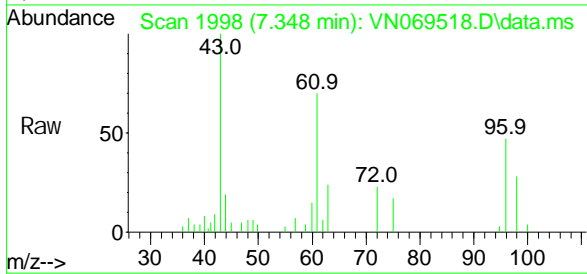

Abundance Scan 1998 (7.348 min): VN069518.D\data.ms (-1882) (-)


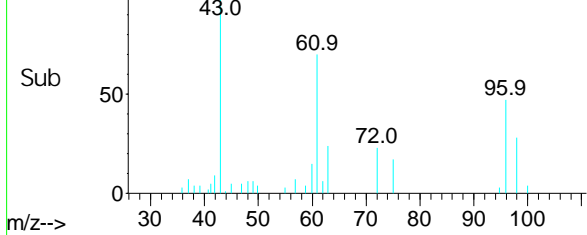


Abundance Scan 1989 (7.324 min): VN069417.D\data.ms (-1962) (-)

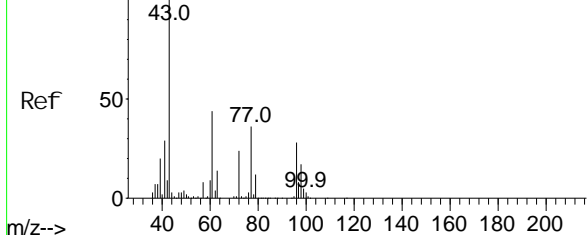



cis-1,2-Dichloroethene
Concen: 1.09 ug/l
RT: 7.327 min Scan# 1990
Delta R.T. 0.003 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23

Tgt Ion: 96 Resp: 17366
Ion Ratio Lower Upper
96 100
61 137.9 0.0 275.0
98 64.3 0.0 129.6

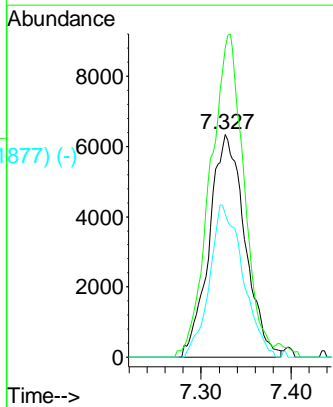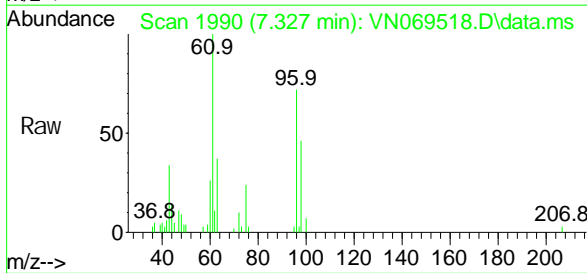

Abundance Scan 1990 (7.327 min): VN069518.D\data.ms (-1877) (-)




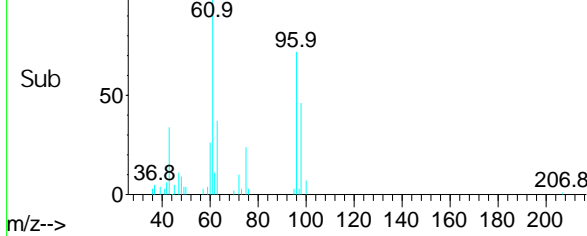


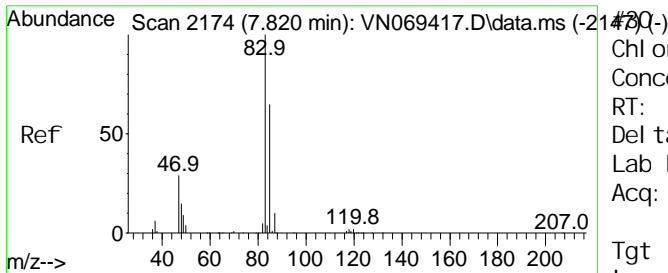

Chloroform
 Concen: 0.61 ug/l
 RT: 7.823 min Scan# 2174
 Delta R.T. 0.003 min
 Lab File: VN069518.D
 Acq: 16 Nov 2021 19:23




Instrument : MSVOA_N
 ClientSampleId :


Tgt Ion: 83 Resp: 17541
 Ion Ratio Lower Upper
 83 100
 85 59.8 51.9 77.9

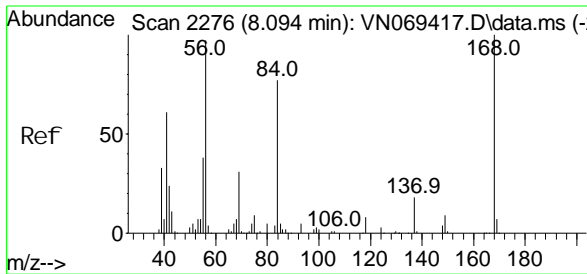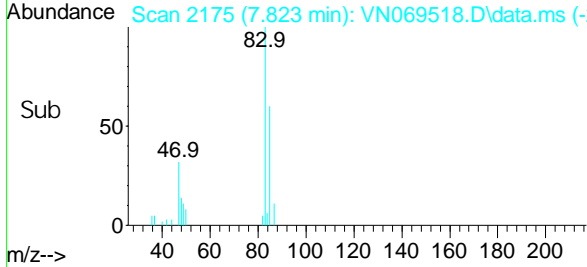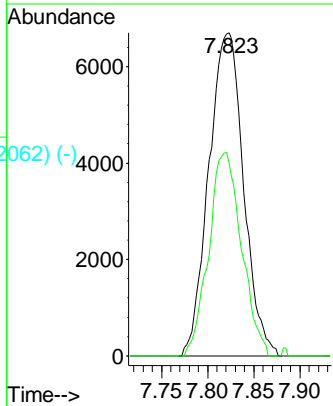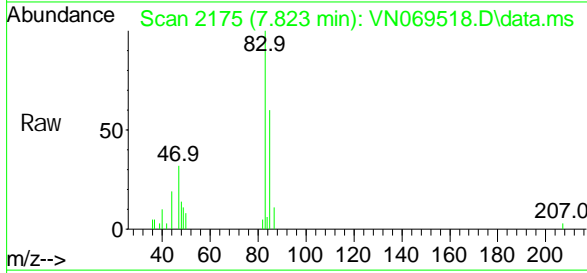

Cyclohexane
 Concen: 1.30 ug/l
 RT: 8.088 min Scan# 2274
 Delta R.T. -0.006 min
 Lab File: VN069518.D
 Acq: 16 Nov 2021 19:23

Tgt Ion: 56 Resp: 36545
 Ion Ratio Lower Upper
 56 100
 69 146.8 27.1 40.7#
 84 102.0 73.4 110.0


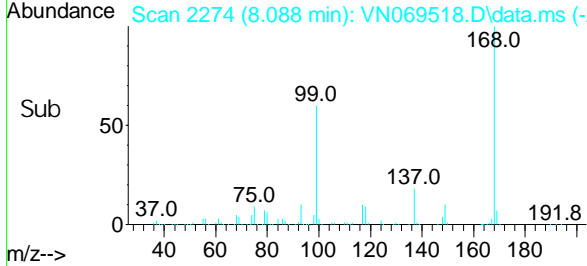
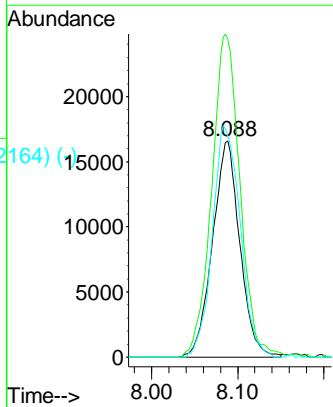
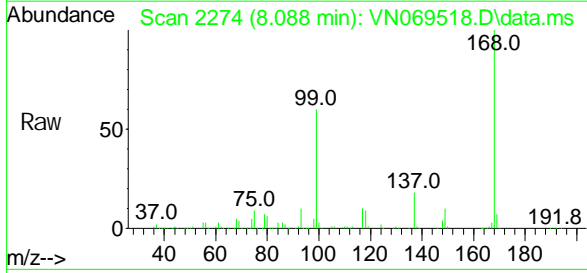


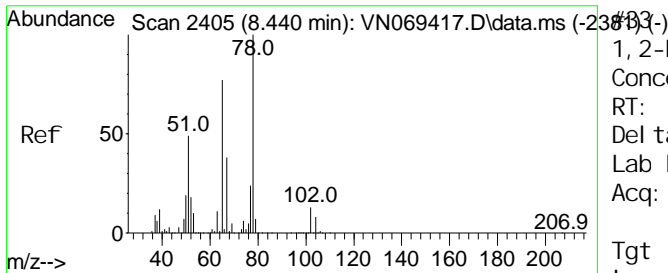

1, 2-Di chl oroethane-d4
 Concen: 50.28 ug/l
 RT: 8.440 mi n Scan# 2405
 Del ta R. T. -0.000 mi n
 Lab Fi le: VN069518.D
 Acq: 16 Nov 2021 19:23




Instrument : MSVOA_N
 ClientSampleId :

Tgt Ion: 65 Resp: 1034546
 Ion Ratio Lower Upper
 65 100
 67 50.4 0.0 103.0

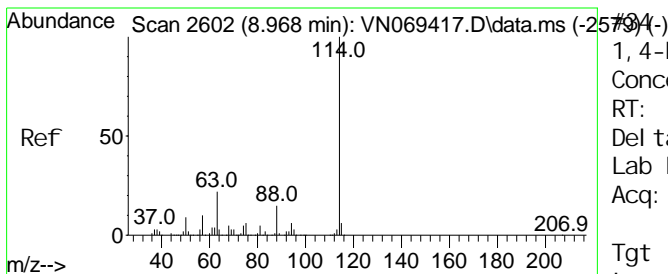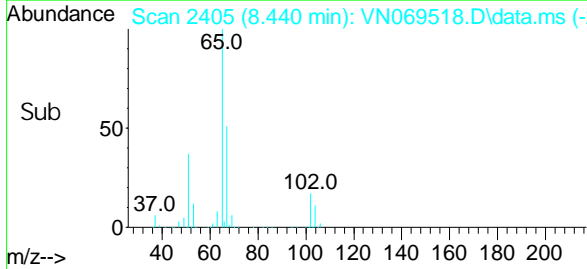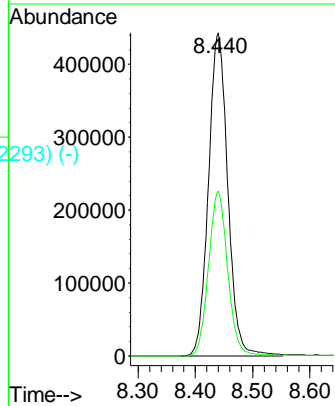


1, 4-Di fl uorobenzene
 Concen: 50.00 ug/l
 RT: 8.968 mi n Scan# 2602
 Del ta R. T. 0.000 mi n
 Lab Fi le: VN069518.D
 Acq: 16 Nov 2021 19:23

Tgt Ion: 114 Resp: 2477114
 Ion Ratio Lower Upper
 114 100
 63 22.8 0.0 37.8
 88 15.8 0.0 27.4

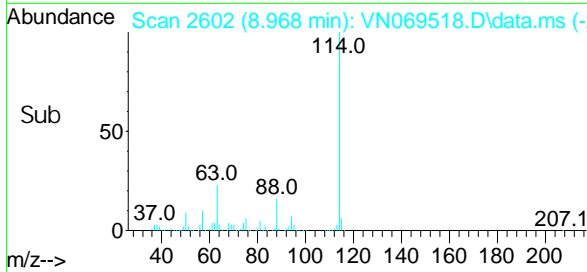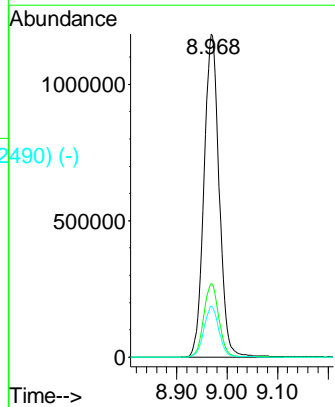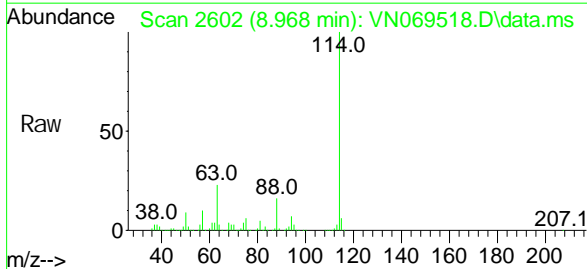


Abundance Scan 2249 (8.021 min): VN069417.D\data.ms (-2249) (-)


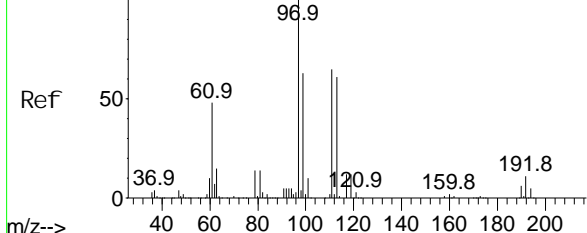


Di bromofluoromethane
Concen: 48.37 ug/l
RT: 8.024 min Scan# 2249
Delta R.T. 0.003 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23


Instrument : MSVOA_N
ClientSampleId :

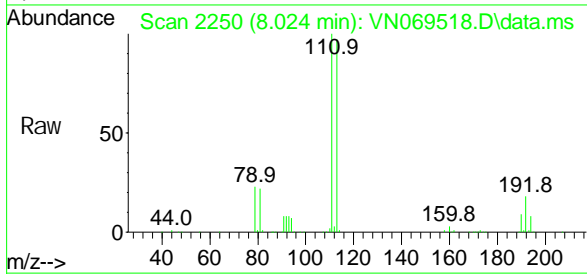

Tgt Ion: 113 Resp: 718634
Ion Ratio Lower Upper
113 100
111 103.5 82.2 123.2
192 17.8 16.9 25.3


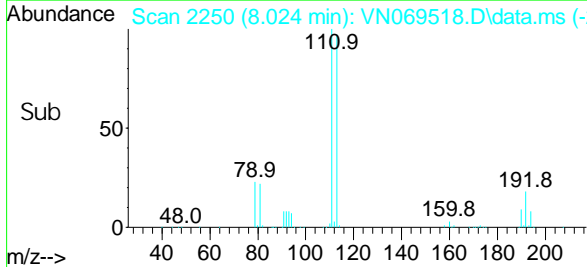
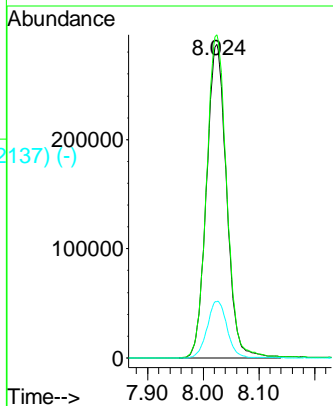


Abundance Scan 2324 (8.223 min): VN069417.D\data.ms (-2324) (-)

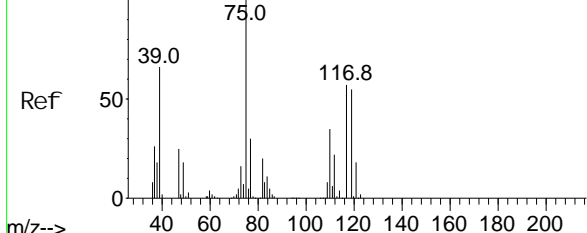


1,1-Dichloropropene
Concen: 5.83 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.137 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23

Tgt Ion: 75 Resp: 121478
Ion Ratio Lower Upper
75 100
110 8.9 18.4 55.2#
77 0.0 24.4 36.6#

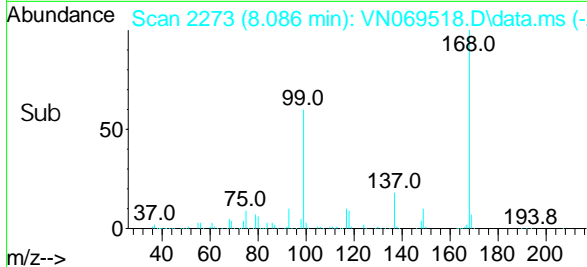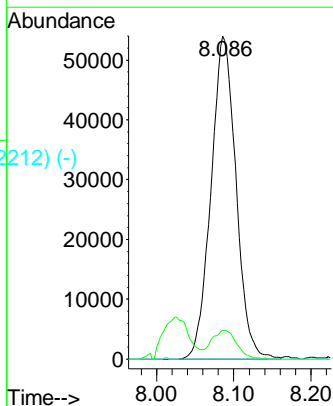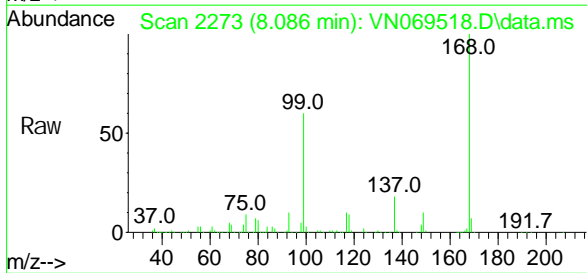


Abundance Scan 2023 (7.415 min): VN069417.D\data.ms (-2047) (-)

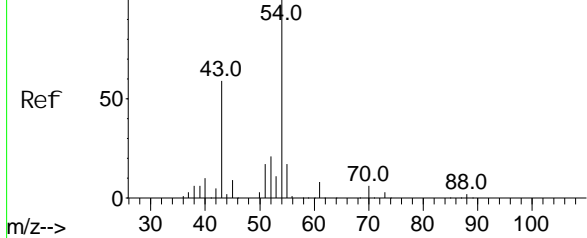



Ethyl Acetate
Concen: 0.74 ug/l
RT: 7.348 min Scan#
Delta R.T. -0.067 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23

Instrument :
MSVOA_N
ClientSampleId :




Tgt Ion: 43 Resp: 20790

Ion	Ratio	Lower	Upper
43	100		
61	115.2	11.5	17.3#
70	0.0	7.9	11.9#

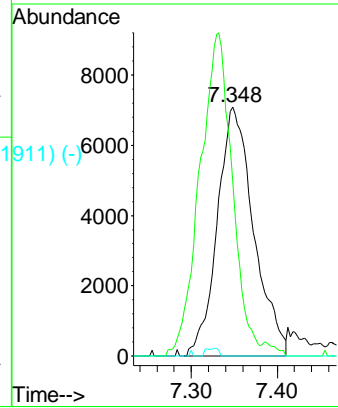




Abundance Scan 2318 (8.206 min): VN069417.D\data.ms (-2294) (-)

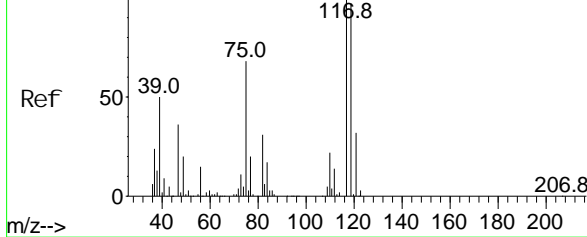


Carbon Tetrachloride
Concen: 7.29 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.120 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23

Tgt Ion: 117 Resp: 146737

Ion	Ratio	Lower	Upper
117	100		
119	5.8	76.1	114.1#
121	0.0	24.2	36.2#

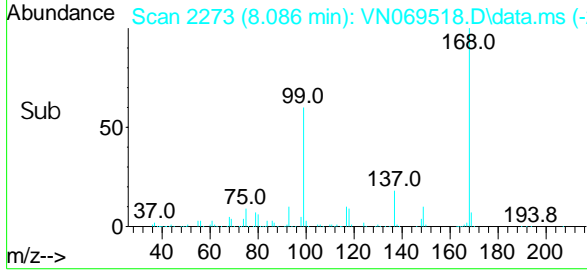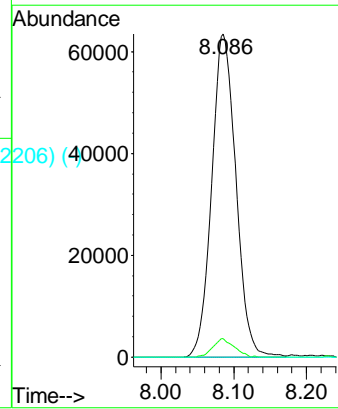


Abundance Scan 2695 (9.218 min): VN069417.D\data.ms (-2674)


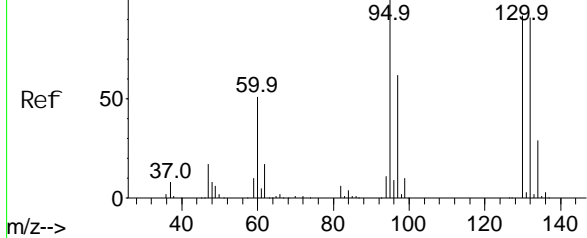


Tri chl oroethene
Concen: 0.73 ug/l
RT: 9.217 min Scan# 1
Del ta R. T. -0.001 min
Lab Fi le: VN069518.D
Acq: 16 Nov 2021 19:23


Instrument : MSVOA_N
Client Sample Id :




Tgt Ion: 130 Resp: 11164
Ion Ratio Lower Upper
130 100
95 105.4 0.0 191.2

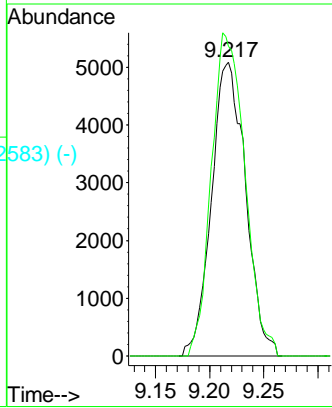



Abundance Scan 2827 (9.572 min): VN069417.D\data.ms (-2879)

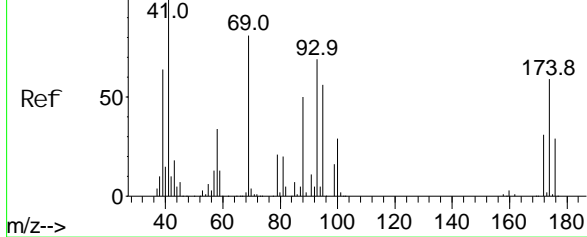

1,4-Di oxane
Concen: 39.20 ug/l
RT: 9.585 min Scan# 2832
Del ta R. T. 0.013 min
Lab Fi le: VN069518.D
Acq: 16 Nov 2021 19:23




Tgt Ion: 88 Resp: 63
Ion Ratio Lower Upper
88 100
43 0.0 23.4 35.2#
58 0.0 50.6 75.8#

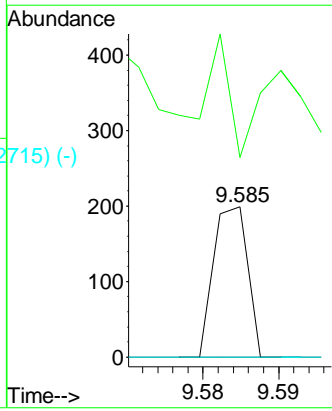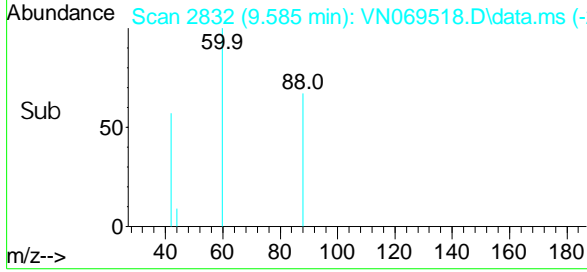

Abundance Scan 2832 (9.585 min): VN069518.D\data.ms (-2715)






Abundance Scan 3151 (10.441 min): VN069417.D\data.ms (-3450) (-)

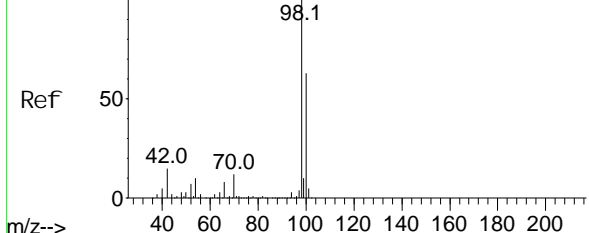


Toluene-d8
Concn: 53.81 ug/l
RT: 10.443 min Scan# 3151
Delta R.T. 0.002 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23

Instrument : MSVOA_N
ClientSampleId :

Tgt Ion: 98 Resp: 3144165
Ion Ratio Lower Upper
98 100
100 63.8 50.4 75.6

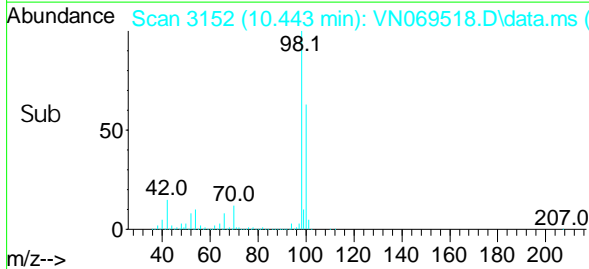
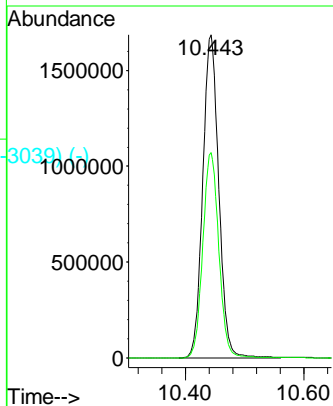
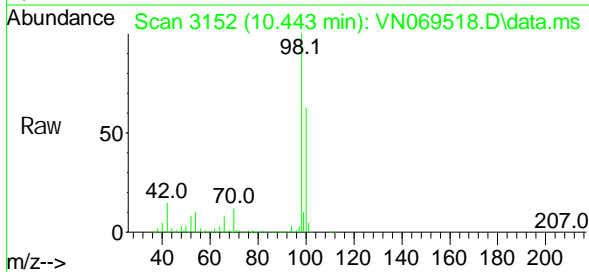



Abundance Scan 3255 (10.719 min): VN069417.D\data.ms (-3256) (-)

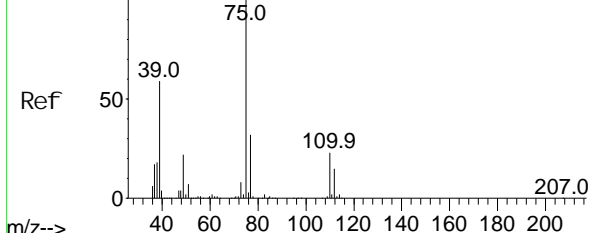

t-1,3-Dichloropropene
Concn: 2.64 ug/l
RT: 10.719 min Scan# 3255
Delta R.T. 0.000 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23

Tgt Ion: 75 Resp: 75
Ion Ratio Lower Upper
75 100
77 0.0 25.6 38.4#

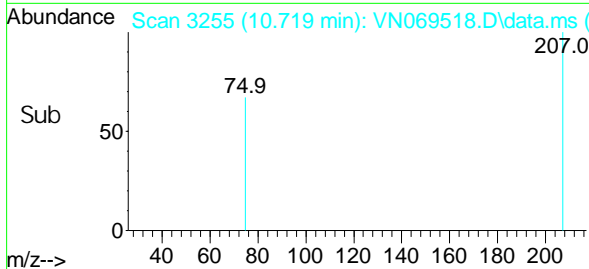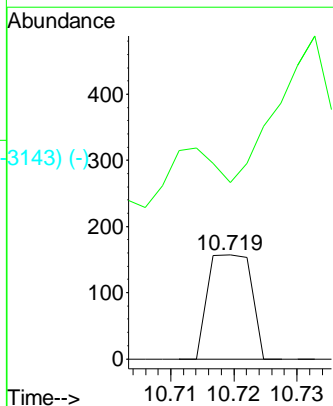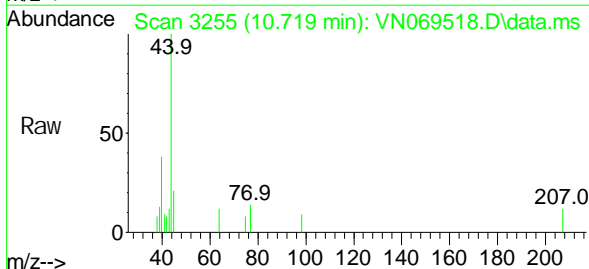




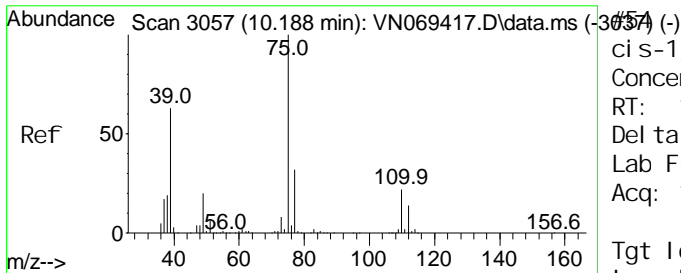


ci s-1, 3-Di chl oropropene
 Concen: 1.74 ug/l
 RT: 10.432 min Scan# 3148
 Del ta R. T. 0.244 min
 Lab Fi le: VN069518.D
 Acq: 16 Nov 2021 19:23

Instrument : MSVOA_N
 ClientSampleId :

Tgt Ion: 75 Resp: 328




Ion	Ratio	Lower	Upper
75	100		
77	314.7	26.4	39.6#
39	324.9	42.5	63.7#

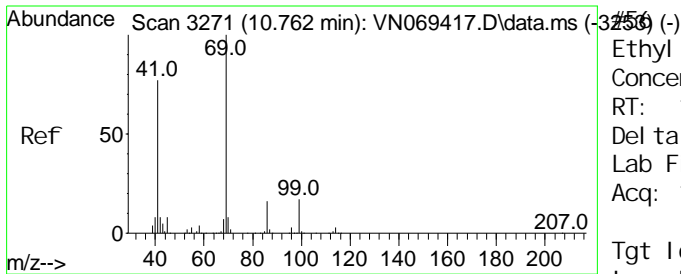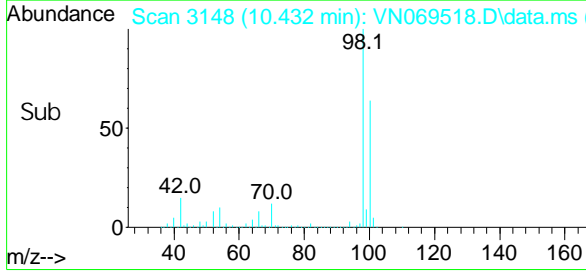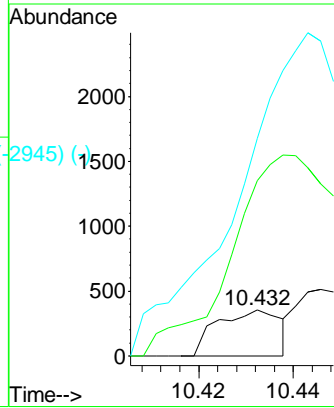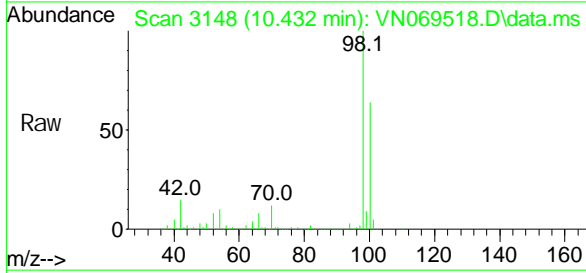


Ethyl methacrylate
 Concen: 2.06 ug/l
 RT: 10.762 min Scan# 3271
 Del ta R. T. 0.000 min
 Lab Fi le: VN069518.D
 Acq: 16 Nov 2021 19:23

Tgt Ion: 69 Resp: 172

Ion	Ratio	Lower	Upper
69	100		
41	194.8	51.4	77.0#
39	122.1	34.6	52.0#

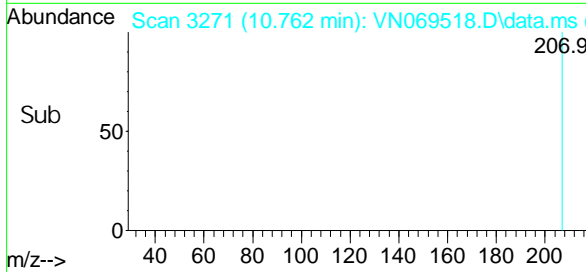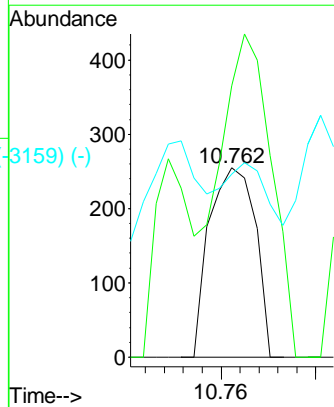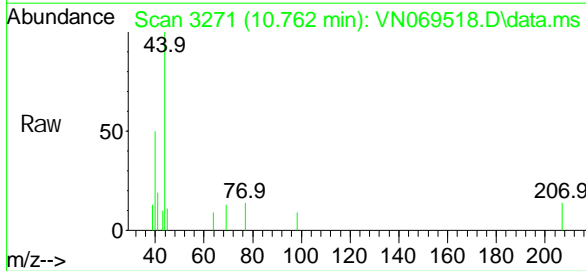

Abundance Scan 3002 (10.041 min): VN069417.D\data.ms (-3358) (-)


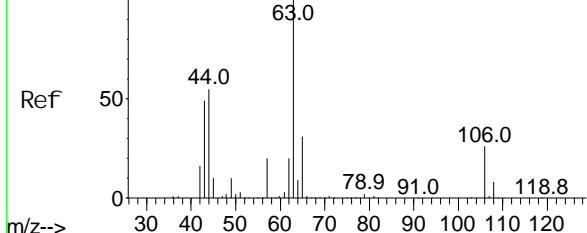


2-Chloroethyl Vinyl ether
Concen: 22.78 ug/l
RT: 9.821 min Scan# 311
Delta R.T. -0.220 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23


Instrument : MSVOA_N
ClientSampleId :

Tgt Ion: 63 Resp: 57
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#


Abundance Scan 2920 (9.821 min): VN069518.D\data.ms

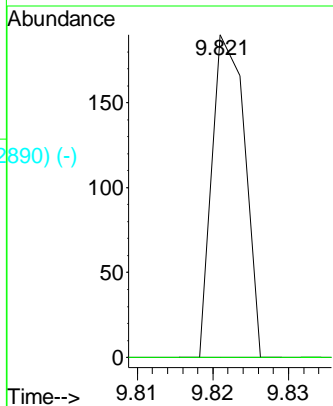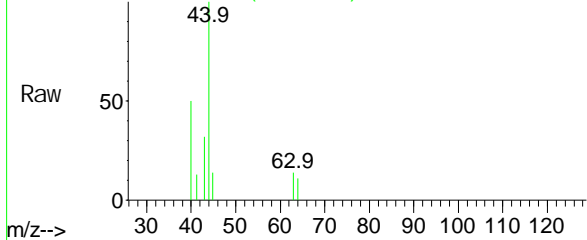

Abundance Scan 2920 (9.821 min): VN069518.D\data.ms (-2890) (-)

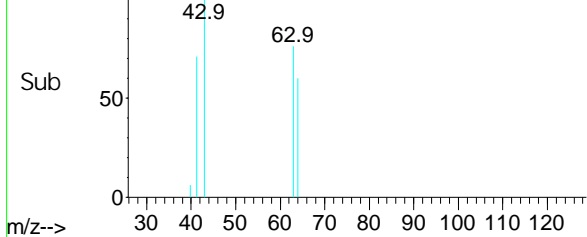



Abundance Scan 3392 (11.087 min): VN069417.D\data.ms (-3359) (-)

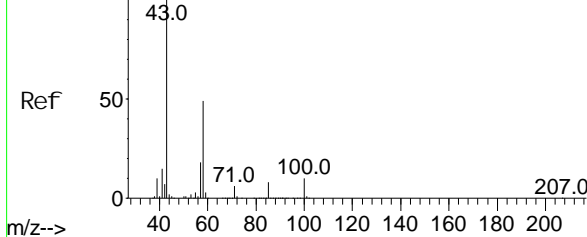


2-Hexanone
Concen: 7.97 ug/l
RT: 11.076 min Scan# 3388
Delta R.T. -0.011 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23


Tgt Ion: 43 Resp: 711
Ion Ratio Lower Upper
43 100
58 50.5 26.9 80.7

Abundance Scan 3388 (11.076 min): VN069518.D\data.ms

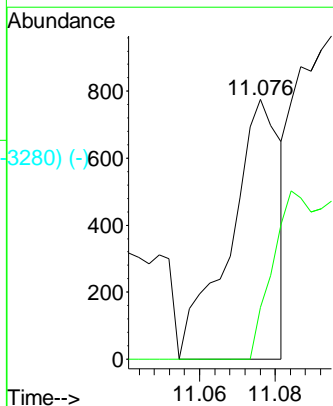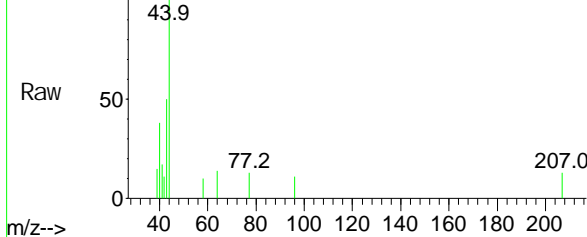

Abundance Scan 3388 (11.076 min): VN069518.D\data.ms (-3280) (-)




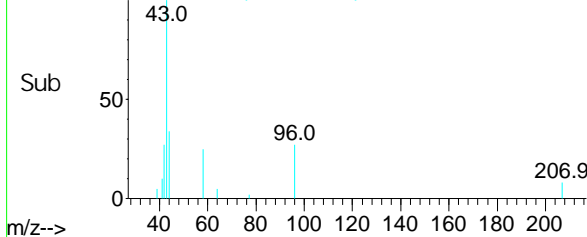


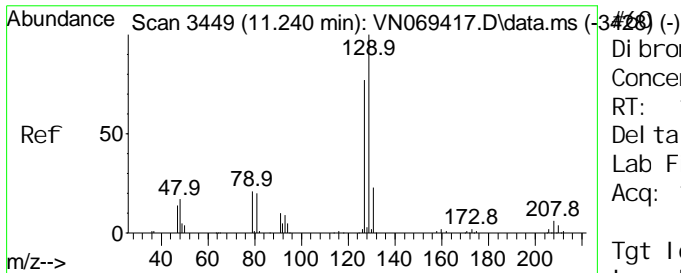

Di bromochloromethane
 Concen: 3.99 ug/l
 RT: 10.977 min Scan# 3351
 Delta R.T. -0.263 min
 Lab File: VN069518.D
 Acq: 16 Nov 2021 19:23




Instrument : MSVOA_N
 ClientSampleId :

Tgt Ion: 129 Resp: 29234
 Ion Ratio Lower Upper
 129 100
 127 0.0 38.6 116.0#

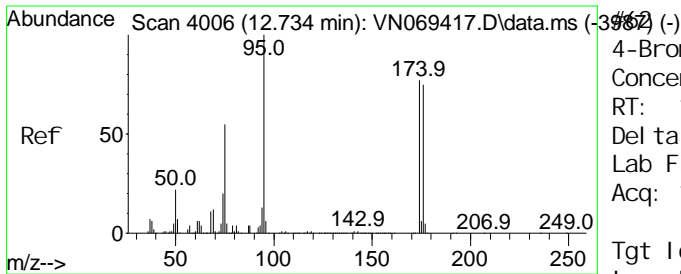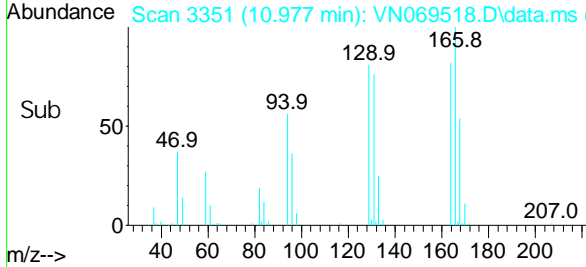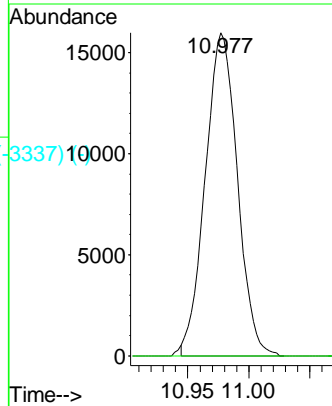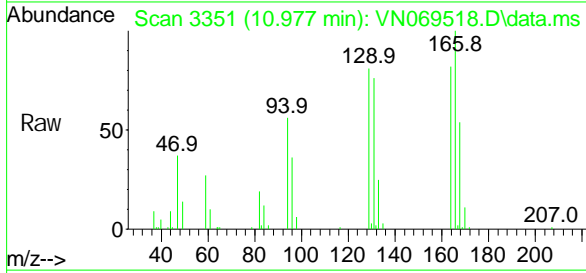


4-Bromofluorobenzene
 Concen: 51.85 ug/l
 RT: 12.734 min Scan# 4006
 Delta R.T. -0.000 min
 Lab File: VN069518.D
 Acq: 16 Nov 2021 19:23

Tgt Ion: 95 Resp: 1112879
 Ion Ratio Lower Upper
 95 100
 174 76.3 0.0 187.2
 176 72.8 0.0 181.4

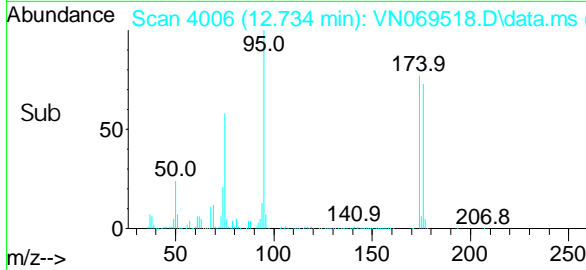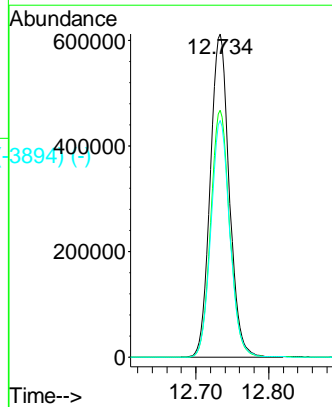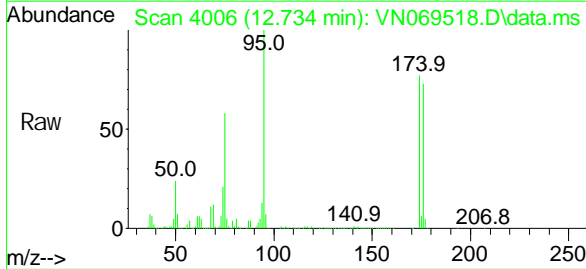


Abundance Scan 3638 (11.747 min): VN069417.D\data.ms (-3668) (-)

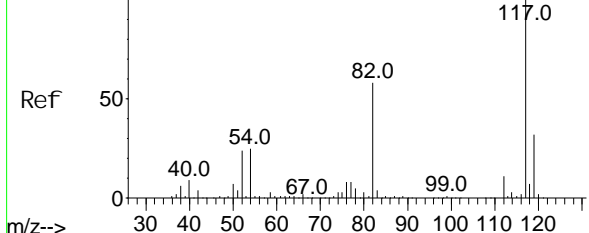


Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23


Instrument : MSVOA_N
ClientSampleId :

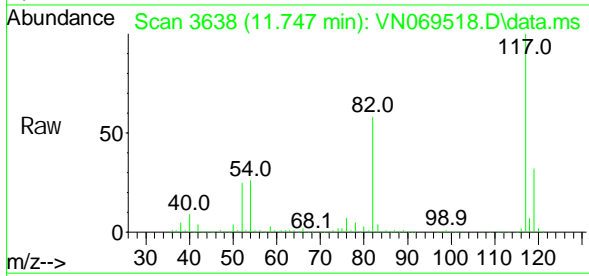


Tgt Ion: 117 Resp: 2447865
Ion Ratio Lower Upper
117 100
82 57.7 42.4 63.6
119 32.4 25.4 38.2

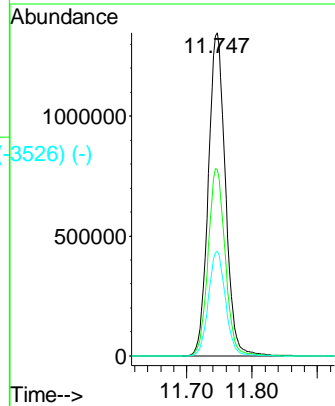

Abundance Scan 3638 (11.747 min): VN069518.D\data.ms (-3526) (-)


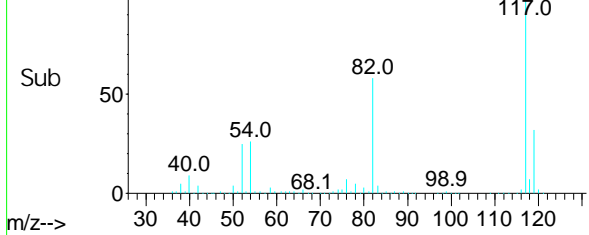


Abundance Scan 3351 (10.977 min): VN069417.D\data.ms (-3362) (-)

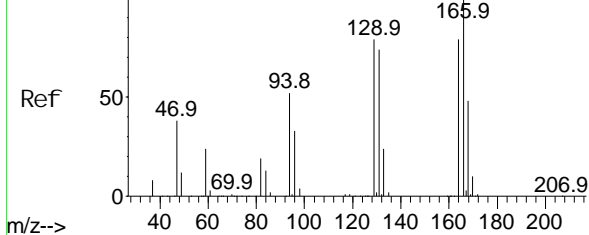



Tetrachloroethene
Concen: 1.99 ug/l
RT: 10.977 min Scan# 3351
Delta R.T. -0.000 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23

Tgt Ion: 164 Resp: 29400
Ion Ratio Lower Upper
164 100
166 122.4 101.9 152.9
129 99.6 72.0 108.0
131 93.1 70.9 106.3

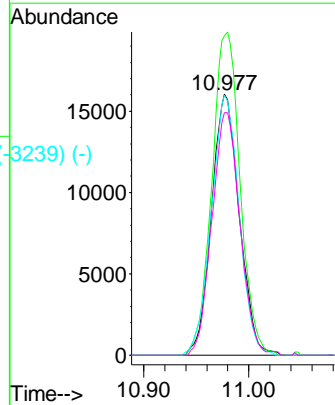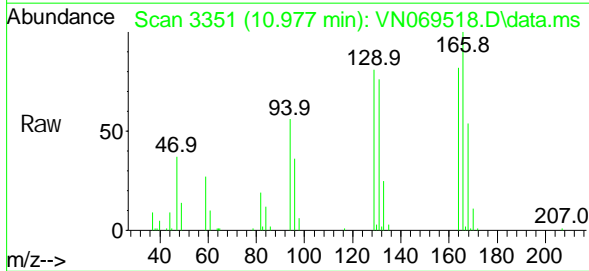

Abundance Scan 3351 (10.977 min): VN069518.D\data.ms (-3239) (-)




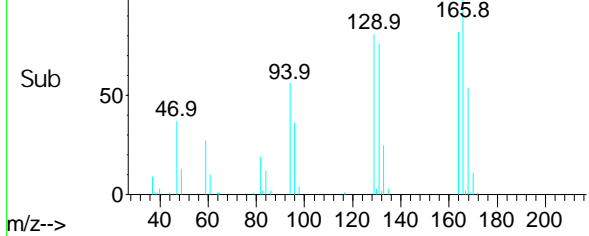


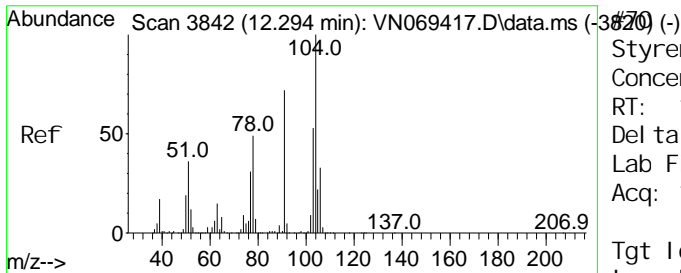

Styrene
 Concen: 1.53 ug/l
 RT: 12.291 min Scan# 3870
 Delta R.T. -0.003 min
 Lab File: VN069518.D
 Acq: 16 Nov 2021 19:23




Instrument : MSVOA_N
 Client Sample Id :


Tgt Ion: 104 Resp: 268
 Ion Ratio Lower Upper
 104 100
 78 0.0 38.7 58.1#
 103 43.7 45.0 67.6#

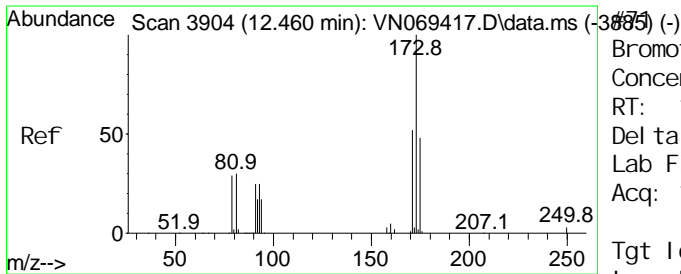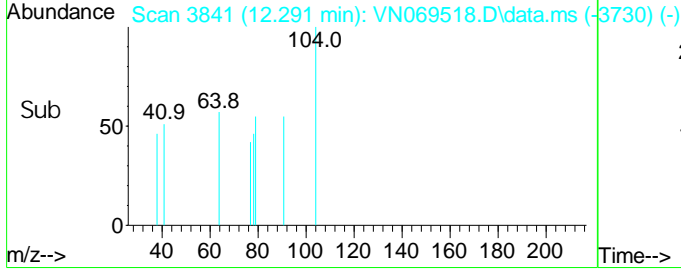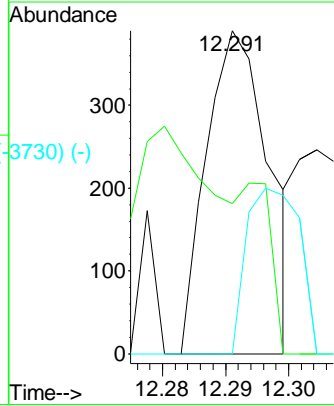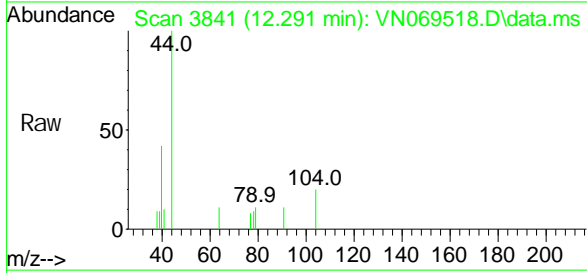

Bromoform
 Concen: 3.47 ug/l
 RT: 12.712 min Scan# 3998
 Delta R.T. 0.252 min
 Lab File: VN069518.D
 Acq: 16 Nov 2021 19:23

Tgt Ion: 173 Resp: 661
 Ion Ratio Lower Upper
 173 100
 175 0.0 24.2 72.6#
 254 0.0 0.0 0.0


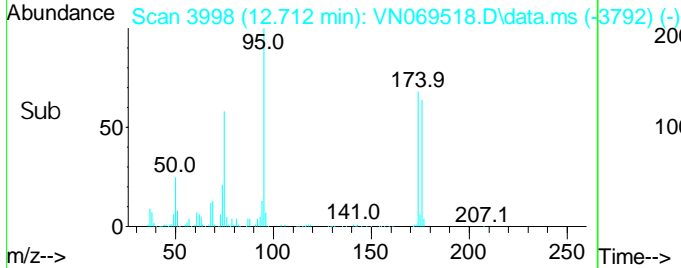
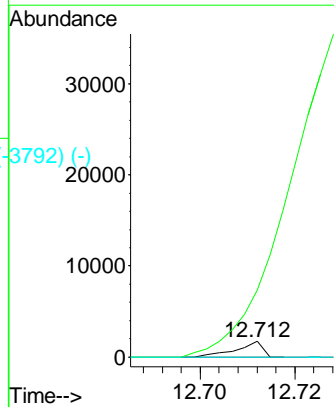



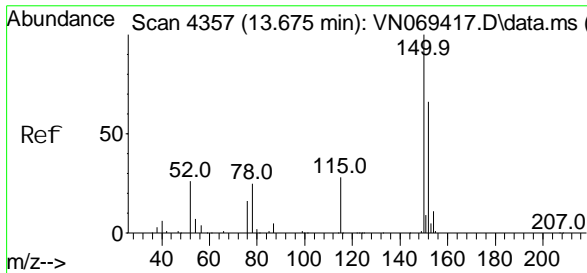

Scan 4357 (13.675 min): VN069417.D\data.ms (-4359) (-)
 1, 4-Di chl oro benzene-d4
 Concen: 50.00 ug/l
 RT: 13.678 min Scan# 4357
 Del ta R. T. 0.003 min
 Lab Fi le: VN069518.D
 Acq: 16 Nov 2021 19:23




Instrument : MSVOA_N
 Client SampleId :

Tgt Ion	Resp	Lower	Upper
152	919963		
115	61.1	27.5	82.5
150	158.5	0.0	344.4

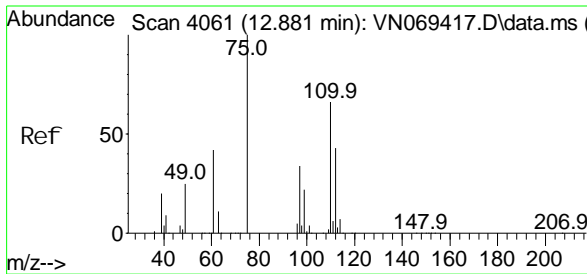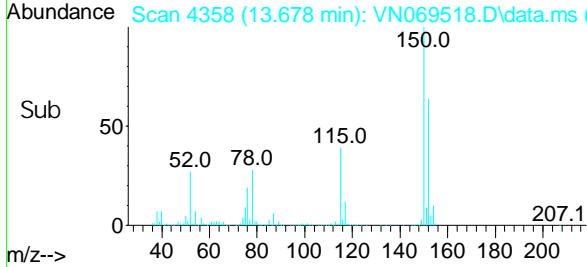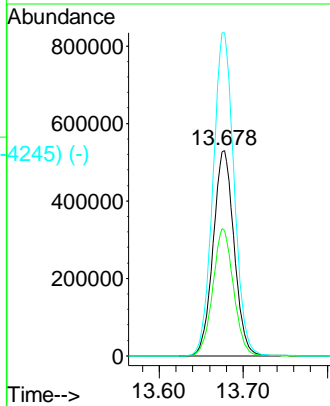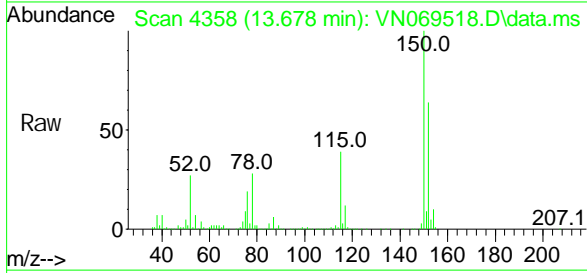


Scan 4061 (12.881 min): VN069417.D\data.ms (-4056) (-)
 1, 2, 3-Tri chl oropropane
 Concen: 29.85 ug/l
 RT: 12.731 min Scan# 4005
 Del ta R. T. -0.150 min
 Lab Fi le: VN069518.D
 Acq: 16 Nov 2021 19:23

Tgt Ion	Resp	Lower	Upper
75	633832		
77	1.0	82.6	247.8#

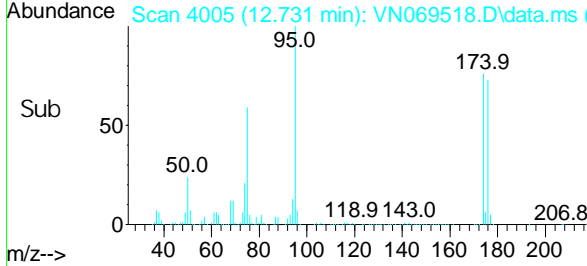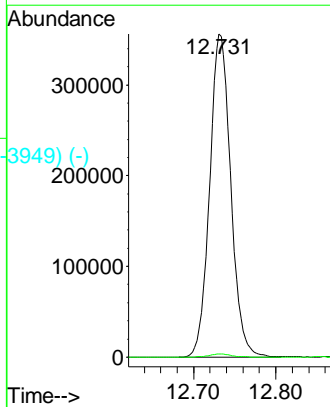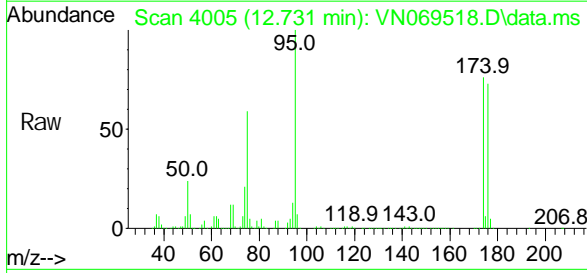

Abundance Scan 3966 (12.626 min): VN069417.D\data.ms (-3966) (-)


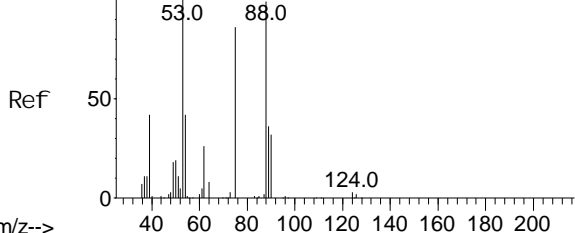


trans-1, 4-Di chloro-2-butene
Concen: 84.37 ug/l
RT: 12.731 min Scan# 4195
Delta R.T. 0.105 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23


Instrument : MSVOA_N
Client SampleId :

Tgt Ion: 75 Resp: 633832
Ion Ratio Lower Upper
75 100
53 0.0 90.5 135.7#
89 0.0 38.2 57.4#


Abundance Scan 4005 (12.731 min): VN069518.D\data.ms

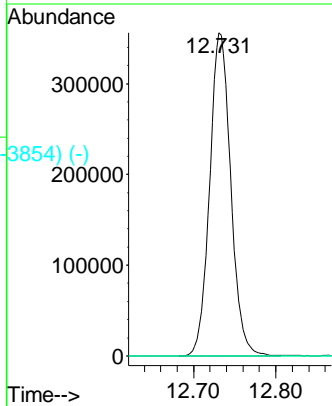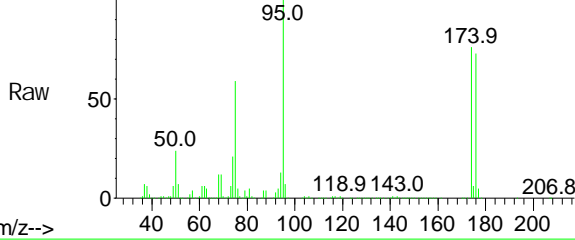

Abundance Scan 4005 (12.731 min): VN069518.D\data.ms (-3854) (-)

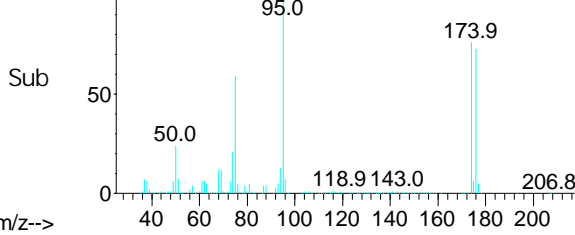



Abundance Scan 4557 (14.211 min): VN069417.D\data.ms (-4557) (-)

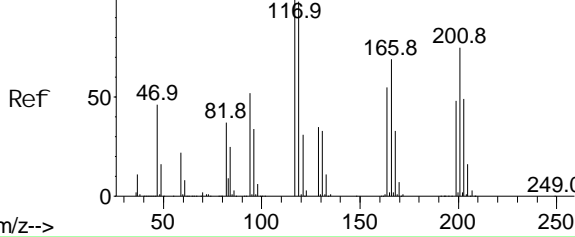


Hexachloroethane
Concen: 2.16 ug/l
RT: 13.981 min Scan# 4471
Delta R.T. -0.230 min
Lab File: VN069518.D
Acq: 16 Nov 2021 19:23


Tgt Ion: 117 Resp: 27
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

Abundance Scan 4471 (13.981 min): VN069518.D\data.ms

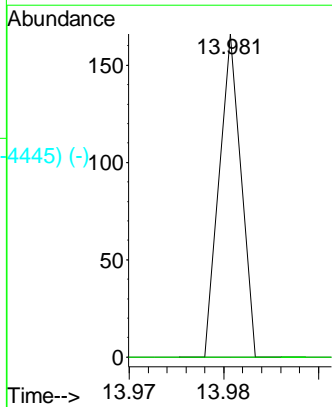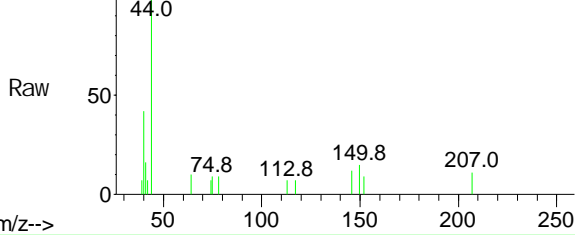

Abundance Scan 4471 (13.981 min): VN069518.D\data.ms (-4445) (-)




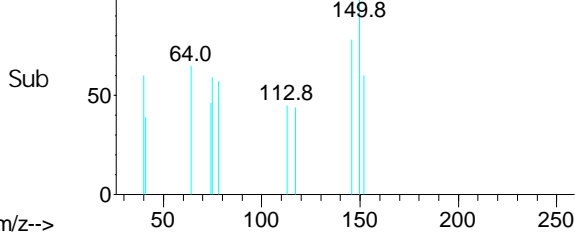


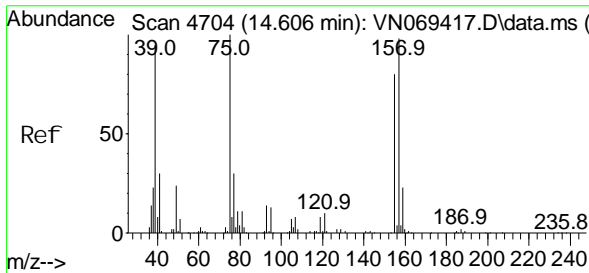

1, 2-Di bromo-3-Chl oropropane
 Concen: 1.82 ug/l
 RT: 14.606 mi n Scan# 4704
 Del ta R. T. -0.000 mi n
 Lab Fi le: VN069518. D
 Acq: 16 Nov 2021 19: 23




Instrument : MSVOA_N
 ClientSampleId :


Tgt Ion	Resp	Lower	Upper
75	100		
155	0.0	46.9	140.7#
157	0.0	60.6	181.7#

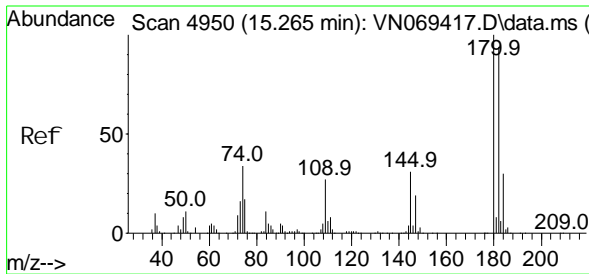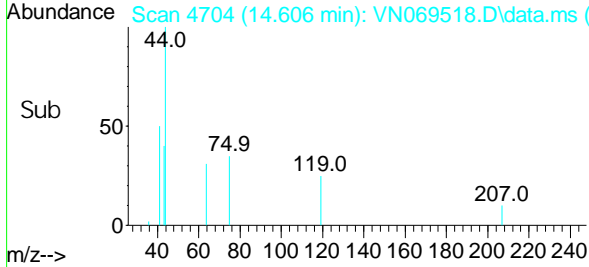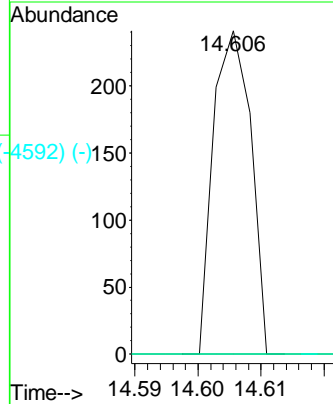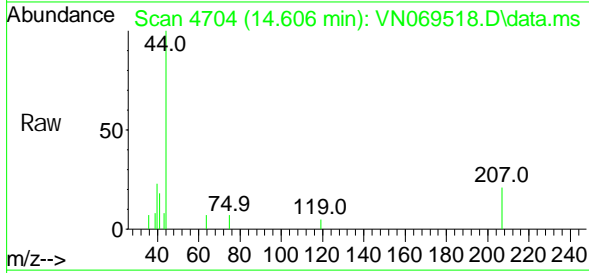

1, 2, 4-Tri chl orobenzene
 Concen: 3.15 ug/l
 RT: 15.257 mi n Scan# 4947
 Del ta R. T. -0.008 mi n
 Lab Fi le: VN069518. D
 Acq: 16 Nov 2021 19: 23


Tgt Ion	Resp	Lower	Upper
180	100		
182	56.7	48.3	144.9
145	4.7	14.5	43.5#

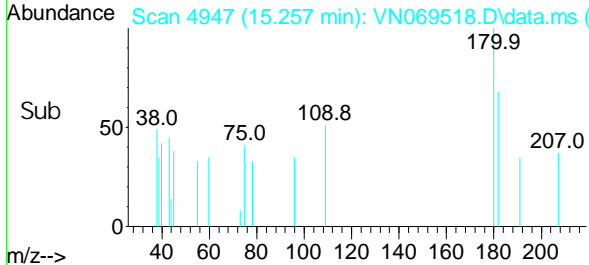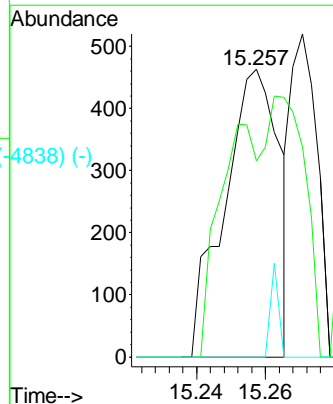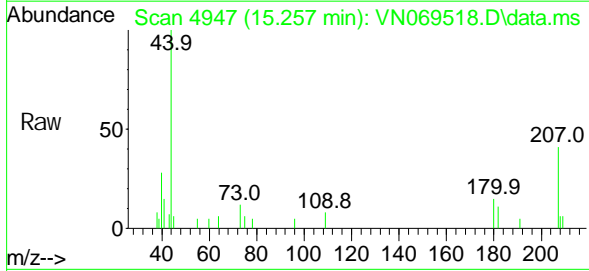



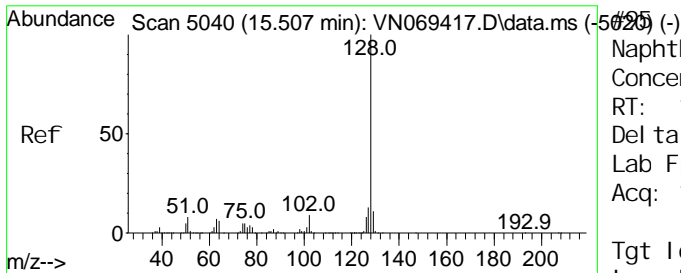


#95 (-)
 Naphthalene
 Concen: 4.54 ug/l
 RT: 15.507 min Scan# 5114
 Delta R.T. -0.000 min
 Lab File: VN069518.D
 Acq: 16 Nov 2021 19:23


Instrument : MSVOA_N
 ClientSampleId :



Tgt Ion: 128 Resp: 4189
 Ion Ratio Lower Upper
 128 100
 127 7.2 10.5 15.7#
 129 7.8 8.7 13.1#

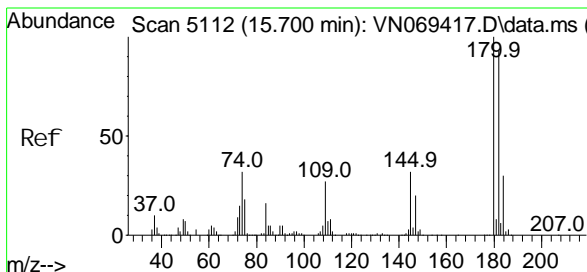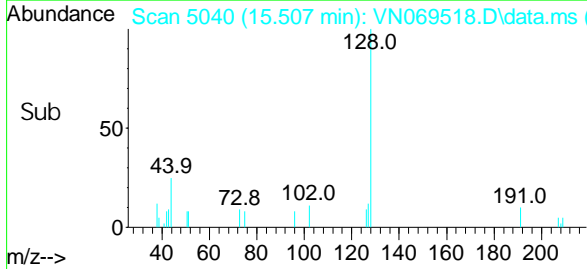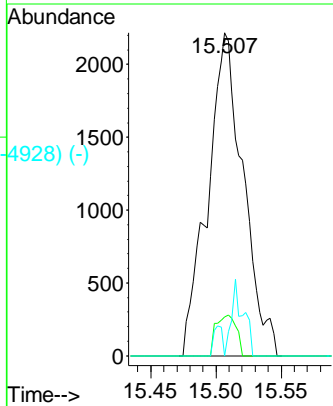

#96 (-)
 1,2,3-Trichlorobenzene
 Concen: 3.23 ug/l
 RT: 15.705 min Scan# 5114
 Delta R.T. 0.005 min
 Lab File: VN069518.D
 Acq: 16 Nov 2021 19:23



Tgt Ion: 180 Resp: 909
 Ion Ratio Lower Upper
 180 100
 182 61.5 47.4 142.2
 145 0.0 15.0 45.1#

