
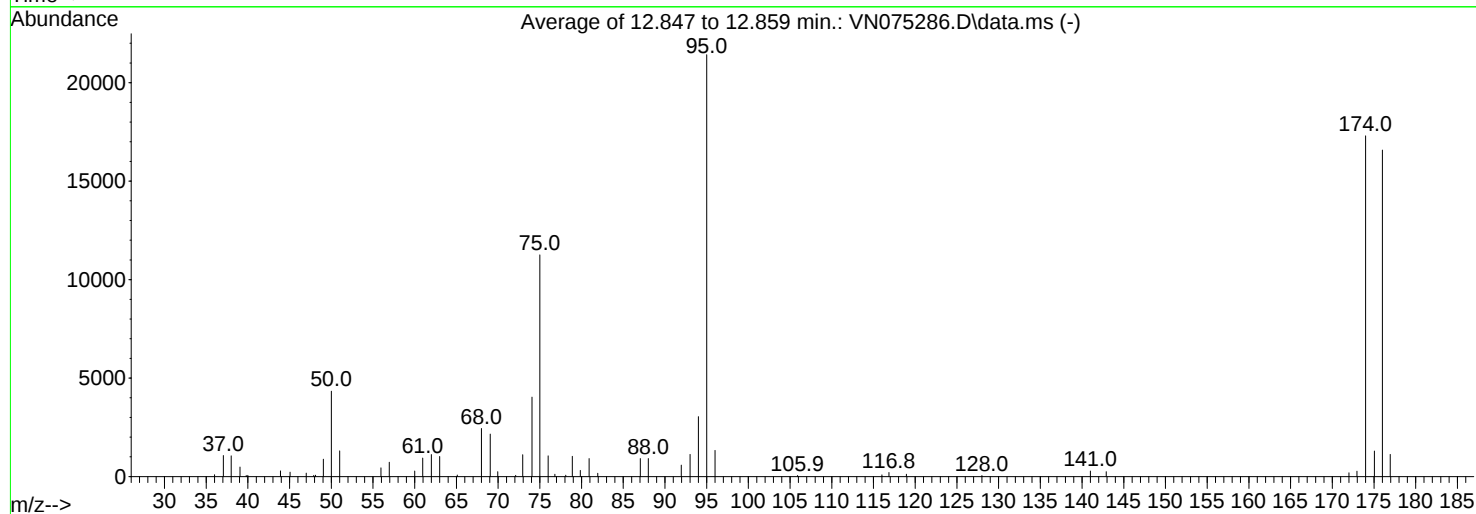


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111622\
Data File : VN075286.D
Acq On : 16 Nov 2022 11:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

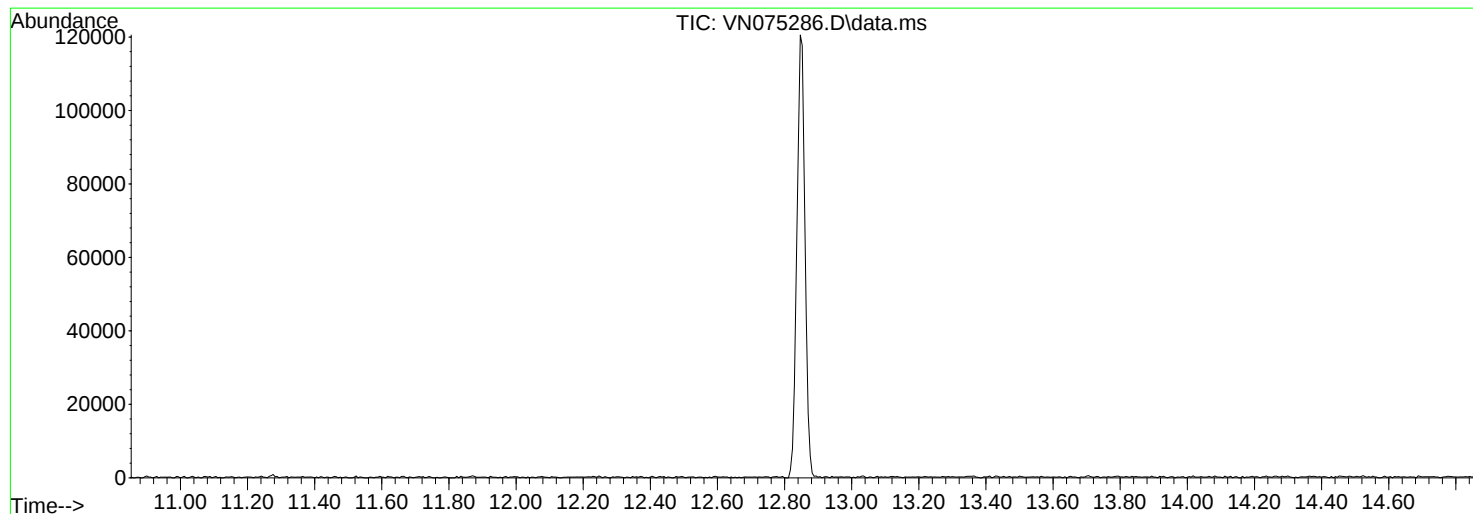

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	4338	PASS
75	95	30	60	52.6	11256	PASS
95	95	100	100	100.0	21416	PASS
96	95	5	9	6.2	1326	PASS
173	174	0.00	2	1.6	276	PASS
174	95	50	100	80.8	17303	PASS
175	174	5	9	7.5	1300	PASS
176	174	95	101	95.8	16577	PASS
177	176	5	9	6.8	1126	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	93	49.05	878	69.05	2157	80.90	911
37.05	1068	50.00	4338	69.95	244	81.95	170
38.00	1054	51.00	1308	72.10	59	87.05	912
39.05	480	55.95	444	72.95	1110	88.00	918
39.80	55	56.95	724	74.05	4035	91.95	579
40.00	63	60.00	280	75.00	11256	93.00	1124
43.90	291	60.95	938	76.00	1052	94.00	3042
45.05	220	62.00	1117	76.80	118	95.00	21416
47.00	173	63.00	1020	78.10	66	96.00	1326
47.90	61	65.10	74	78.90	1029	105.90	56
48.10	72	68.00	2444	79.85	313	116.00	82

Average of 12.847 to 12.859 min.: VN075286.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.85	204						
118.95	115						
128.00	55						
141.00	283						
142.90	250						
172.00	191						
172.95	276						
174.00	17303						
175.05	1300						
176.00	16577						
176.95	1126						

Instrument :

MSVOA_N

ClientSampleId :

BFB