
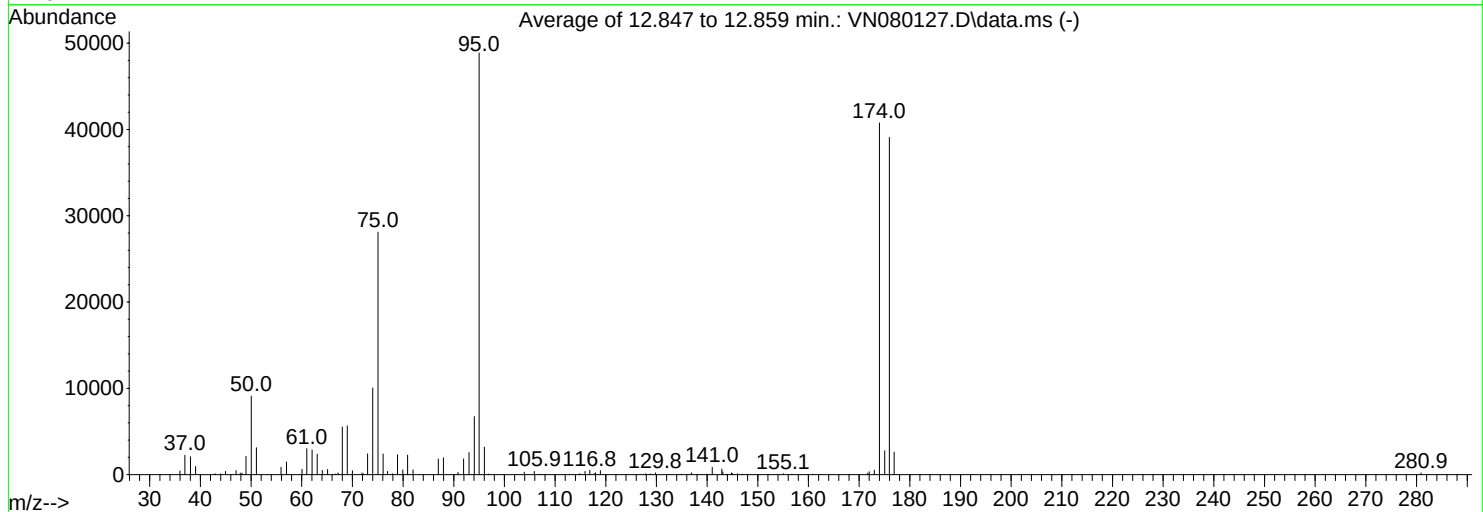


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111623\
Data File : VN080127.D
Acq On : 16 Nov 2023 09:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

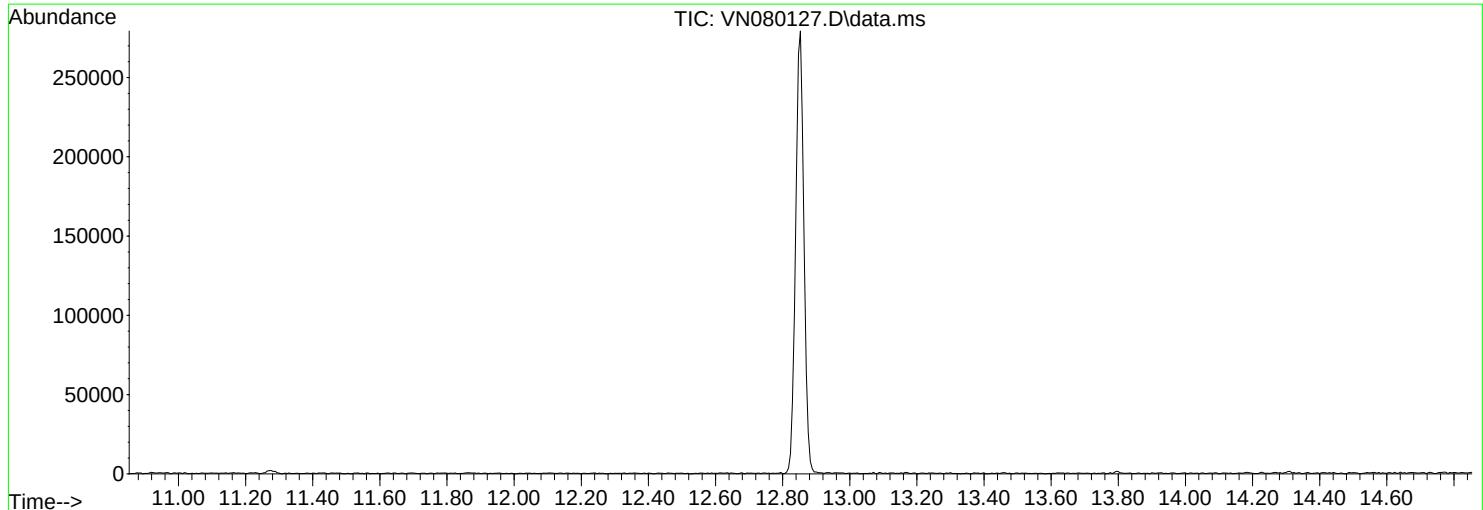

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	9096	PASS
75	95	30	60	57.5	28104	PASS
95	95	100	100	100.0	48875	PASS
96	95	5	9	6.5	3183	PASS
173	174	0.00	2	1.3	517	PASS
174	95	50	100	83.4	40747	PASS
175	174	5	9	6.8	2759	PASS
176	174	95	101	95.9	39083	PASS
177	176	5	9	6.7	2617	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	431	50.05	9096	67.15	201	77.90	111
36.95	2251	51.05	3113	68.00	5531	78.90	229
38.05	2068	55.90	855	69.00	5652	79.95	56
39.05	951	57.00	1466	70.00	468	80.90	225
42.90	112	60.05	620	71.90	208	81.95	552
44.00	96	61.00	3031	72.20	93	86.95	1810
44.95	377	62.05	2881	73.00	2410	87.95	1942
47.05	489	63.05	2375	74.00	10059	90.85	258
47.85	195	64.05	494	75.05	28104	91.95	1822
48.20	192	65.10	595	76.05	2384	93.00	2568
49.00	2133	66.70	68	76.90	374	94.05	6727

Average of 12.847 to 12.859 min.: VN080127.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	48875	118.00	219	143.80	60	173.00	517
96.05	3183	118.95	468	144.80	205	174.00	40747
96.90	69	127.90	120	145.00	131	175.05	2759
103.90	283	128.80	76	146.00	111	175.95	39083
105.90	373	129.80	200	146.90	53	176.90	2617
107.00	52	135.00	62	147.90	60	280.90	202
112.80	65	136.90	208	155.05	115		
114.85	113	139.90	56	156.70	53		
115.90	381	141.00	850	160.80	52		
116.85	494	142.90	646	171.70	172		
117.70	122	143.10	336	172.00	333		

Instrument :

MSVOA_N

ClientSampleId :

BFB