


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111722\
Data File : VN075297.D
Acq On : 17 Nov 2022 09:48
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

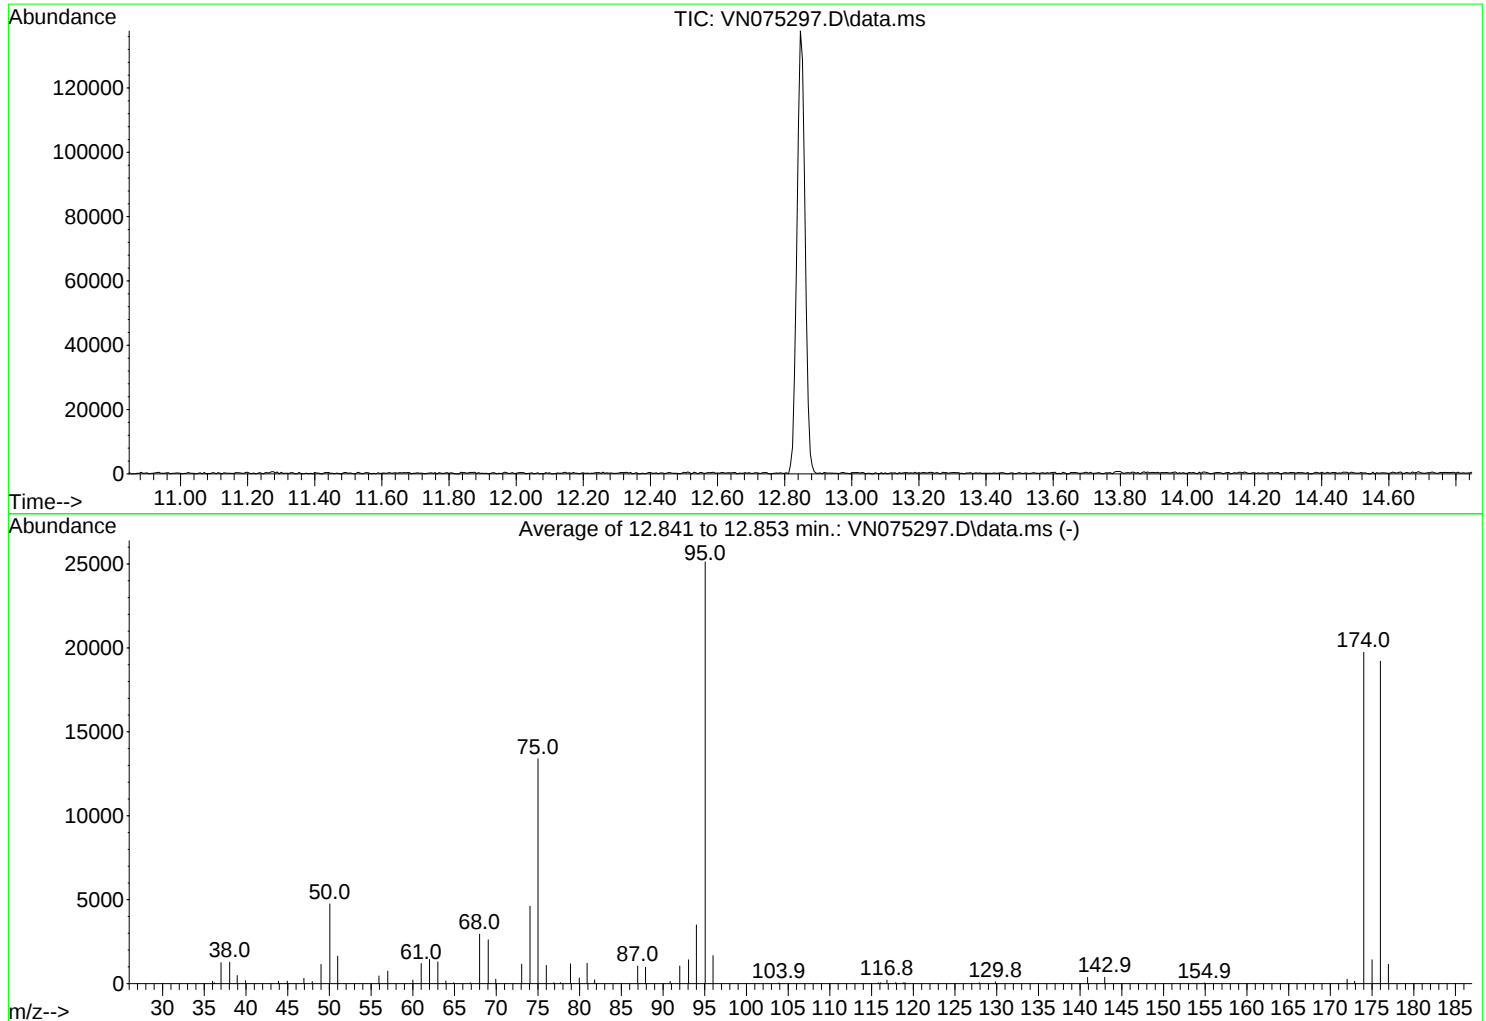

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	4743	PASS
75	95	30	60	53.4	13406	PASS
95	95	100	100	100.0	25128	PASS
96	95	5	9	6.6	1671	PASS
173	174	0.00	2	0.7	142	PASS
174	95	50	100	78.5	19737	PASS
175	174	5	9	7.2	1419	PASS
176	174	95	101	97.3	19204	PASS
177	176	5	9	6.0	1157	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	141	50.05	4743	68.00	2947	80.90	1211
36.20	57	51.00	1640	69.05	2612	81.80	221
37.00	1251	55.95	458	69.95	269	86.95	105
38.05	1280	57.00	744	73.05	1165	87.90	97
38.95	485	60.00	220	74.05	4610	90.85	137
39.95	177	61.00	1205	75.00	13406	92.00	1049
43.90	141	62.00	1446	76.00	1083	93.05	1419
44.95	151	63.00	1293	76.90	60	94.00	3500
46.95	313	63.95	161	77.70	71	95.05	25128
47.95	124	64.90	61	78.90	1186	96.00	1671
49.00	1145	66.90	54	79.95	341	103.90	51

Instrument :

MSVOA_N

ClientSampleId :

BFB

Average of 12.841 to 12.853 min.: VN075297.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
115.80	59	172.00	268				
116.10	61	172.90	142				
116.85	207	174.00	19737				
117.90	64	175.00	1419				
118.80	62	176.00	19204				
119.00	64	176.95	1157				
127.90	53						
129.85	106						
140.90	369						
142.95	381						
154.90	50						