
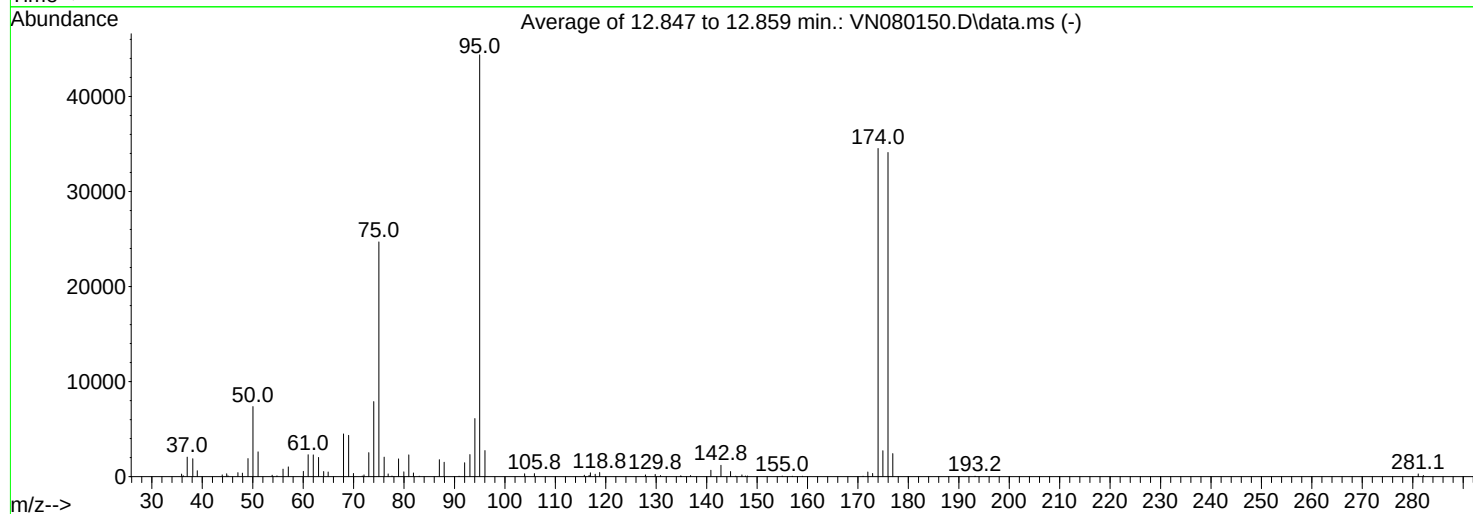


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111723\
Data File : VN080150.D
Acq On : 17 Nov 2023 09:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

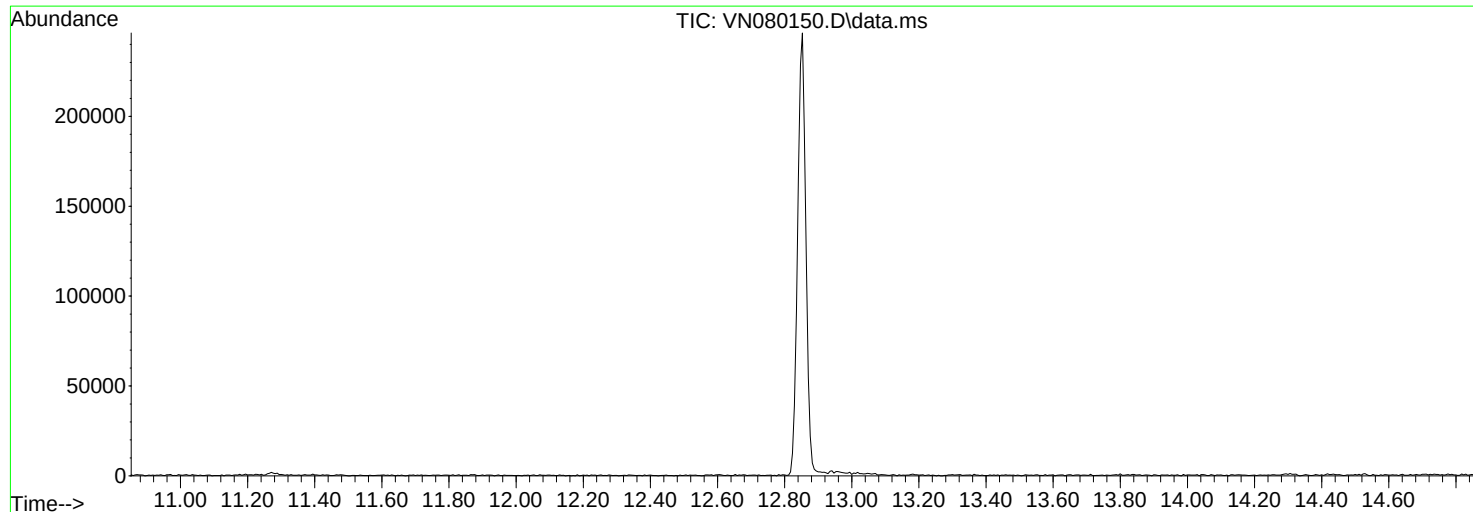

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	7376	PASS
75	95	30	60	55.6	24691	PASS
95	95	100	100	100.0	44376	PASS
96	95	5	9	6.2	2744	PASS
173	174	0.00	2	1.0	333	PASS
174	95	50	100	77.8	34520	PASS
175	174	5	9	7.9	2731	PASS
176	174	95	101	98.8	34109	PASS
177	176	5	9	7.1	2421	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	263	50.05	7376	64.95	496	77.60	61
36.20	107	51.05	2618	68.00	4499	78.90	186
37.00	2054	53.85	148	69.00	4351	79.95	50
38.10	1884	54.80	83	69.95	333	80.95	229
39.00	631	56.00	799	71.70	73	81.85	395
43.95	188	57.05	1029	72.05	185	83.00	50
44.85	302	60.05	561	73.00	2532	87.00	1793
45.10	85	61.00	2313	74.00	7889	87.95	1508
47.05	424	62.00	2286	75.00	24691	90.90	53
47.95	379	63.05	2016	76.05	2048	92.00	1466
49.05	1897	64.05	547	76.85	280	93.05	2325

Average of 12.847 to 12.859 min.: VN080150.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	6116	129.80	244	148.10	60	193.20	50
95.00	44376	130.85	123	155.00	60	281.10	294
96.05	2744	134.80	85	157.00	51	282.10	119
103.90	305	135.00	58	159.00	57		
105.85	327	136.80	118	171.00	59		
115.75	161	140.85	679	171.95	483		
116.70	131	142.85	1198	172.90	333		
116.95	413	144.75	534	174.00	34520		
117.90	261	145.80	57	174.95	2731		
118.80	447	147.00	187	175.95	34109		
127.85	183	147.70	69	176.90	2421		

Instrument :

MSVOA_N

ClientSampleId :

BFB