

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111724\
 Data File : VN084886.D
 Acq On : 17 Nov 2024 11:26
 Operator : JC\MD
 Sample : VN1117WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN1117WBL01

Quant Time: Nov 18 00:16:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 31 18:45:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.218	168	155503	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	272839	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	236144	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	104526	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.571	65	115215	51.298	ug/l	0.00
Spiked Amount	50.000	Range 74 - 125	Recovery	=	102.600%	
35) Dibromofluoromethane	8.165	113	94278	51.050	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	=	102.100%	
50) Toluene-d8	10.565	98	311458	45.783	ug/l	0.00
Spiked Amount	50.000	Range 86 - 113	Recovery	=	91.560%	
62) 4-Bromofluorobenzene	12.847	95	114265	44.942	ug/l	0.00
Spiked Amount	50.000	Range 77 - 121	Recovery	=	89.880%	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111724\
Data File : VN084886.D
Acq On : 17 Nov 2024 11:26
Operator : JC\MD
Sample : VN1117WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN1117WBL01

Quant Time: Nov 18 00:16:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 31 18:45:38 2024
Response via : Initial Calibration




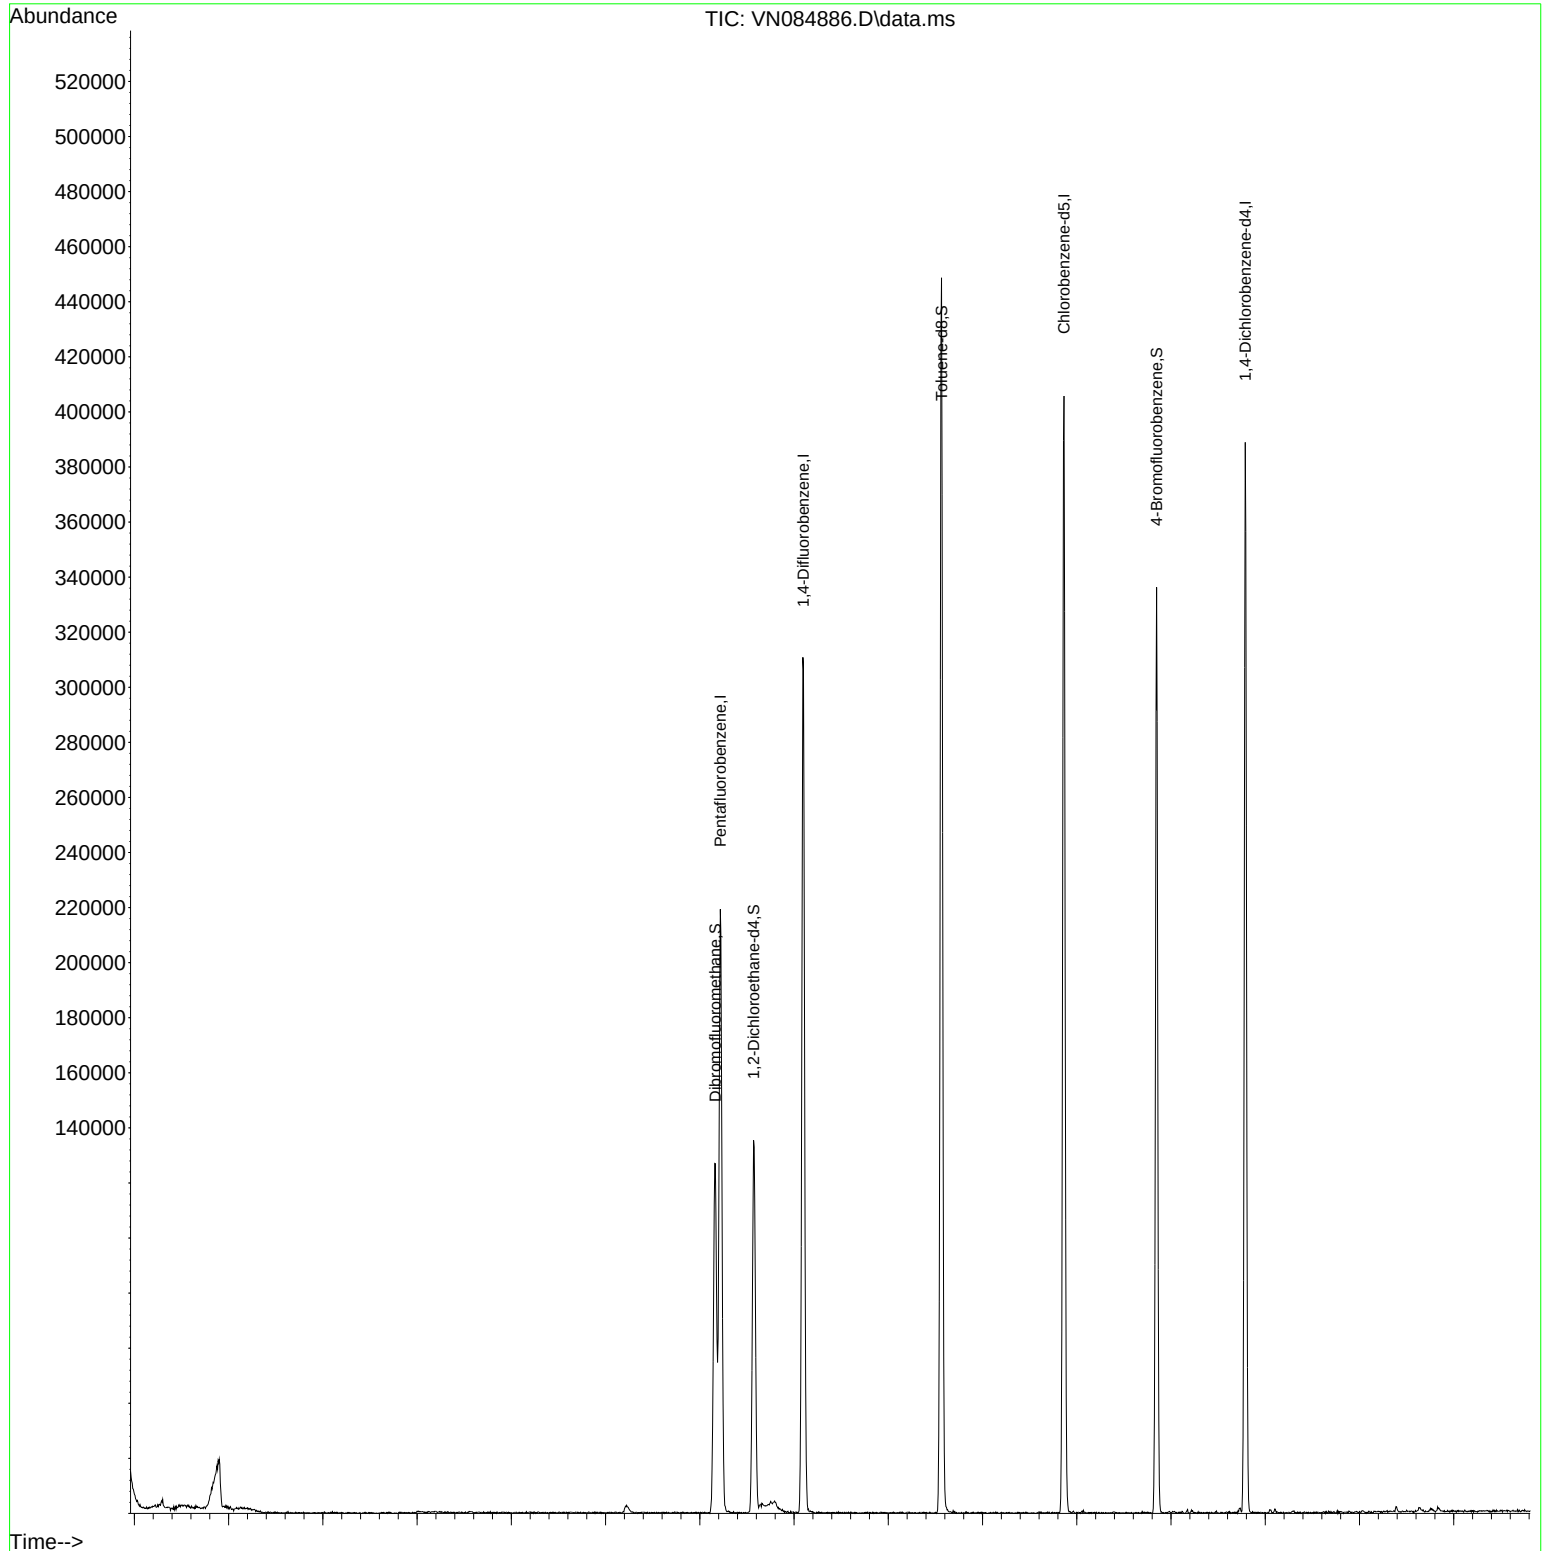


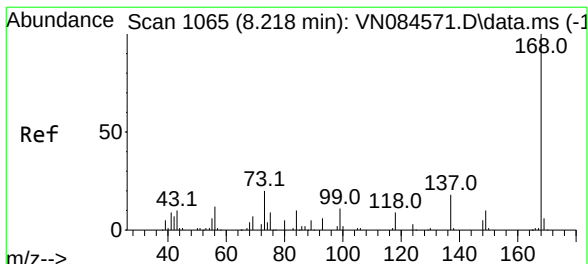

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.006 min
Lab File: VN084886.D
Acq: 17 Nov 2024 11:26




Instrument :
MSVOA_N
ClientSampleId :
VN1117WBL01


Tgt Ion:168 Resp: 155503
Ion Ratio Lower Upper
168 100
99 60.7 54.2 81.2

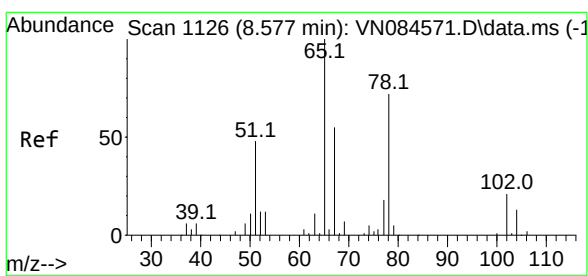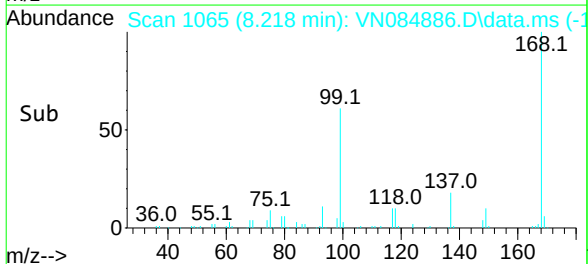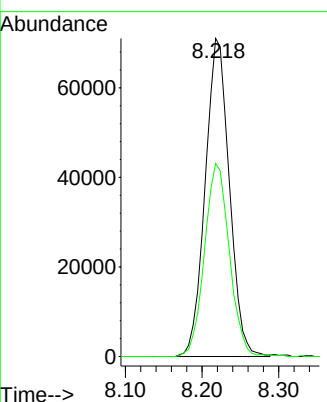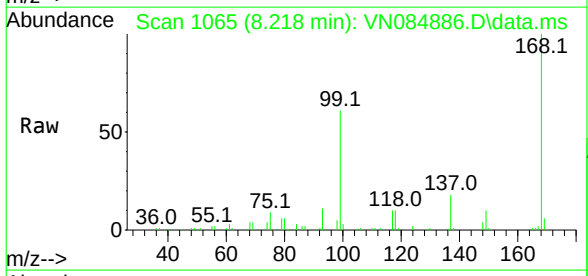

#33
1,2-Dichloroethane-d4
Concen: 51.298 ug/l
RT: 8.571 min Scan# 1125
Delta R.T. -0.006 min
Lab File: VN084886.D
Acq: 17 Nov 2024 11:26

Tgt Ion: 65 Resp: 115215
Ion Ratio Lower Upper
65 100
67 50.9 0.0 102.0


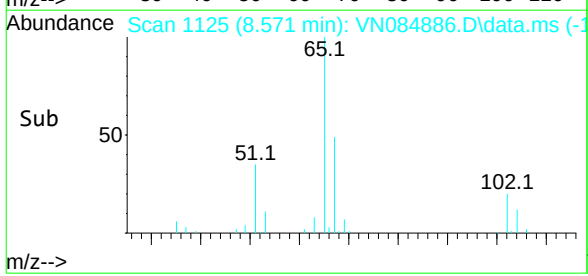
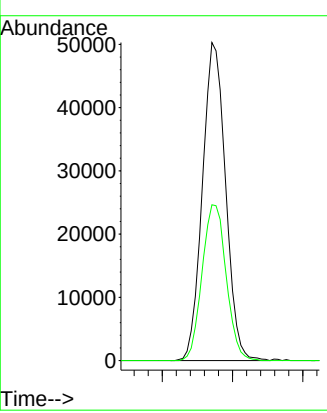
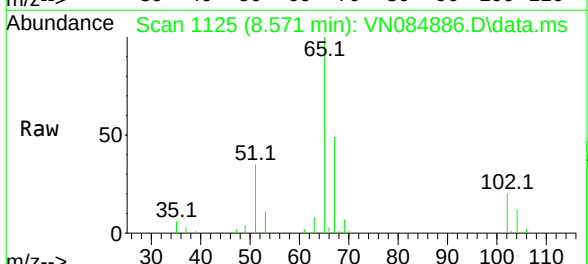


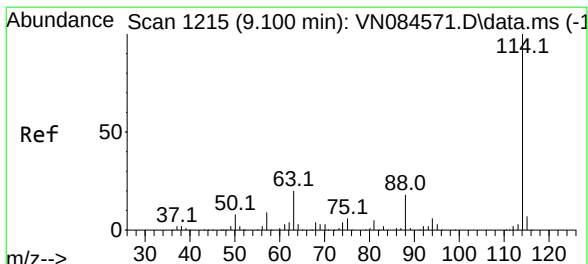

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 9.100 min Scan# 12
 Delta R.T. 0.000 min
 Lab File: VN084886.D
 Acq: 17 Nov 2024 11:26




Instrument :
 MSVOA_N
 ClientSampleId :
 VN1117WBL01


Tgt Ion:	114	Resp:	272839
Ion	Ratio	Lower	Upper
114	100		
63	19.5	0.0	43.8
88	15.8	0.0	31.6

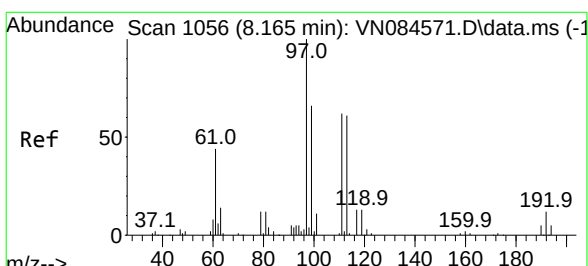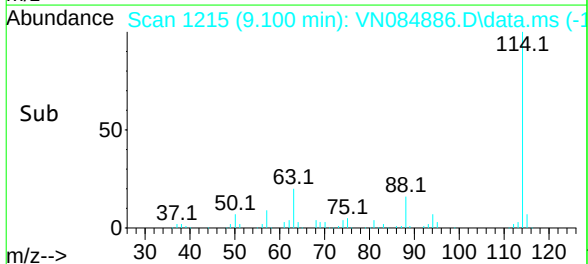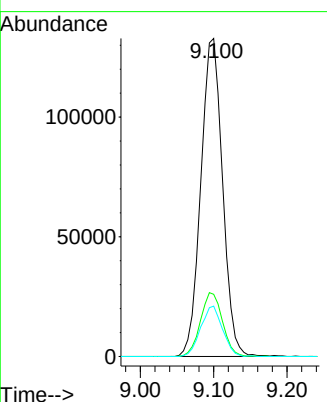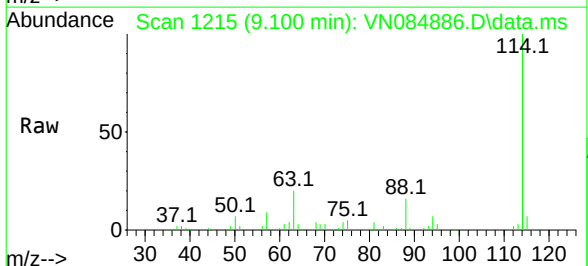

#35
 Dibromofluoromethane
 Concen: 51.050 ug/l
 RT: 8.165 min Scan# 1056
 Delta R.T. -0.000 min
 Lab File: VN084886.D
 Acq: 17 Nov 2024 11:26

Tgt Ion:	113	Resp:	94278
Ion	Ratio	Lower	Upper
113	100		
111	101.6	83.3	124.9
192	18.2	13.5	20.3

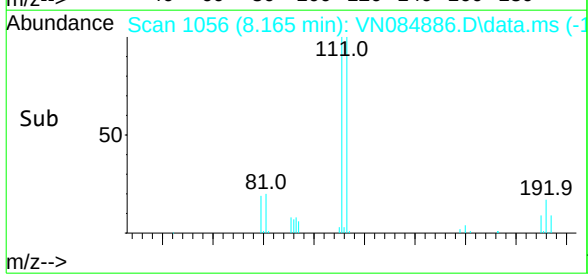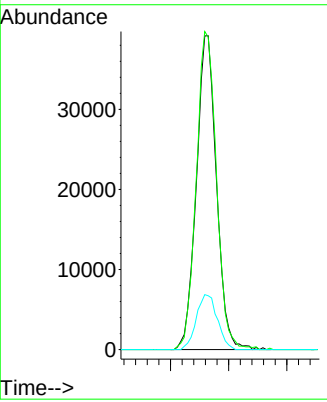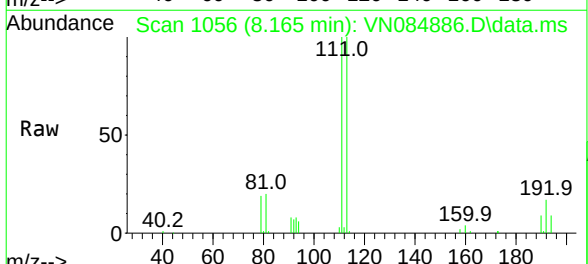

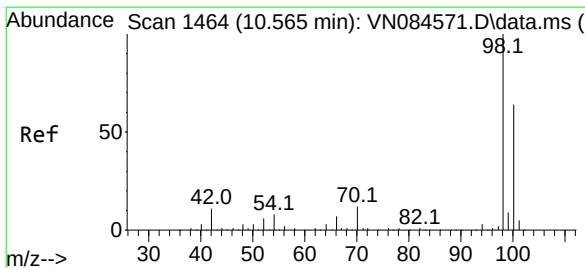

#50

Toluene-d8

Concen: 45.783 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. -0.000 min

Lab File: VN084886.D

Acq: 17 Nov 2024 11:26

Instrument :

MSVOA_N

ClientSampleId :





VN1117WBL01

Tgt Ion: 98 Resp: 311458

Ion Ratio Lower Upper

98 100

100 64.5 52.7 79.1

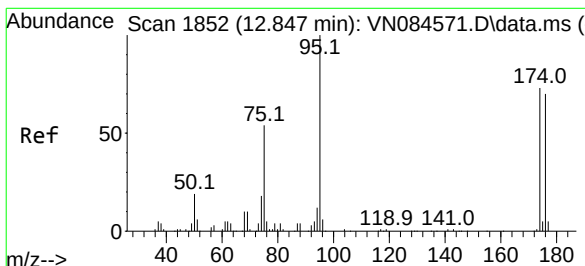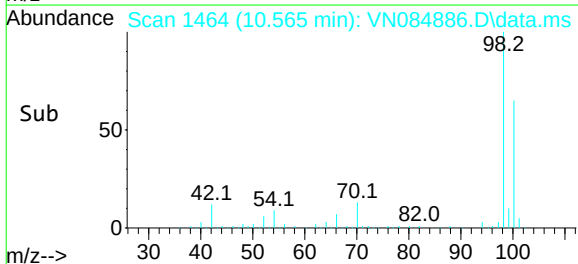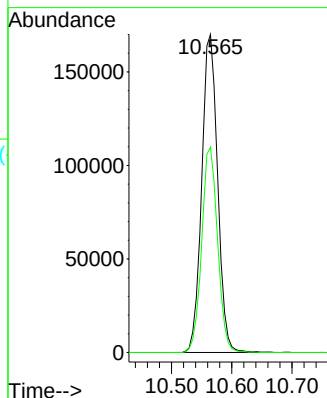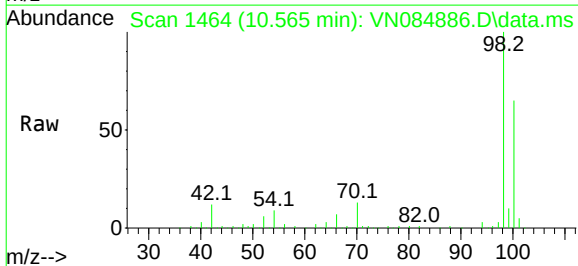

#62

4-Bromofluorobenzene

Concen: 44.942 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. -0.000 min

Lab File: VN084886.D

Acq: 17 Nov 2024 11:26




Tgt Ion: 95 Resp: 114265


Ion Ratio Lower Upper

95 100

174 77.2 0.0 145.2

176 72.5 0.0 140.0


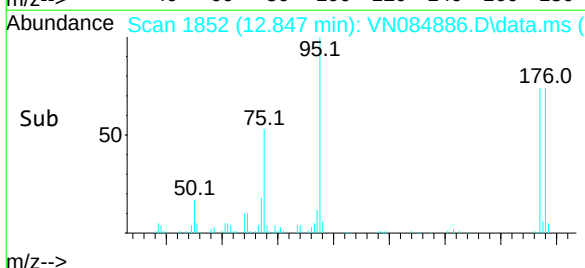
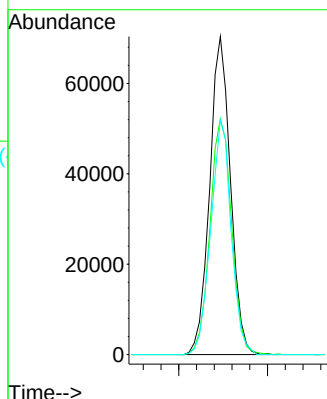
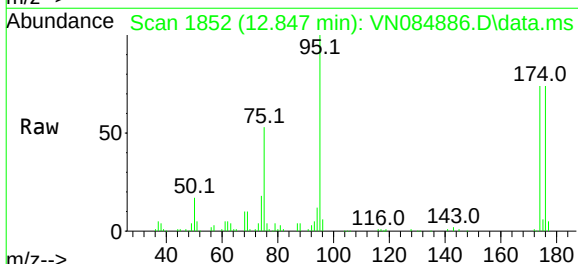


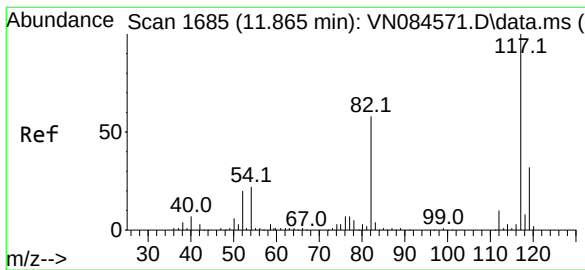

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. -0.000 min
Lab File: VN084886.D
Acq: 17 Nov 2024 11:26

Instrument :
MSVOA_N
ClientSampleId :
VN1117WBL01

Tgt Ion:117 Resp: 236144
Ion Ratio Lower Upper
117 100
82 54.5 47.2 70.8
119 31.6 25.4 38.0

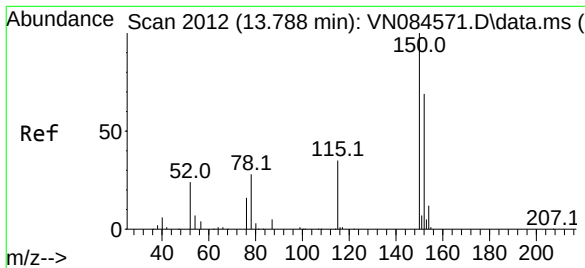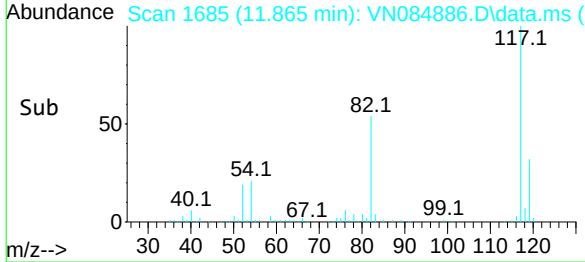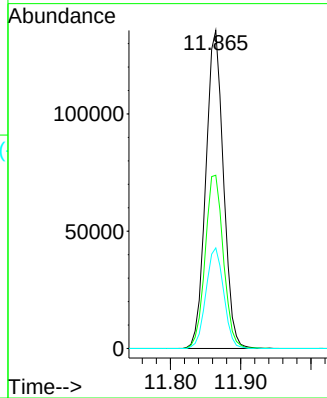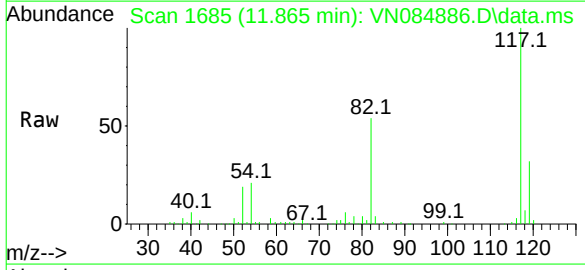

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN084886.D
Acq: 17 Nov 2024 11:26

Tgt Ion:152 Resp: 104526
Ion Ratio Lower Upper
152 100
115 62.2 31.3 93.9
150 158.6 0.0 349.8

