
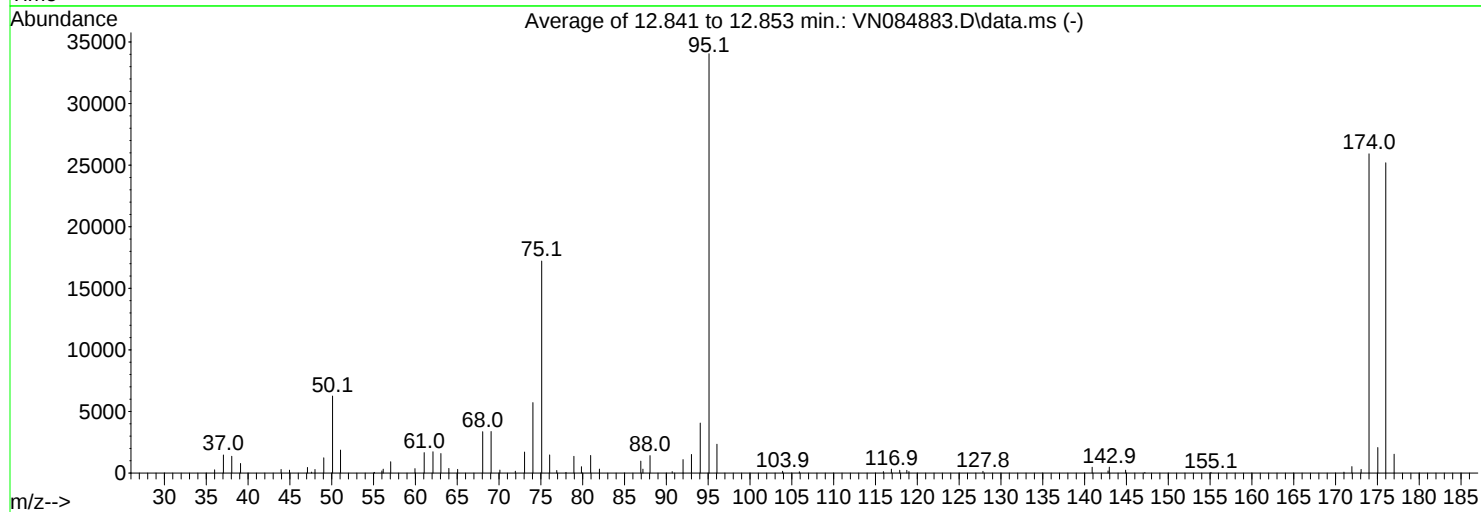


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111724\
Data File : VN084883.D
Acq On : 17 Nov 2024 10:03
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

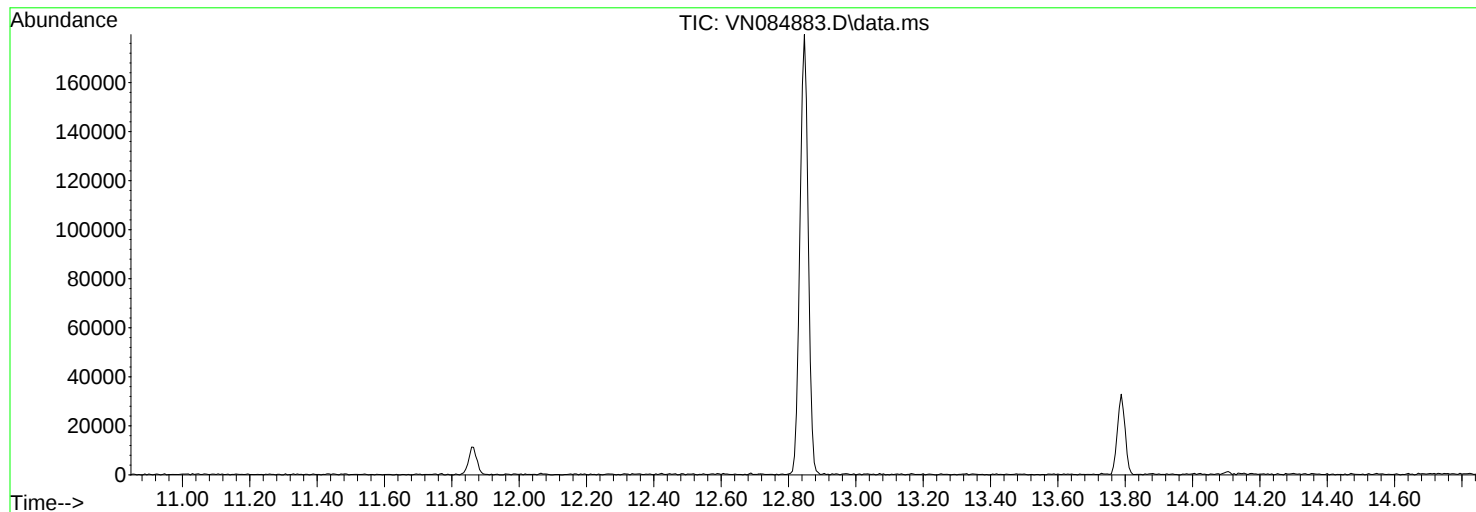

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	6255	PASS
75	95	30	60	50.6	17216	PASS
95	95	100	100	100.0	34048	PASS
96	95	5	9	6.9	2344	PASS
173	174	0.00	2	1.1	298	PASS
174	95	50	100	76.1	25923	PASS
175	174	5	9	8.0	2075	PASS
176	174	95	101	97.2	25195	PASS
177	176	5	9	6.1	1531	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	264	51.05	1866	68.05	3360	79.85	518
37.05	1468	55.10	59	69.05	3375	80.95	1430
38.05	1367	56.00	174	70.10	245	82.00	325
39.10	781	56.15	321	71.95	155	86.95	971
43.95	298	57.05	920	73.05	1707	87.20	320
44.95	239	59.95	365	74.05	5723	88.05	1419
47.10	456	61.05	1661	75.10	17216	90.70	117
47.60	79	62.10	1731	76.05	1473	92.00	1095
48.00	292	63.05	1588	76.90	212	93.00	1515
49.05	1241	64.00	379	78.00	58	94.05	4061
50.10	6255	65.05	301	78.95	1362	95.10	34048

Average of 12.841 to 12.853 min.: VN084883.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.05	2344	142.95	483				
103.90	149	144.90	237				
105.90	110	147.20	57				
115.95	123	155.10	52				
116.90	318	171.00	80				
117.90	232	171.95	527				
118.75	225	173.05	298				
119.00	122	174.00	25923				
127.85	145	175.05	2075				
140.90	475	176.00	25195				
142.80	176	177.00	1531				

Instrument :

MSVOA_N

ClientSampleId :

BFB