

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111725\
 Data File : VN088297.D
 Acq On : 17 Nov 2025 12:37
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Nov 18 02:58:38 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
 Quant Title : SW846 8260
 QLast Update : Mon Nov 03 01:16:06 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.206	168	190582	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.083	114	427343	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.841	117	405111	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.770	152	189838	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.559	65	177181	53.764	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	107.520%
35) Dibromofluoromethane	8.147	113	139847	48.712	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.420%
50) Toluene-d8	10.547	98	494417	44.695	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.380%
62) 4-Bromofluorobenzene	12.829	95	179468	45.938	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	91.880%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111725\
Data File : VN088297.D
Acq On : 17 Nov 2025 12:37
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Nov 18 02:58:38 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Quant Title : SW846 8260
QLast Update : Mon Nov 03 01:16:06 2025
Response via : Initial Calibration




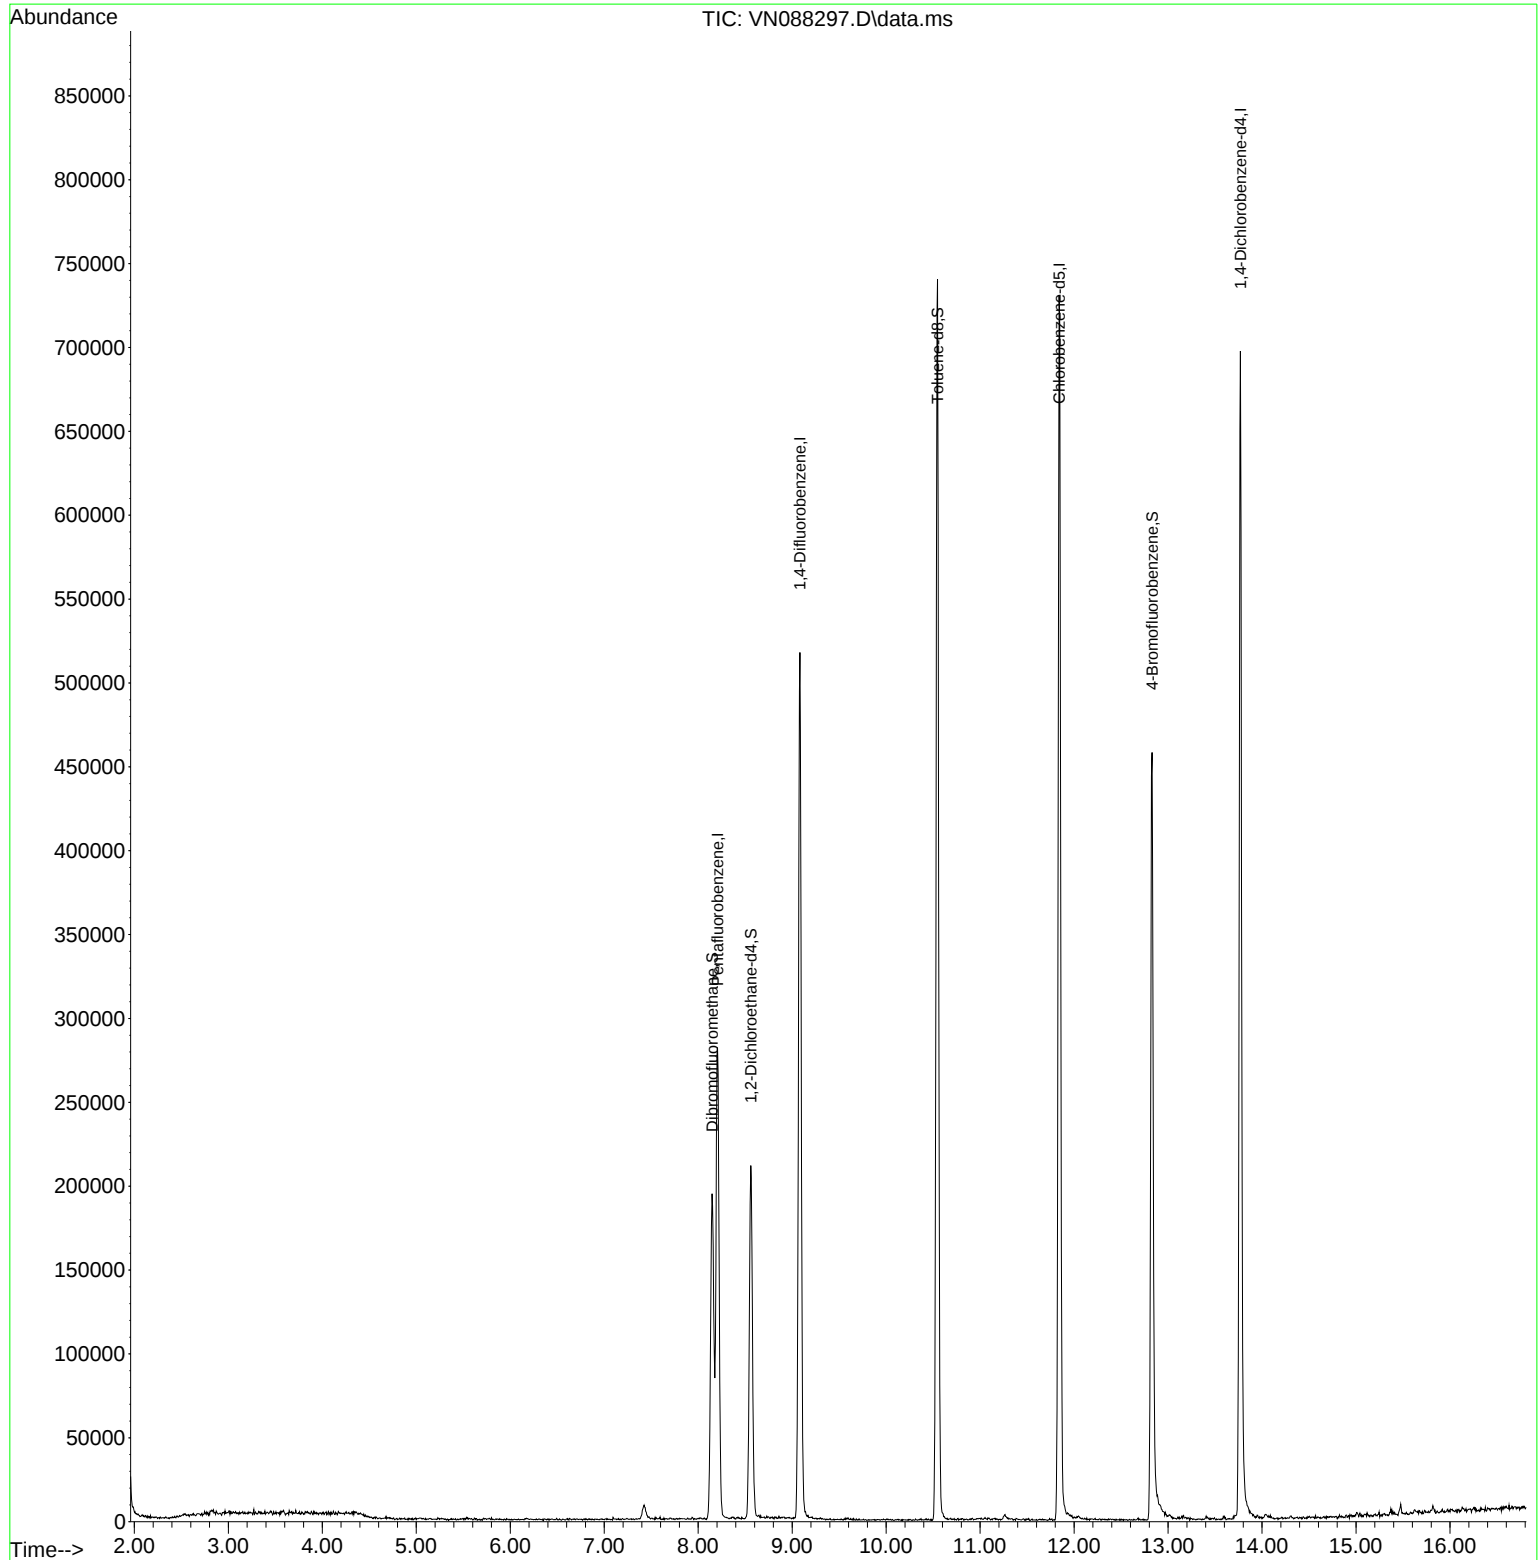


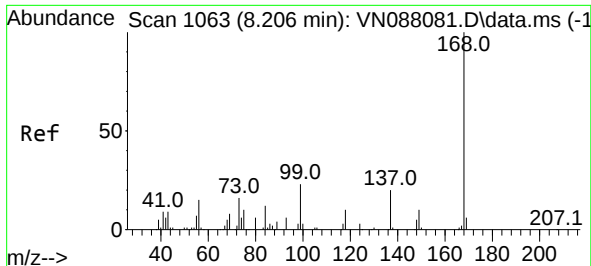

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.206 min Scan# 1063
Delta R.T. 0.000 min
Lab File: VN088297.D
Acq: 17 Nov 2025 12:37




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 190582
Ion Ratio Lower Upper
168 100
99 64.3 57.2 85.8

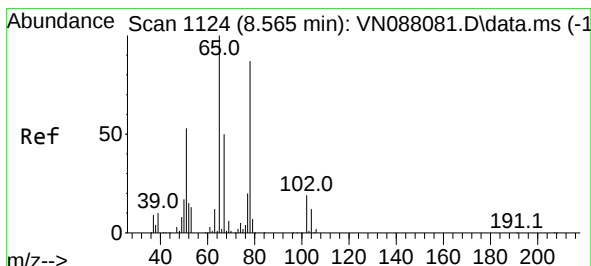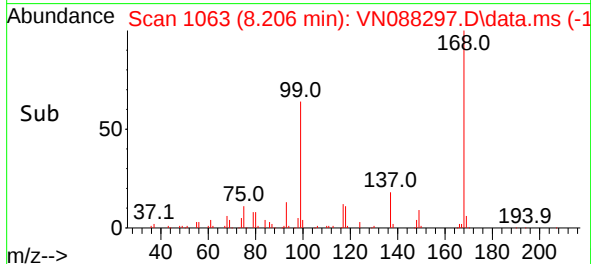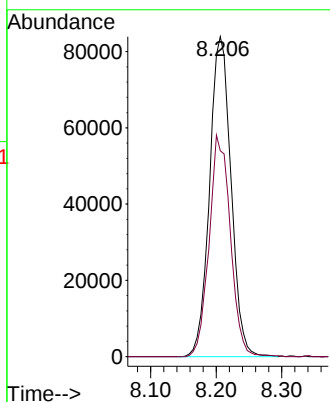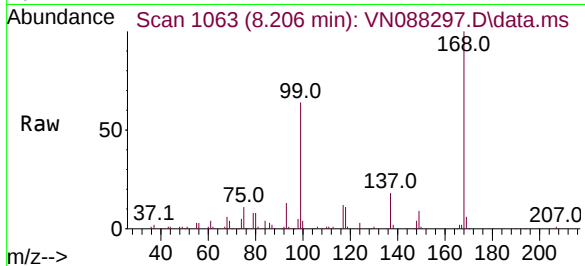

#33
1,2-Dichloroethane-d4
Concen: 53.764 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. -0.000 min
Lab File: VN088297.D
Acq: 17 Nov 2025 12:37

Tgt Ion: 65 Resp: 177181
Ion Ratio Lower Upper
65 100
67 50.4 0.0 100.0

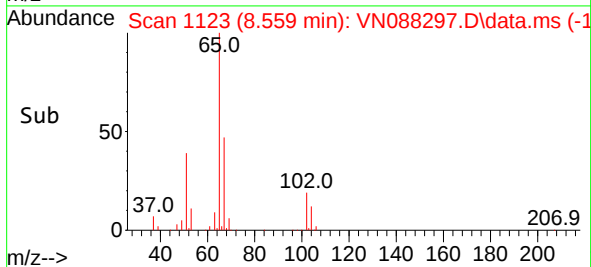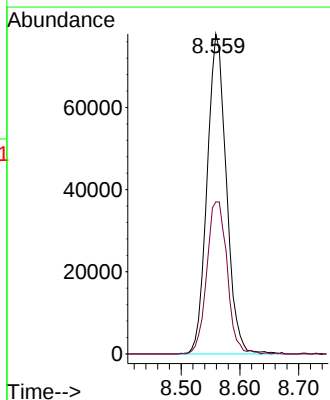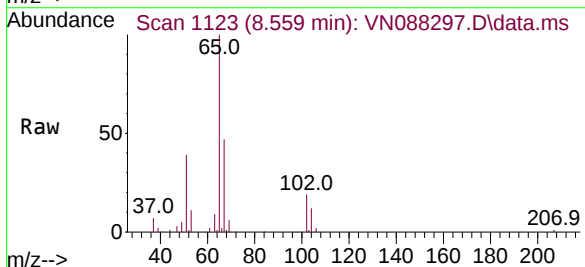

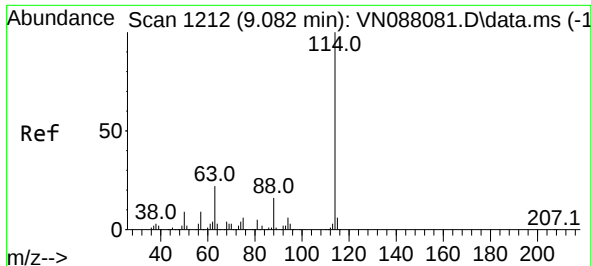

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.083 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN088297.D

Acq: 17 Nov 2025 12:37

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion:114 Resp: 427343

Ion Ratio Lower Upper

114 100

63 22.5 0.0 45.2

88 16.7 0.0 33.4

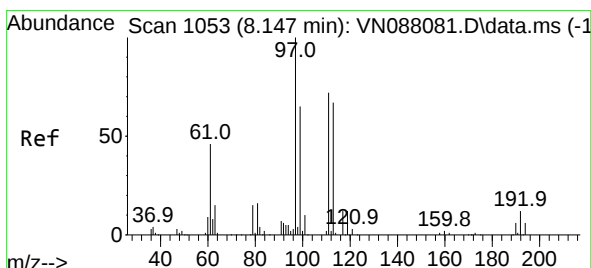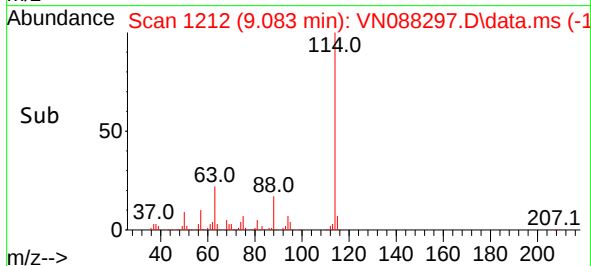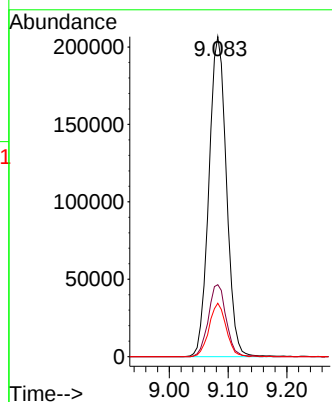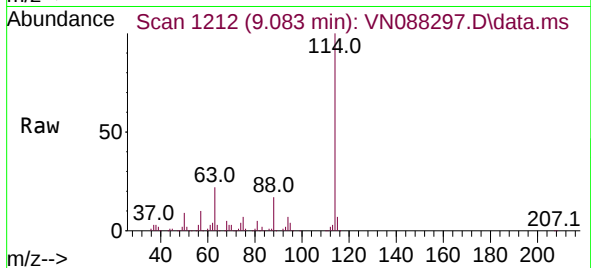

#35

Dibromofluoromethane

Concen: 48.712 ug/l

RT: 8.147 min Scan# 1053

Delta R.T. -0.006 min

Lab File: VN088297.D

Acq: 17 Nov 2025 12:37




Tgt Ion:113 Resp: 139847


Ion Ratio Lower Upper

113 100

111 103.6 82.8 124.2

192 16.4 12.8 19.2


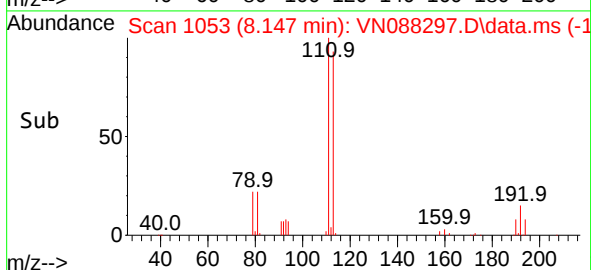
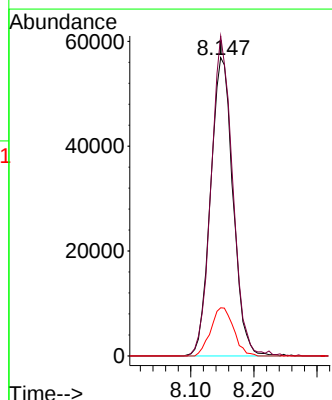
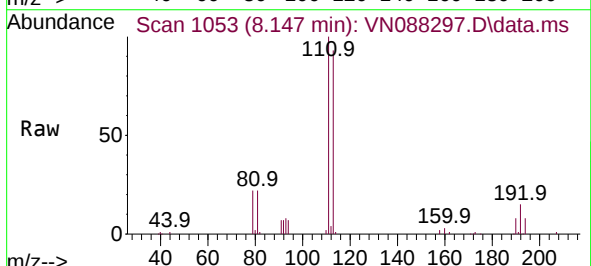


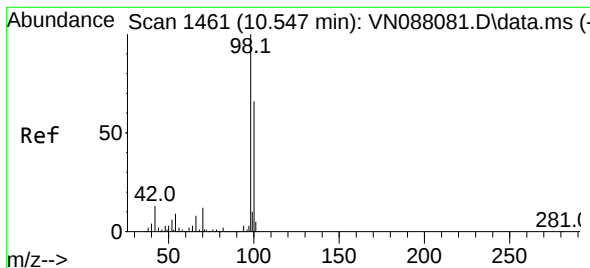

#50
Toluene-d8
Concen: 44.695 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. -0.000 min
Lab File: VN088297.D
Acq: 17 Nov 2025 12:37




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 494417
Ion Ratio Lower Upper
98 100
100 64.9 52.8 79.2

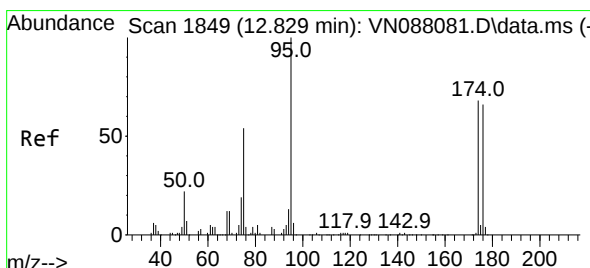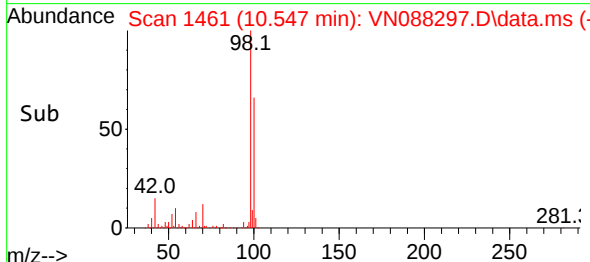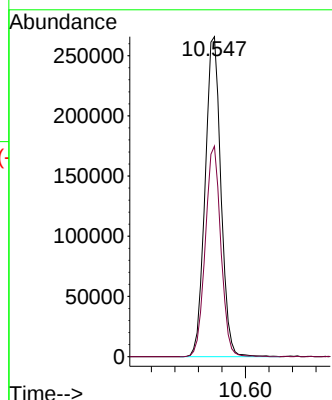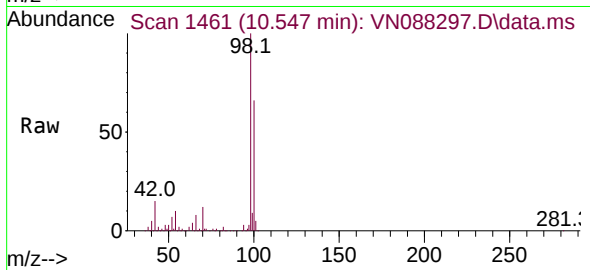

#62
4-Bromofluorobenzene
Concen: 45.938 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. 0.006 min
Lab File: VN088297.D
Acq: 17 Nov 2025 12:37

Tgt Ion: 95 Resp: 179468
Ion Ratio Lower Upper
95 100
174 70.7 0.0 138.4
176 64.3 0.0 132.6


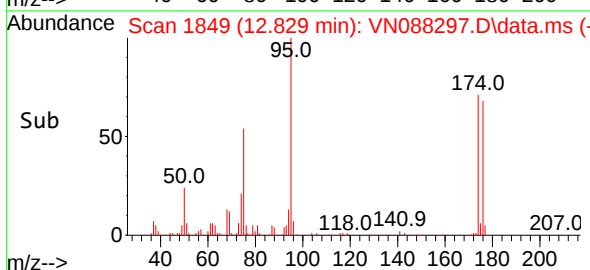
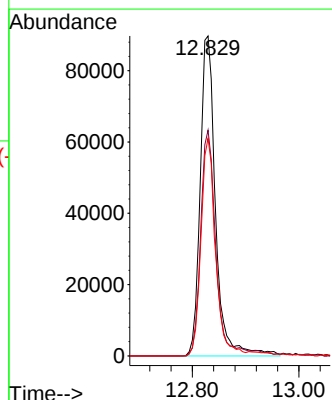
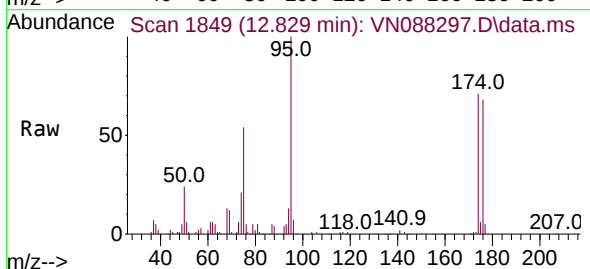


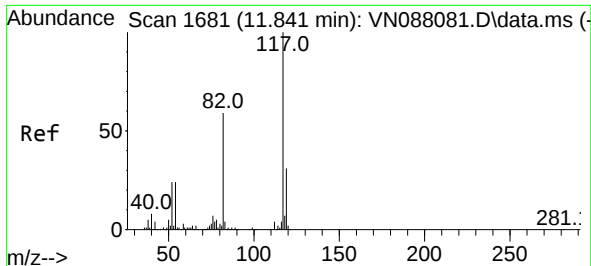

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.841 min Scan# 1681
Delta R.T. -0.000 min
Lab File: VN088297.D
Acq: 17 Nov 2025 12:37

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 405111
Ion Ratio Lower Upper
117 100
82 59.1 47.4 71.2
119 31.0 24.3 36.5

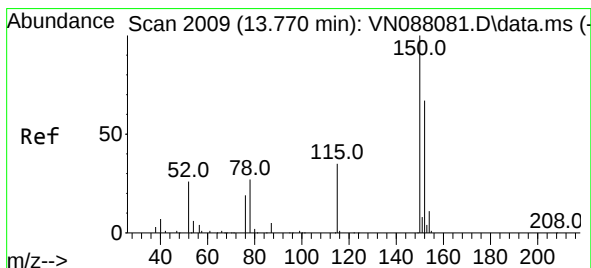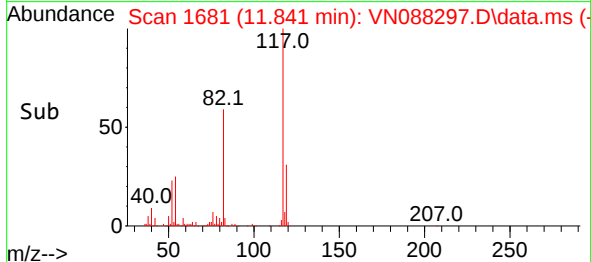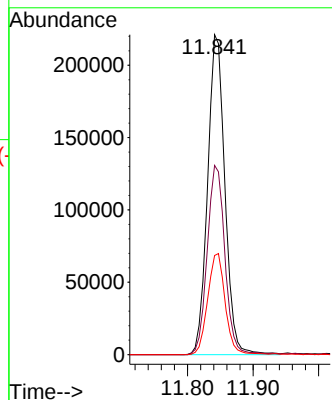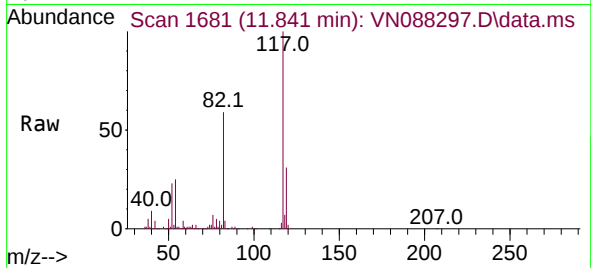

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.770 min Scan# 2009
Delta R.T. 0.006 min
Lab File: VN088297.D
Acq: 17 Nov 2025 12:37

Tgt Ion:152 Resp: 189838
Ion Ratio Lower Upper
152 100
115 64.0 32.3 96.8
150 157.4 0.0 351.0

