


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN111819\
Data File : VN059272.D
Acq On : 18 Nov 2019 9:30
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N110619W.M
Title : SW846 8260
Last Update : Thu Nov 07 04:00:41 2019

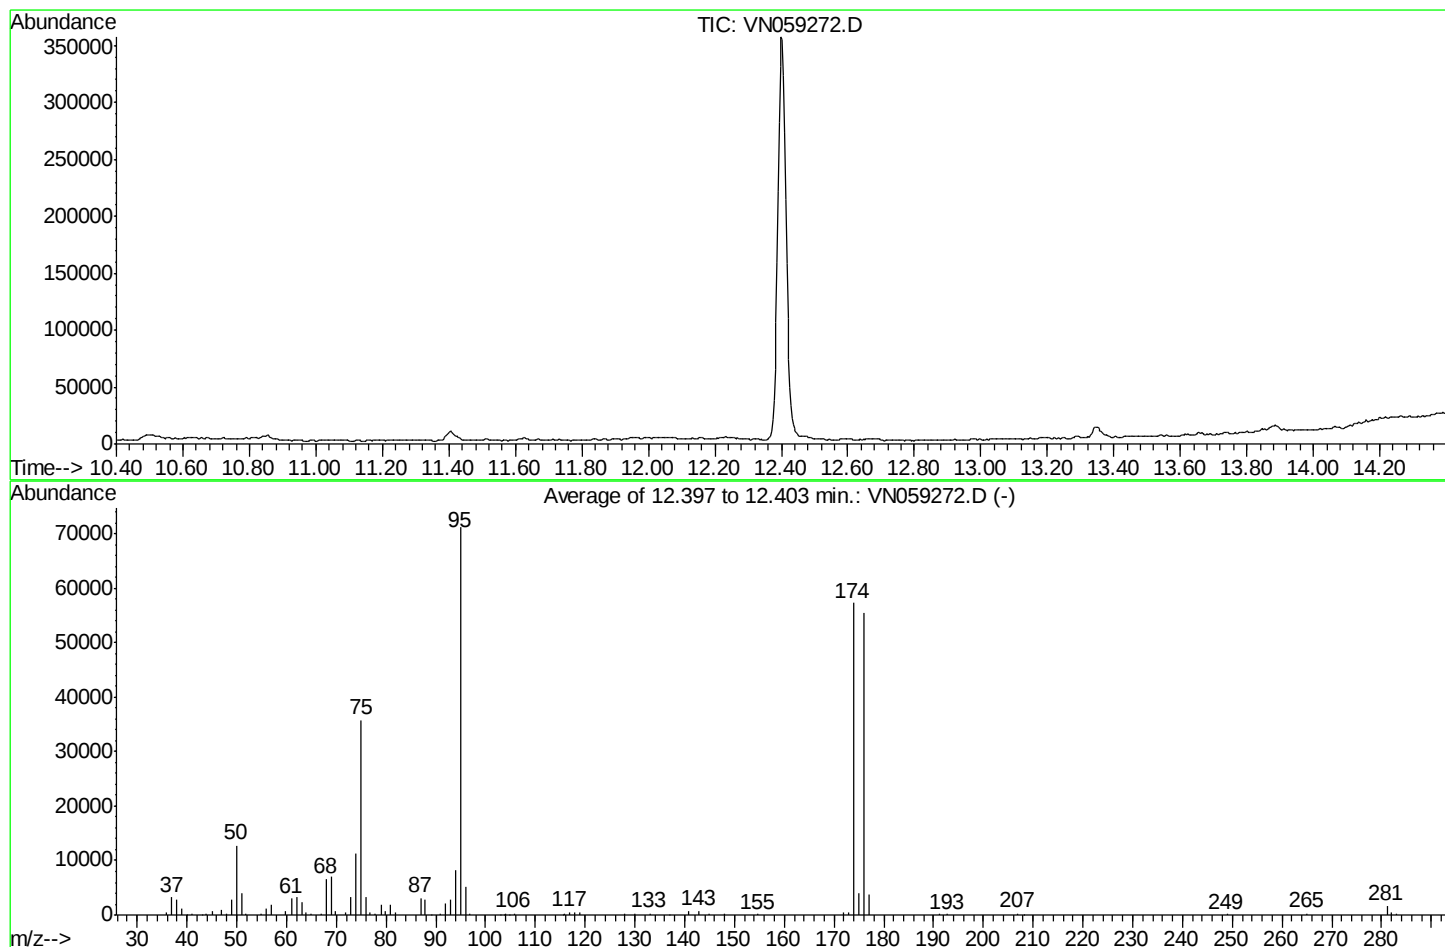

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	12805	PASS
75	95	30	60	50.3	35850	PASS
95	95	100	100	100.0	71205	PASS
96	95	5	9	7.3	5191	PASS
173	174	0.00	2	1.0	593	PASS
174	95	50	100	80.5	57336	PASS
175	174	5	9	7.0	4031	PASS
176	174	95	101	96.7	55456	PASS
177	176	5	9	6.8	3791	PASS