




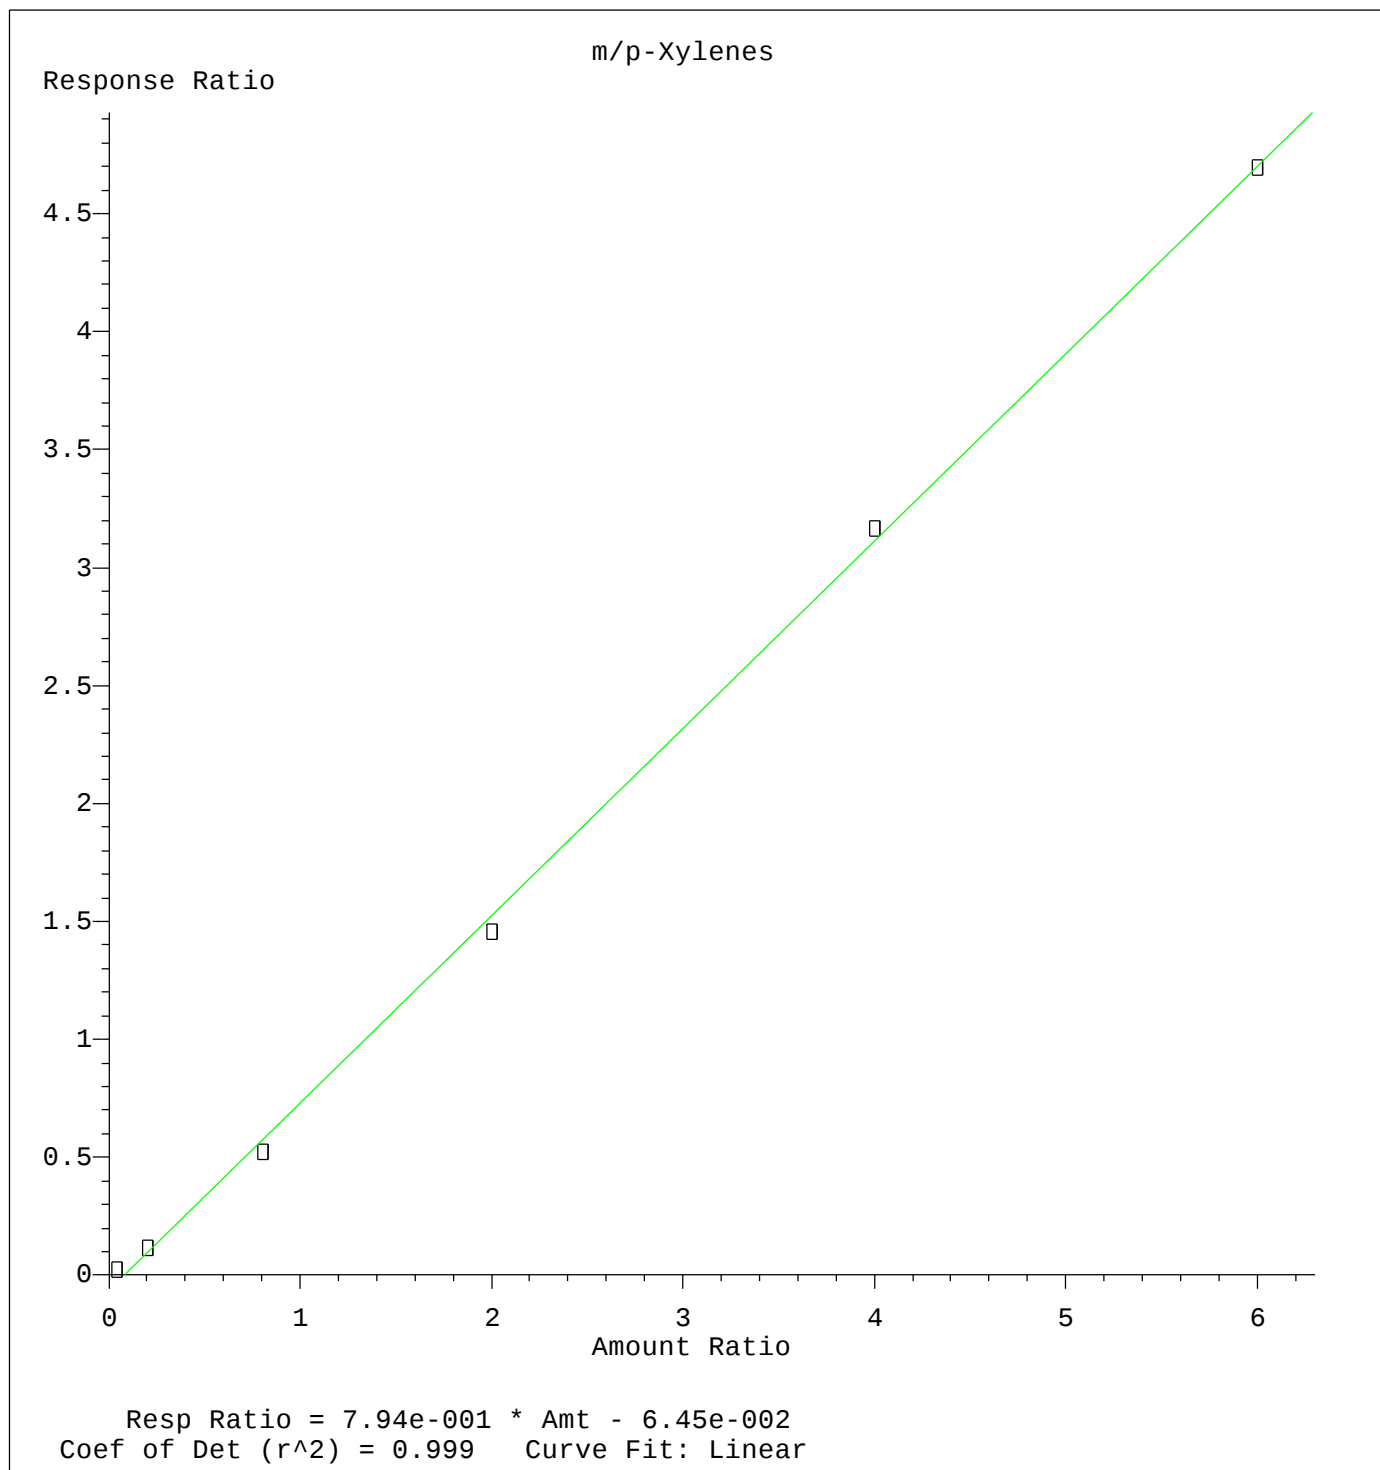

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020

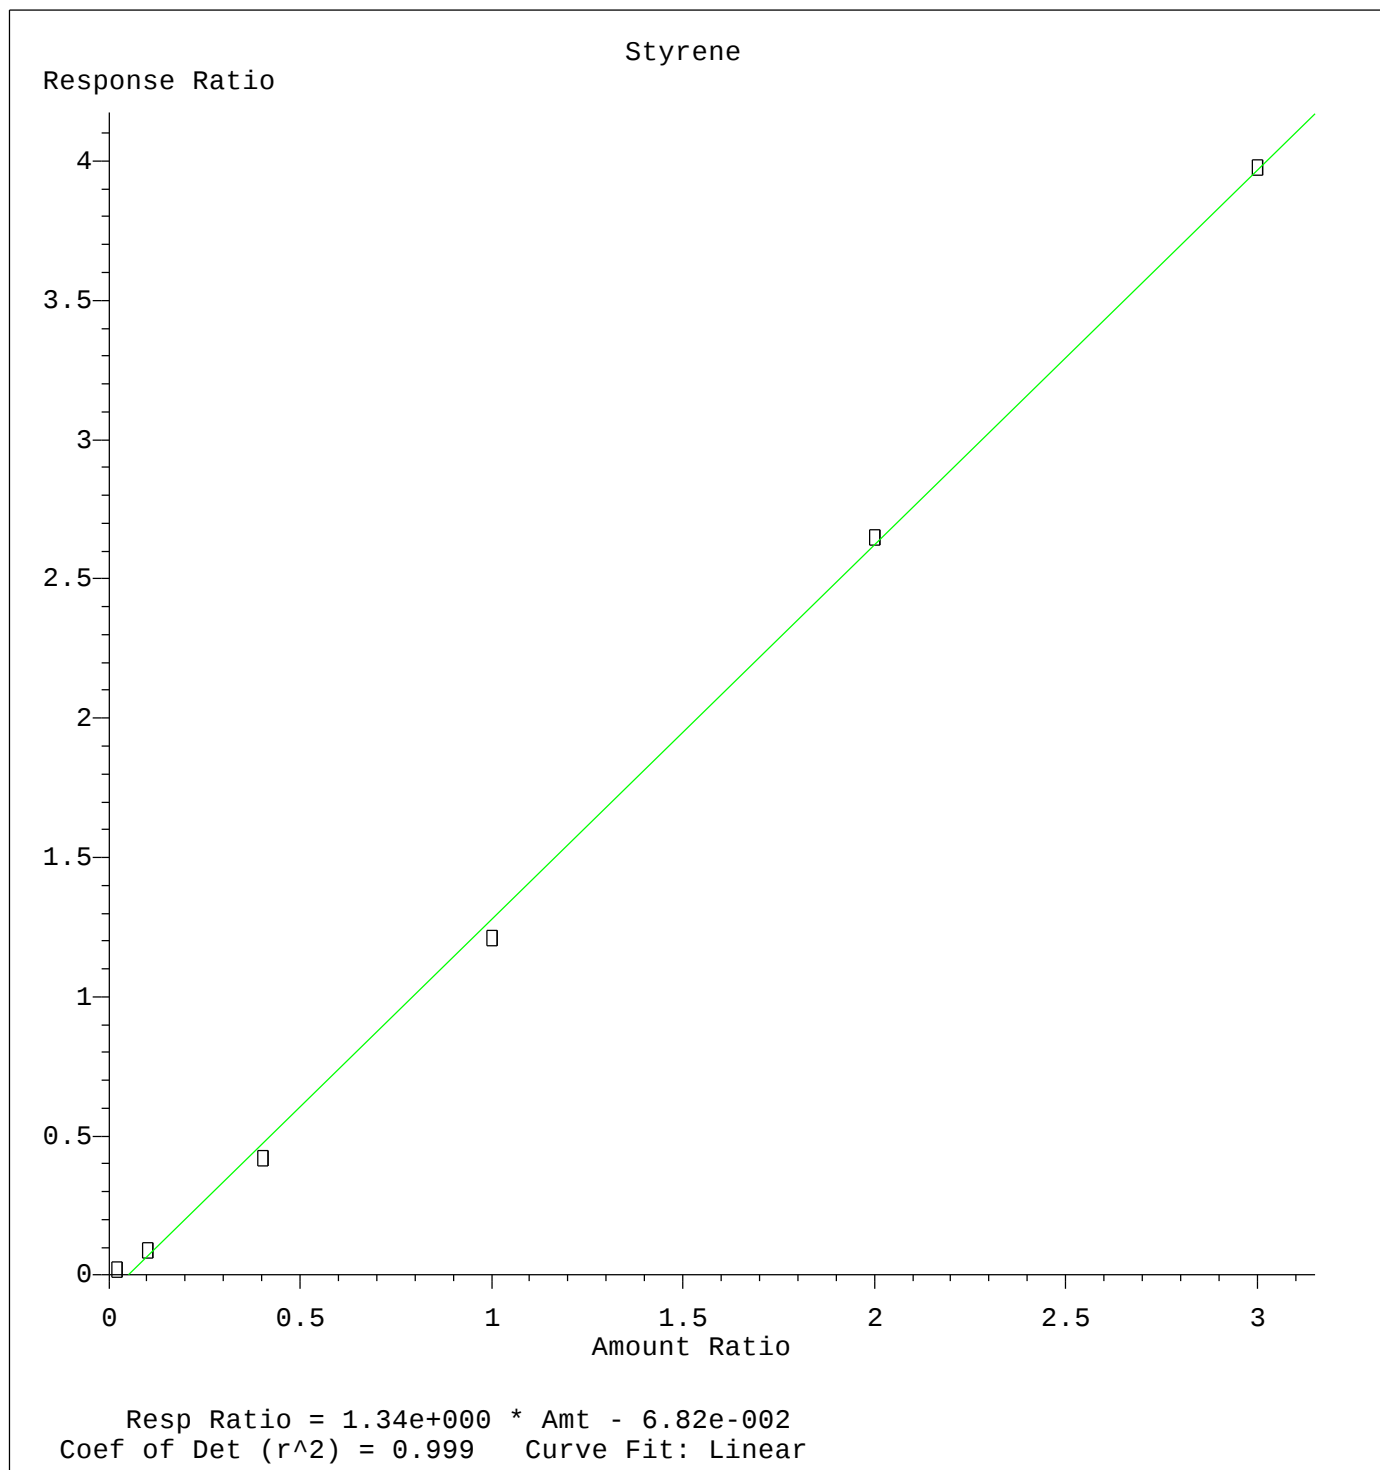


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020

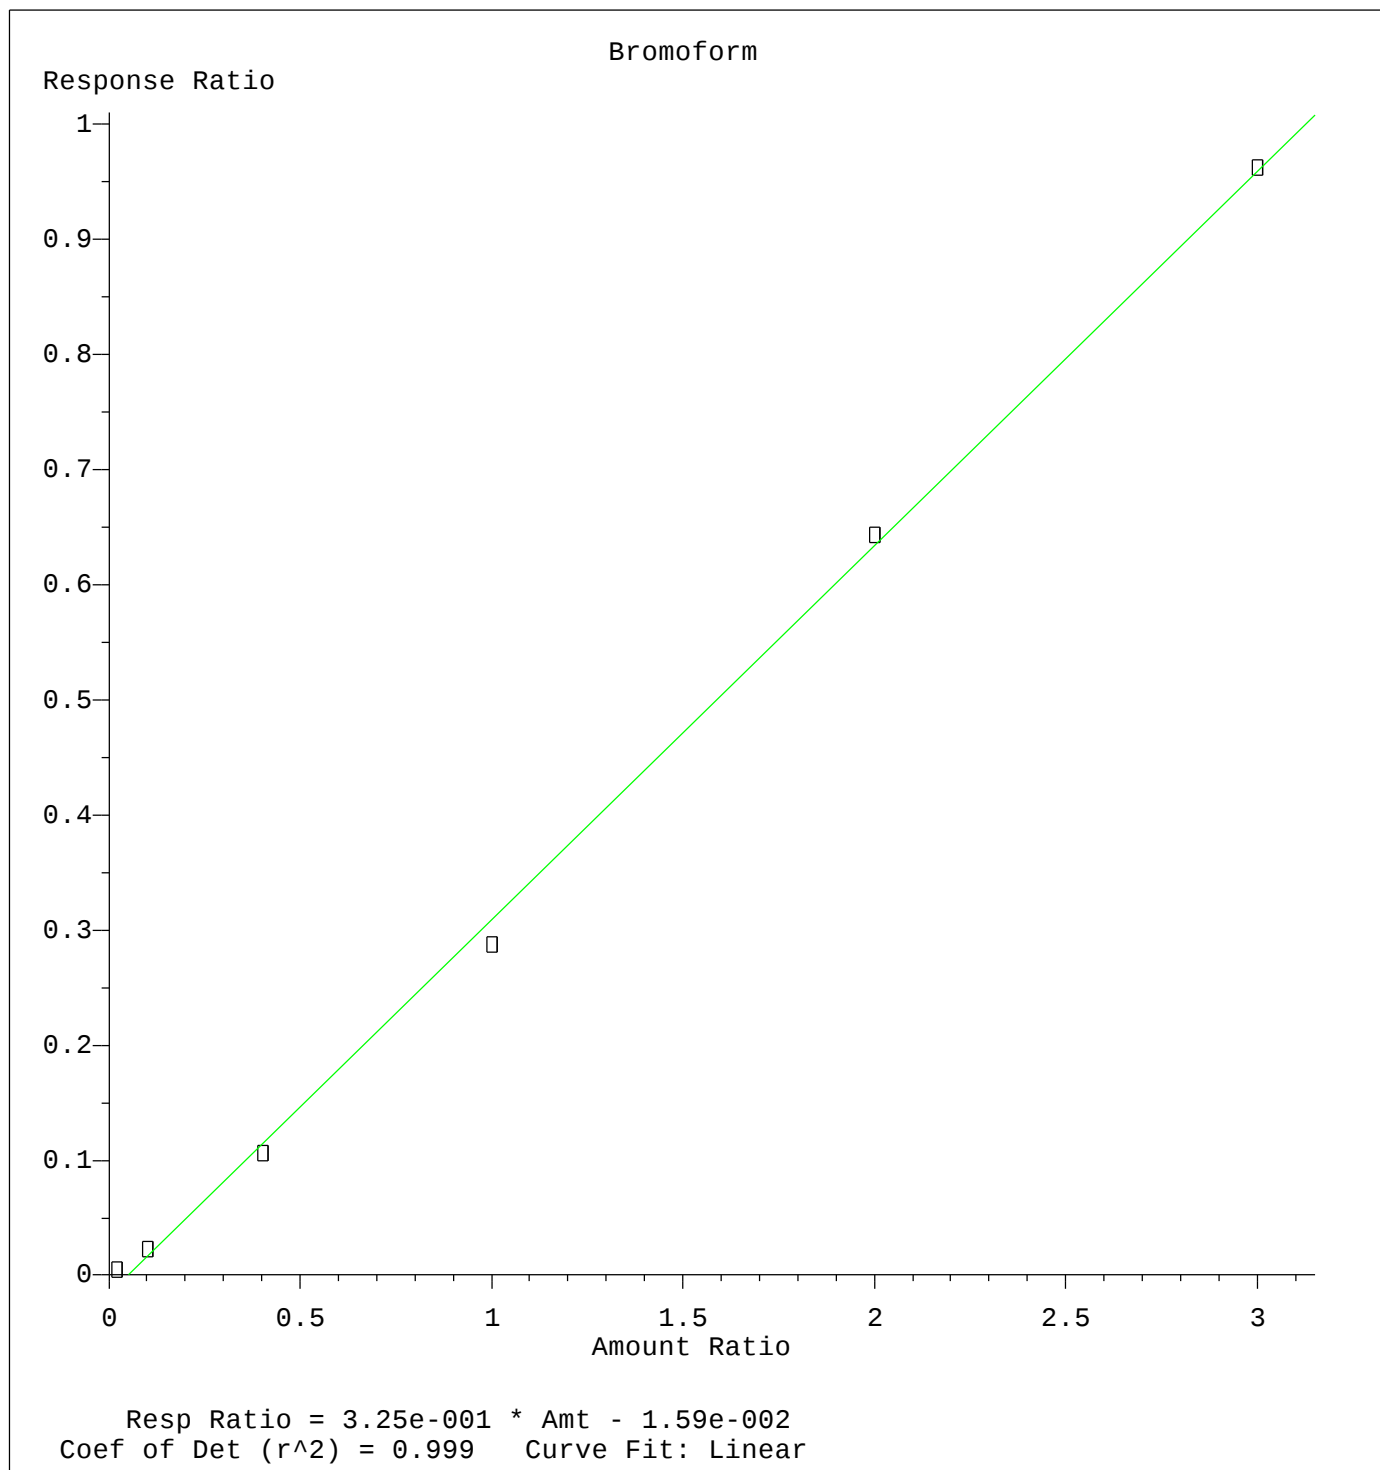

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020

trans-1,4-Dichloro-2-butene

Response Ratio

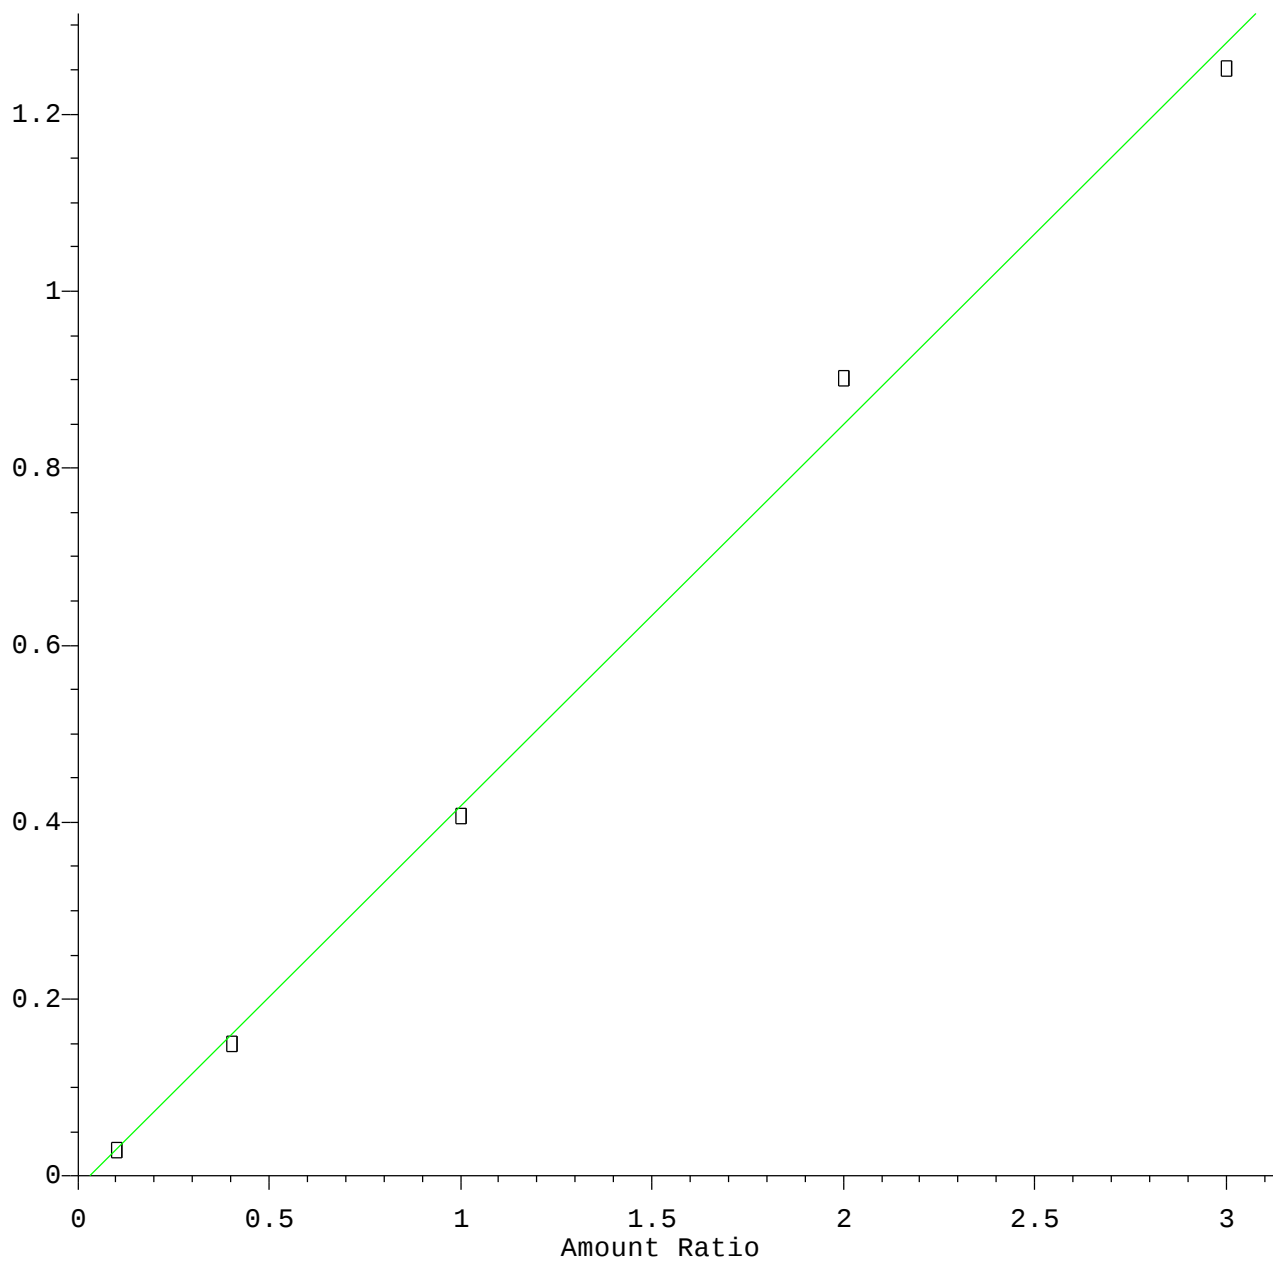


Resp Ratio = $4.31 \times 10^{-1} \times \text{Amt} - 1.32 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020


1,2,4-Trichlorobenzene

Response Ratio

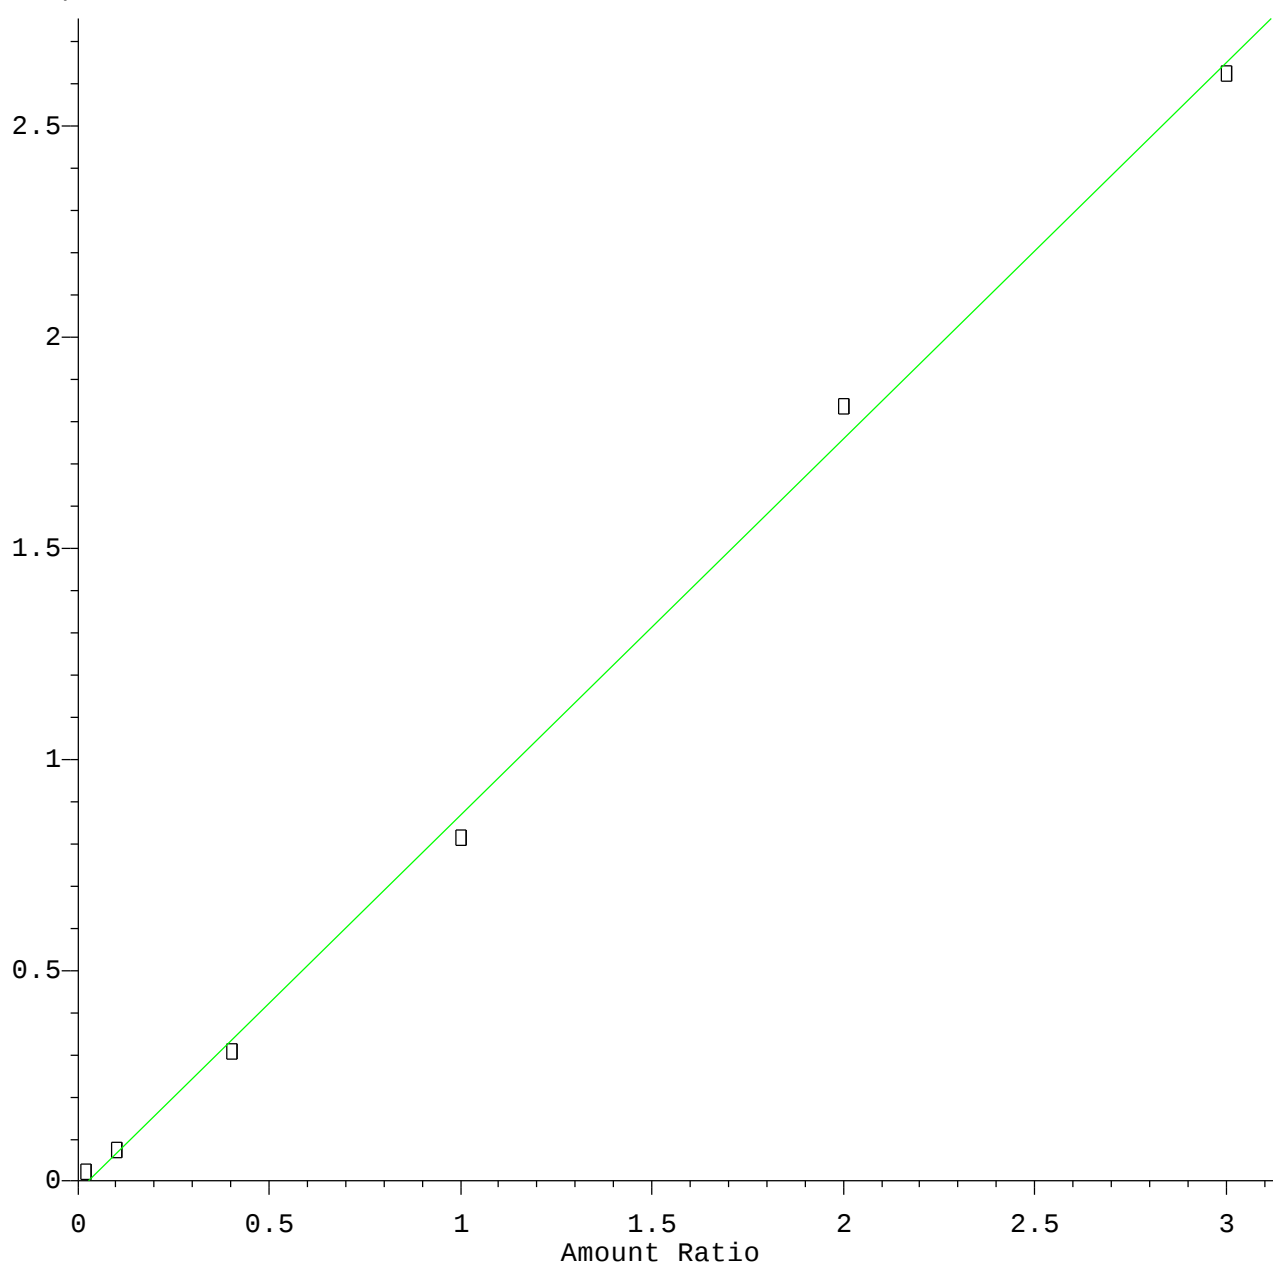

Resp Ratio = 8.91×10^{-1} * Amt - 2.37×10^{-2}
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020

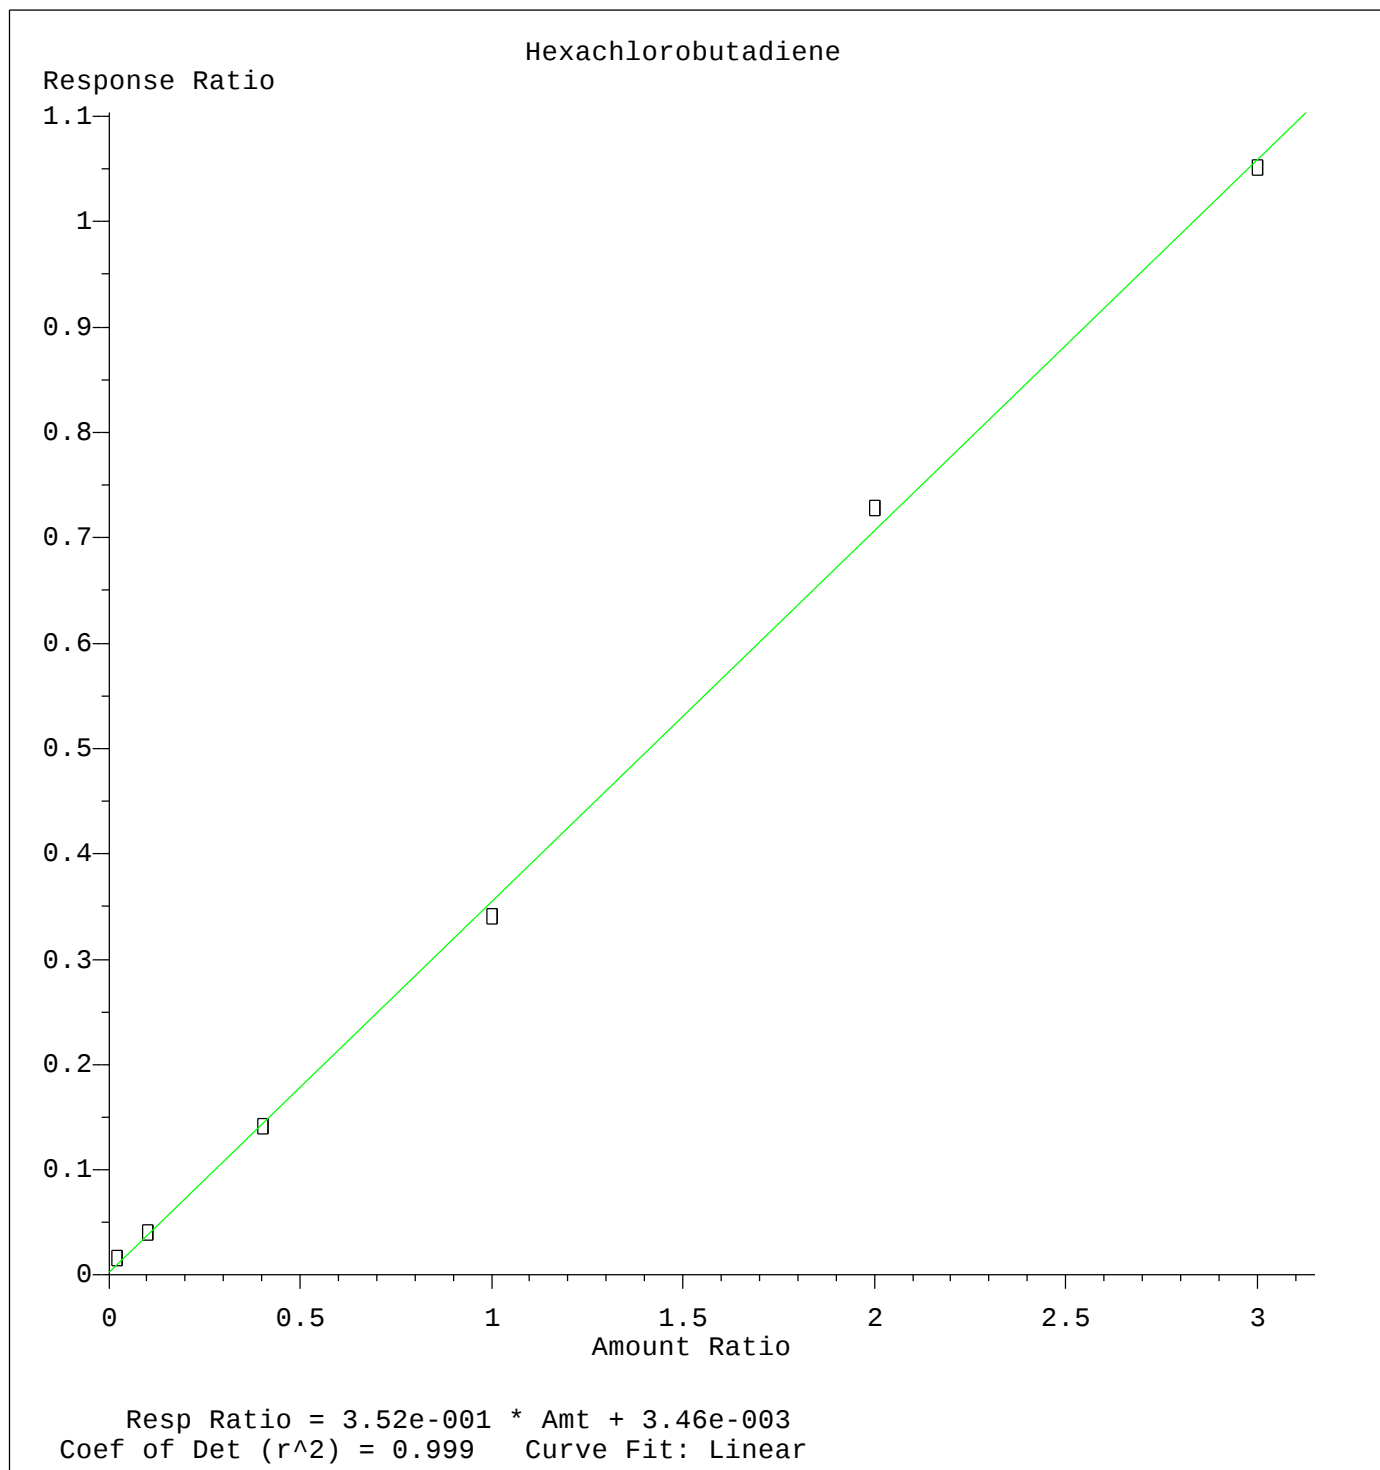

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020


1,2,3-Trichlorobenzene

Response Ratio

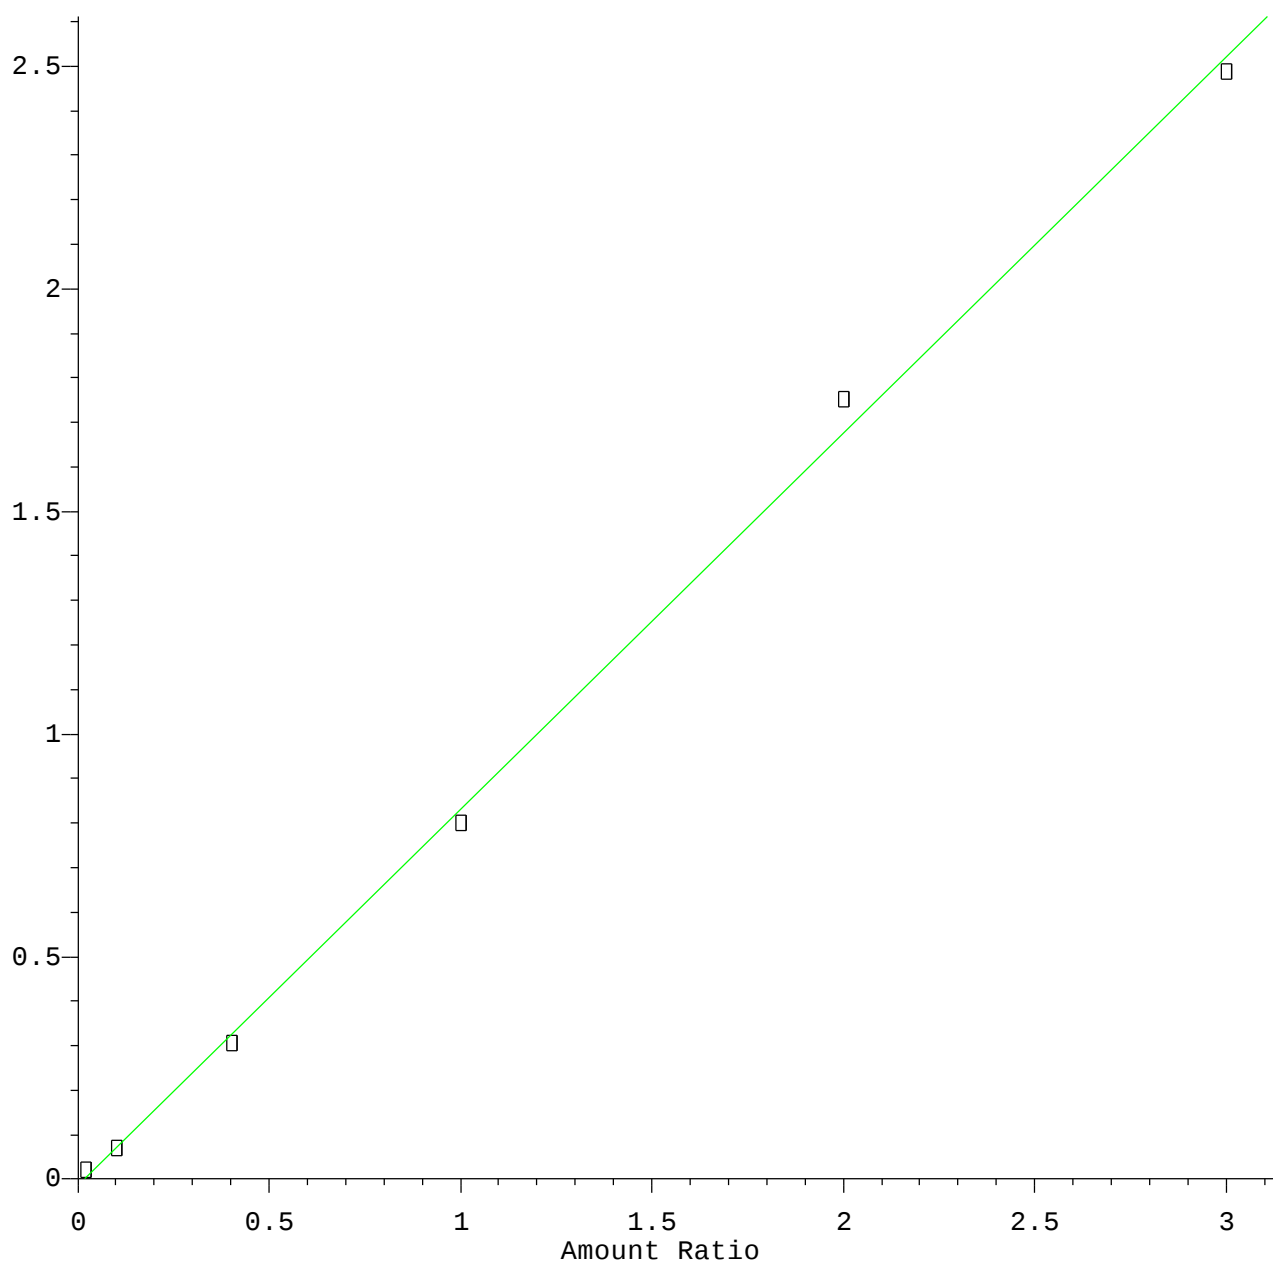


Resp Ratio = $8.45 \times 10^{-1} \times \text{Amt} - 1.28 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020

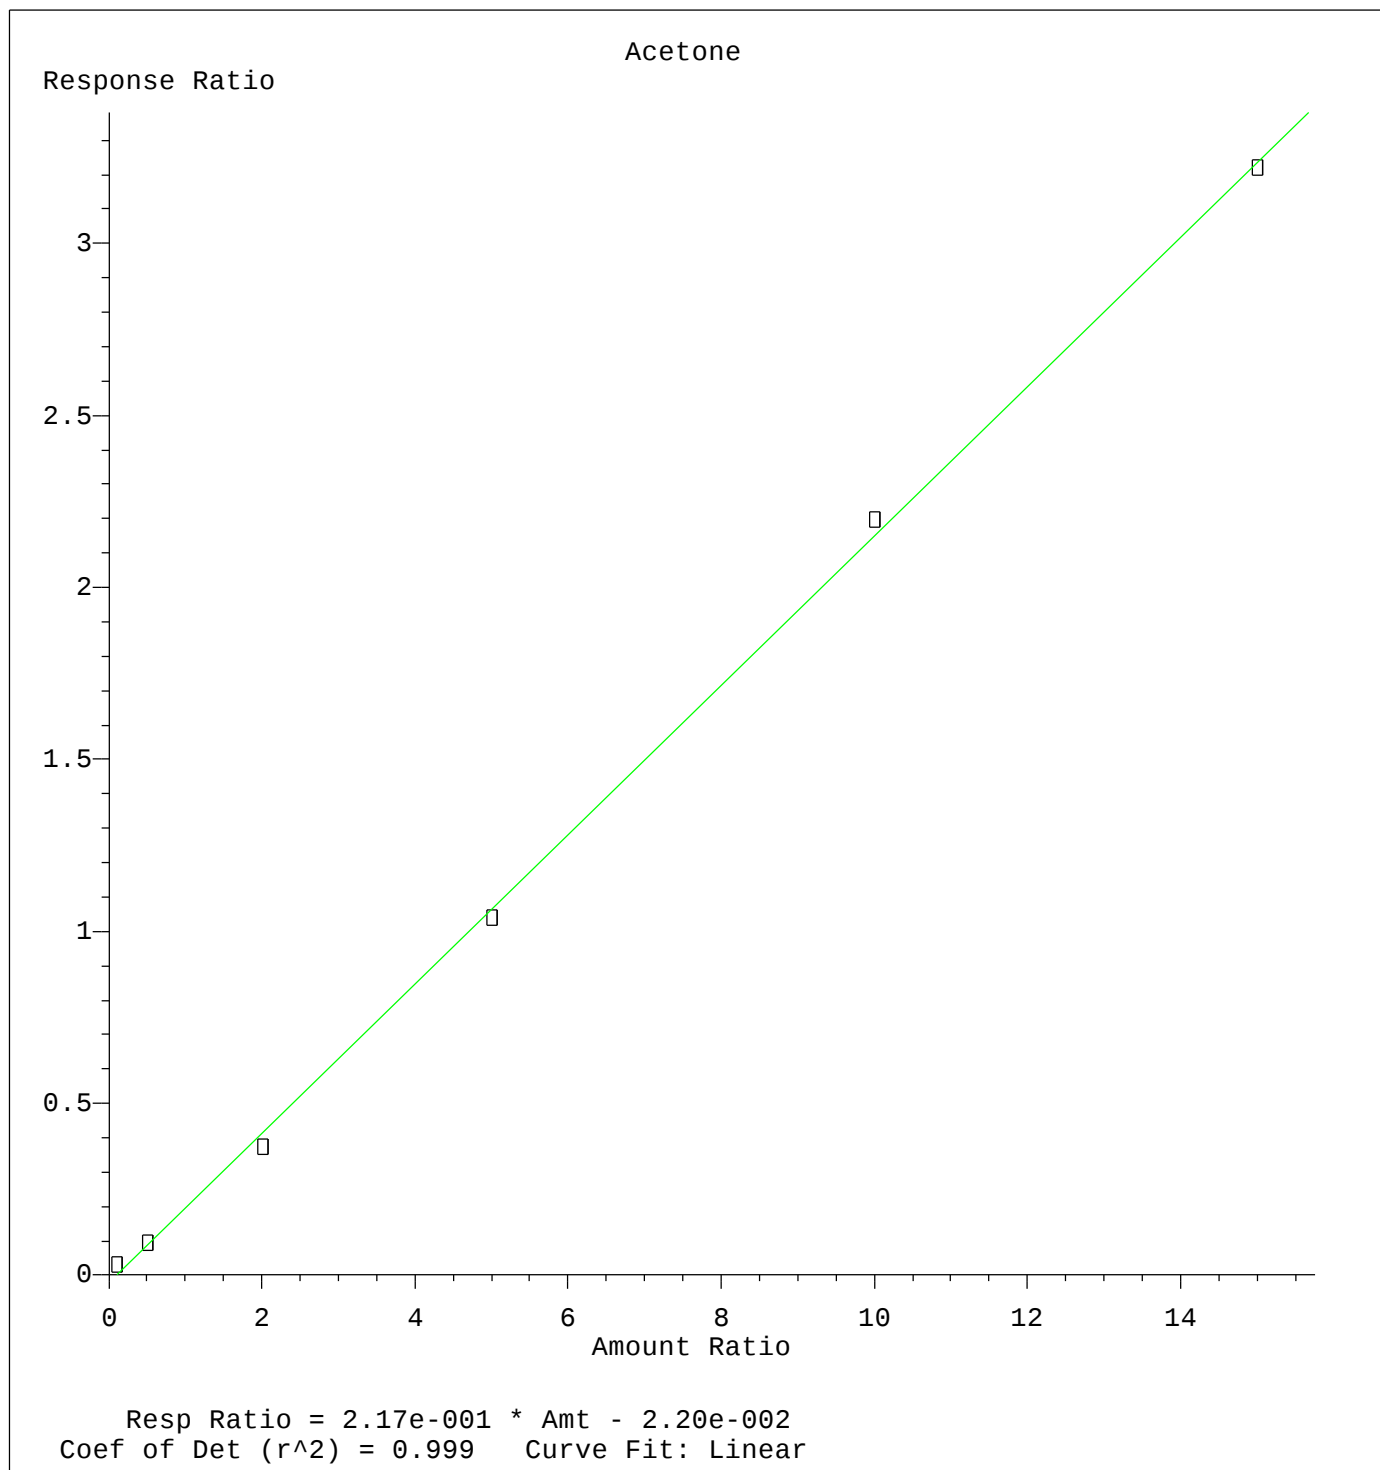

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020

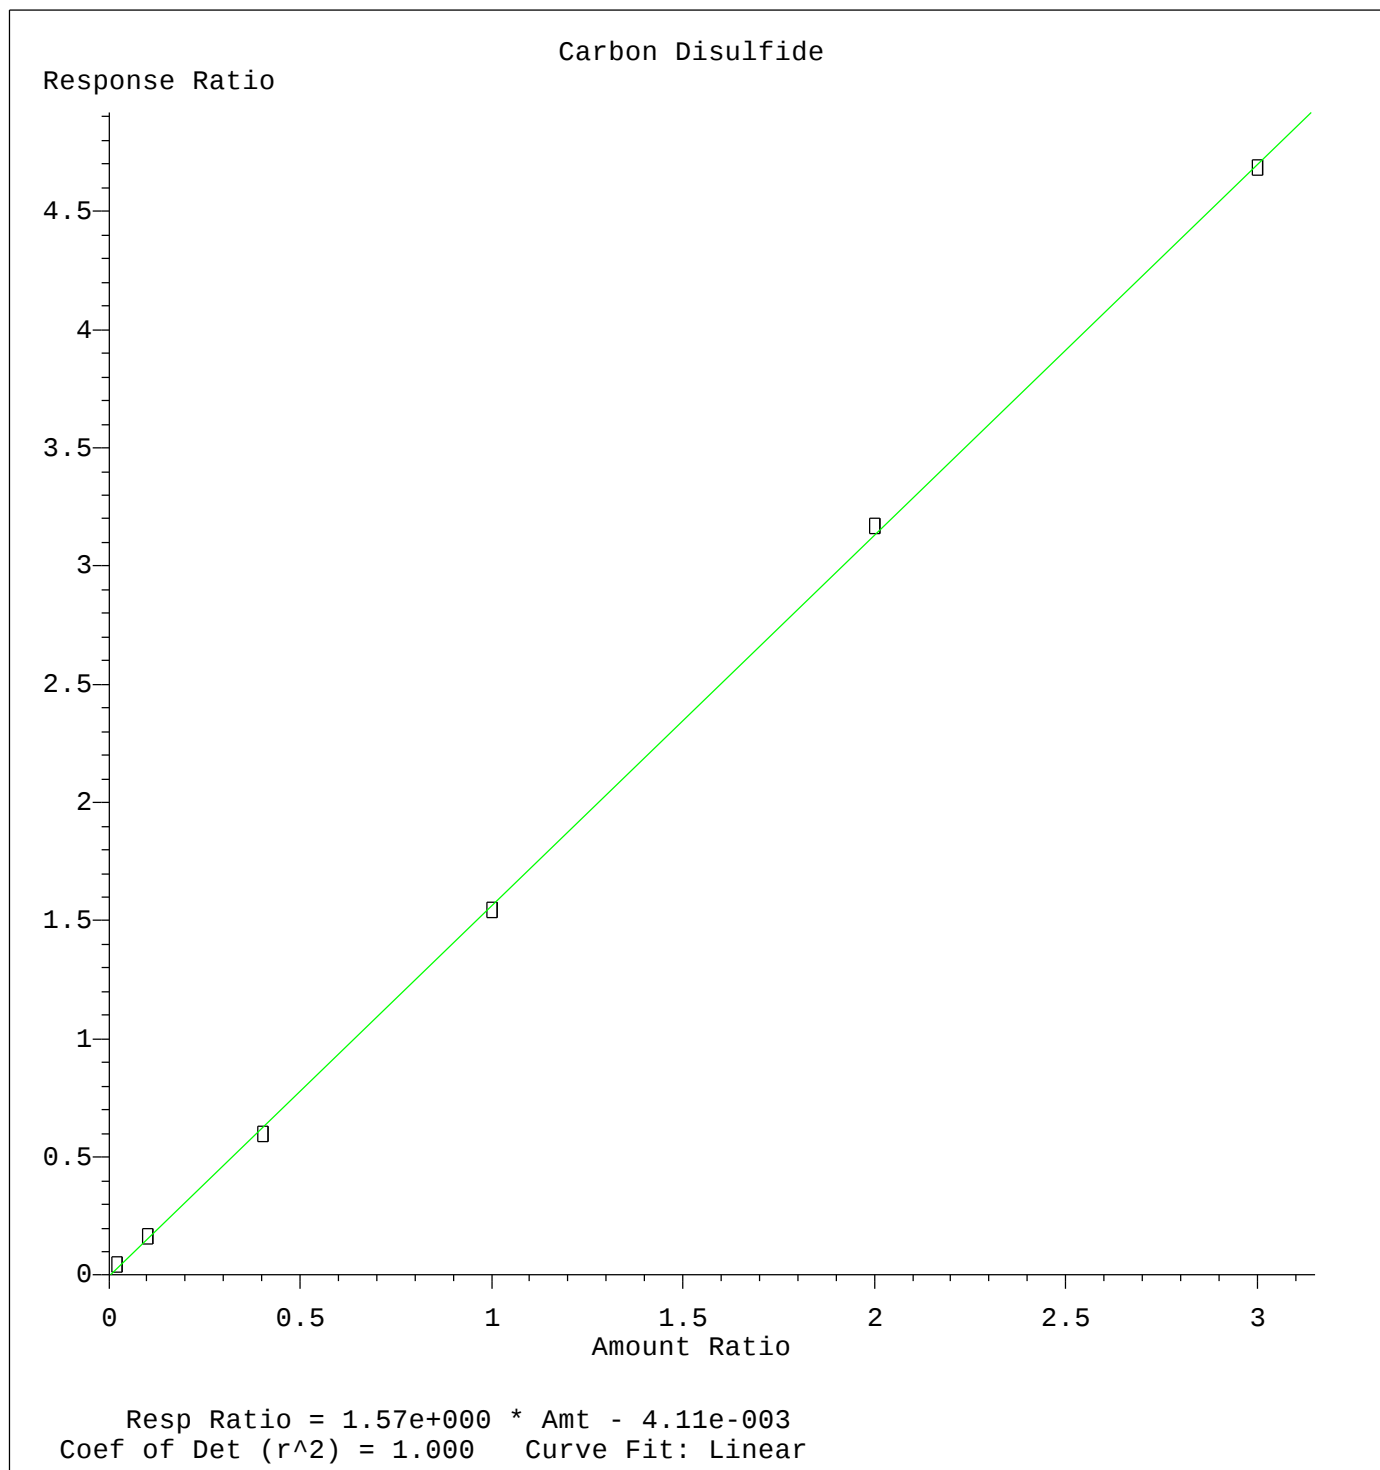


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020

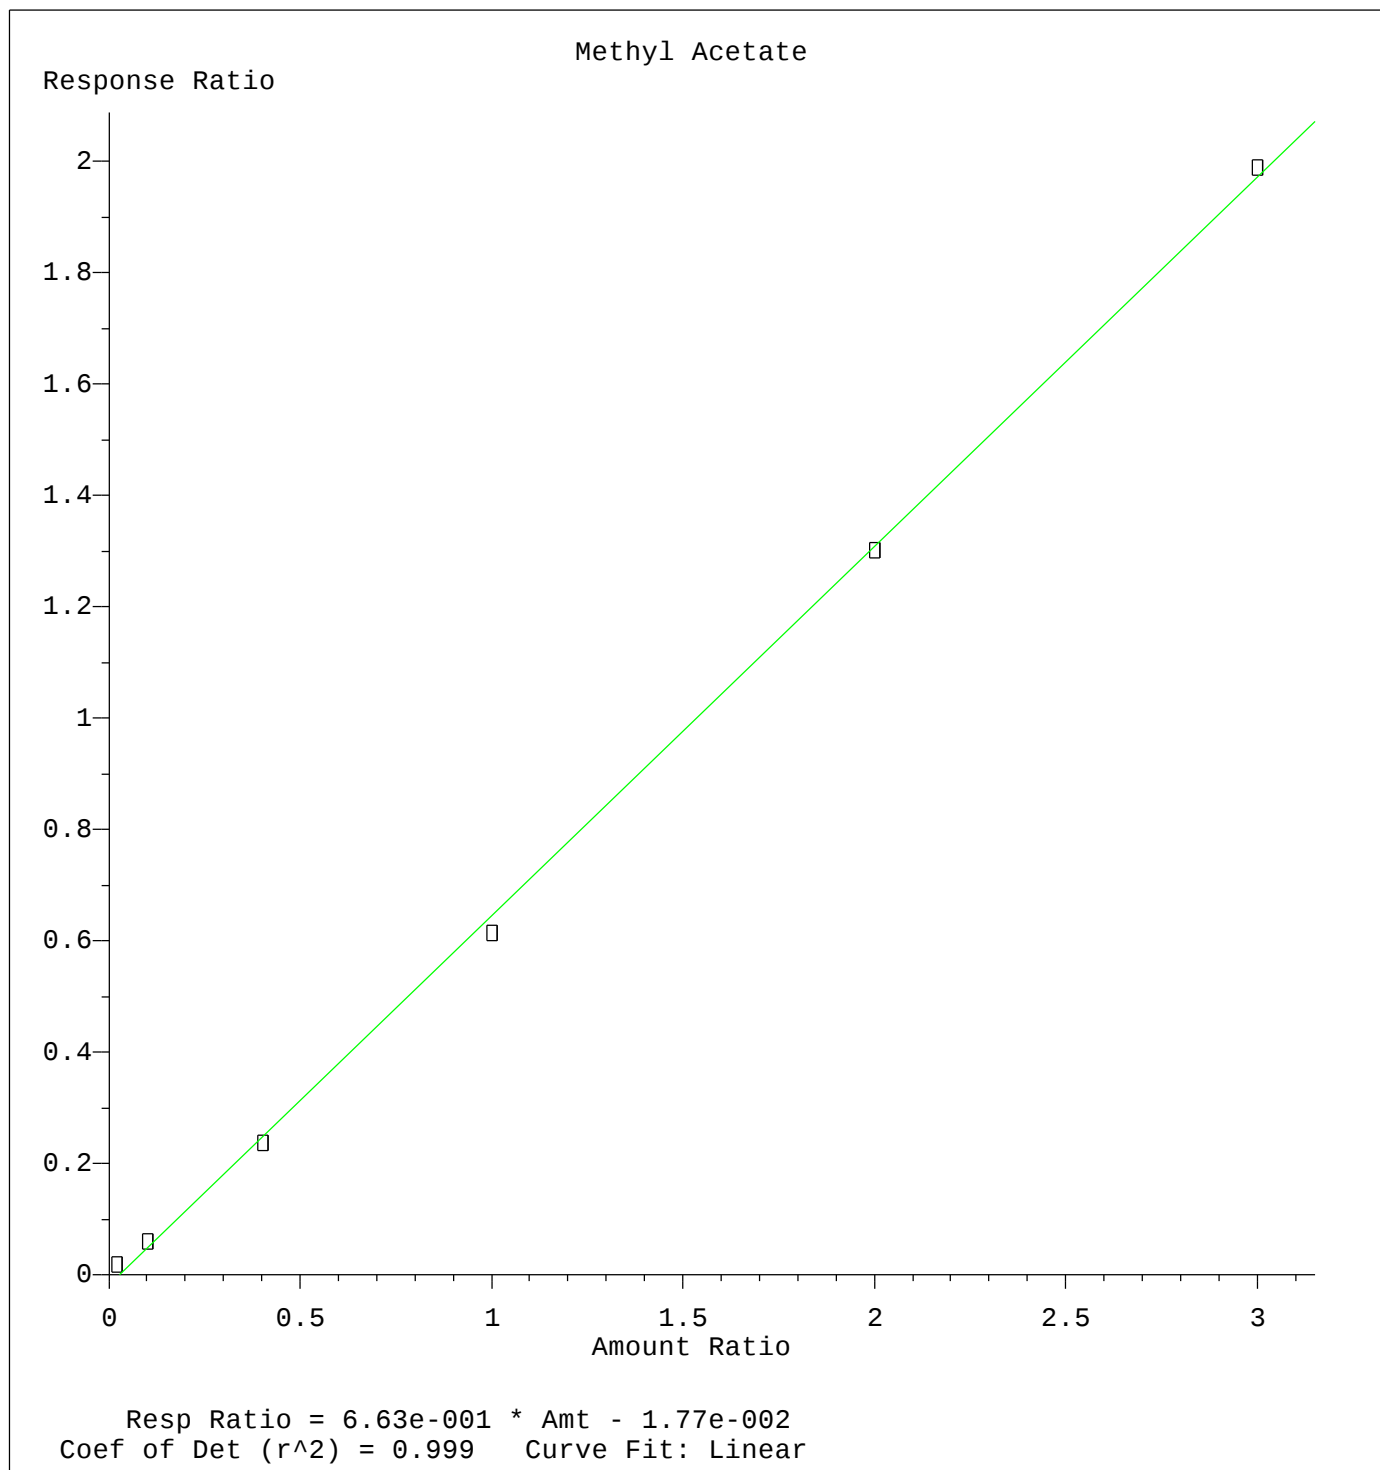

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020


4-Methyl-2-Pentanone

Response Ratio

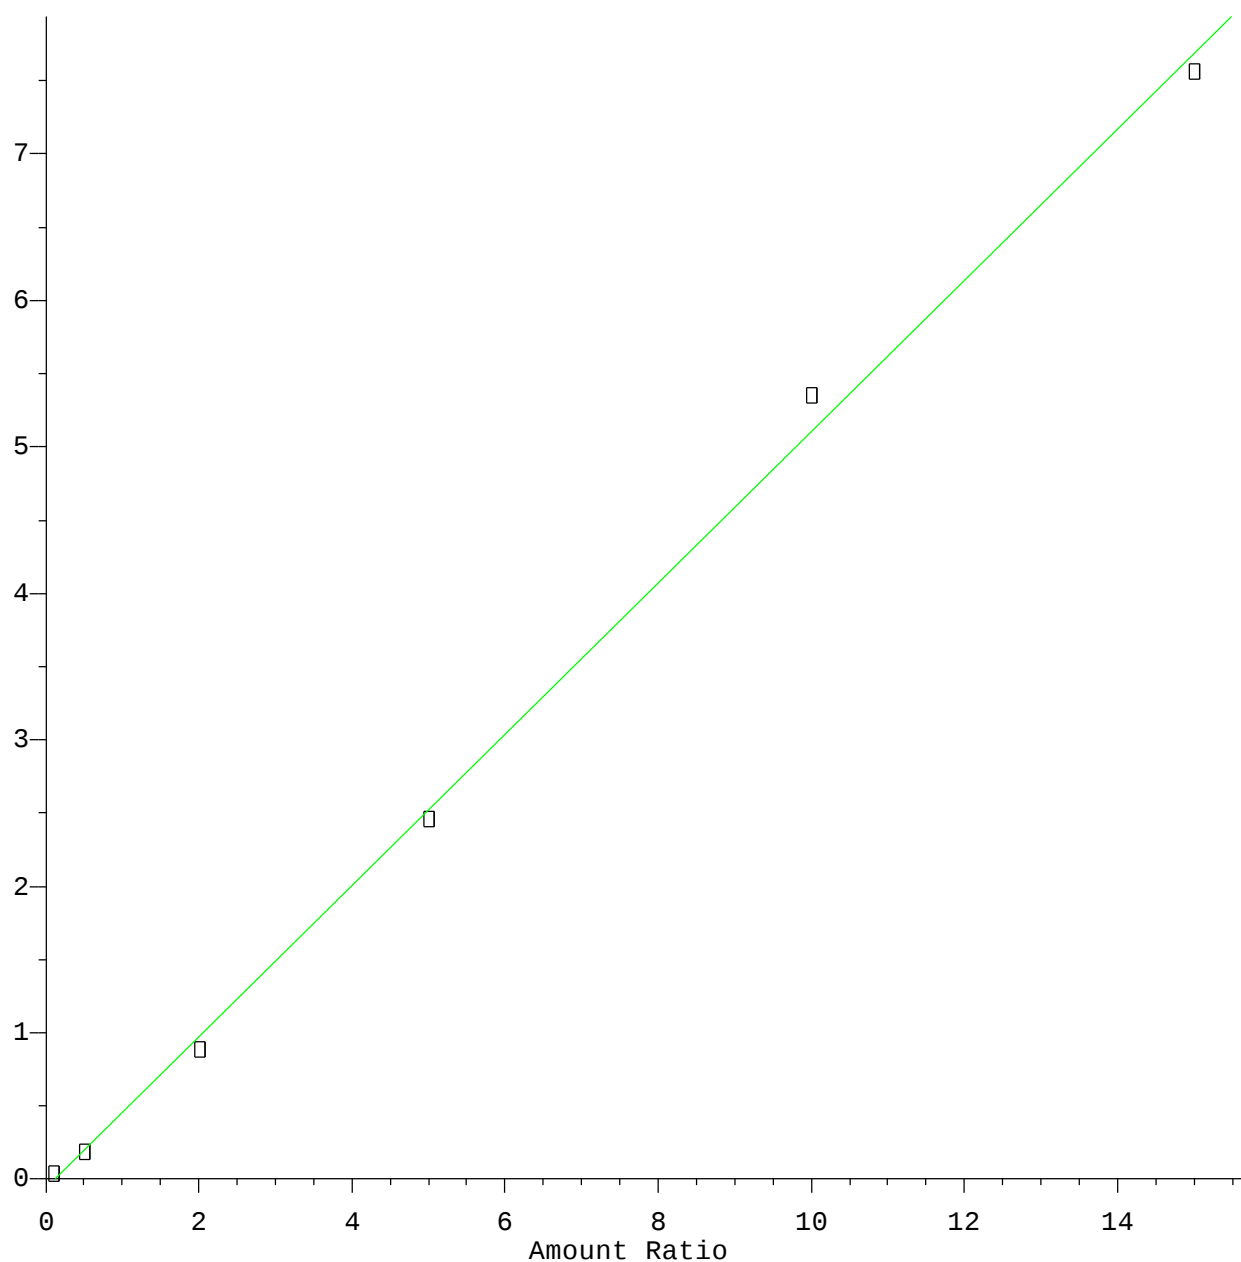

Resp Ratio = $5.17 \times 10^{-1} \times \text{Amt} - 6.33 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020

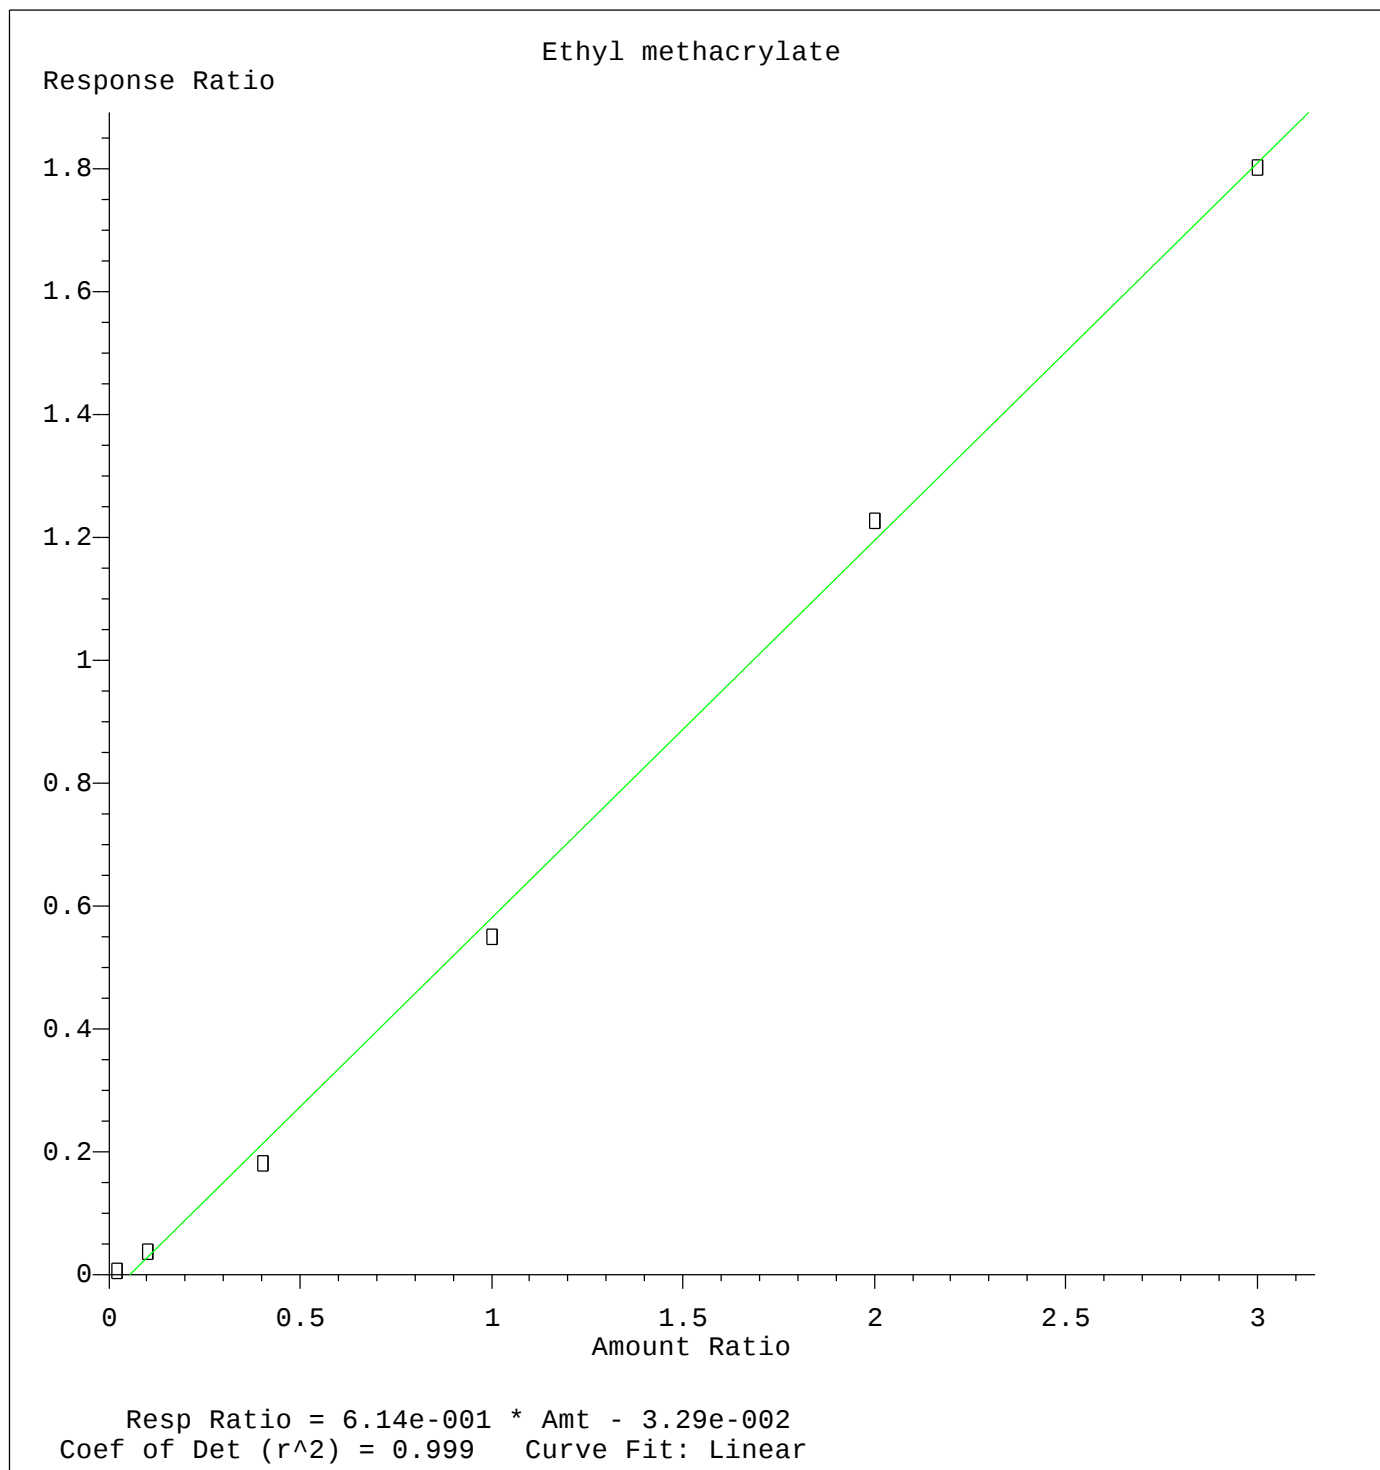

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020

2-Chloroethyl Vinyl ether

Response Ratio

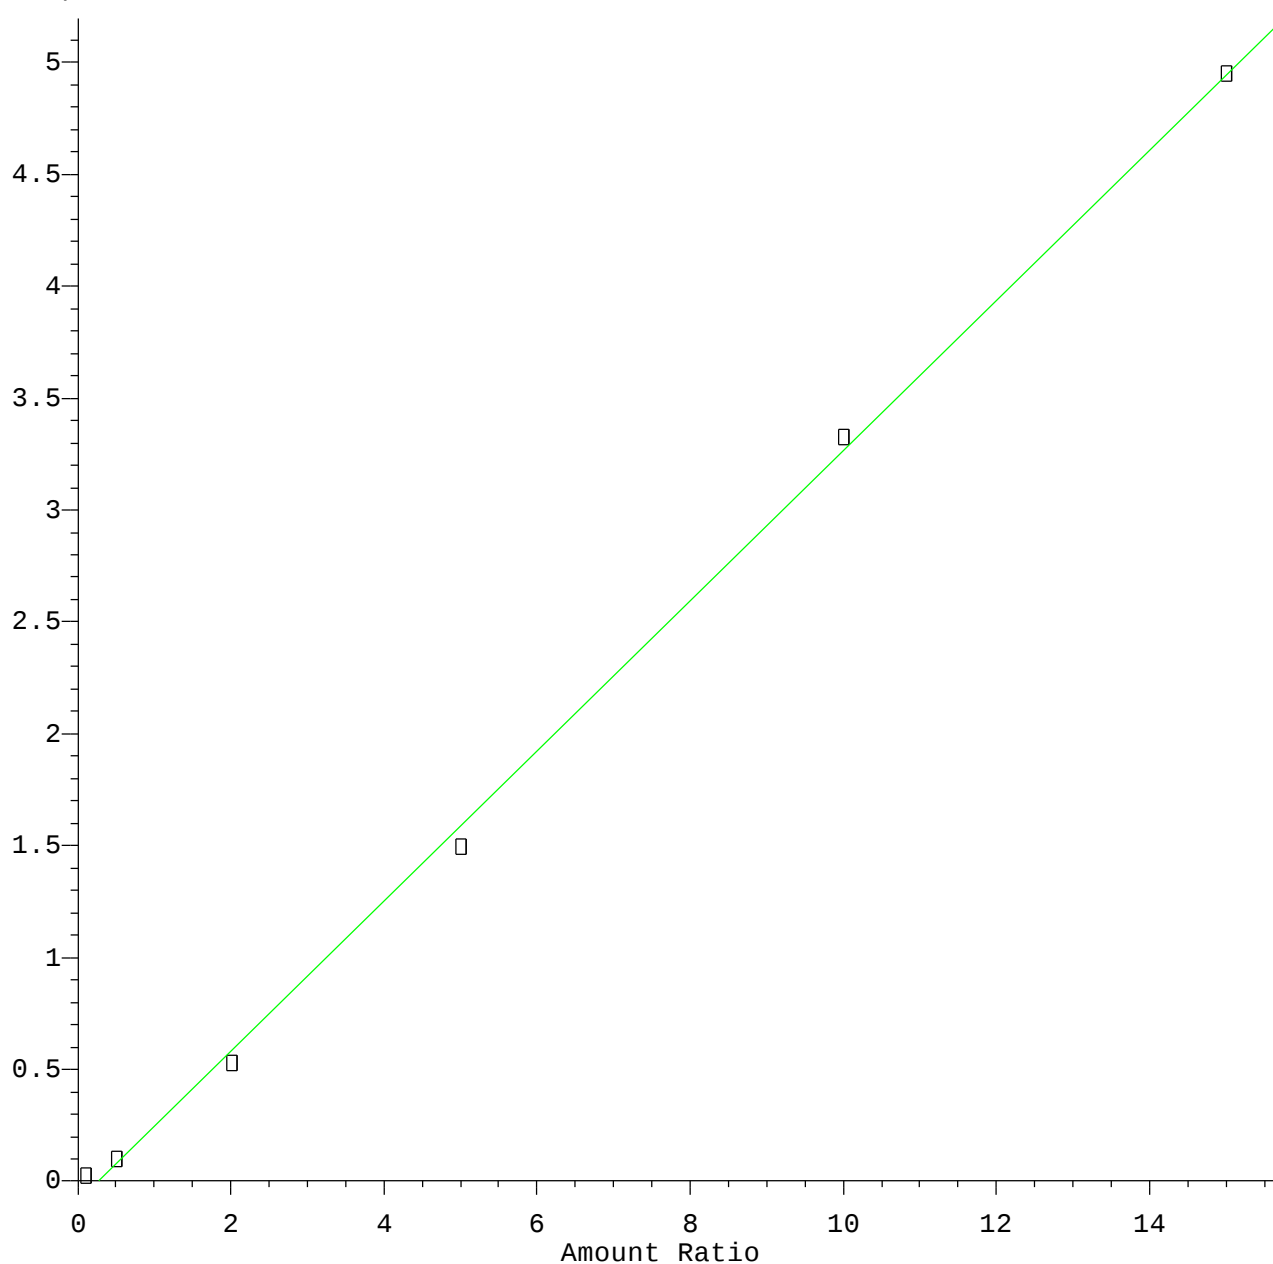


Resp Ratio = $3.36 \times 10^{-1} \times \text{Amt} - 8.91 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020

2-Hexanone

Response Ratio

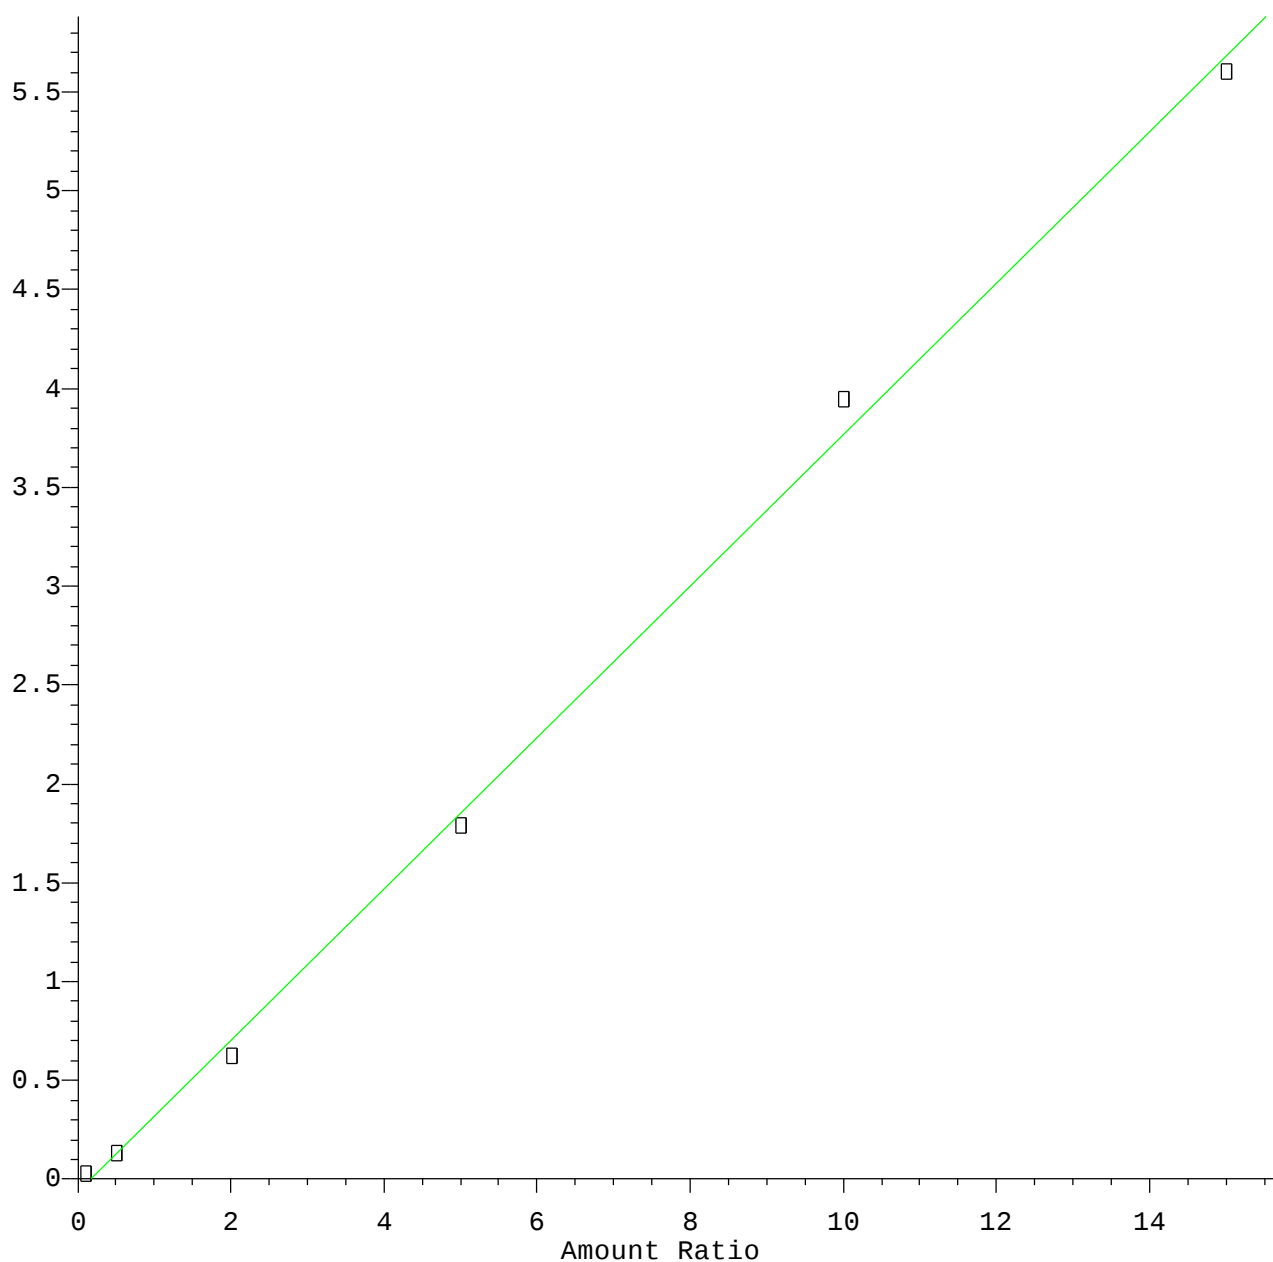

Resp Ratio = $3.83 \times 10^{-1} \times \text{Amt} - 6.47 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Calibration Table Last Updated: Wed Nov 18 15:29:54 2020