

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111821\
 Data File : VN069544.D
 Acq On : 18 Nov 2021 10:35
 Operator : JC/MD
 Sample : VN1118MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :


Quant Time: Nov 19 03:16:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 09 18:18:22 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	1365437	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2355150	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	2292816	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	833482	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	992229	50.117	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 100.240%			
35) Dibromofluoromethane	8.024	113	686633	48.611	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 97.220%			
50) Toluene-d8	10.443	98	2963175	53.339	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 106.680%			
62) 4-Bromofluorobenzene	12.734	95	1018850	49.923	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 99.840%			
Target Compounds			Qvalue			
13) Acrolein	4.047	56	998	Below Cal #	62	
15) Acrylonitrile	5.557	53	2835	0.310 ug/l #	32	
16) Acetone	4.301	43	10515	0.984 ug/l	98	
29) Tetrahydrofuran	7.702	42	1889	0.213 ug/l #	43	
31) Cyclohexane	8.088	56	34970	1.293 ug/l #	29	
36) 1,1-Dichloropropene	8.086	75	116779	5.893 ug/l #	49	
38) Carbon Tetrachloride	8.088	117	141242	7.382 ug/l #	16	
49) 1,4-Dioxane	9.569	88	455	40.149 ug/l #	68	
51) 4-Methyl-2-Pentanone	10.341	43	9414	0.339 ug/l	93	
53) t-1,3-Dichloropropene	10.714	75	235	2.646 ug/l	94	
54) cis-1,3-Dichloropropene	10.191	75	180	1.739 ug/l #	41	
56) Ethyl methacrylate	10.765	69	1624	2.107 ug/l #	73	
58) 2-Chloroethyl Vinyl ether	9.893	63	54	22.777 ug/l #	45	
59) 2-Hexanone	11.089	43	19851	8.761 ug/l	89	
60) Dibromochloromethane	11.242	129	188	2.428 ug/l	68	
61) 1,2-Dibromoethane	11.339	107	154	1.080 ug/l #	25	
70) Styrene	12.294	104	1589	1.550 ug/l #	67	
71) Bromoform	12.465	173	53	3.432 ug/l #	29	
74) N-amyl acetate	12.398	43	10226	0.364 ug/l #	89	
76) 1,2,3-Trichloropropane	12.734	75	570844	29.678 ug/l #	1	
81) trans-1,4-Dichloro-2-b...	12.734	75	570844	83.903 ug/l #	5	
87) 1,3-Dichlorobenzene	13.627	146	5346	0.203 ug/l	96	
88) 1,4-Dichlorobenzene	13.627	146	5346	0.207 ug/l	96	
89) n-Butylbenzene	13.943	91	12300	0.283 ug/l	97	
90) Hexachloroethane	14.209	117	62	2.168 ug/l #	6	
91) 1,2-Dichlorobenzene	13.991	146	5742	0.229 ug/l	88	
92) 1,2-Dibromo-3-Chloropr...	14.600	75	1122	2.057 ug/l #	12	
93) 1,2,4-Trichlorobenzene	15.263	180	10185	3.841 ug/l	96	
95) Naphthalene	15.509	128	43259	5.516 ug/l	98	
96) 1,2,3-Trichlorobenzene	15.708	180	13065	4.145 ug/l	96	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Nov 19 03:16:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 09 18:18:22 2021
Response via : Initial Calibration




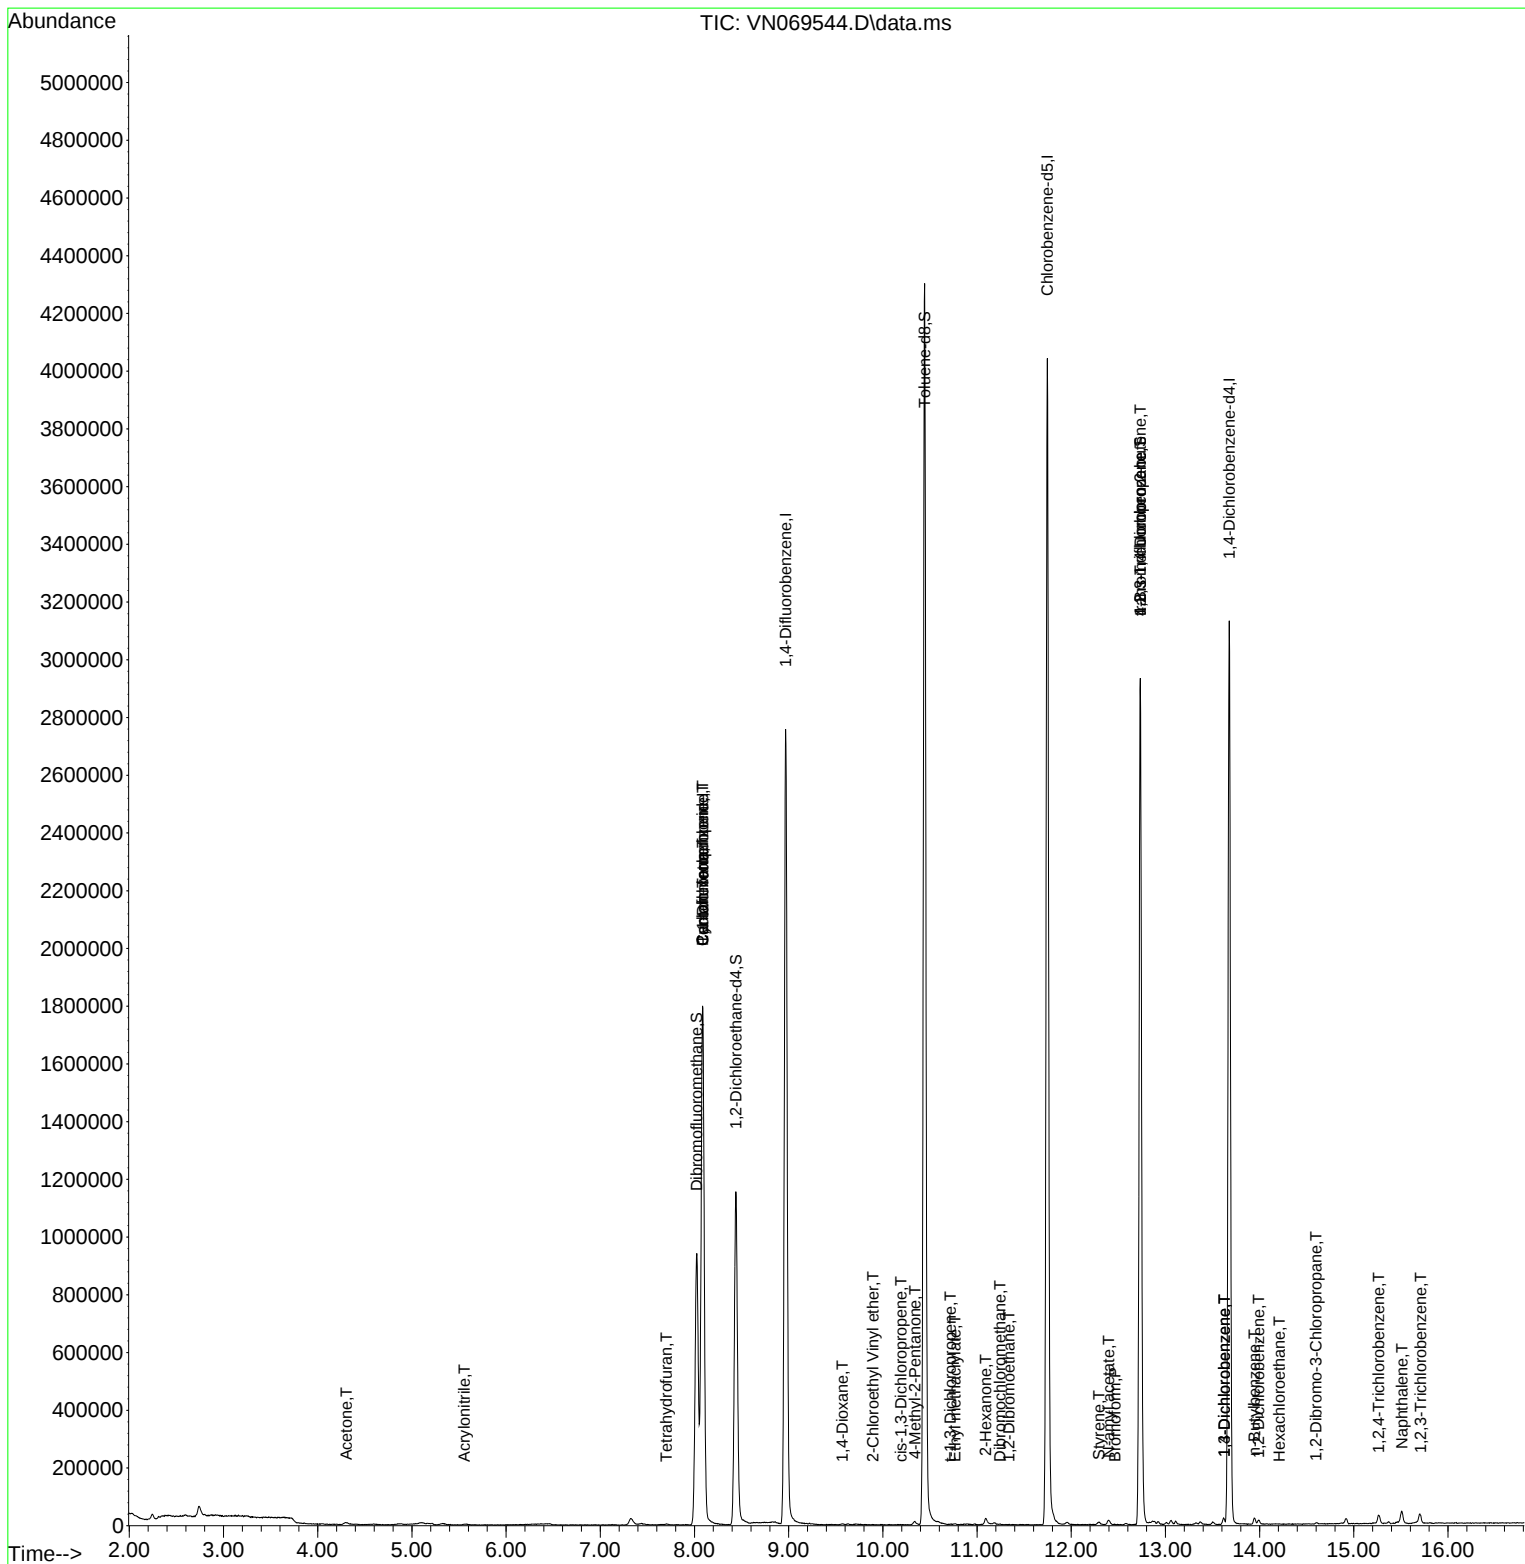




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 1365437
Ion Ratio Lower Upper
168 100
99 60.4 41.3 61.9

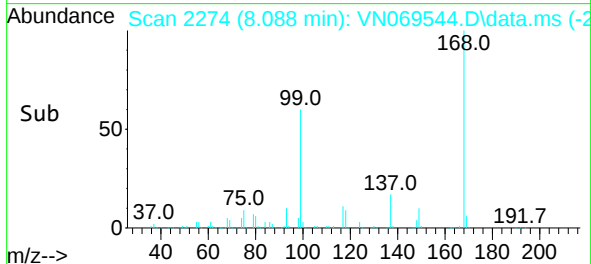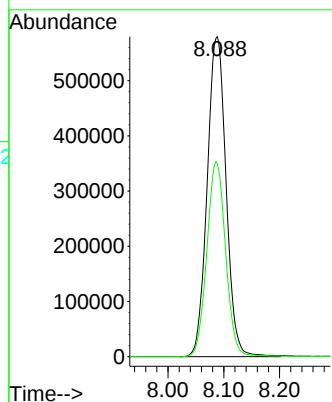

#13
Acrolein
Concen: Below Cal
RT: 4.047 min Scan# 767
Delta R.T. 0.006 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

Tgt Ion: 56 Resp: 998
Ion Ratio Lower Upper
56 100
55 39.4 56.6 85.0#


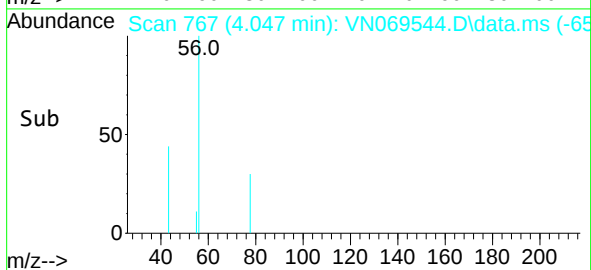
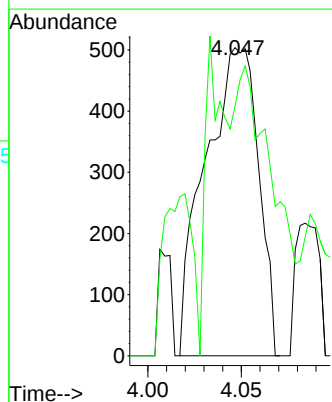
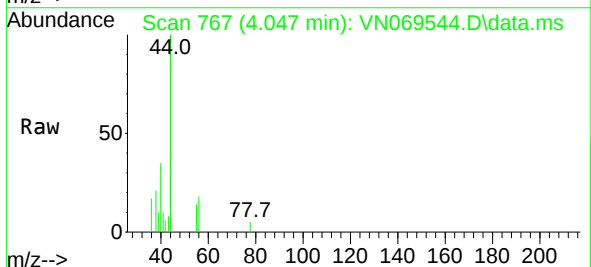


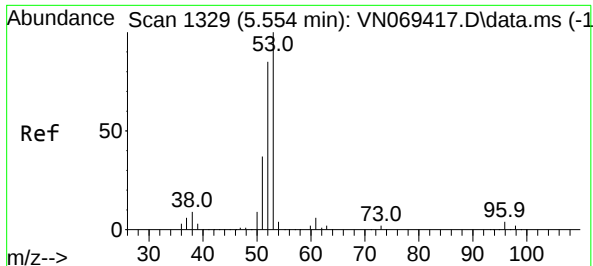

#15
Acrylonitrile
Concen: 0.310 ug/l
RT: 5.557 min Scan# 11
Delta R.T. 0.003 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 53 Resp: 2835
Ion Ratio Lower Upper
53 100
52 8.5 66.2 99.2#
51 15.9 29.6 44.4#

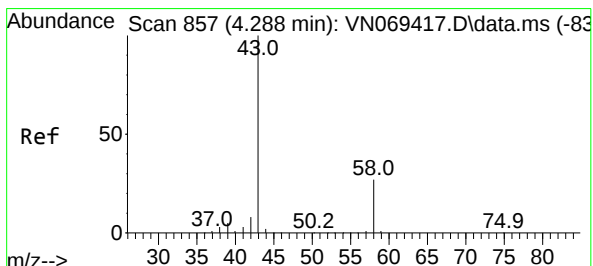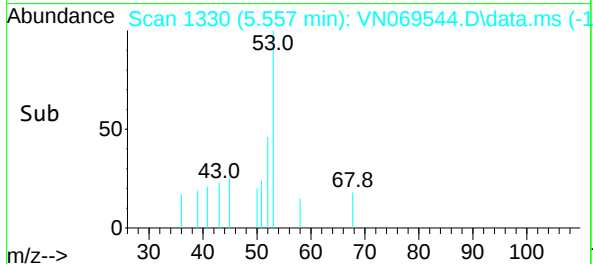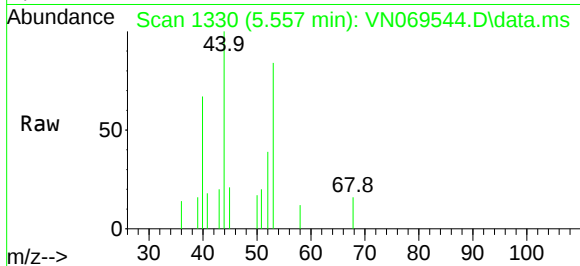

#16
Acetone
Concen: 0.984 ug/l
RT: 4.301 min Scan# 862
Delta R.T. 0.013 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

Tgt Ion: 43 Resp: 10515
Ion Ratio Lower Upper
43 100
58 28.0 23.1 34.7

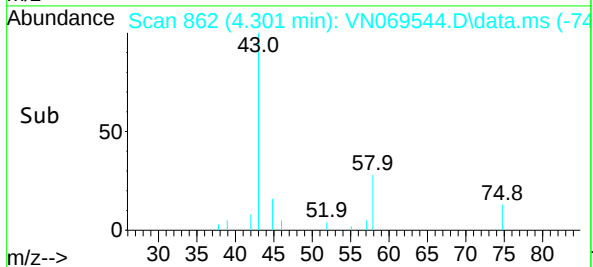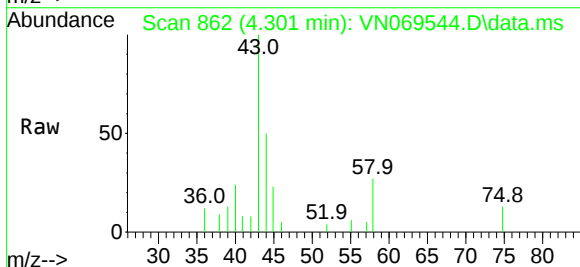



#29

Tetrahydrofuran

Concen: 0.213 ug/l

RT: 7.702 min Scan# 21

Delta R.T. 0.016 min


Lab File: VN069544.D

Acq: 18 Nov 2021 10:35




Instrument :

MSVOA_N

ClientSampleId :



Tgt Ion:	42	Resp:	1889
Ion	Ratio	Lower	Upper
42	100		
72	6.2	36.3	54.5#
71	8.0	34.7	52.1#

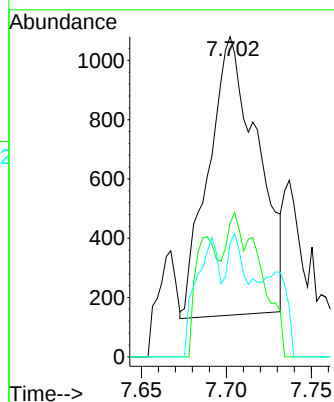

#31

Cyclohexane

Concen: 1.293 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.006 min

Lab File: VN069544.D

Acq: 18 Nov 2021 10:35


Tgt Ion:	56	Resp:	34970
Ion	Ratio	Lower	Upper
56	100		
69	146.2	27.1	40.7#
84	115.8	73.4	110.0#

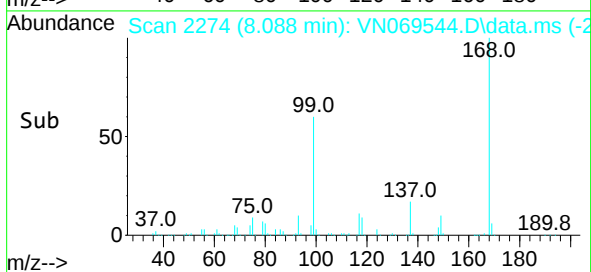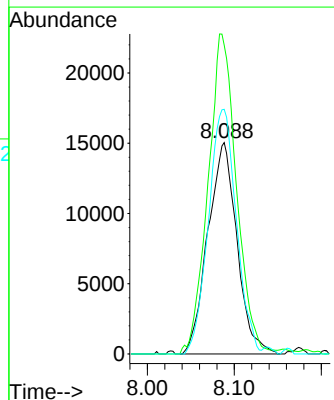






#33
 1,2-Dichloroethane-d4
 Concen: 50.117 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. -0.000 min
 Lab File: VN069544.D
 Acq: 18 Nov 2021 10:35

Instrument :
 MSVOA_N
 ClientSampleId :



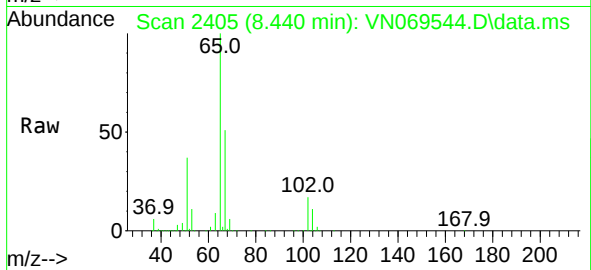



Tgt Ion: 65 Resp: 992229
 Ion Ratio Lower Upper
 65 100
 67 51.4 0.0 103.0

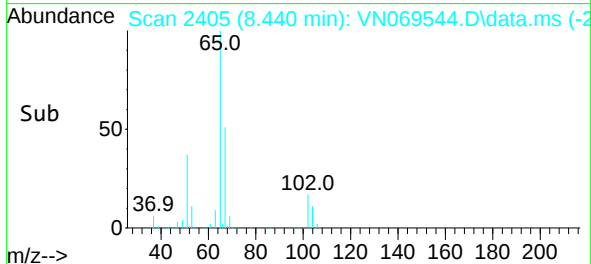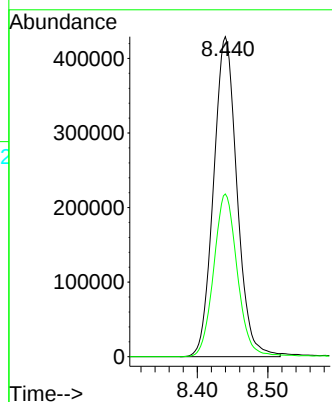

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.968 min Scan# 2602
 Delta R.T. 0.000 min
 Lab File: VN069544.D
 Acq: 18 Nov 2021 10:35

Tgt Ion: 114 Resp: 2355150
 Ion Ratio Lower Upper
 114 100
 63 22.2 0.0 37.8
 88 15.9 0.0 27.4


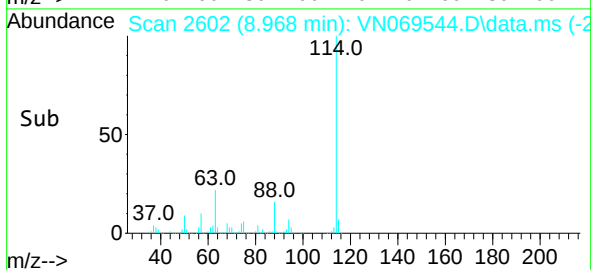

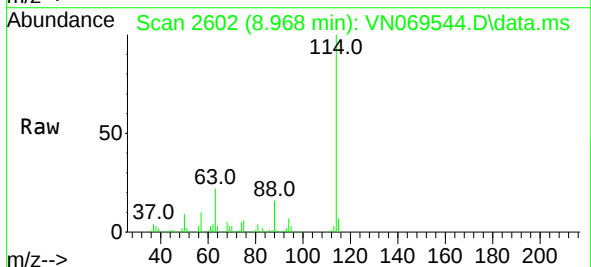




#35
Dibromofluoromethane
Concen: 48.611 ug/l
RT: 8.024 min Scan# 21
Delta R.T. 0.003 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:113 Resp: 686633
Ion Ratio Lower Upper
113 100
111 103.2 82.2 123.2
192 18.5 16.9 25.3

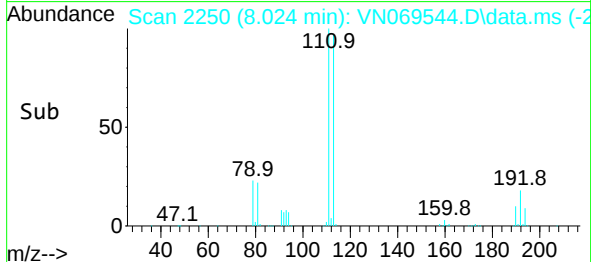

#36
1,1-Dichloropropene
Concen: 5.893 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.137 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35


Tgt Ion: 75 Resp: 116779
Ion Ratio Lower Upper
75 100
110 8.8 18.4 55.2#
77 0.0 24.4 36.6#

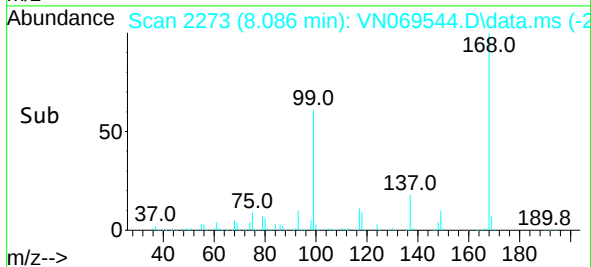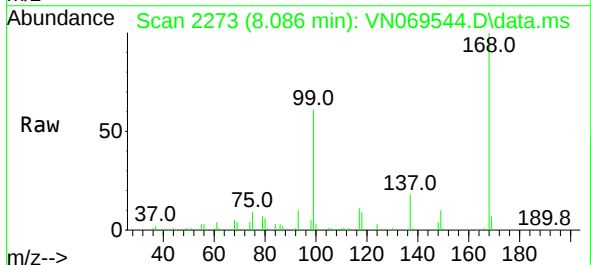






#38
Carbon Tetrachloride
Concen: 7.382 ug/l
RT: 8.088 min Scan# 211
Delta R.T. -0.118 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 141242
Ion Ratio Lower Upper
117 100
119 4.5 76.1 114.1#
121 0.0 24.2 36.2#

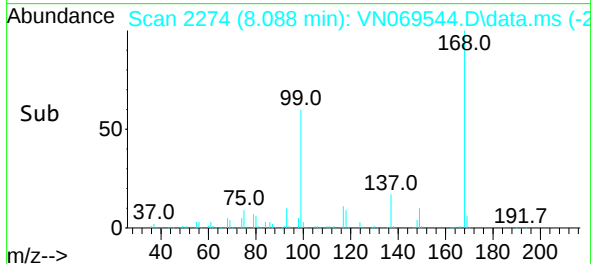

#49
1,4-Dioxane
Concen: 40.149 ug/l
RT: 9.569 min Scan# 2826
Delta R.T. -0.003 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

Tgt Ion: 88 Resp: 455
Ion Ratio Lower Upper
88 100
43 54.1 23.4 35.2#
58 43.1 50.6 75.8#


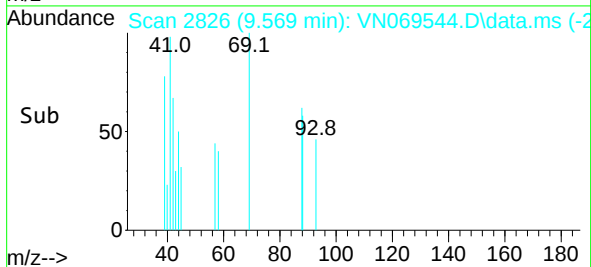

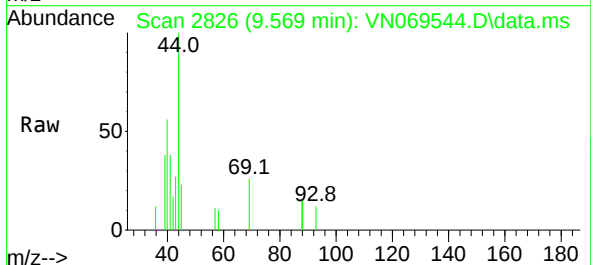




#50
Toluene-d8
Concen: 53.339 ug/l
RT: 10.443 min Scan# 3151
Delta R.T. 0.002 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 2963175
Ion Ratio Lower Upper
98 100
100 63.7 50.4 75.6

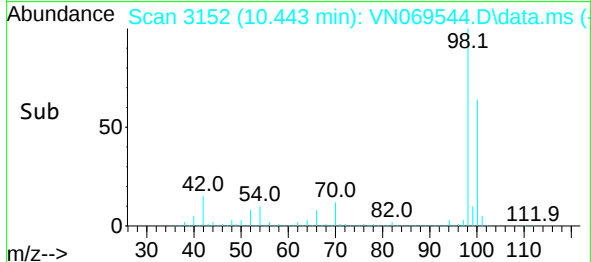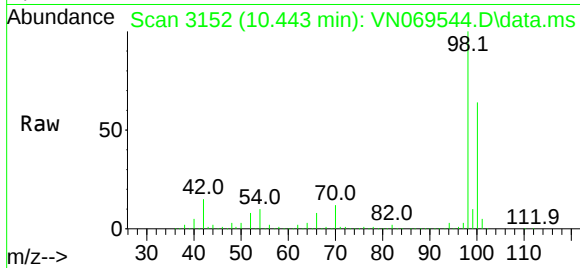

#51
4-Methyl-2-Pentanone
Concen: 0.339 ug/l
RT: 10.341 min Scan# 3114
Delta R.T. 0.010 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35


Tgt Ion: 43 Resp: 9414
Ion Ratio Lower Upper
43 100
58 33.9 30.4 45.6

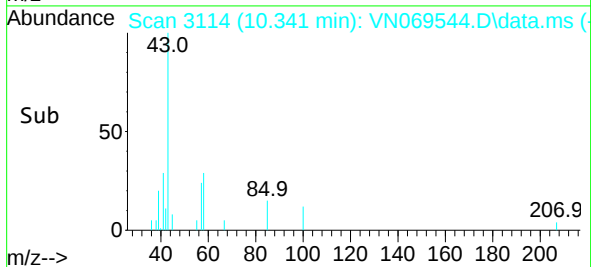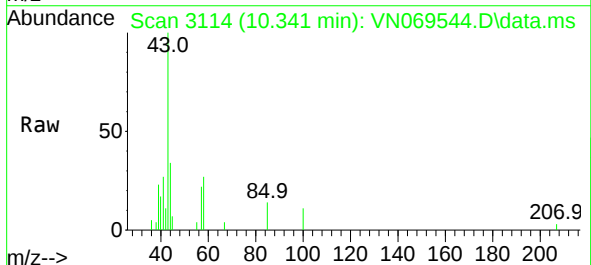






#53
 t-1,3-Dichloropropene
 Concen: 2.646 ug/l
 RT: 10.714 min Scan# 31
 Delta R.T. -0.005 min
 Lab File: VN069544.D
 Acq: 18 Nov 2021 10:35

Instrument :
 MSVOA_N
 ClientSampleId :



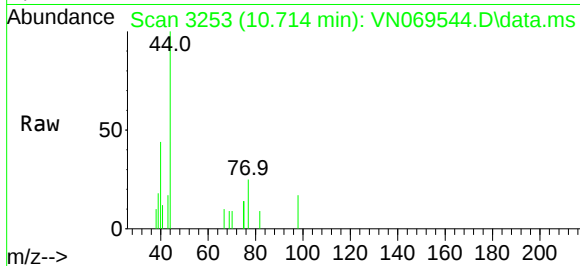



Tgt Ion: 75 Resp: 235
 Ion Ratio Lower Upper
 75 100
 77 28.7 25.6 38.4

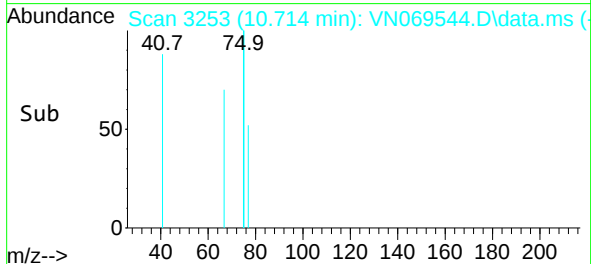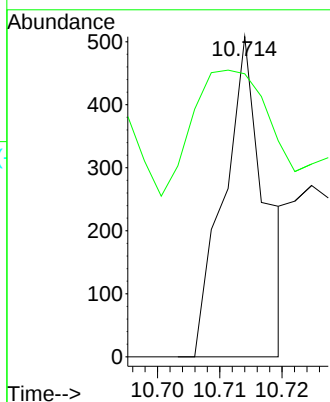

#54
 cis-1,3-Dichloropropene
 Concen: 1.739 ug/l
 RT: 10.191 min Scan# 3058
 Delta R.T. 0.003 min
 Lab File: VN069544.D
 Acq: 18 Nov 2021 10:35

Tgt Ion: 75 Resp: 180
 Ion Ratio Lower Upper
 75 100
 77 0.0 26.4 39.6#
 39 11.0 42.5 63.7#


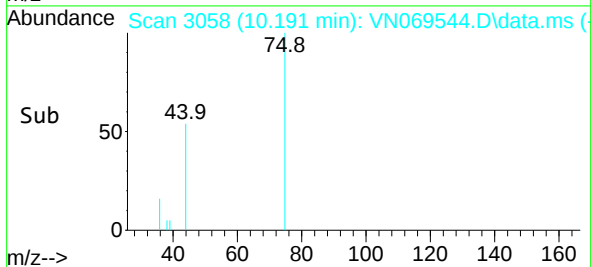
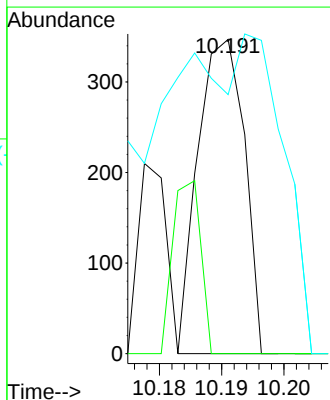
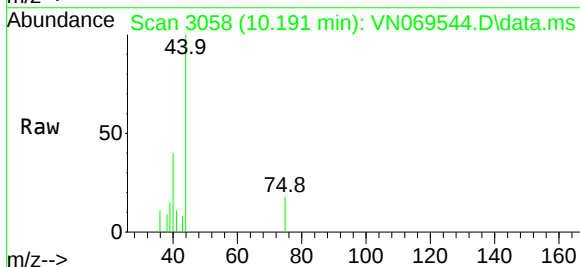




#56
Ethyl methacrylate
Concen: 2.107 ug/l
RT: 10.765 min Scan# 31
Delta R.T. 0.003 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 69 Resp: 1624
Ion Ratio Lower Upper
69 100
41 30.7 51.4 77.0#
39 40.3 34.6 52.0

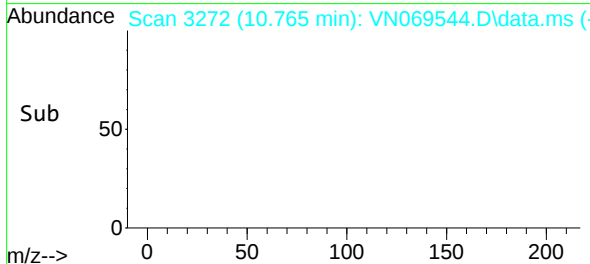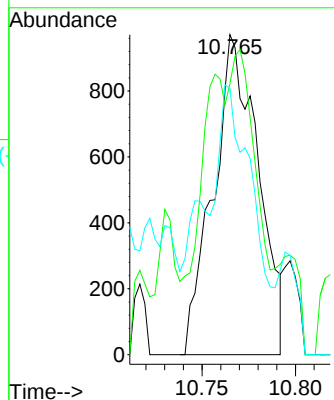

#58
2-Chloroethyl Vinyl ether
Concen: 22.777 ug/l
RT: 9.893 min Scan# 2947
Delta R.T. -0.148 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

Tgt Ion: 63 Resp: 54
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#



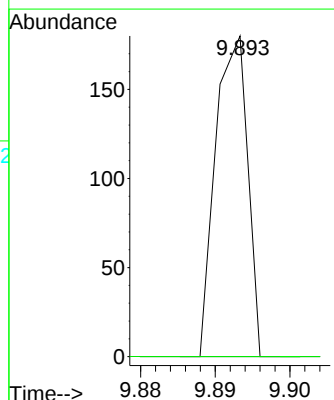
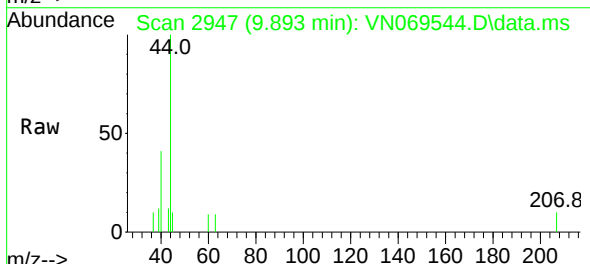




#59
2-Hexanone
Concen: 8.761 ug/l
RT: 11.089 min Scan# 31
Delta R.T. 0.002 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 19851
Ion Ratio Lower Upper
43 100
58 45.9 26.9 80.7

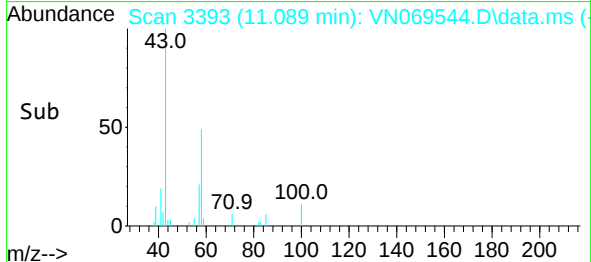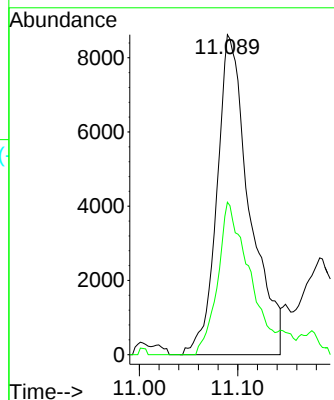

#60
Dibromochloromethane
Concen: 2.428 ug/l
RT: 11.242 min Scan# 3450
Delta R.T. 0.002 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

Tgt Ion: 129 Resp: 188
Ion Ratio Lower Upper
129 100
127 50.0 38.6 116.0


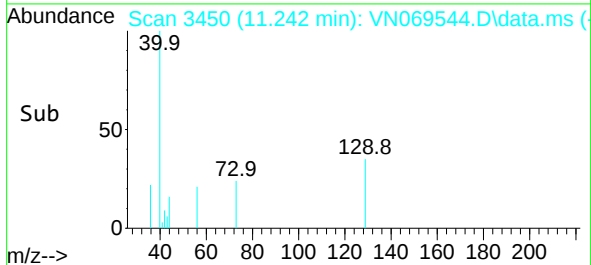
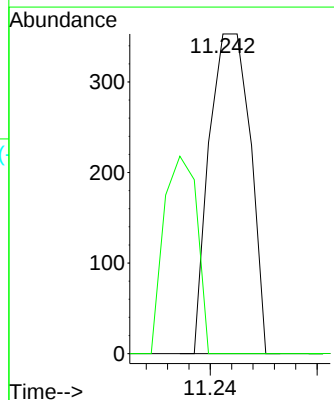
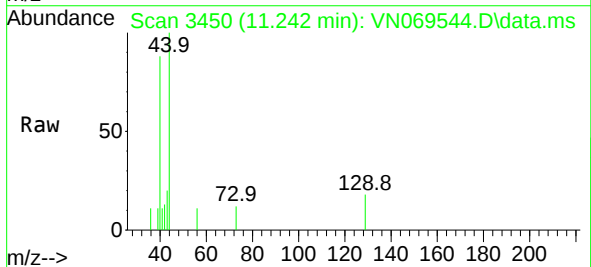




#61
1,2-Dibromoethane
Concen: 1.080 ug/l
RT: 11.339 min Scan# 3486
Delta R.T. -0.008 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:107 Resp: 154
Ion Ratio Lower Upper
107 100
109 167.5 75.7 113.5#

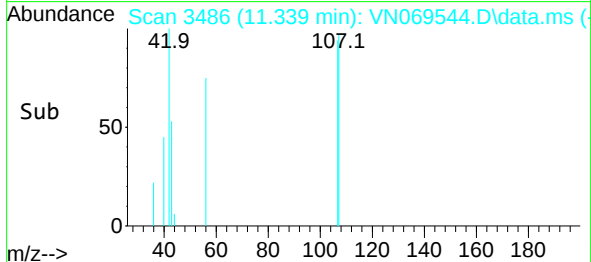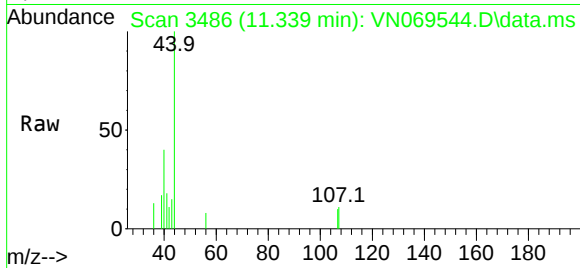

#62
4-Bromofluorobenzene
Concen: 49.923 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.000 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35


Tgt Ion: 95 Resp: 1018850
Ion Ratio Lower Upper
95 100
174 76.5 0.0 187.2
176 74.2 0.0 181.4

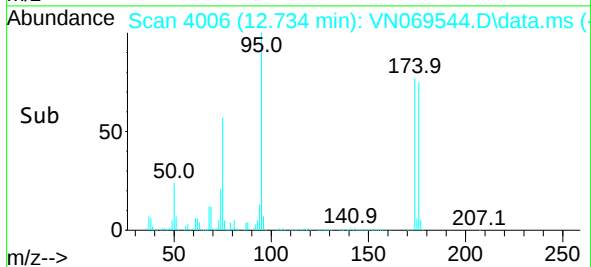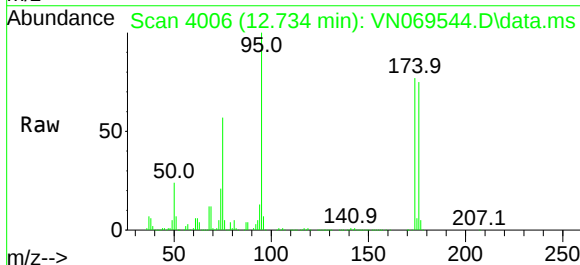






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:117 Resp: 2292816
Ion Ratio Lower Upper
117 100
82 57.9 42.4 63.6
119 32.2 25.4 38.2

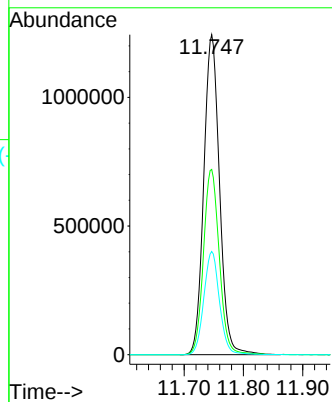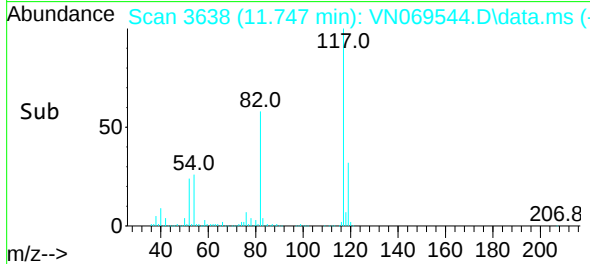


#70
Styrene
Concen: 1.550 ug/l
RT: 12.294 min Scan# 3842
Delta R.T. -0.000 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

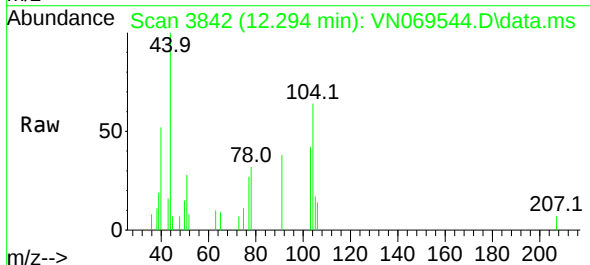

Tgt Ion:104 Resp: 1589
Ion Ratio Lower Upper
104 100
78 40.3 38.7 58.1
103 93.8 45.0 67.6#

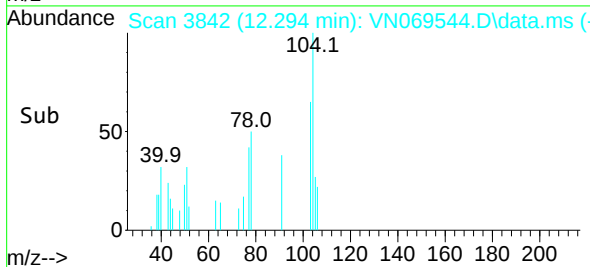

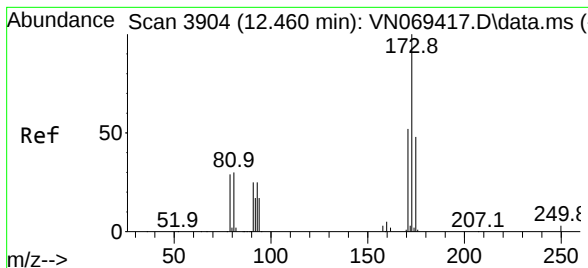

#71

Bromoform

Concen: 3.432 ug/l

RT: 12.465 min Scan# 3906

Delta R.T. 0.005 min

Lab File: VN069544.D





Acq: 18 Nov 2021 10:35

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:173	Resp:	53
Ion Ratio	Lower	Upper
173	100	
175	0.0	24.2 72.6#
254	0.0	0.0 0.0

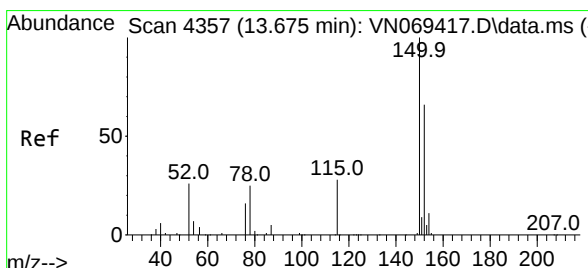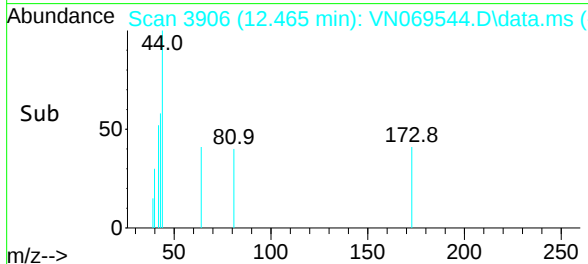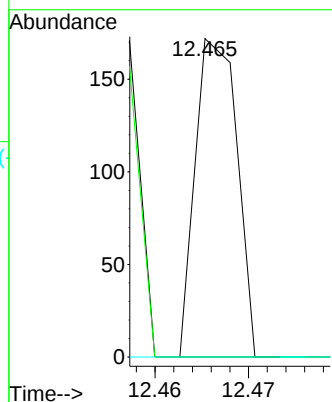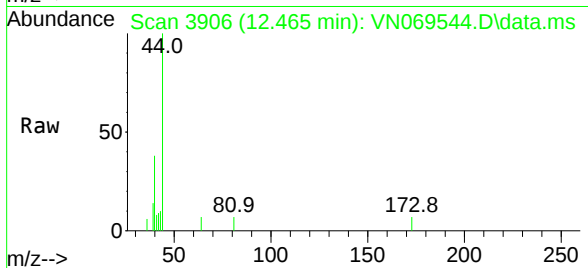

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l




RT: 13.678 min Scan# 4358


Delta R.T. 0.003 min

Lab File: VN069544.D

Acq: 18 Nov 2021 10:35


Tgt Ion:152	Resp:	833482
Ion Ratio	Lower	Upper
152	100	
115	60.8	27.5 82.5
150	157.7	0.0 344.4

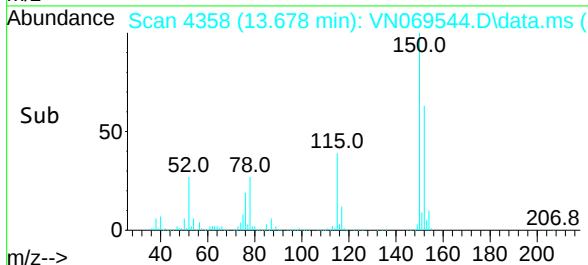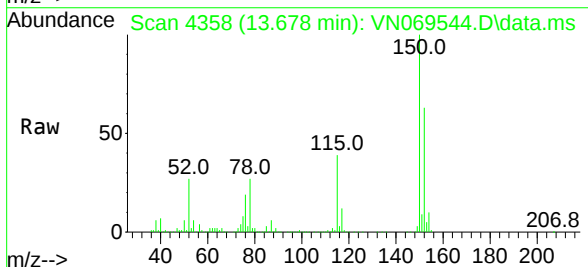






#74
N-amy1 acetate
Concen: 0.364 ug/l
RT: 12.398 min Scan# 31
Delta R.T. 0.010 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

Instrument :
MSVOA_N
ClientSampleId :



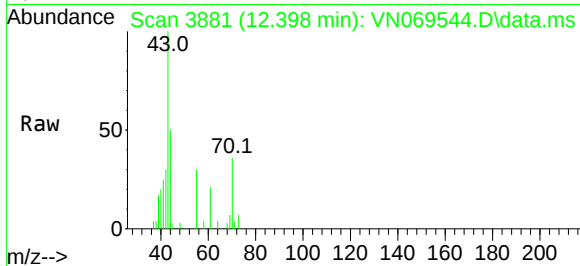



Tgt Ion: 43	Resp: 10226
Ion Ratio	Lower Upper
43 100	
70 42.6	33.4 50.0
55 32.0	19.3 28.9#
61 11.6	18.5 27.7#

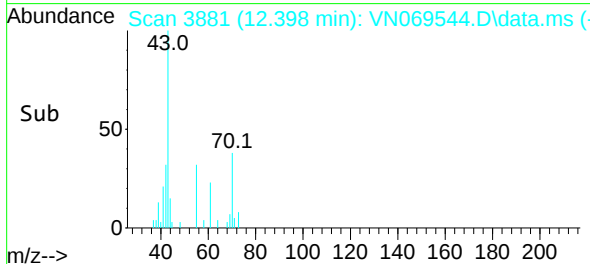

#76
1,2,3-Trichloropropane
Concen: 29.678 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.147 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

Tgt Ion: 75	Resp: 570844
Ion Ratio	Lower Upper
75 100	
77 1.0	82.6 247.8#


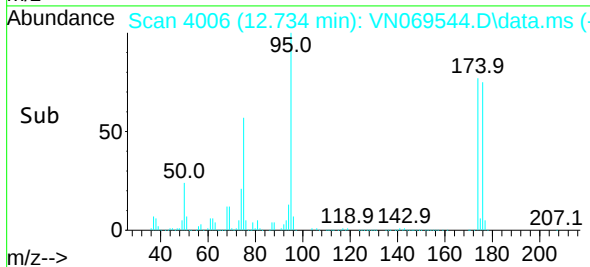

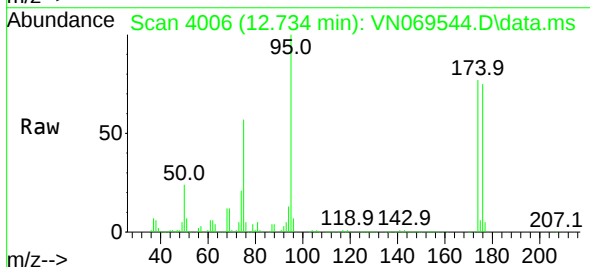




#81
trans-1,4-Dichloro-2-butene
Concen: 83.903 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.108 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 570844
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

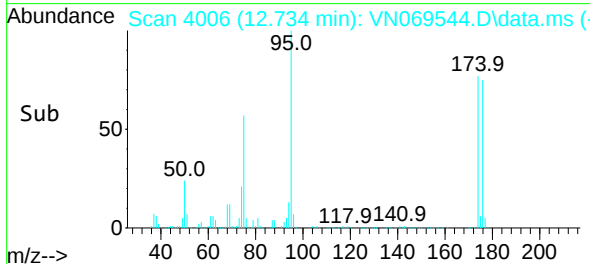

#87
1,3-Dichlorobenzene
Concen: 0.203 ug/l
RT: 13.627 min Scan# 4339
Delta R.T. 0.011 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35


Tgt Ion: 146 Resp: 5346
Ion Ratio Lower Upper
146 100
111 40.9 18.6 55.6
148 61.6 31.6 95.0

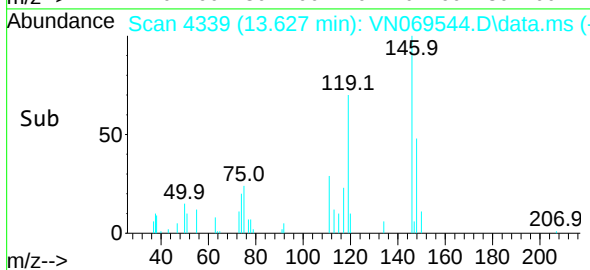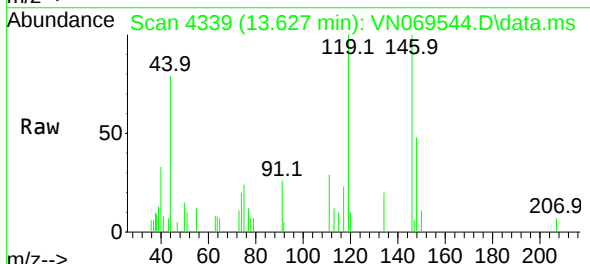






#88
1,4-Dichlorobenzene
Concen: 0.207 ug/l
RT: 13.627 min Scan# 41
Delta R.T. -0.069 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion	Ratio	Lower	Upper
146	100		
111	40.9	18.3	54.8
148	61.6	31.8	95.4

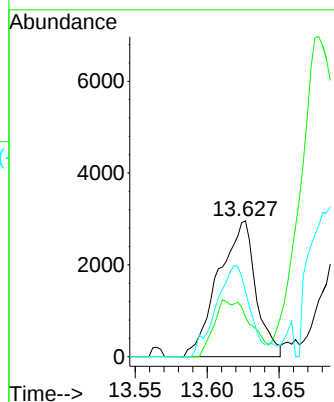

#89
n-Butylbenzene
Concen: 0.283 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. 0.000 min
Lab File: VN069544.D
Acq: 18 Nov 2021 10:35

Tgt Ion	Ratio	Lower	Upper
91	100		
92	51.3	25.4	76.0
134	24.3	13.6	40.8

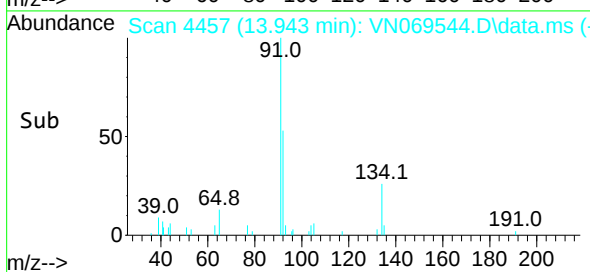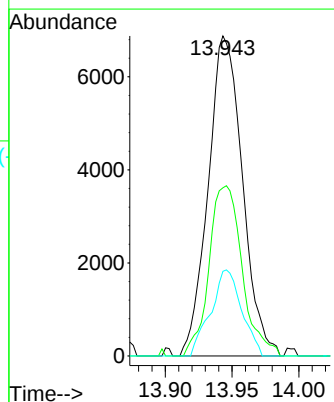



#90

Hexachloroethane

Concen: 2.168 ug/l

RT: 14.209 min Scan# 4556

Delta R.T. -0.002 min

Lab File: VN069544.D

Acq: 18 Nov 2021 10:35

Instrument :

MSVOA_N





ClientSampleId :

Tgt Ion:117 Resp: 62

Ion Ratio Lower Upper

117 100

201 0.0 43.9 131.6#

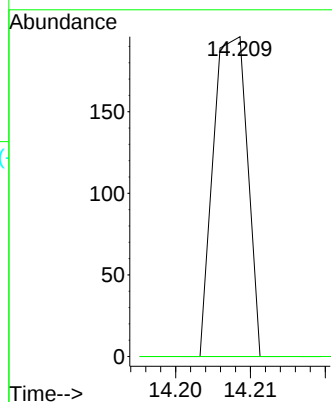

#91

1,2-Dichlorobenzene

Concen: 0.229 ug/l

RT: 13.991 min Scan# 4475

Delta R.T. 0.002 min

Lab File: VN069544.D

Acq: 18 Nov 2021 10:35




Tgt Ion:146 Resp: 5742


Ion Ratio Lower Upper

146 100

111 24.4 19.1 57.3

148 68.7 32.1 96.3


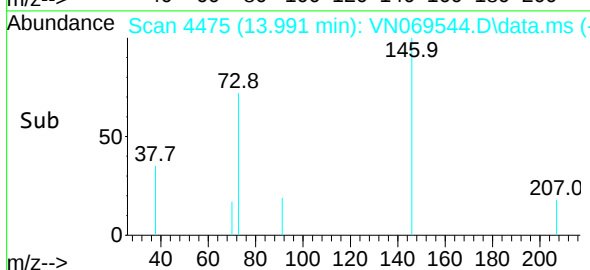






#92
 1,2-Dibromo-3-Chloropropane
 Concen: 2.057 ug/l
 RT: 14.600 min Scan# 41
 Delta R.T. -0.006 min
 Lab File: VN069544.D
 Acq: 18 Nov 2021 10:35




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 1122
 Ion Ratio Lower Upper
 75 100
 155 33.3 46.9 140.7#
 157 0.0 60.6 181.7#

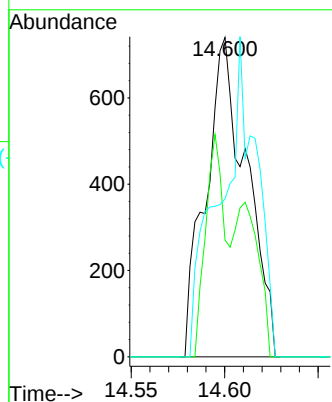

#93
 1,2,4-Trichlorobenzene
 Concen: 3.841 ug/l
 RT: 15.263 min Scan# 4949
 Delta R.T. -0.002 min
 Lab File: VN069544.D
 Acq: 18 Nov 2021 10:35

Tgt Ion: 180 Resp: 10185
 Ion Ratio Lower Upper
 180 100
 182 92.2 48.3 144.9
 145 31.4 14.5 43.5

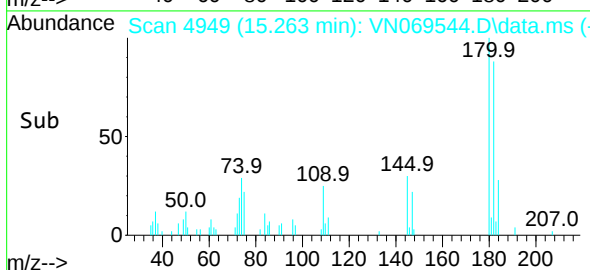



#95

Naphthalene

Concen: 5.516 ug/l

RT: 15.509 min Scan# 5040

Delta R.T. 0.002 min

Lab File: VN069544.D





Acq: 18 Nov 2021 10:35

Instrument :

MSVOA_N

ClientSampleId :

Tgt Ion:	128	Resp:	43259
Ion Ratio	Lower	Upper	
128	100		
127	12.8	10.5	15.7
129	9.8	8.7	13.1

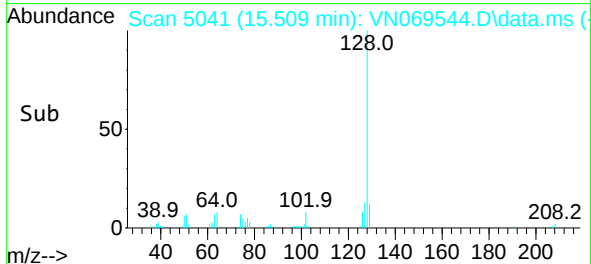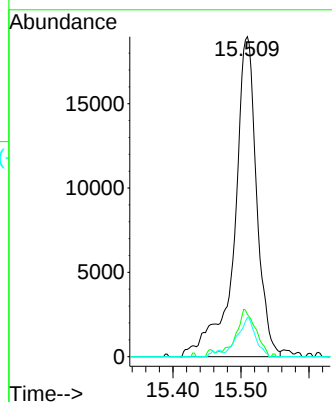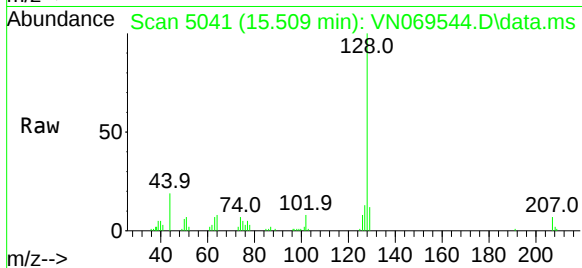

#96

1,2,3-Trichlorobenzene

Concen: 4.145 ug/l

RT: 15.708 min Scan# 5115

Delta R.T. 0.008 min

Lab File: VN069544.D

Acq: 18 Nov 2021 10:35

Tgt Ion:	180	Resp:	13065
Ion Ratio	Lower	Upper	
180	100		
182	91.9	47.4	142.2
145	33.3	15.0	45.1

