


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111821\
Data File : VN069542.D
Acq On : 18 Nov 2021 9:24
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
Title : SW846 8260
Last Update : Tue Nov 09 18:18:22 2021

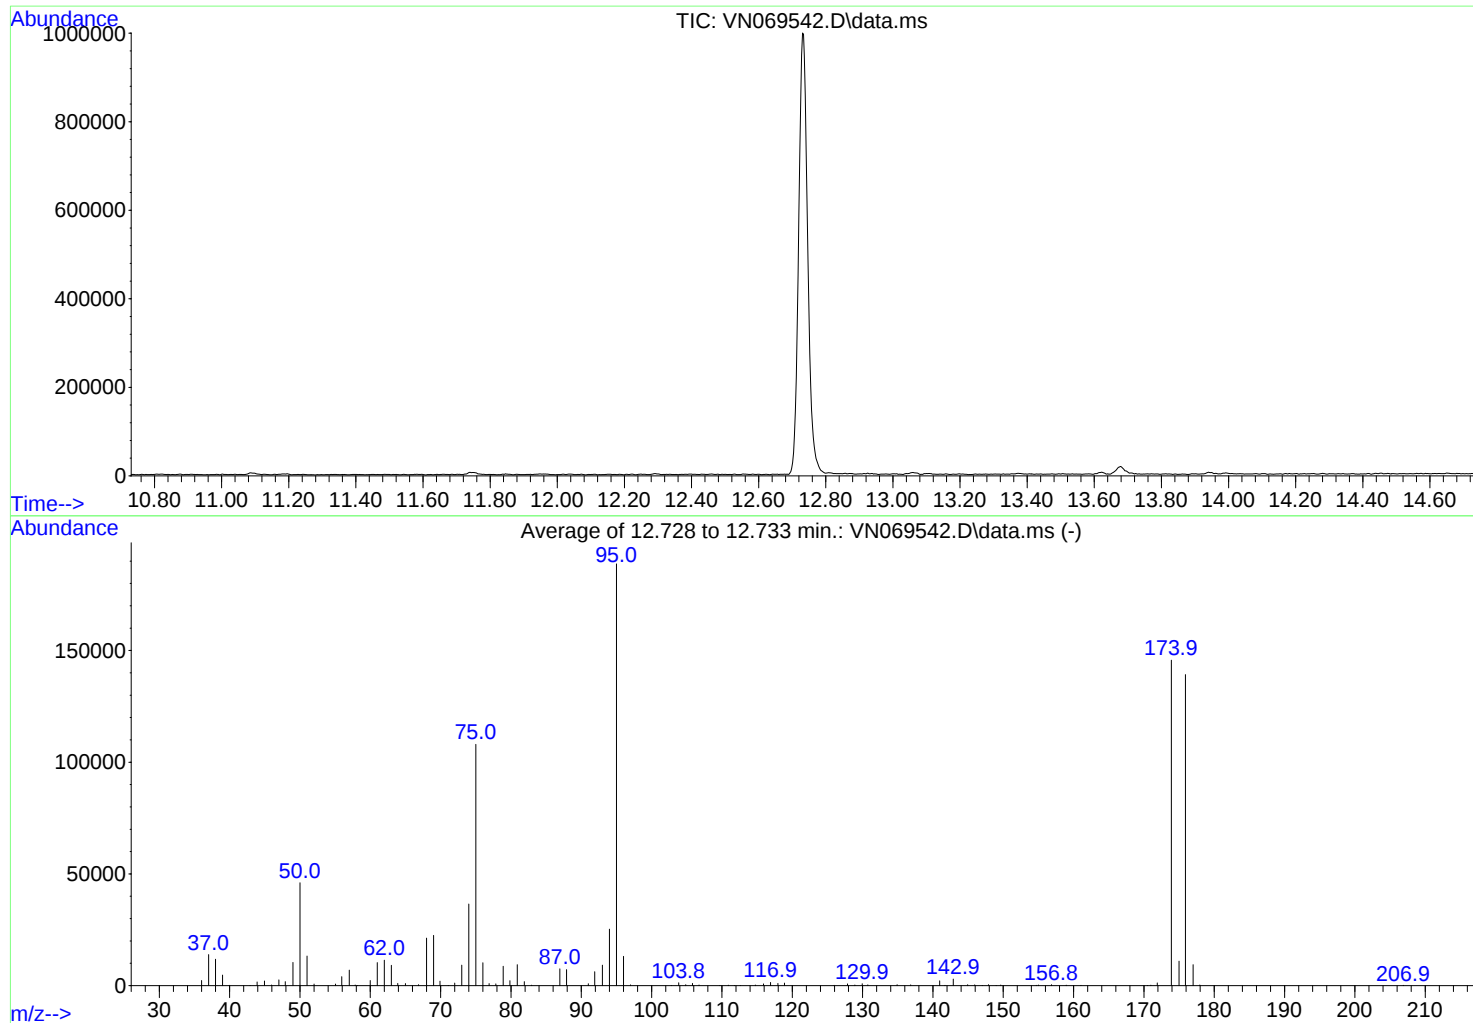

AutoFind: Scans 4004, 4005, 4006; Background Corrected with Scan 3987

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.4	46035	PASS
75	95	30	60	57.2	108016	PASS
95	95	100	100	100.0	188779	PASS
96	95	5	9	6.9	13080	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.2	145643	PASS
175	174	5	9	7.5	10987	PASS
176	174	95	101	95.6	139179	PASS
177	176	5	9	6.8	9406	PASS