


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111821\
 Data File : VN069568.D
 Acq On : 18 Nov 2021 22:07
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Title : SW846 8260
 Last Update : Tue Nov 09 18:18:22 2021

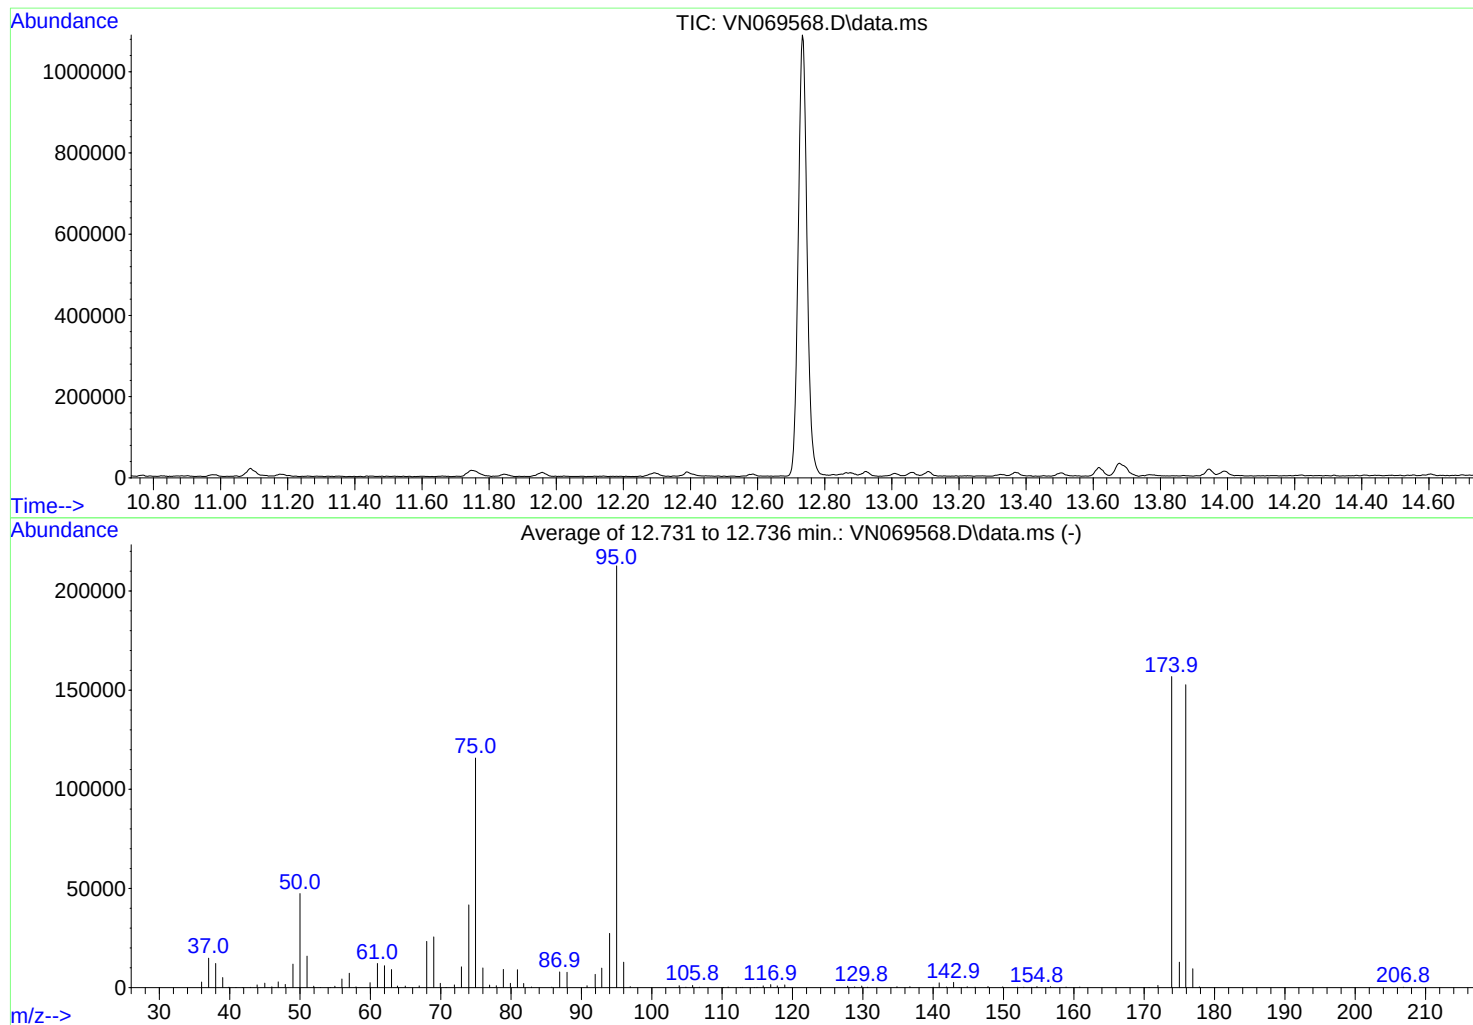

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	47424	PASS
75	95	30	60	54.4	115759	PASS
95	95	100	100	100.0	212672	PASS
96	95	5	9	6.0	12862	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.8	156864	PASS
175	174	5	9	8.2	12849	PASS
176	174	95	101	97.3	152683	PASS
177	176	5	9	6.2	9519	PASS