
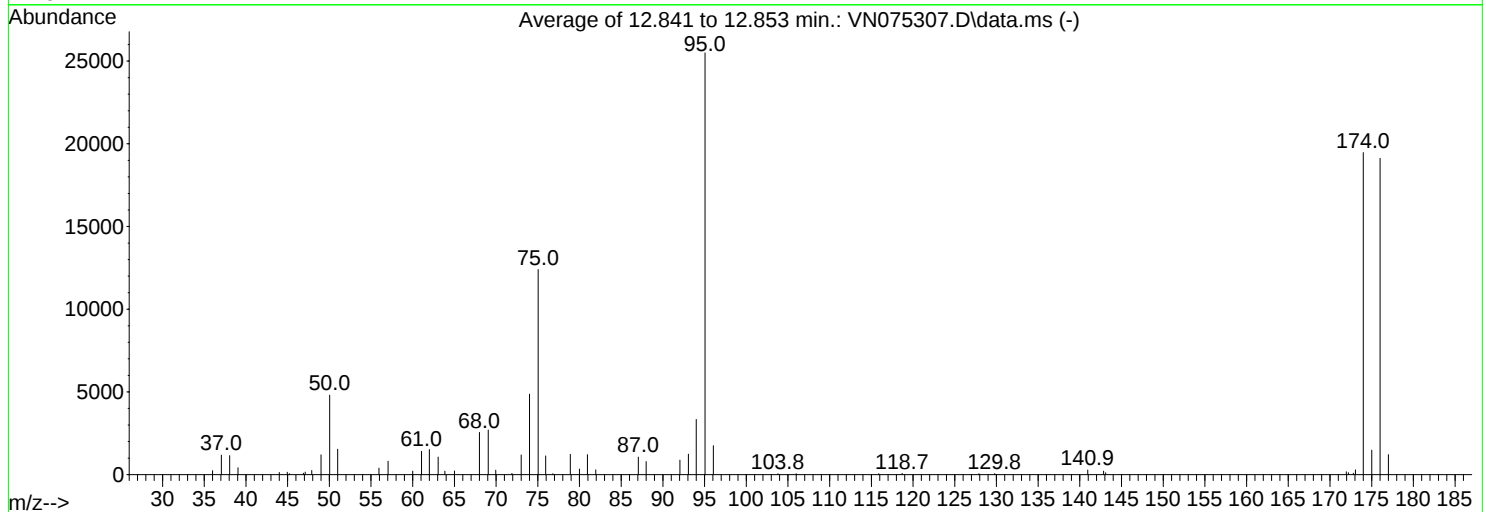


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111822\
Data File : VN075307.D
Acq On : 18 Nov 2022 11:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102622W.M
Title : SW846 8260
Last Update : Thu Oct 27 09:48:49 2022

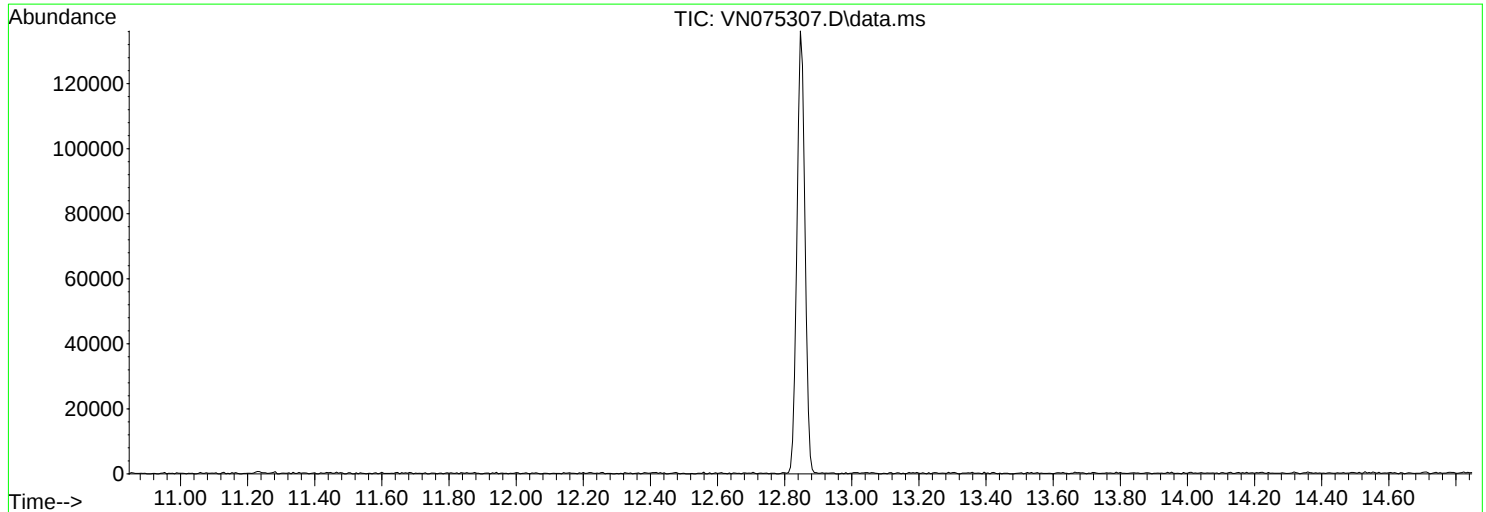

AutoFind: Scans 1834, 1835, 1836; Background Corrected with Scan 1826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	4803	PASS
75	95	30	60	48.6	12404	PASS
95	95	100	100	100.0	25499	PASS
96	95	5	9	6.9	1749	PASS
173	174	0.00	2	1.5	287	PASS
174	95	50	100	76.4	19475	PASS
175	174	5	9	7.6	1480	PASS
176	174	95	101	98.2	19119	PASS
177	176	5	9	6.3	1211	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	240	50.05	4803	69.05	2701	81.95	294
37.05	1184	51.00	1538	69.95	268	87.05	106
38.05	1153	55.95	401	71.90	74	88.00	79
39.05	419	57.05	808	73.00	1194	92.05	88
44.00	135	60.00	216	74.00	4864	93.05	1241
44.95	141	61.05	1417	75.05	12404	94.00	3334
45.20	57	62.00	1516	75.95	1132	95.05	25499
46.90	91	63.05	1065	76.80	55	96.05	1749
47.10	156	63.85	216	78.90	1229	103.80	63
47.90	252	65.00	226	80.00	341	106.00	58
49.00	1203	68.00	2553	80.95	1205	115.90	56

Average of 12.841 to 12.853 min.: VN075307.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
118.70	76	175.00	1480				
127.90	54	176.00	19119				
129.80	64	177.00	1211				
140.95	283						
142.85	211						
143.10	117						
171.95	178						
172.20	115						
172.80	91						
173.05	287						
174.00	19475						

Instrument :

MSVOA_N

ClientSampleId :

BFB