

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111823\
 Data File : VN080184.D
 Acq On : 18 Nov 2023 14:31
 Operator : JC\MD
 Sample : 05470-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-1

Quant Time: Nov 20 01:25:24 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
 Quant Title : SW846 8260
 QLast Update : Fri Nov 17 01:19:32 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	153161	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	283524	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	299626	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	130370	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	140747	55.655	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	111.300%
35) Dibromofluoromethane	8.171	113	108518	51.872	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.740%
50) Toluene-d8	10.571	98	376670	49.947	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	99.900%
62) 4-Bromofluorobenzene	12.853	95	145960	51.241	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.480%
Target Compounds						
16) Acetone	4.448	43	4497	5.294	ug/l	Qvalue # 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111823\
Data File : VN080184.D
Acq On : 18 Nov 2023 14:31
Operator : JC\MD
Sample : 05470-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-1

Quant Time: Nov 20 01:25:24 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Quant Title : SW846 8260
QLast Update : Fri Nov 17 01:19:32 2023
Response via : Initial Calibration




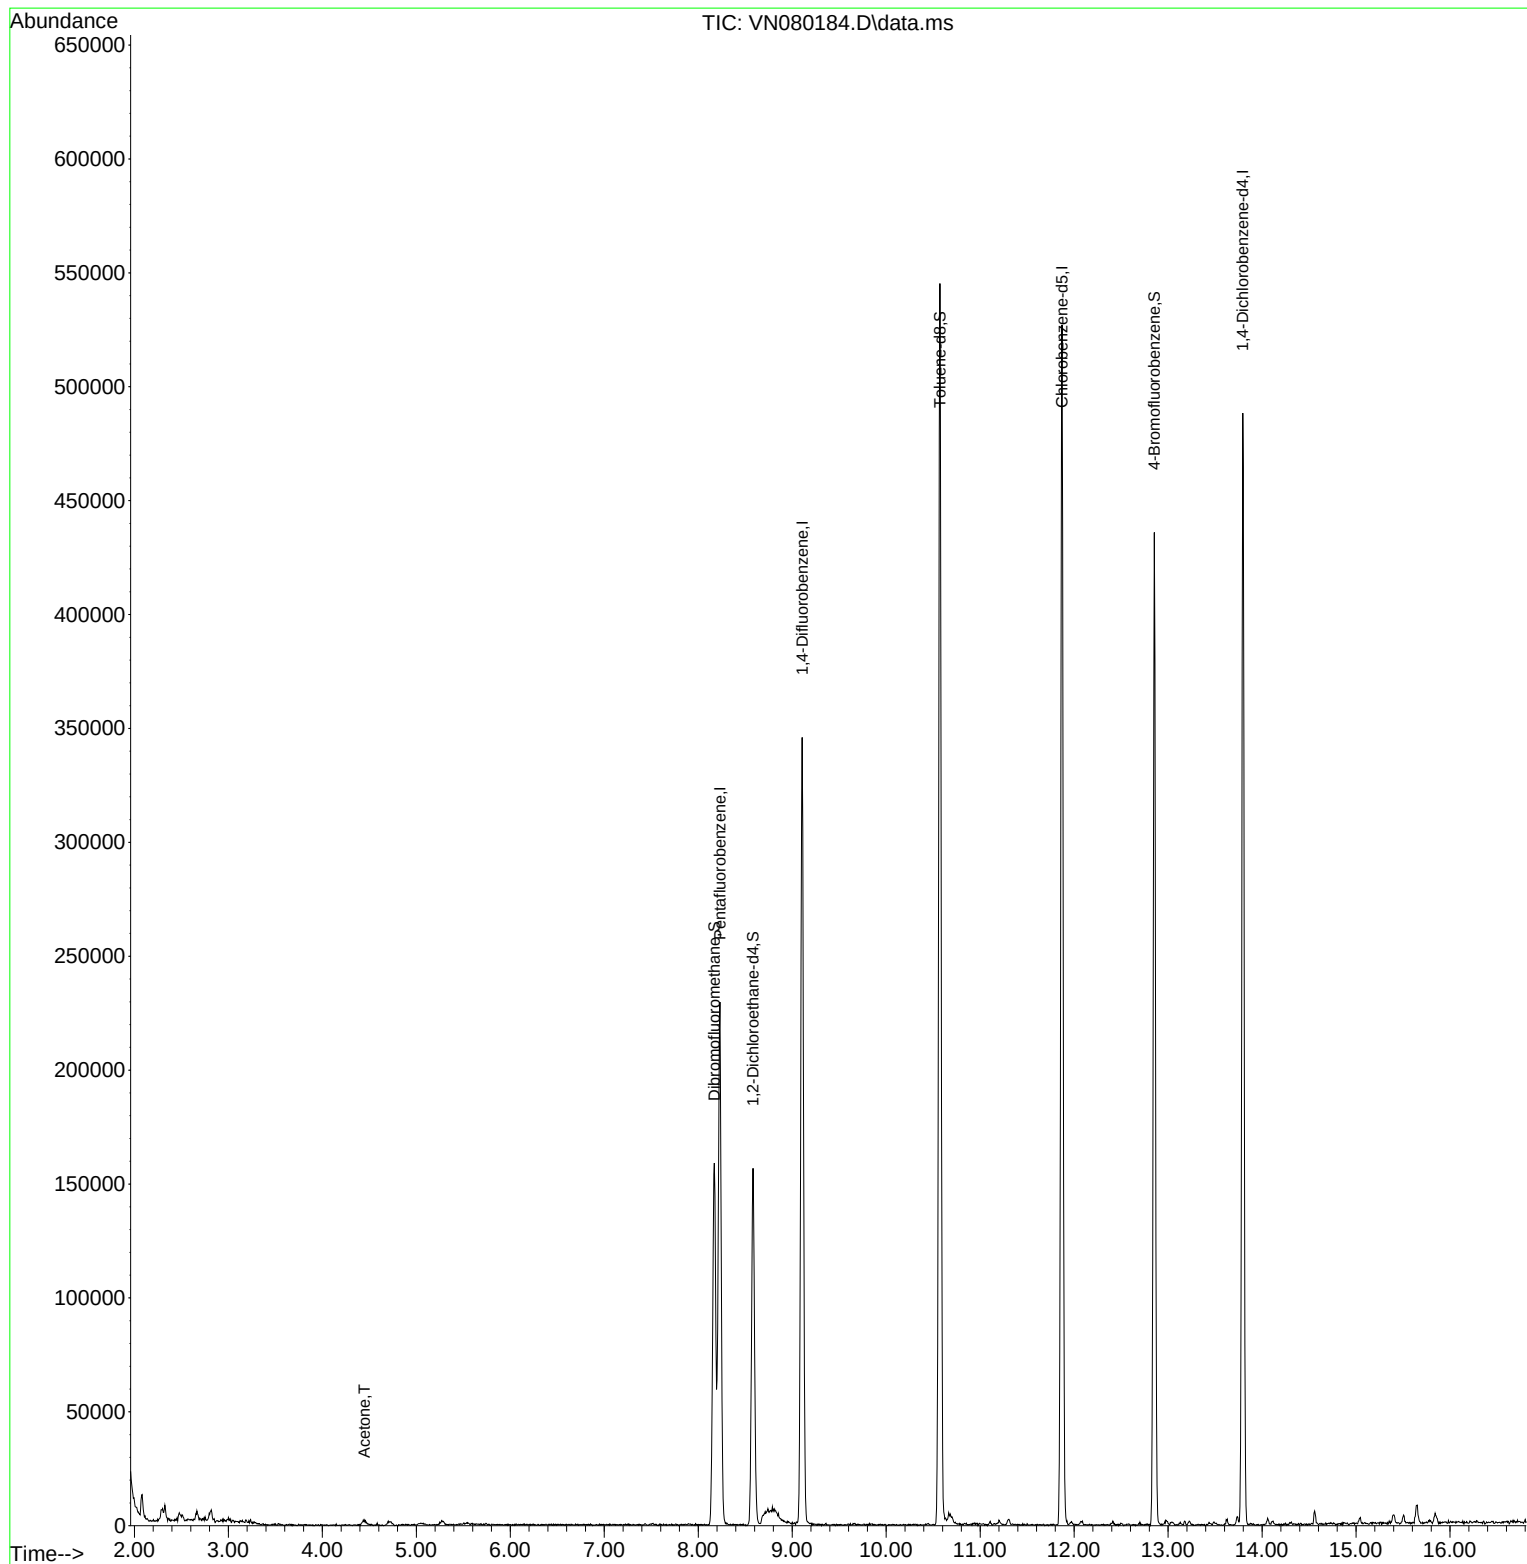


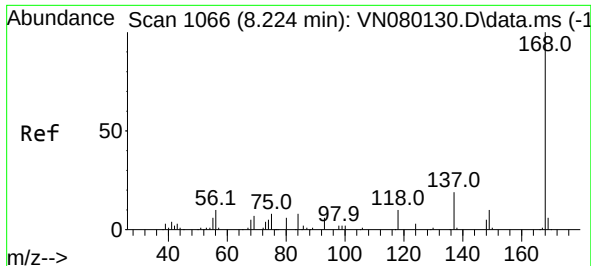

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN080184.D
Acq: 18 Nov 2023 14:31




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion:168 Resp: 153161
Ion Ratio Lower Upper
168 100
99 64.0 53.0 79.6

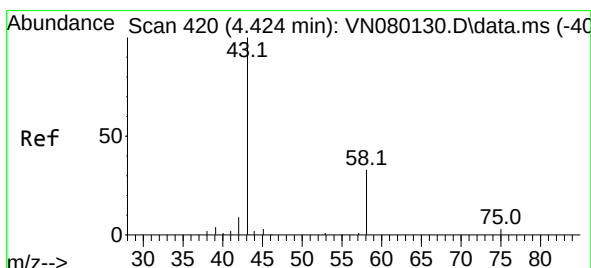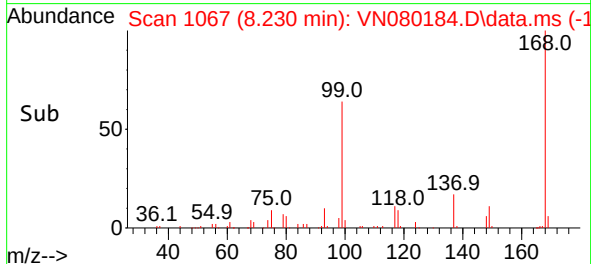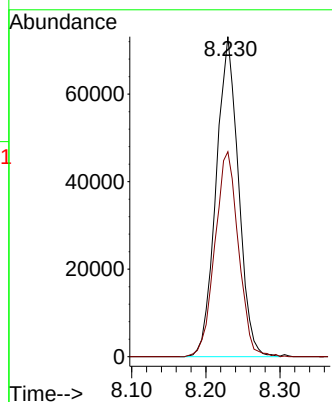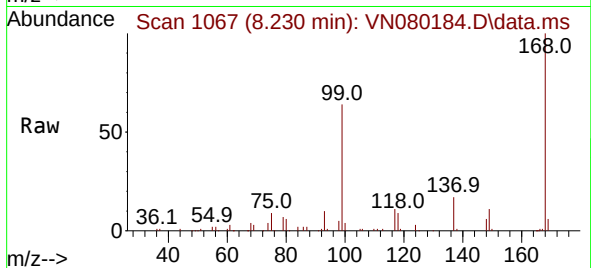

#16
Acetone
Concen: 5.294 ug/l
RT: 4.448 min Scan# 424
Delta R.T. 0.024 min
Lab File: VN080184.D
Acq: 18 Nov 2023 14:31

Tgt Ion: 43 Resp: 4497
Ion Ratio Lower Upper
43 100
58 27.8 28.0 42.0#

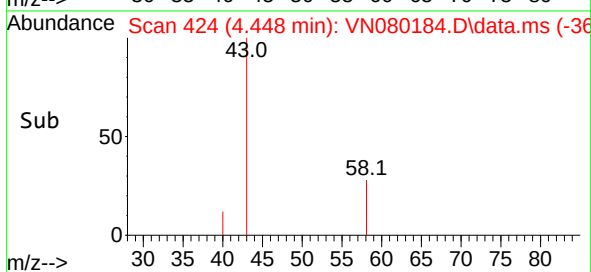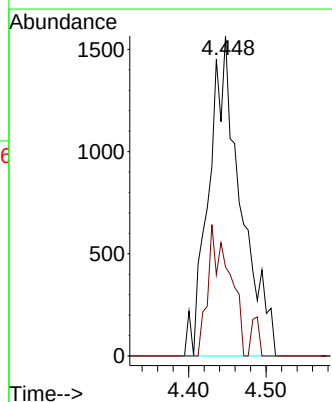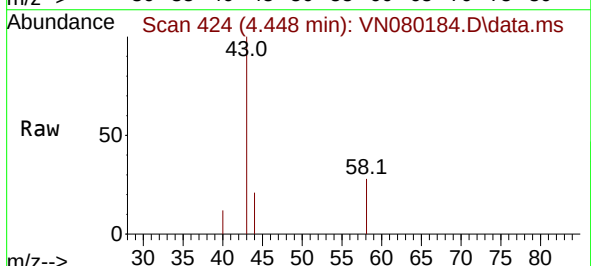

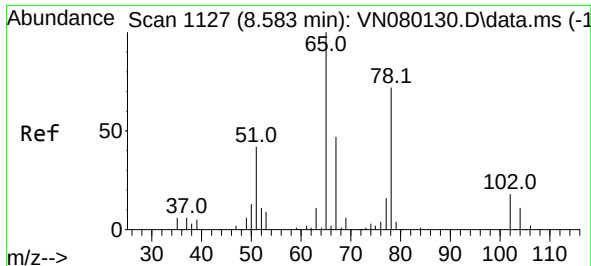

#33

1,2-Dichloroethane-d4

Concen: 55.655 ug/l

RT: 8.583 min Scan# 1127

Delta R.T. 0.000 min

Lab File: VN080184.D

Acq: 18 Nov 2023 14:31

Instrument :

MSVOA_N

ClientSampleId :





TP-1

Tgt Ion: 65 Resp: 140747

Ion Ratio Lower Upper

65 100

67 47.8 0.0 106.6

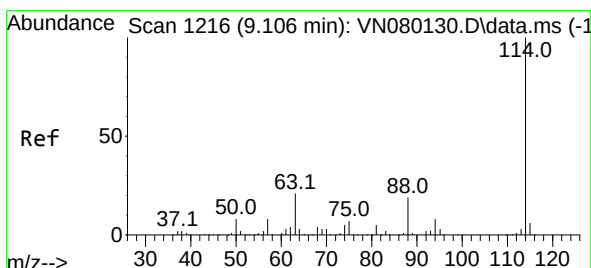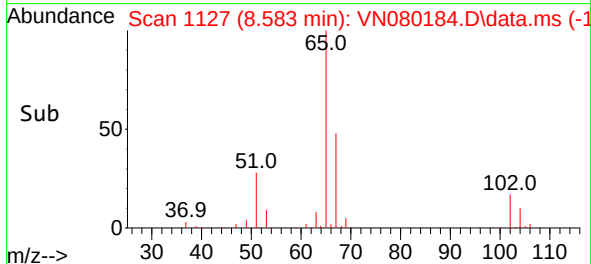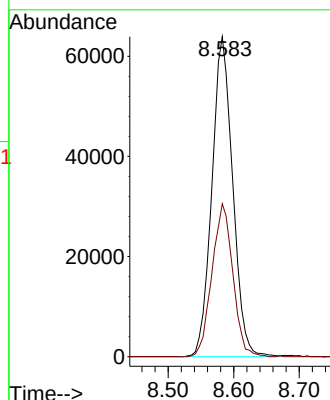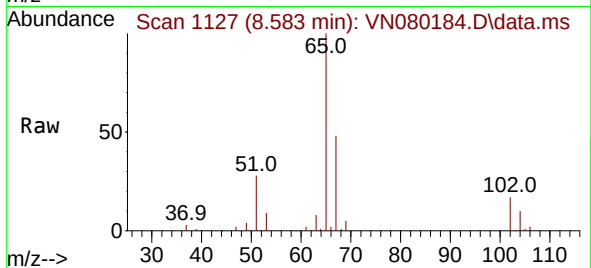

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. -0.000 min

Lab File: VN080184.D

Acq: 18 Nov 2023 14:31




Tgt Ion: 114 Resp: 283524


Ion Ratio Lower Upper

114 100

63 20.3 0.0 36.4

88 18.2 0.0 30.6

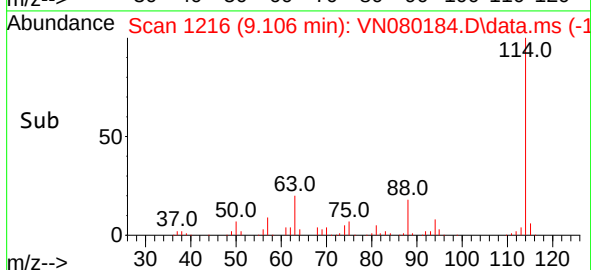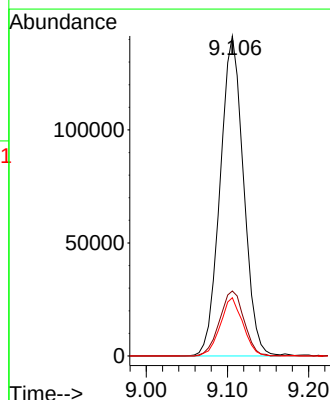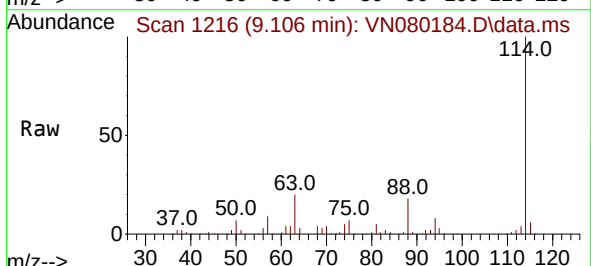

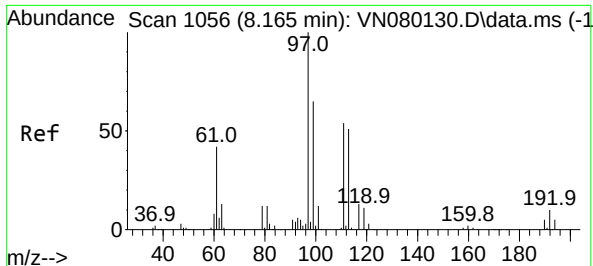

#35

Dibromofluoromethane

Concen: 51.872 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN080184.D

Acq: 18 Nov 2023 14:31

Instrument :

MSVOA_N

ClientSampleId :

TP-1





Tgt Ion:113 Resp: 108518

Ion Ratio Lower Upper

113 100

111 103.4 82.6 123.8

192 19.4 12.7 19.1#

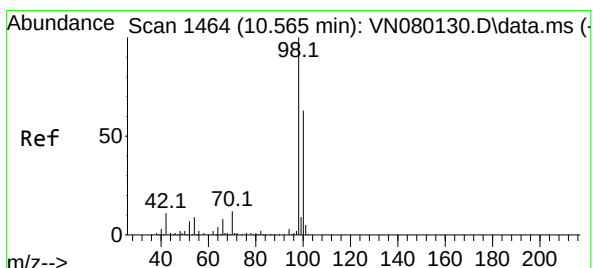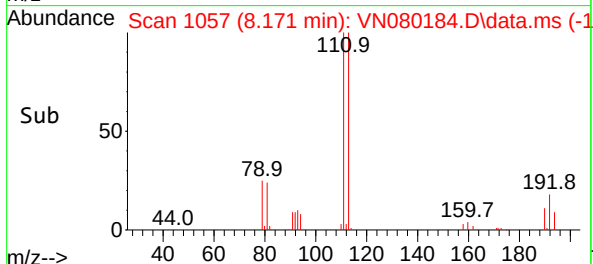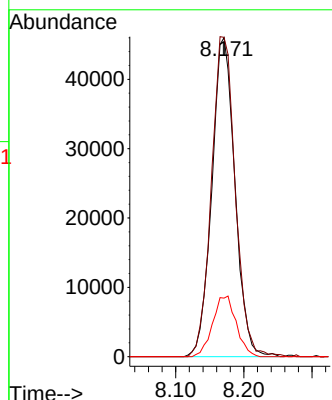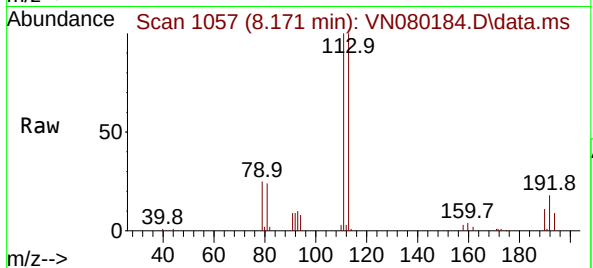

#50

Toluene-d8

Concen: 49.947 ug/l

RT: 10.571 min Scan# 1465

Delta R.T. 0.006 min

Lab File: VN080184.D




Acq: 18 Nov 2023 14:31


Tgt Ion: 98 Resp: 376670

Ion Ratio Lower Upper

98 100

100 63.5 52.0 78.0


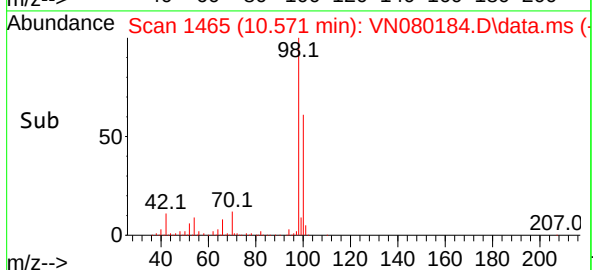
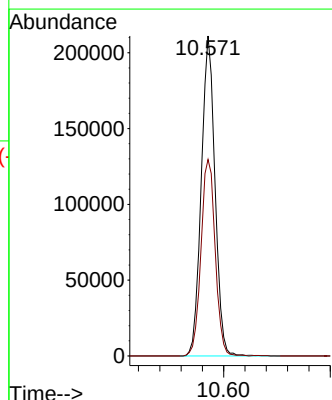
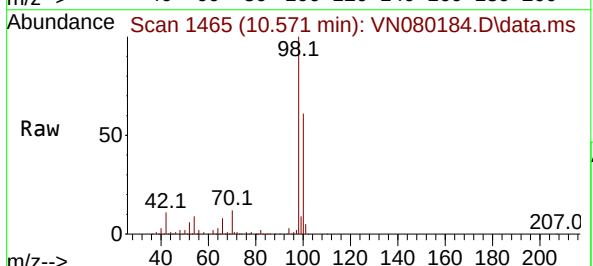


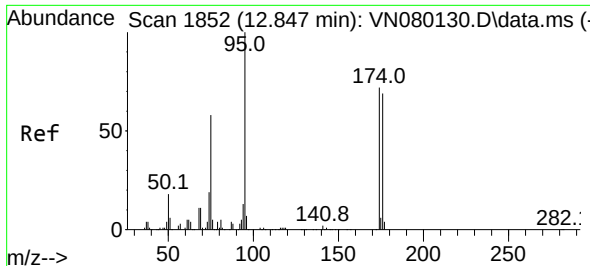

#62
4-Bromofluorobenzene
Concen: 51.241 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN080184.D
Acq: 18 Nov 2023 14:31




Instrument :
MSVOA_N
ClientSampleId :
TP-1


Tgt Ion: 95 Resp: 145960
Ion Ratio Lower Upper
95 100
174 75.6 0.0 143.8
176 71.2 0.0 135.8

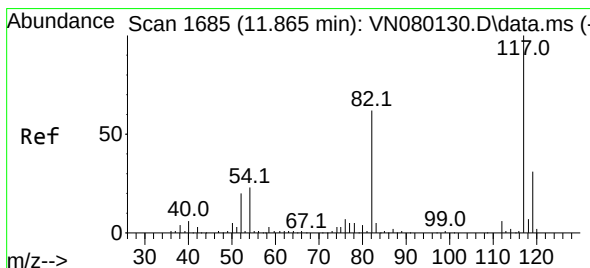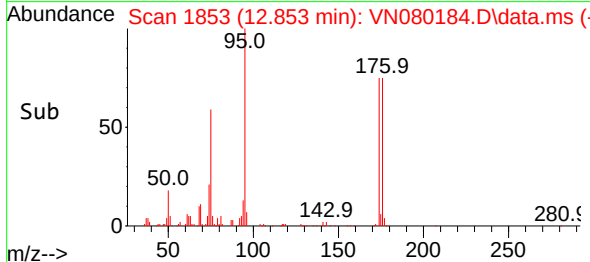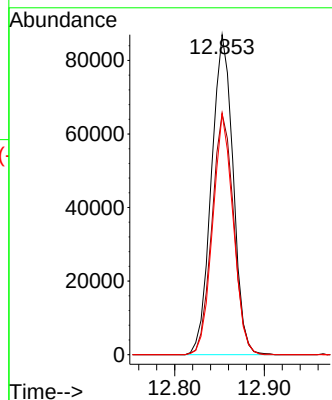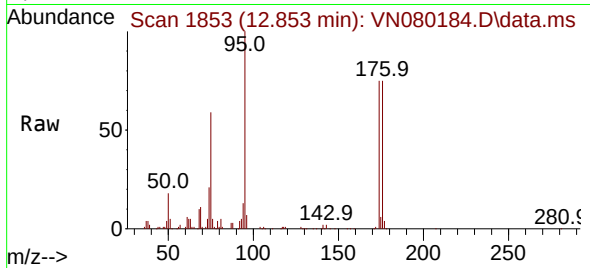

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.006 min
Lab File: VN080184.D
Acq: 18 Nov 2023 14:31


Tgt Ion: 117 Resp: 299626
Ion Ratio Lower Upper
117 100
82 59.3 44.0 66.0
119 33.1 25.6 38.4

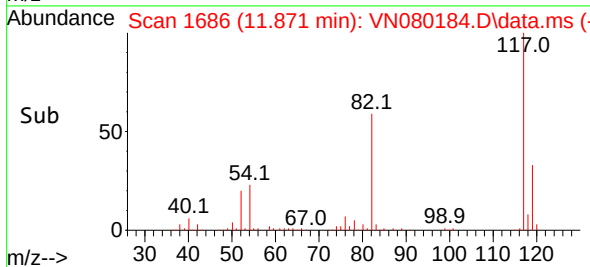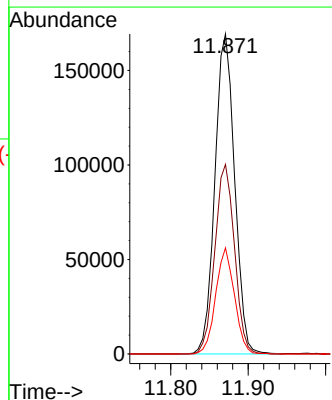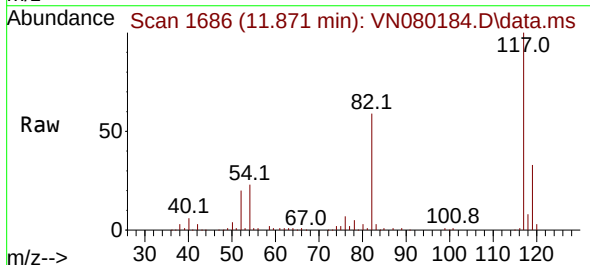

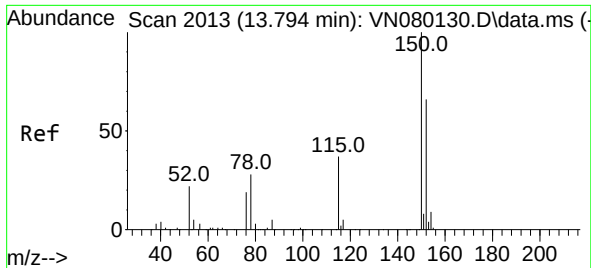

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VN080184.D
 Acq: 18 Nov 2023 14:31

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-1

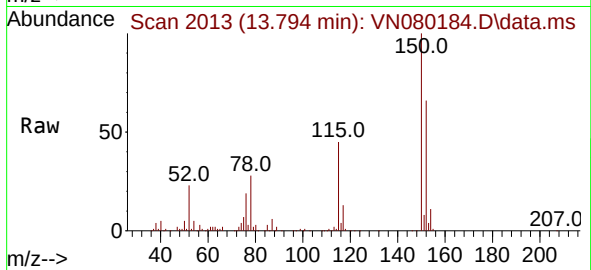

Tgt Ion:152 Resp: 130370
 Ion Ratio Lower Upper
 152 100
 115 65.6 32.3 96.8
 150 156.1 0.0 355.8

