


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111823\
Data File : VN080178.D
Acq On : 18 Nov 2023 11:48
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

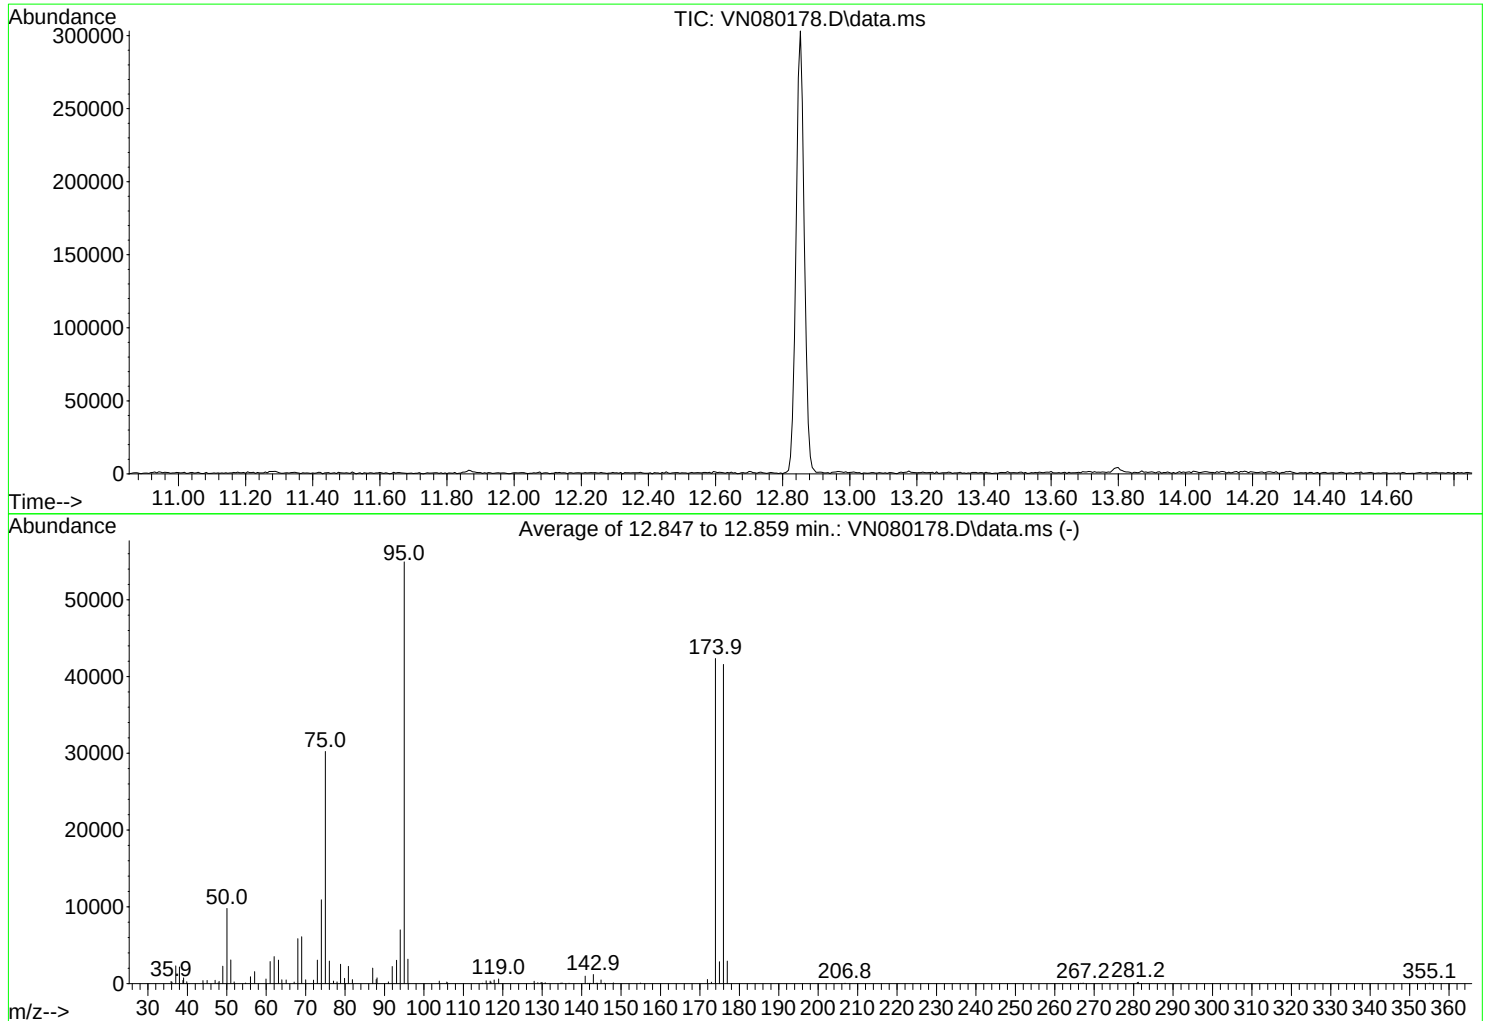

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.8	9794	PASS
75	95	30	60	55.1	30243	PASS
95	95	100	100	100.0	54936	PASS
96	95	5	9	5.8	3194	PASS
173	174	0.00	2	0.5	194	PASS
174	95	50	100	77.1	42339	PASS
175	174	5	9	6.7	2848	PASS
176	174	95	101	98.2	41579	PASS
177	176	5	9	7.1	2946	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	293	48.05	303	63.10	3073	76.00	2941
36.10	203	49.00	2273	63.95	511	77.05	33
37.05	2325	50.05	9794	65.05	482	77.95	23
38.00	2176	51.00	3078	67.10	219	78.85	251
38.90	415	51.85	227	68.00	5854	79.85	685
39.05	759	54.80	95	69.00	6106	80.85	2246
39.85	258	56.00	901	70.00	509	81.85	516
43.95	397	57.05	1556	72.00	455	87.00	2013
45.00	421	59.95	602	72.95	3068	87.90	549
47.05	441	61.00	2879	74.00	10910	88.10	753
47.80	109	62.00	3530	75.00	30243	91.00	234

Average of 12.847 to 12.859 min.: VN080178.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.95	2220	117.00	214	140.90	978	172.90	194
93.05	3038	117.80	488	141.60	55	173.95	42339
94.00	7004	118.95	614	142.10	63	174.95	2848
95.00	54936	127.95	306	142.95	1180	175.95	41579
95.95	3194	128.90	123	143.70	55	176.95	2946
103.90	324	129.70	139	144.00	60	206.80	66
105.80	218	129.95	165	144.90	485	266.60	59
106.00	103	130.75	135	145.80	57	267.20	94
114.80	62	134.70	62	148.05	115	280.95	165
115.80	371	135.00	106	154.90	75	281.20	186
116.80	342	136.80	58	171.90	543	355.10	87

Instrument :

MSVOA_N

ClientSampleId :

BFB