
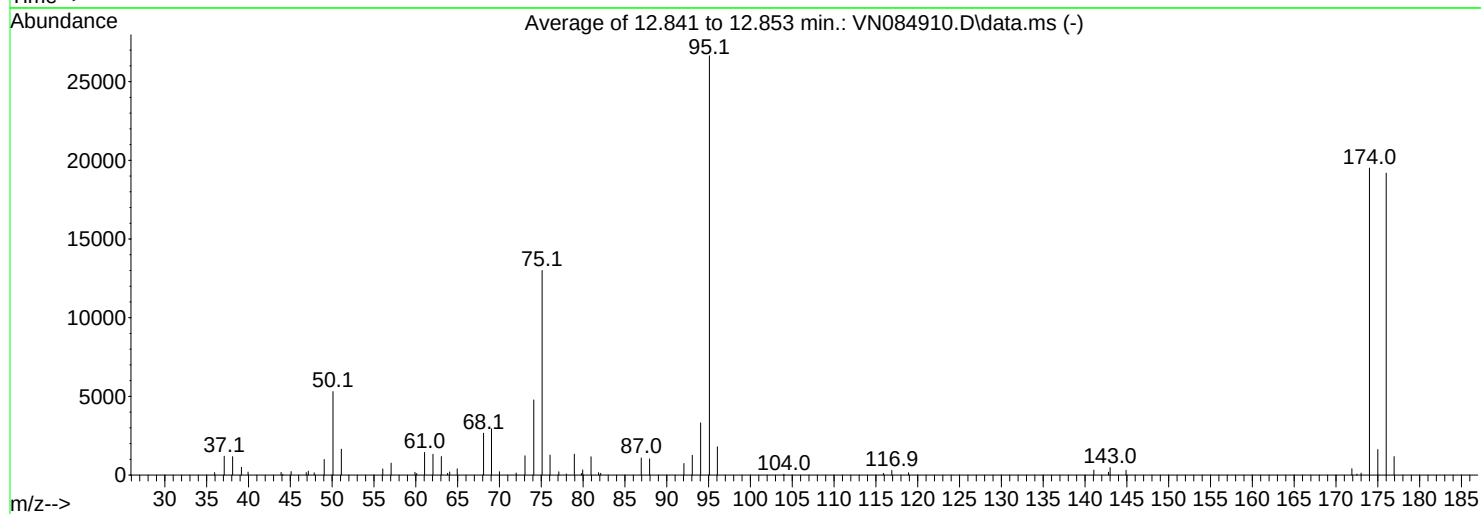


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111824\
Data File : VN084910.D
Acq On : 18 Nov 2024 08:47
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

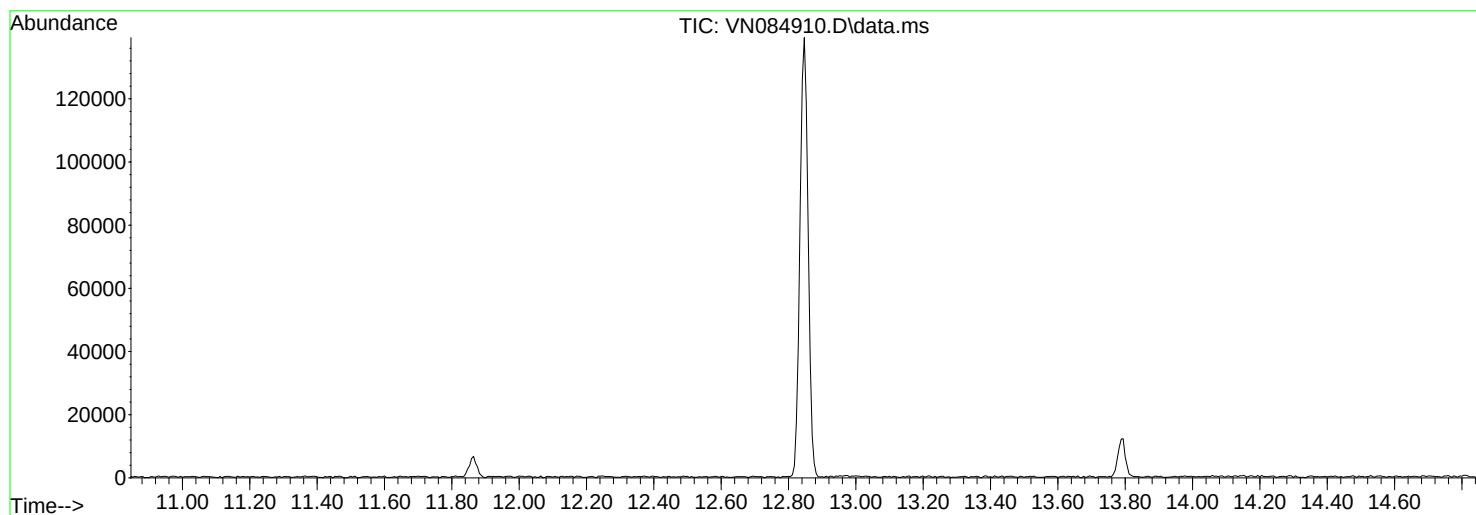

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	5305	PASS
75	95	30	60	48.8	13002	PASS
95	95	100	100	100.0	26645	PASS
96	95	5	9	6.8	1800	PASS
173	174	0.00	2	0.6	124	PASS
174	95	50	100	73.2	19507	PASS
175	174	5	9	8.3	1624	PASS
176	174	95	101	98.4	19189	PASS
177	176	5	9	6.1	1178	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	158	49.05	991	64.05	202	78.00	69
37.10	1200	50.10	5305	64.95	396	78.95	1328
38.10	1172	51.10	1647	68.10	2662	79.80	101
39.15	495	56.05	392	69.05	2940	79.95	329
39.95	191	57.05	760	70.00	216	80.95	1166
43.90	171	59.90	177	72.00	134	81.85	156
44.10	50	60.10	97	73.05	1225	82.10	113
45.10	223	61.05	1439	74.10	4775	86.95	1087
46.90	160	62.05	1320	75.10	13002	87.95	1029
47.15	251	63.05	1176	76.05	1275	92.05	735
47.85	145	63.80	111	77.10	212	93.05	1259

Average of 12.841 to 12.853 min.: VN084910.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.05	3316	171.90	407				
95.10	26645	172.50	68				
96.05	1800	173.00	124				
104.00	54	174.00	19507				
115.90	111	175.00	1624				
116.90	299	176.00	19189				
118.90	145	176.95	1178				
141.05	316						
142.80	184						
143.00	474						
144.90	309						

Instrument :

MSVOA_N

ClientSampleId :

BFB