
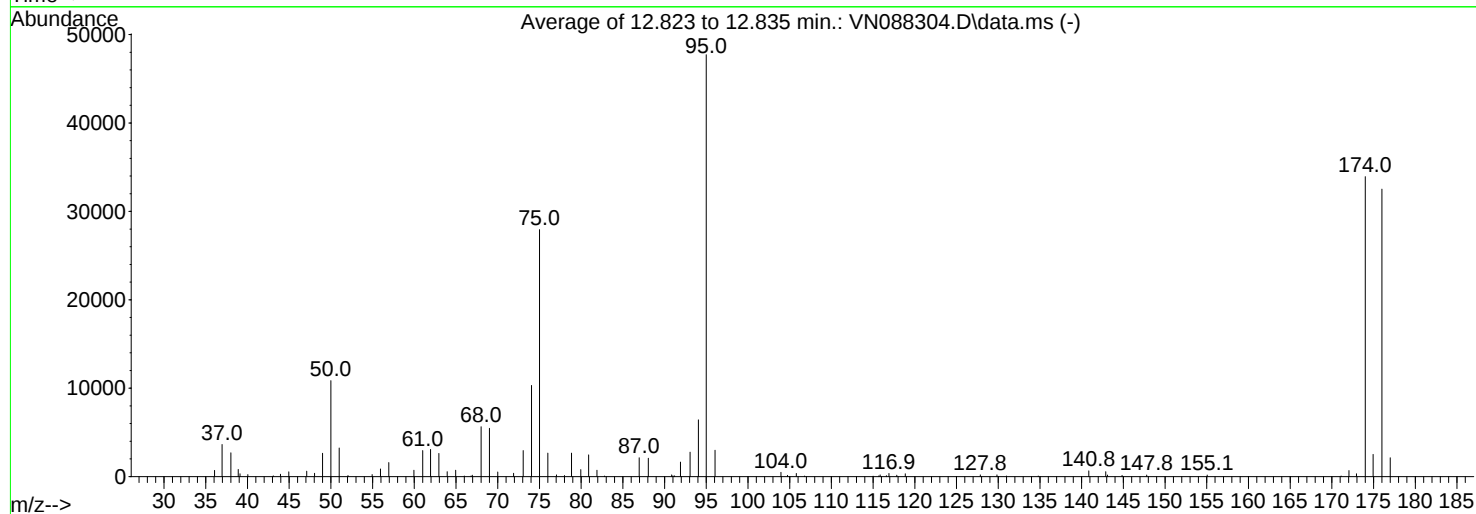


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111825\
Data File : VN088304.D
Acq On : 18 Nov 2025 08:28
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N102325W.M
Title : SW846 8260
Last Update : Mon Nov 03 01:16:06 2025

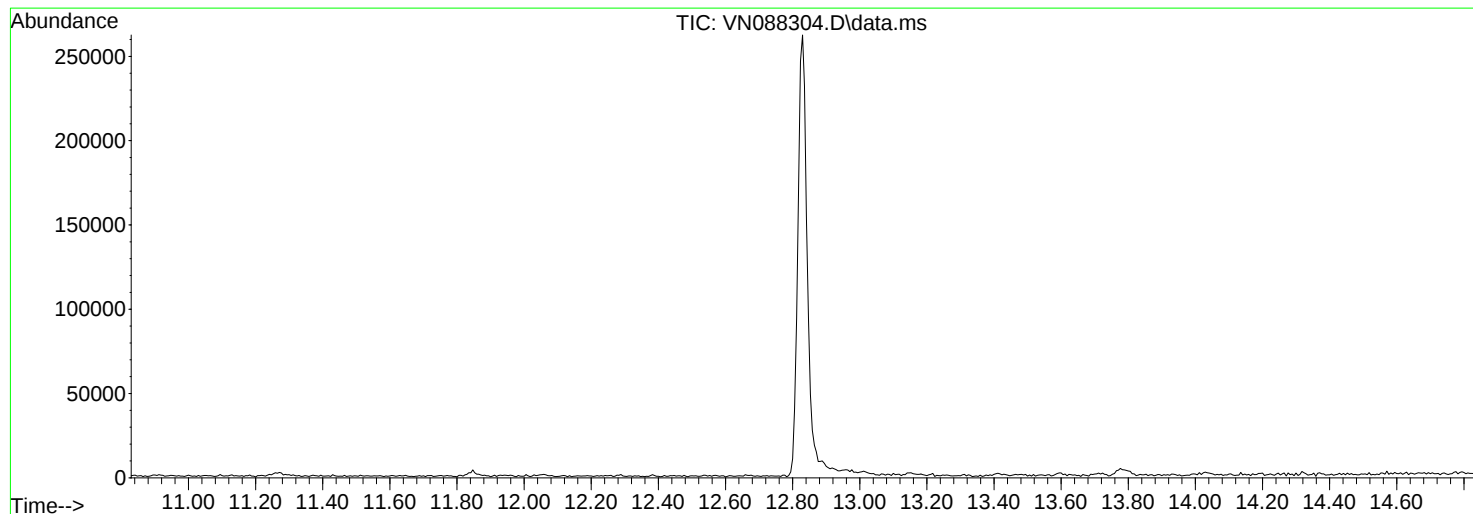

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.7	10855	PASS
75	95	30	60	58.5	27939	PASS
95	95	100	100	100.0	47723	PASS
96	95	5	9	6.3	2987	PASS
173	174	0.00	2	1.0	324	PASS
174	95	50	100	71.1	33933	PASS
175	174	5	9	7.4	2505	PASS
176	174	95	101	95.8	32515	PASS
177	176	5	9	6.5	2120	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	696	49.00	2631	63.95	544	75.00	27939
36.95	3630	50.00	10855	64.95	720	76.00	2660
38.00	2688	51.00	3237	66.00	66	77.05	182
38.90	806	52.05	117	66.80	60	78.00	122
39.10	321	54.95	230	66.95	161	78.85	2661
40.05	220	55.95	858	68.00	5642	79.95	788
43.10	79	56.95	1579	69.00	5458	80.90	2458
43.95	266	59.95	722	70.00	517	81.90	719
44.95	531	61.00	2939	71.90	380	82.80	56
47.10	608	61.95	3060	73.05	2948	86.95	2123
48.05	378	62.95	2618	74.05	10311	88.05	2072

Average of 12.823 to 12.835 min.: VN088304.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.85	182	106.80	63	134.80	73	174.95	2505
91.00	79	115.00	54	140.85	647	176.00	32515
91.20	88	115.70	77	142.90	546	177.00	2120
91.90	1635	115.85	193	143.10	177		
93.05	2770	116.60	102	144.85	141		
94.05	6412	116.90	359	147.80	170		
95.00	47723	117.85	157	155.05	165		
96.05	2987	118.85	312	171.10	62		
103.95	489	127.85	194	172.05	680		
104.75	145	129.85	188	172.95	324		
105.80	357	131.00	67	174.00	33933		

Instrument :

MSVOA_N

ClientSampleId :

BFB