


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN111918\
 Data File : VN052375.D
 Acq On : 19 Nov 2018 9:02
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
 Title : SW846 8260
 Last Update : Thu Nov 15 03:02:37 2018

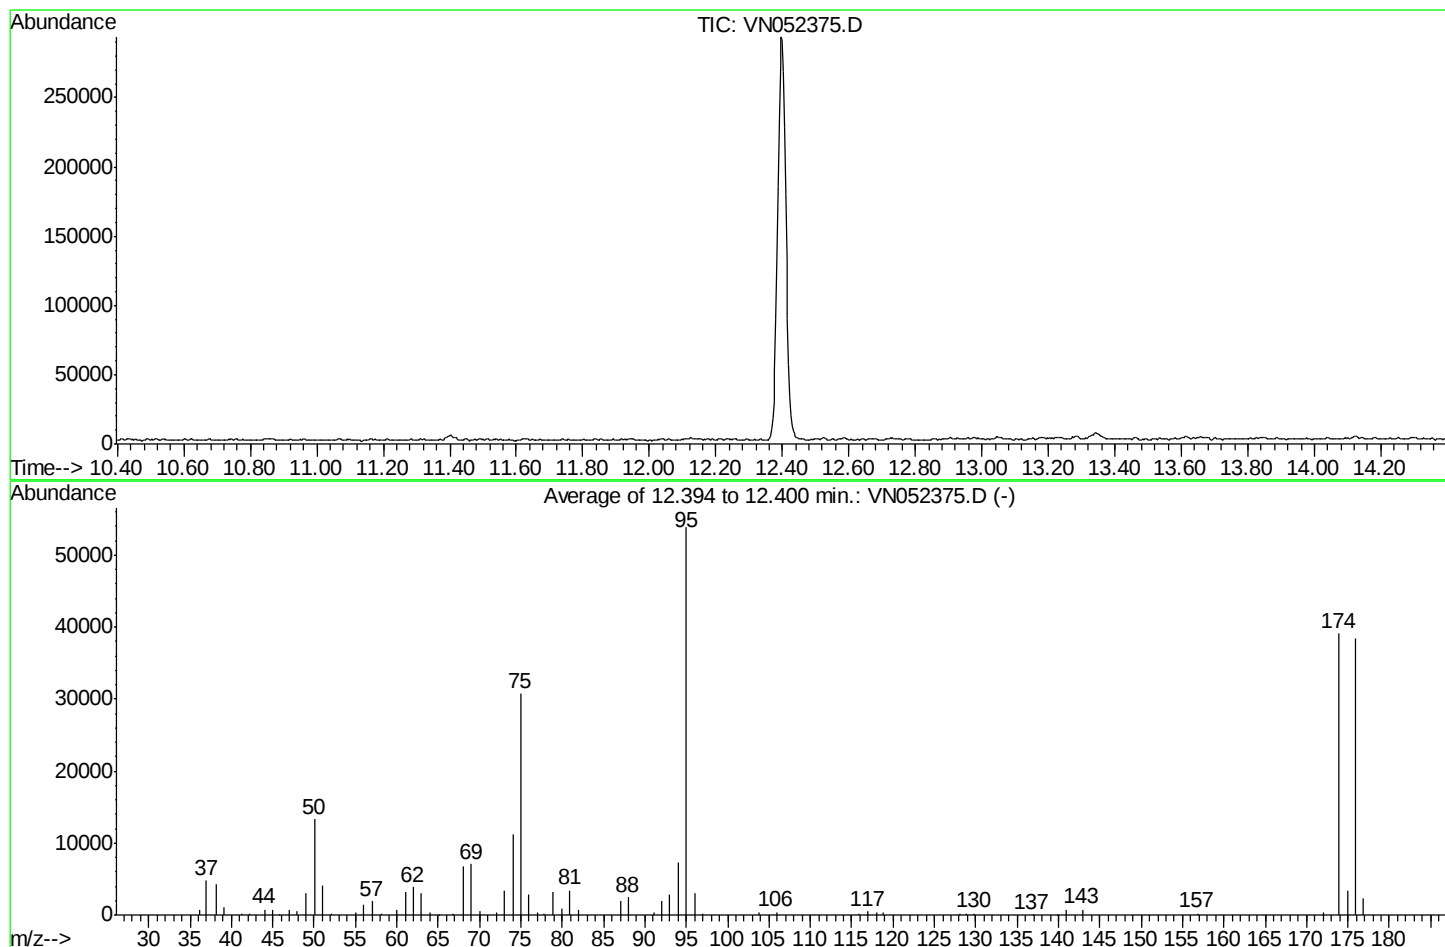

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	13252	PASS
75	95	30	60	57.0	30677	PASS
95	95	100	100	100.0	53845	PASS
96	95	5	9	5.7	3095	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.6	39112	PASS
175	174	5	9	8.7	3395	PASS
176	174	95	101	98.0	38320	PASS
177	176	5	9	6.2	2391	PASS