

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN111920\
 Data File : VN064768.D
 Acq On : 20 Nov 2020 8:19
 Operator : JC/MD
 Sample : L4779-02 50X
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 1641

Quant Time: Nov 20 13:46:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
 Quant Title : SW846 8260
 QLast Update : Wed Nov 18 15:29:54 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.63	168	217072	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.55	114	523885	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.38	117	502369	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.32	152	288322	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.99	65	254967	66.77	ug/l	0.00
Spiked Amount			Recovery	=	133.54%	
35) Dibromofluoromethane	7.55	113	152430	51.12	ug/l	0.00
Spiked Amount			Recovery	=	102.24%	
50) Toluene-d8	10.06	98	569194	42.00	ug/l	0.00
Spiked Amount			Recovery	=	84.00%	
62) 4-Bromofluorobenzene	12.37	95	315058	62.20	ug/l	0.00
Spiked Amount			Recovery	=	124.40%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.73	59	260	0.702	ug/l #	70
13) Acrolein	3.49	56	70	0.807	ug/l #	11
16) Acetone	3.78	43	8412	13.985	ug/l	98
18) Methyl Acetate	4.28	43	1003	1.683	ug/l #	54
20) Methylene Chloride	4.51	84	1129	0.399	ug/l #	78
22) Diisopropyl ether	5.99	45	7714	0.912	ug/l #	1
23) Vinyl Acetate	5.99	43	22478	3.291	ug/l #	75
25) 2-Butanone	6.78	43	369	0.253	ug/l #	51
27) cis-1,2-Dichloroethene	6.78	96	1413	0.492	ug/l	45
29) Tetrahydrofuran	7.17	42	219	0.222	ug/l #	35
30) Chloroform	7.33	83	8696	1.614	ug/l	91
31) Cyclohexane	7.62	56	6803	1.648	ug/l #	30
36) 1,1-Dichloropropene	7.62	75	20592	3.821	ug/l #	50
38) Carbon Tetrachloride	7.63	117	25802	4.505	ug/l #	17
43) Isopropyl Acetate	8.21	43	3449	0.394	ug/l #	64
44) Trichloroethene	8.79	130	1370	0.318	ug/l	86
51) 4-Methyl-2-Pentanone	9.95	43	1470	6.401	ug/l #	39
56) Ethyl methacrylate	10.37	69	66	2.685	ug/l #	1
59) 2-Hexanone	10.72	43	169	8.482	ug/l #	53
68) m/p-Xylenes	11.48	106	68	4.071	ug/l #	43
70) Styrene	11.92	104	31	2.539	ug/l #	24
71) Bromoform	12.37	173	1251	2.830	ug/l #	1
76) 1,2,3-Trichloropropane	12.37	75	164722	26.515	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.37	75	164722	67.770	ug/l #	5
95) Naphthalene	15.10	128	3605	0.222	ug/l #	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN111920\
Data File : VN064768.D
Acq On : 20 Nov 2020 8:19
Operator : JC/MD
Sample : L4779-02 50X
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
1641

Quant Time: Nov 20 13:46:14 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
Quant Title : SW846 8260
QLast Update : Wed Nov 18 15:29:54 2020
Response via : Initial Calibration

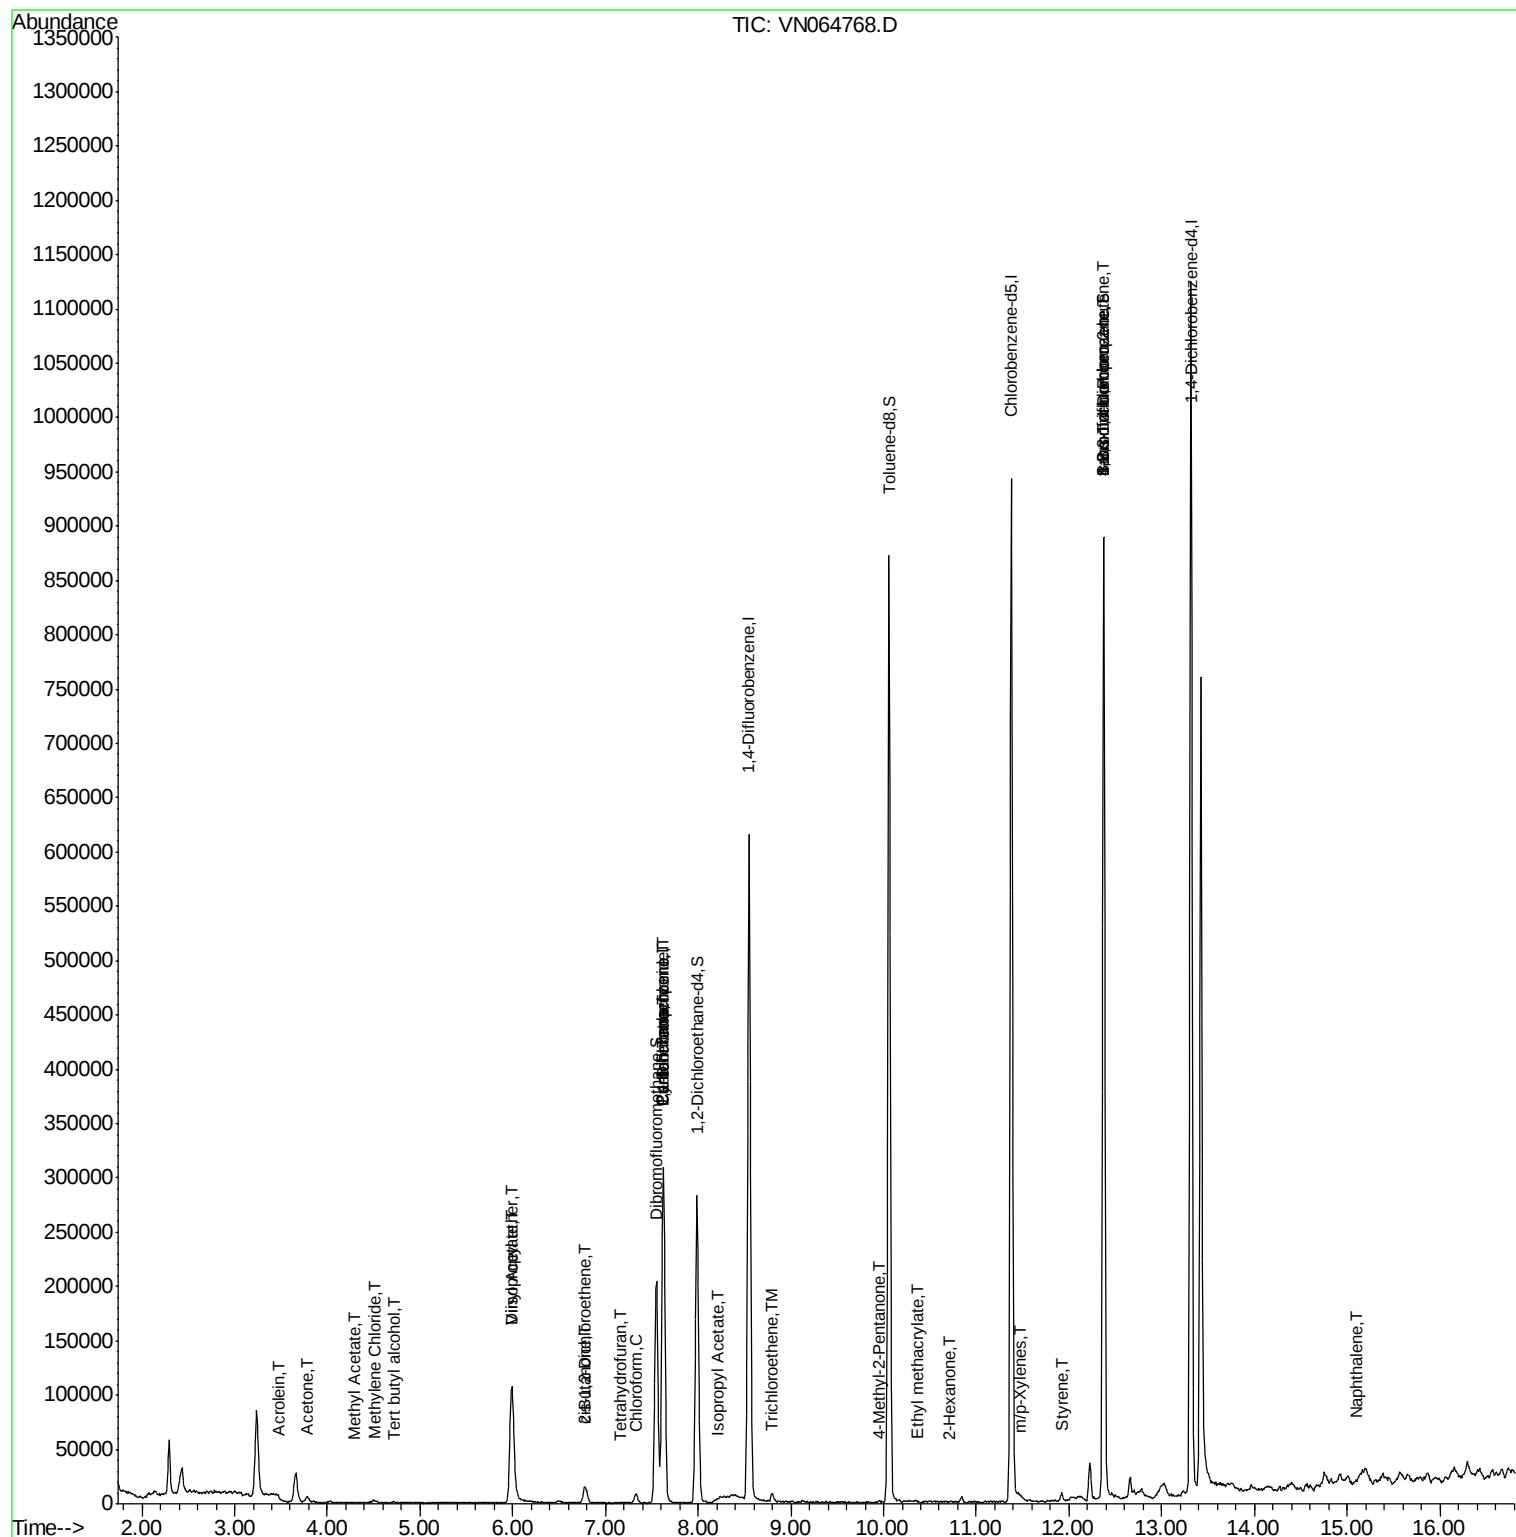



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.63 min Scan# 1831

Delta R.T. 0.00 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19

Instrument :

MSVOA_N

ClientSampled :


1641

Tgt Ion:168 Resp: 217072

Ion Ratio Lower Upper

168 100

99 67.8 55.7 83.5

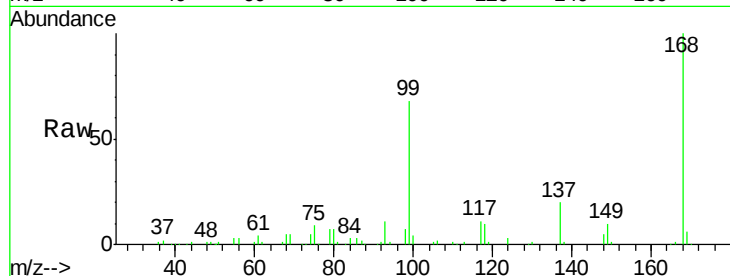

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.63

100000

80000



60000

40000

20000

0

Time--> 7.50 7.60 7.70



#11

Tert butyl alcohol

Concen: 0.702 ug/l

RT: 4.73 min Scan# 931

Delta R.T. -0.00 min

Lab File: VN064768.D


Acq: 20 Nov 2020 8:19

Tgt Ion: 59 Resp: 260

Ion Ratio Lower Upper

59 100

57 0.0 9.1 13.7#



Abundance Ion 59.00 (58.70 to 59.70): VNO

Ion 57.00 (56.70 to 57.70): VNO

4.73


300


200

100

0

Time--> 4.71 4.72 4.73 4.74 4.75



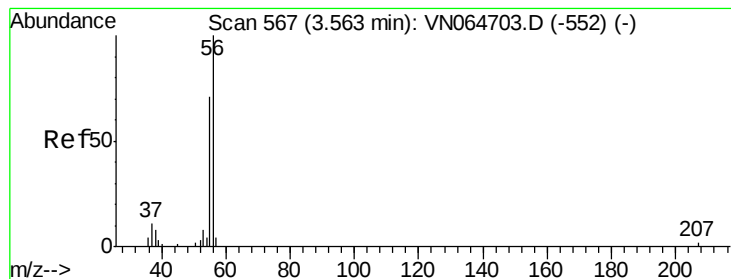

#13

Acrolein

Concen: 0.807 ug/l

RT: 3.49 min Scan# 545

Delta R.T. -0.07 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19

Instrument :

MSVOA_N

ClientSampled :


1641

Tgt Ion: 56 Resp: 70

Ion Ratio Lower Upper




56 100

55 0.0 61.8 92.6#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 55.00 (54.70 to 55.70): VN0

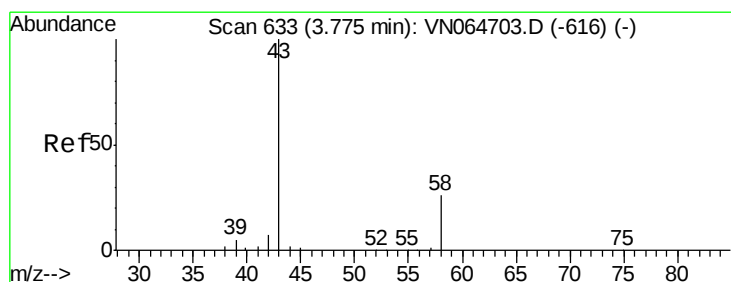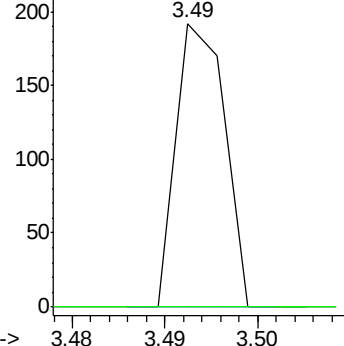

#16

Acetone

Concen: 13.985 ug/l

RT: 3.78 min Scan# 635

Delta R.T. 0.01 min

Lab File: VN064768.D


Acq: 20 Nov 2020 8:19

Tgt Ion: 43 Resp: 8412

Ion Ratio Lower Upper



43 100


58 25.6 21.2 31.8

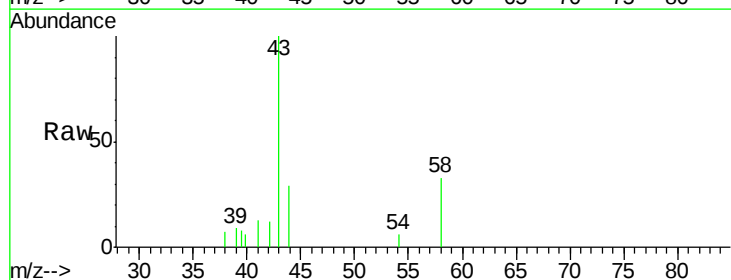

Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0




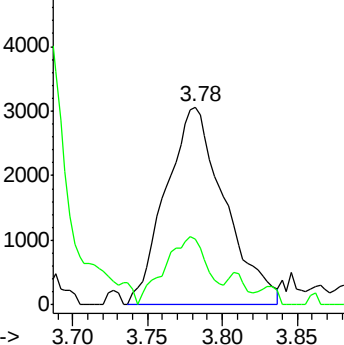




#18
Methyl Acetate
Concen: 1.683 ug/l
RT: 4.28 min Scan# 790
Delta R.T. 0.00 min
Lab File: VN064768.D
Acq: 20 Nov 2020 8:19




Instrument :
MSVOA_N
ClientSampleId :
1641


Tgt Ion: 43 Resp: 1003
Ion Ratio Lower Upper
43 100
74 0.0 17.6 26.4#

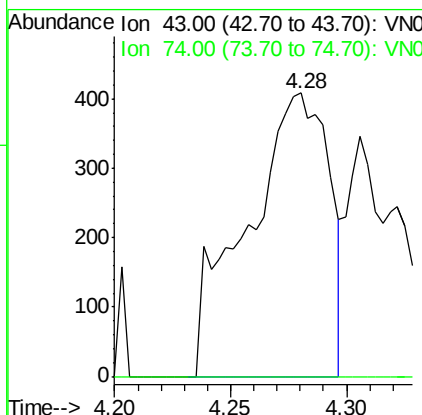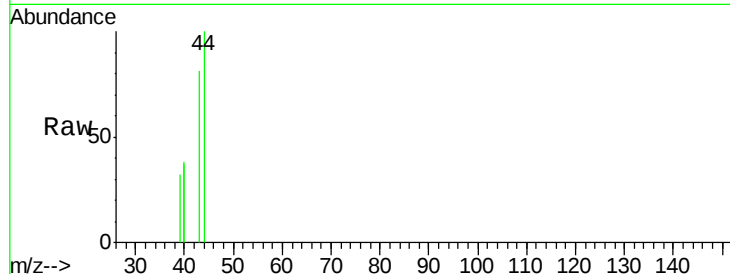

#20
Methylene Chloride
Concen: 0.399 ug/l
RT: 4.51 min Scan# 862
Delta R.T. 0.01 min
Lab File: VN064768.D
Acq: 20 Nov 2020 8:19

Tgt Ion: 84 Resp: 1129
Ion Ratio Lower Upper
84 100
49 107.0 102.4 153.6
51 39.4 29.4 44.2
86 34.1 51.2 76.8#

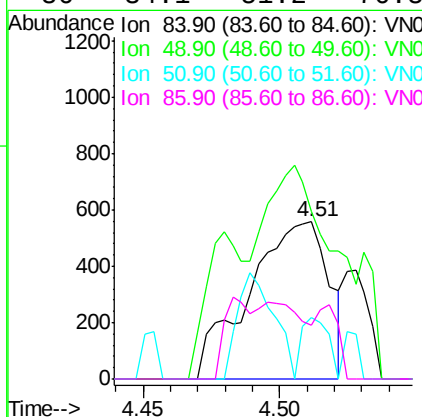

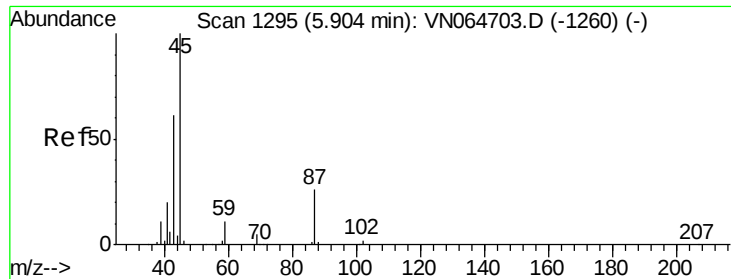

#22

Diisopropyl ether

Concen: 0.912 ug/l

RT: 5.99 min Scan# 1321

Delta R.T. 0.08 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19

Instrument :

MSVOA_N

ClientSampleId :

1641

Tgt Ion: 45 Resp: 7714


Ion Ratio Lower Upper

45 100

43 277.2 52.3 78.5#

87 0.0 21.6 32.4#

59 881.9 8.7 13.1#



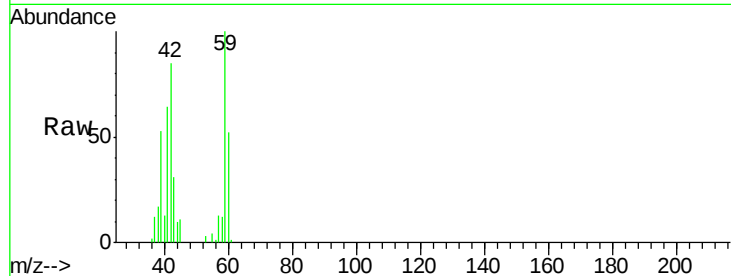


Abundance Ion 45.00 (44.70 to 45.70): VN0

Ion 43.00 (42.70 to 43.70): VN0

Ion 87.00 (86.70 to 87.70): VN0

Ion 59.00 (58.70 to 59.70): VN0

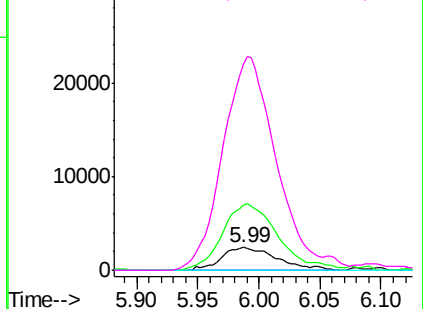

#23

Vinyl Acetate

Concen: 3.291 ug/l

RT: 5.99 min Scan# 1322

Delta R.T. 0.14 min

Lab File: VN064768.D


Acq: 20 Nov 2020 8:19

Tgt Ion: 43 Resp: 22478

Ion Ratio Lower Upper



43 100


86 0.0 7.4 11.0#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 86.00 (85.70 to 86.70): VN0




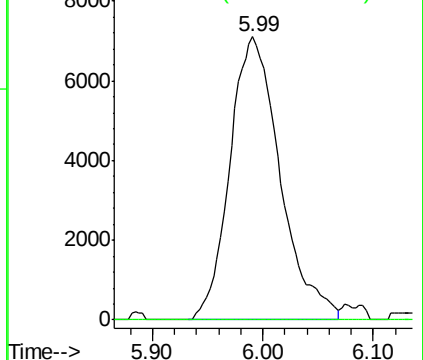


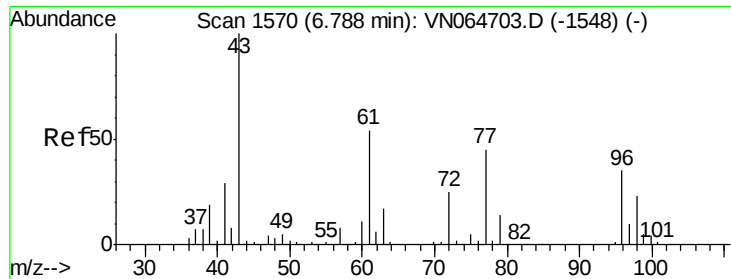

#25
2-Butanone
Concen: 0.253 ug/l
RT: 6.78 min Scan# 1569
Delta R.T. -0.00 min
Lab File: VN064768.D
Acq: 20 Nov 2020 8:19




Instrument :
MSVOA_N
ClientSampled :
1641


Tgt Ion: 43 Resp: 369
Ion Ratio Lower Upper
43 100
72 0.0 19.7 29.5#

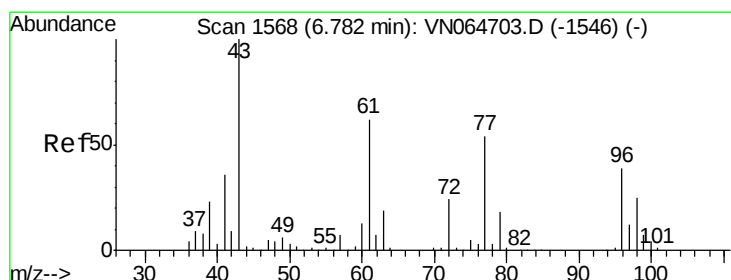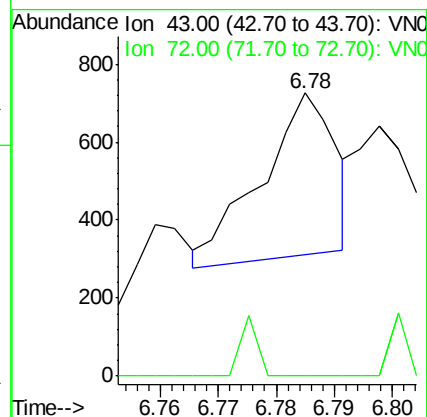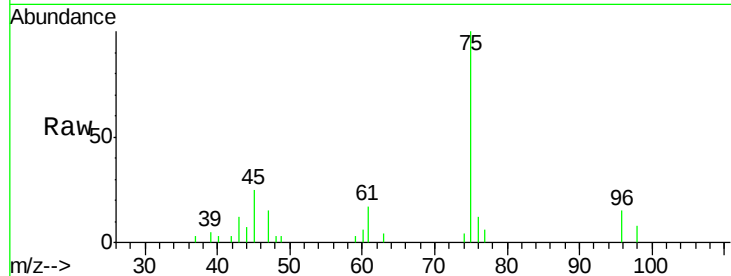

#27
cis-1,2-Dichloroethene
Concen: 0.492 ug/l
RT: 6.78 min Scan# 1569
Delta R.T. 0.00 min
Lab File: VN064768.D
Acq: 20 Nov 2020 8:19

Tgt Ion: 96 Resp: 1413
Ion Ratio Lower Upper
96 100
61 68.0 0.0 322.6
98 77.4 0.0 128.6

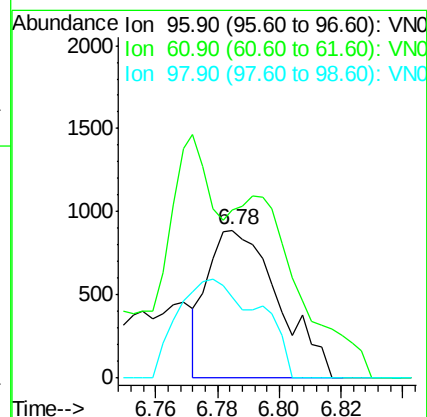



#29

Tetrahydrofuran

Concen: 0.222 ug/l

RT: 7.17 min Scan# 1690

Delta R.T. 0.01 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19

Instrument :

MSVOA_N

ClientSampled :

1641





Tgt Ion: 42 Resp: 219

Ion Ratio Lower Upper

42 100

72 0.0 33.0 49.4#

71 0.0 31.8 47.6#

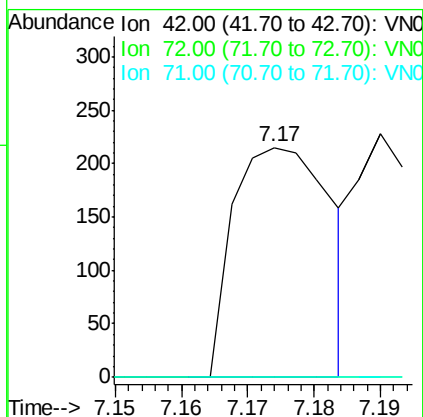

#30

Chloroform

Concen: 1.614 ug/l

RT: 7.33 min Scan# 1738

Delta R.T. -0.00 min

Lab File: VN064768.D




Acq: 20 Nov 2020 8:19


Tgt Ion: 83 Resp: 8696

Ion Ratio Lower Upper

83 100

85 56.0 50.6 75.8

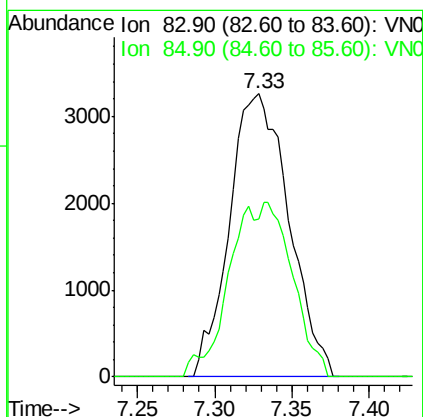


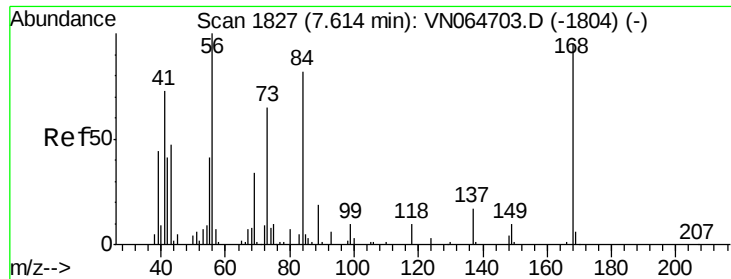




#31
Cyclohexane
Concen: 1.648 ug/l
RT: 7.62 min Scan# 1830
Delta R.T. 0.01 min
Lab File: VN064768.D
Acq: 20 Nov 2020 8:19

Instrument :
MSVOA_N
ClientSampleId :
1641

Tgt Ion: 56 Resp: 6803
Ion Ratio Lower Upper
56 100
69 133.8 27.2 40.8#
84 106.7 65.9 98.9#

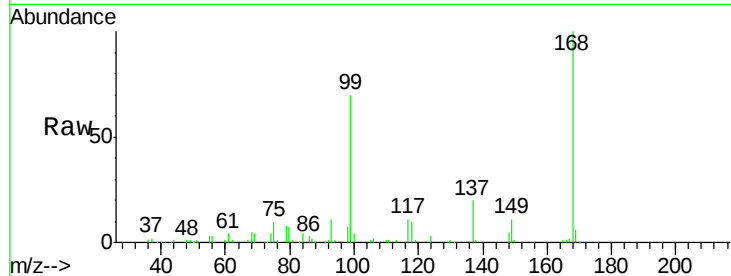


Abundance Ion 56.00 (55.70 to 56.70): VN0
Ion 69.00 (68.70 to 69.70): VN0
Ion 84.00 (83.70 to 84.70): VN0


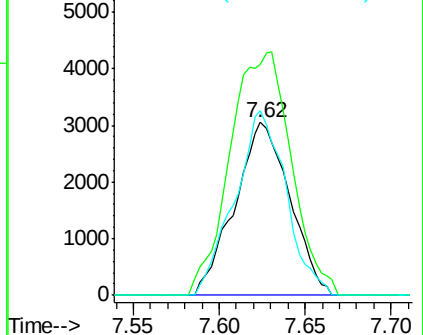



#33
1,2-Dichloroethane-d4
Concen: 66.769 ug/l
RT: 7.99 min Scan# 1943
Delta R.T. -0.00 min
Lab File: VN064768.D
Acq: 20 Nov 2020 8:19

Tgt Ion: 65 Resp: 254967
Ion Ratio Lower Upper
65 100
67 50.9 0.0 99.8



Abundance Ion 64.90 (64.60 to 65.60): VN0
Ion 66.90 (66.60 to 67.60): VN0

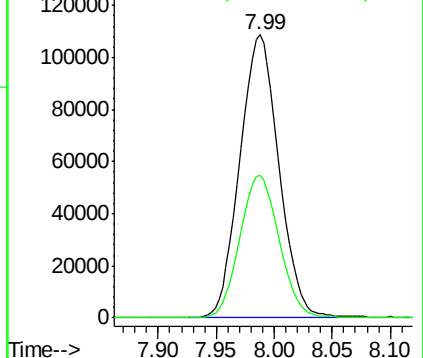


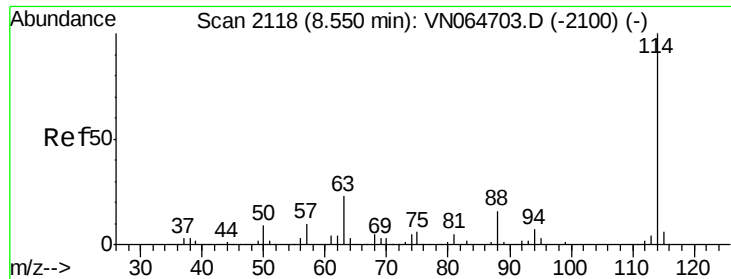




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.55 min Scan# 2118
 Delta R.T. -0.00 min
 Lab File: VN064768.D
 Acq: 20 Nov 2020 8:19

Instrument :
 MSVOA_N
 ClientSampleId :
 1641

Tgt Ion	Ratio	Lower	Upper
114	100		
63	22.0	0.0	46.0
88	16.4	0.0	31.2

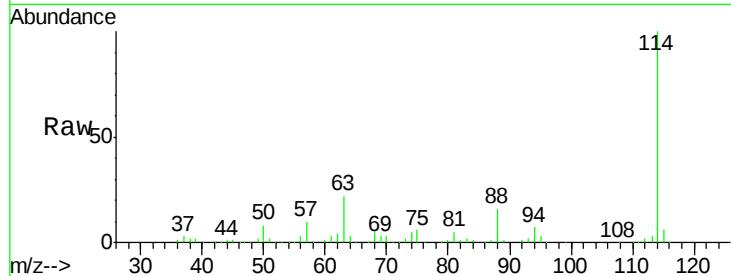


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN


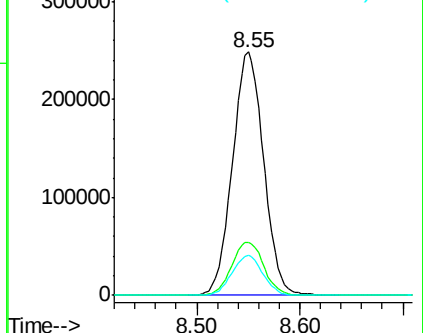



#35
 Dibromofluoromethane
 Concen: 51.120 ug/l
 RT: 7.55 min Scan# 1806
 Delta R.T. -0.00 min
 Lab File: VN064768.D
 Acq: 20 Nov 2020 8:19

Tgt Ion	Ratio	Lower	Upper
113	100		
111	104.0	82.2	123.4
192	15.6	12.7	19.1



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V




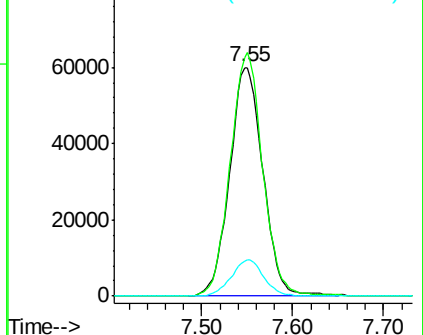


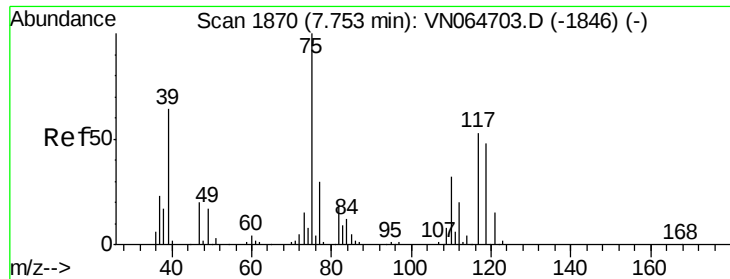

#36
 1,1-Dichloropropene
 Concen: 3.821 ug/l
 RT: 7.62 min Scan# 1830
 Delta R.T. -0.13 min
 Lab File: VN064768.D
 Acq: 20 Nov 2020 8:19




Instrument :
 MSVOA_N
 ClientSampleId :
 1641


Tgt Ion	Ratio	Lower	Upper
75	100		
110	7.1	16.2	48.6#
77	0.0	24.4	36.6#

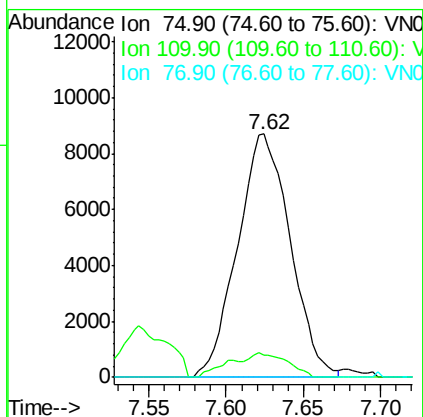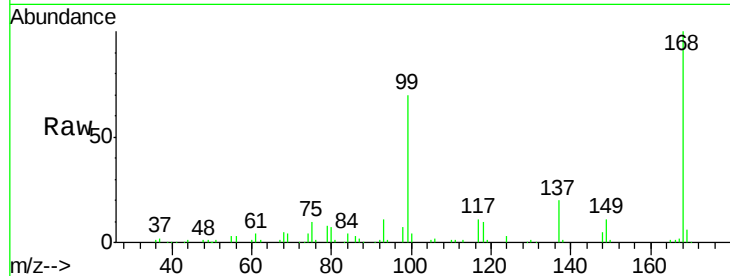

#38
 Carbon Tetrachloride
 Concen: 4.505 ug/l
 RT: 7.63 min Scan# 1832
 Delta R.T. -0.10 min
 Lab File: VN064768.D
 Acq: 20 Nov 2020 8:19

Tgt Ion	Ratio	Lower	Upper
117	100		
119	7.1	77.8	116.6#
121	0.0	24.9	37.3#

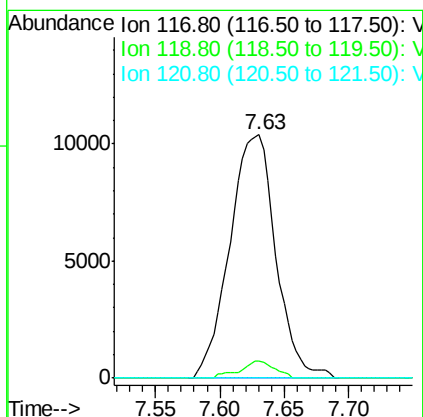



#43

Isopropyl Acetate

Concen: 0.394 ug/l

RT: 8.21 min Scan# 2013

Delta R.T. 0.09 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19

Instrument :

MSVOA_N

ClientSampleId :

1641


Tgt Ion: 43 Resp: 3449

Ion Ratio Lower Upper

43 100

61 0.0 14.1 21.1#




87 0.0 9.1 13.7#

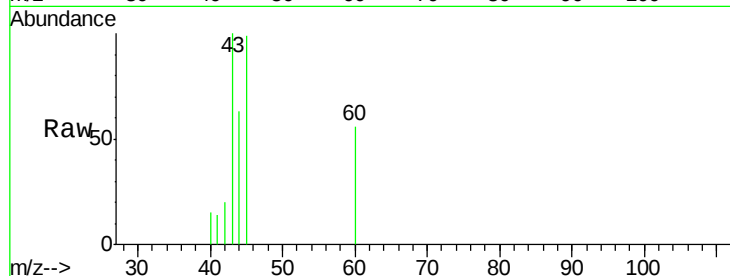

Abundance Ion 43.00 (42.70 to 43.70): VN064768.D (-2013) (-)

Ion 61.00 (60.70 to 61.70): VN064768.D (-2013) (-)

Ion 87.00 (86.70 to 87.70): VN064768.D (-2013) (-)

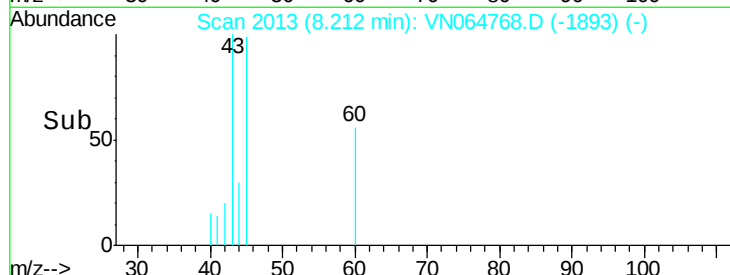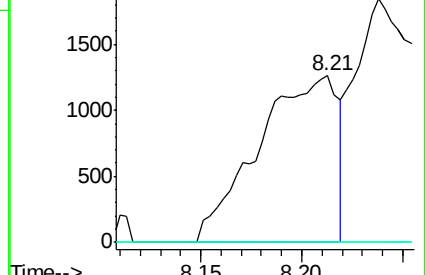

#44

Trichloroethene

Concen: 0.318 ug/l

RT: 8.79 min Scan# 2193

Delta R.T. -0.01 min

Lab File: VN064768.D


Acq: 20 Nov 2020 8:19

Tgt Ion: 130 Resp: 1370

Ion Ratio Lower Upper



130 100


95 92.7 0.0 214.2



Abundance Ion 129.80 (129.50 to 130.50): VN064768.D (-2193) (-)

Ion 94.90 (94.60 to 95.60): VN064768.D (-2193) (-)

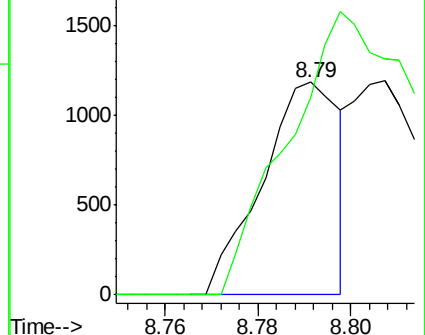



#50

Toluene-d8

Concen: 42.001 ug/l

RT: 10.06 min Scan# 2587

Delta R.T. -0.00 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19

Instrument :

MSVOA_N

ClientSampled :


1641

Tgt Ion: 98 Resp: 569194

Ion Ratio Lower Upper

98 100

100 63.0 50.4 75.6



Abundance Ion 98.00 (97.70 to 98.70): VN064703.D (-2571) (-)

Ion 100.00 (99.70 to 100.70): VN064703.D (-2571) (-)

10.06



300000

200000

100000

0

Time-->



#51

4-Methyl-2-Pentanone

Concen: 6.401 ug/l

RT: 9.95 min Scan# 2553

Delta R.T. -0.00 min

Lab File: VN064768.D


Acq: 20 Nov 2020 8:19

Tgt Ion: 43 Resp: 1470

Ion Ratio Lower Upper

43 100

58 0.0 28.5 42.7#



Abundance Ion 43.00 (42.70 to 43.70): VN064703.D (-2539) (-)

Ion 58.00 (57.70 to 58.70): VN064703.D (-2539) (-)

9.95

1000

800


600


400

200

0

Time-->



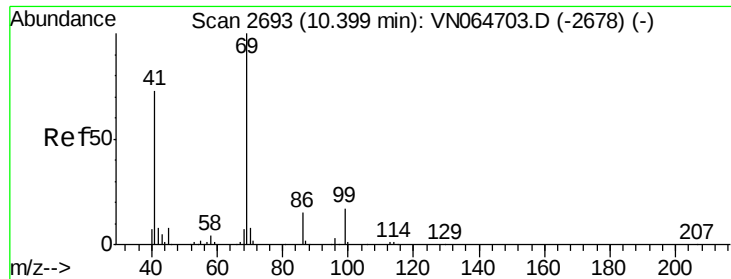

#56

Ethyl methacrylate

Concen: 2.685 ug/l

RT: 10.37 min Scan# 2685

Delta R.T. -0.02 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19





Instrument :

MSVOA_N

ClientSampled :

1641

Tgt Ion:	69	Resp:	66
Ion	Ratio	Lower	Upper
69	100		
41	289.4	59.0	88.4#
39	533.3	38.4	57.6#

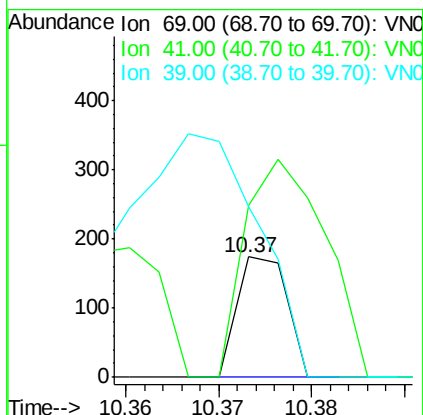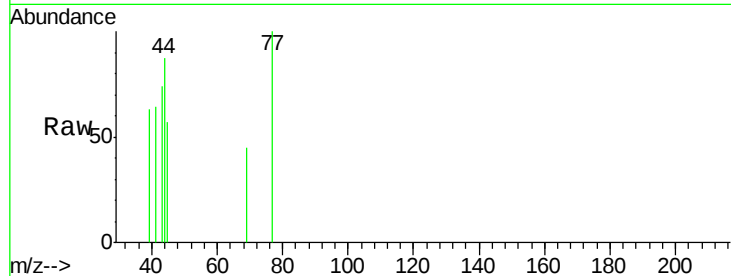

#59

2-Hexanone

Concen: 8.482 ug/l




RT: 10.72 min Scan# 2792


Delta R.T. -0.00 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19

Tgt Ion:	43	Resp:	169
Ion	Ratio	Lower	Upper
43	100		
58	17.2	24.4	73.4#

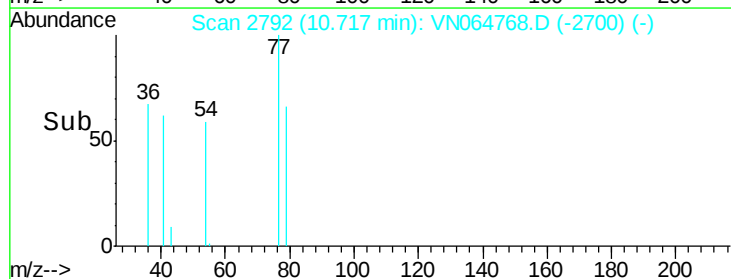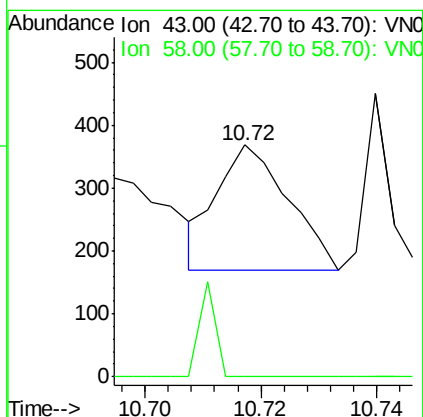



#62

4-Bromofluorobenzene

Concen: 62.198 ug/l

RT: 12.37 min Scan# 3307

Delta R.T. -0.00 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19

Instrument :

MSVOA_N

ClientSampled :

1641


Tgt Ion: 95 Resp: 315058

Ion Ratio Lower Upper

95 100

174 72.1 0.0 136.8




176 69.5 0.0 134.2

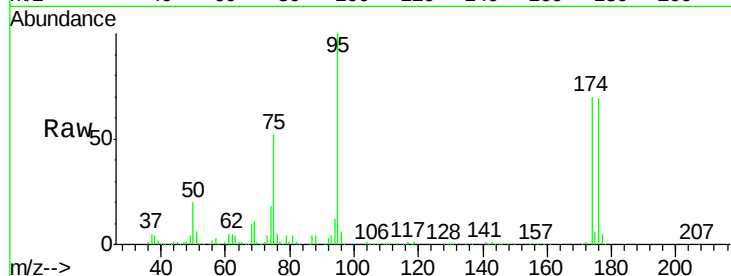

Abundance Ion 94.90 (94.60 to 95.60): VN064768.D (-3214) (-)

Ion 173.80 (173.50 to 174.50): VN064768.D (-3214) (-)

Ion 175.80 (175.50 to 176.50): VN064768.D (-3214) (-)

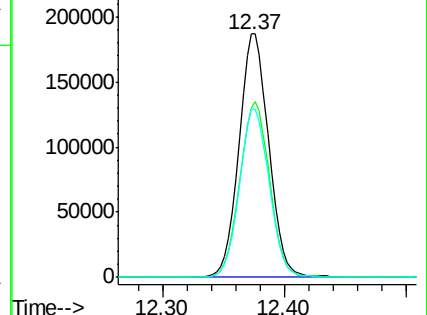

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.38 min Scan# 2998

Delta R.T. 0.00 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19


Tgt Ion: 117 Resp: 502369

Ion Ratio Lower Upper

117 100

82 58.1 47.0 70.6



119 32.1 25.4 38.2




Abundance Ion 116.90 (116.60 to 117.60): VN064768.D (-2904) (-)

Ion 82.00 (81.70 to 82.70): VN064768.D (-2904) (-)

Ion 118.90 (118.60 to 119.60): VN064768.D (-2904) (-)



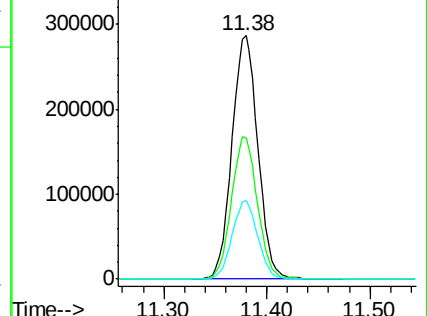



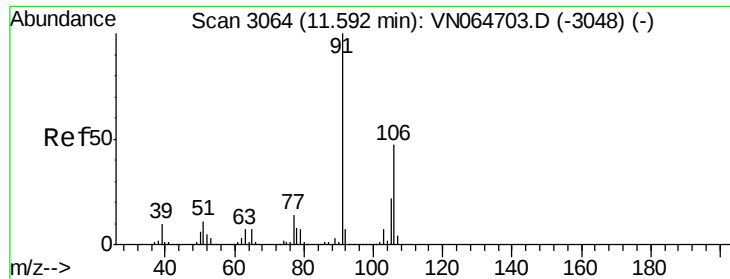

#68
m/p-Xylenes
Concen: 4.071 ug/l
RT: 11.48 min Scan# 3030
Delta R.T. -0.11 min
Lab File: VN064768.D
Acq: 20 Nov 2020 8:19




Instrument :
MSVOA_N
ClientSampleId :
1641


Tgt Ion:106 Resp: 68
Ion Ratio Lower Upper
106 100
91 125.0 171.9 257.9#

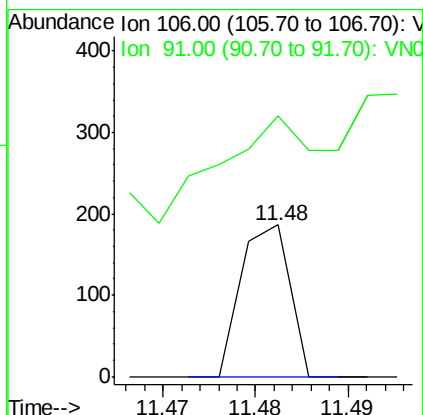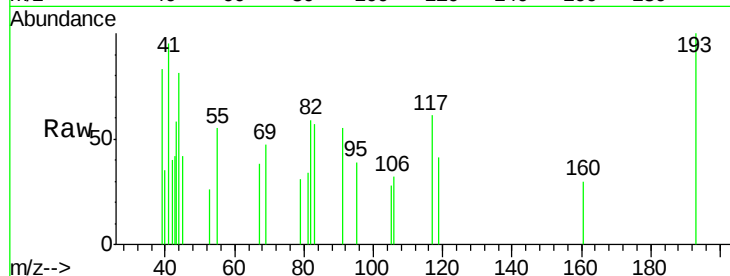

#70
Styrene
Concen: 2.539 ug/l
RT: 11.92 min Scan# 3167
Delta R.T. -0.01 min
Lab File: VN064768.D
Acq: 20 Nov 2020 8:19

Tgt Ion:104 Resp: 31
Ion Ratio Lower Upper
104 100
78 0.0 44.1 66.1#
103 0.0 43.7 65.5#

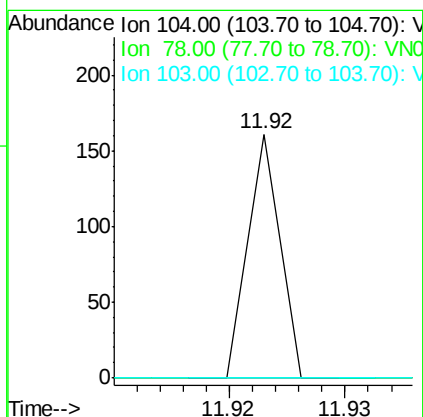



#71

Bromoform

Concen: 2.830 ug/l

RT: 12.37 min Scan# 3306

Delta R.T. 0.27 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19

Instrument :

MSVOA_N

ClientSampleId :

1641


Tgt Ion:173 Resp: 1251

Ion Ratio Lower Upper

173 100

175 1198.1 24.3 72.9#




254 0.0 0.1 0.1#

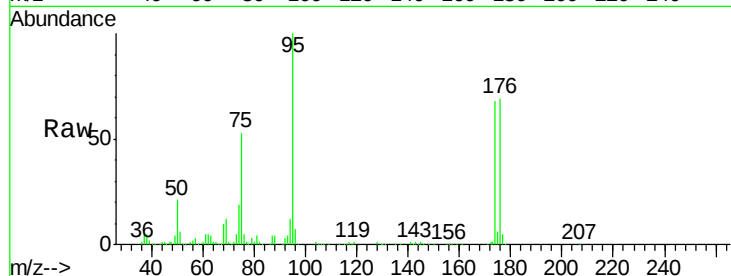

Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

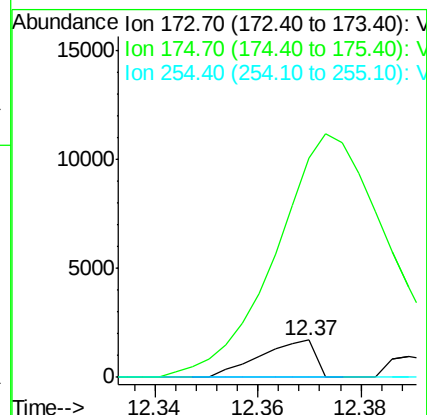

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.32 min Scan# 3600

Delta R.T. -0.00 min

Lab File: VN064768.D

Acq: 20 Nov 2020 8:19


Tgt Ion:152 Resp: 288322

Ion Ratio Lower Upper

152 100

115 63.7 32.1 96.3



150 157.0 0.0 344.8




Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V



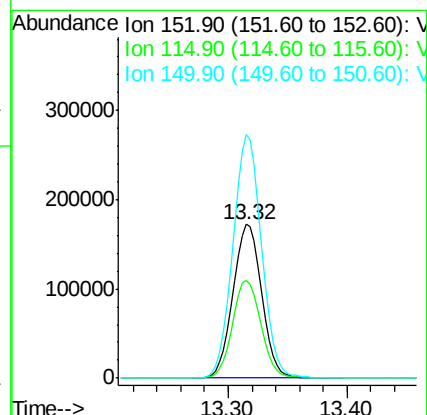





#76
 1,2,3-Trichloropropane
 Concen: 26.515 ug/l
 RT: 12.37 min Scan# 3307
 Delta R.T. -0.15 min
 Lab File: VN064768.D
 Acq: 20 Nov 2020 8:19




Instrument :
 MSVOA_N
 ClientSampled :
 1641


Tgt Ion: 75 Resp: 164722
 Ion Ratio Lower Upper
 75 100
 77 1.3 0.0 0.0#

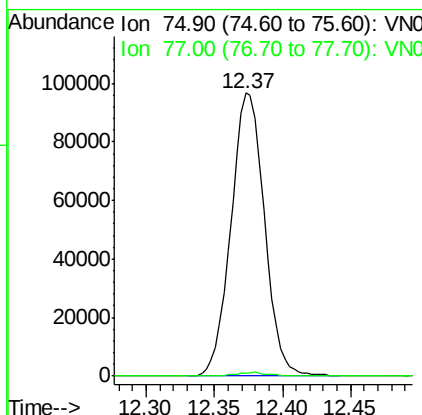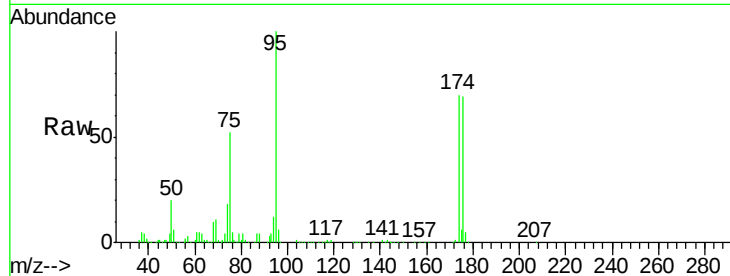

#81
 trans-1,4-Dichloro-2-butene
 Concen: 67.770 ug/l
 RT: 12.37 min Scan# 3307
 Delta R.T. 0.10 min
 Lab File: VN064768.D
 Acq: 20 Nov 2020 8:19

Tgt Ion: 75 Resp: 164722
 Ion Ratio Lower Upper
 75 100
 53 0.2 88.8 133.2#
 89 0.0 43.1 64.7#

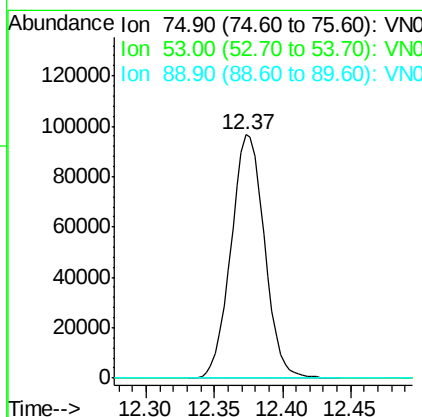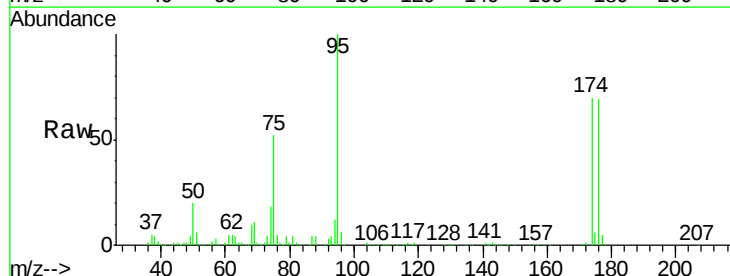

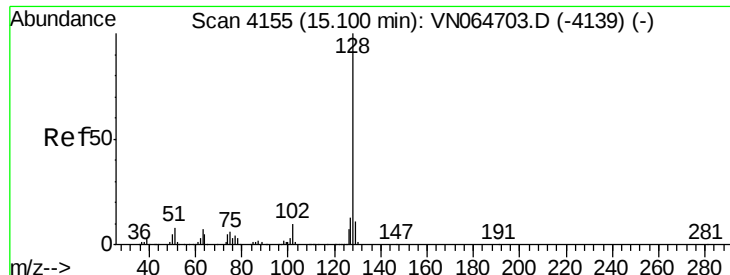

#95

Naphthalene

Concen: 0.222 ug/l

RT: 15.10 min Scan# 4156

Delta R.T. 0.00 min

Lab File: VN064768.D


Acq: 20 Nov 2020 8:19

Instrument :

MSVOA_N

ClientSampleId :

1641




Tgt Ion:128 Resp: 3605

Ion Ratio Lower Upper

128 100

127 3.7 10.8 16.2#

129 0.0 8.9 13.3#



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

