


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN111920\
 Data File : VN064723.D
 Acq On : 19 Nov 2020 10:29
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111820W.M
 Title : SW846 8260
 Last Update : Sat Nov 21 00:39:10 2020

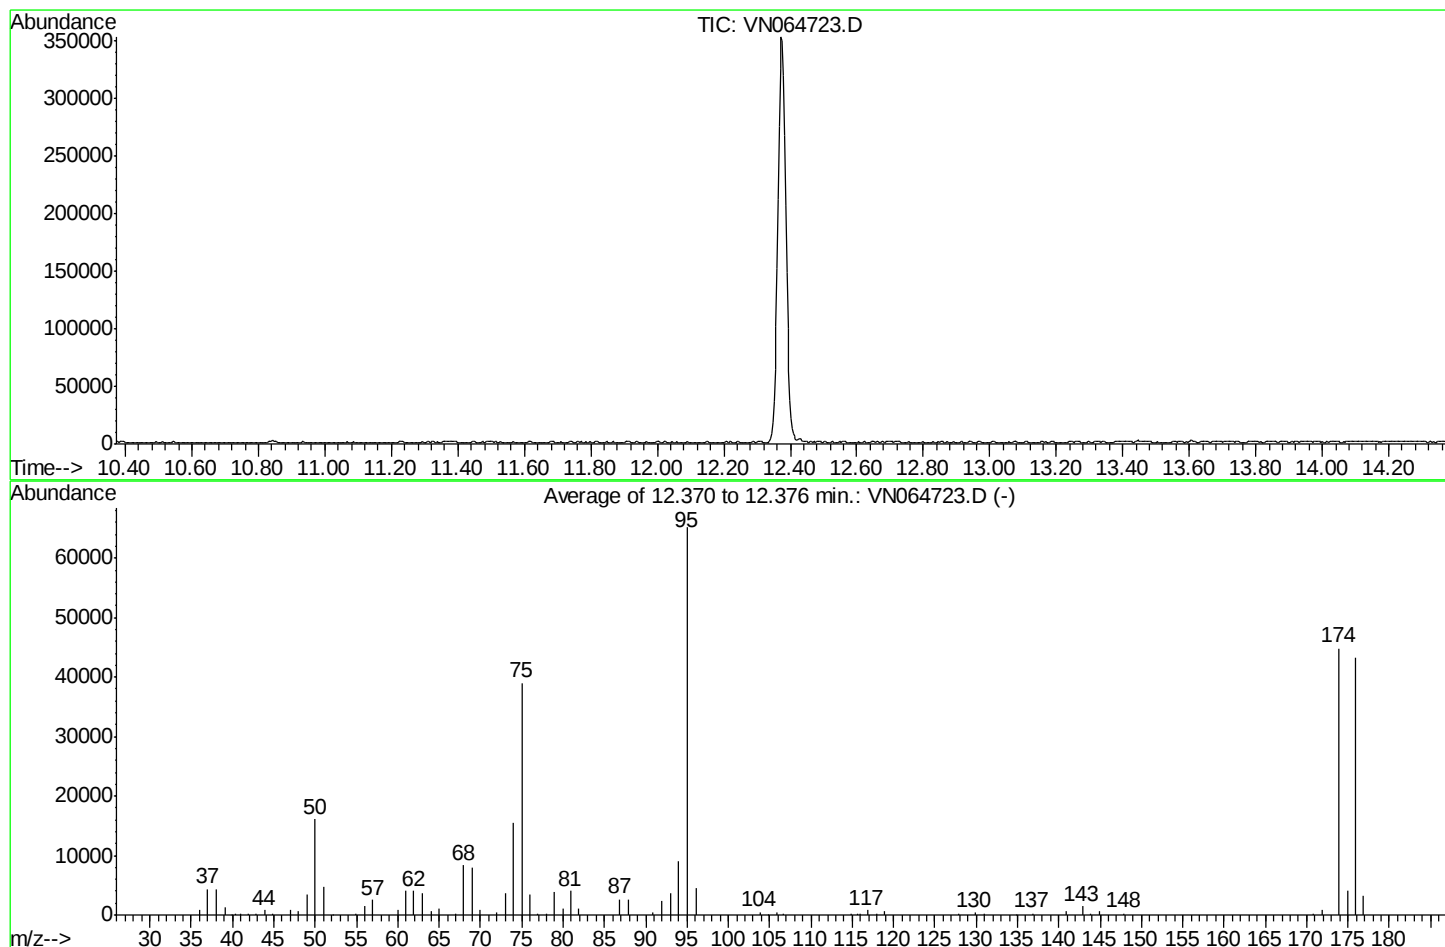

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	16117	PASS
75	95	30	60	59.8	38981	PASS
95	95	100	100	100.0	65186	PASS
96	95	5	9	7.1	4626	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	68.8	44864	PASS
175	174	5	9	8.9	3996	PASS
176	174	95	101	96.7	43362	PASS
177	176	5	9	7.4	3228	PASS