

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111921\
 Data File : VN069598.D
 Acq On : 19 Nov 2021 20:46
 Operator : JC/MD
 Sample : M4768-03
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Nov 22 05:09:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
 Quant Title : SW846 8260
 QLast Update : Tue Nov 09 18:18:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	1341998	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	2325883	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	2342810	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.675	152	929008	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.437	65	987230	50.736	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 101.480%			
35) Dibromofluoromethane	8.024	113	680329	48.770	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 97.540%			
50) Toluene-d8	10.443	98	2953966	53.842	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 107.680%			
62) 4-Bromofluorobenzene	12.734	95	1109478	55.048	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 110.100%			
Target Compounds					Qvalue	
13) Acrolein	4.044	56	500	Below Cal	#	1
16) Acetone	4.293	43	8454	0.805	ug/l #	86
18) Methyl Acetate	4.873	43	9090	0.266	ug/l #	74
31) Cyclohexane	8.086	56	36812	1.385	ug/l #	20
36) 1,1-Dichloropropene	8.088	75	114079	5.829	ug/l #	49
37) Ethyl Acetate	7.421	43	8975	0.339	ug/l #	82
38) Carbon Tetrachloride	8.086	117	139978	7.408	ug/l #	16
43) Isopropyl Acetate	8.636	43	9184	0.216	ug/l #	55
52) Toluene	10.508	92	60621	1.611	ug/l	95
53) t-1,3-Dichloropropene	10.722	75	110	2.642	ug/l #	60
54) cis-1,3-Dichloropropene	10.363	75	58	1.735	ug/l #	65
56) Ethyl methacrylate	10.760	69	297	2.063	ug/l #	24
59) 2-Hexanone	11.092	43	2182	8.033	ug/l	77
60) Dibromochloromethane	11.218	129	54	2.420	ug/l #	11
67) Ethyl Benzene	11.846	91	53300	0.663	ug/l	90
68) m/p-Xylenes	11.950	106	91175	3.082	ug/l	89
69) o-Xylene	12.280	106	42124	1.428	ug/l	90
70) Styrene	12.280	104	3057	1.576	ug/l #	1
73) Isopropylbenzene	12.581	105	57550	0.778	ug/l	94
76) 1,2,3-Trichloropropane	12.731	75	620921	28.962	ug/l #	1
78) n-propylbenzene	12.921	91	69666	0.837	ug/l	95
80) 1,3,5-Trimethylbenzene	13.061	105	14917	0.249	ug/l	93
81) trans-1,4-Dichloro-2-b...	12.731	75	620921	82.018	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.369	105	52826	0.915	ug/l	94
85) sec-Butylbenzene	13.503	105	43404	0.593	ug/l	93
90) Hexachloroethane	14.217	117	8897	2.959	ug/l #	6
92) 1,2-Dibromo-3-Chloropr...	14.640	75	109	1.820	ug/l	69
93) 1,2,4-Trichlorobenzene	15.271	180	552	3.149	ug/l #	1
95) Naphthalene	15.507	128	19279	4.877	ug/l #	93
96) 1,2,3-Trichlorobenzene	15.700	180	782	3.222	ug/l #	55


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111921\
Data File : VN069598.D
Acq On : 19 Nov 2021 20:46
Operator : JC/MD
Sample : M4768-03
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Nov 22 05:09:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N110921W.M
Quant Title : SW846 8260
QLast Update : Tue Nov 09 18:18:22 2021
Response via : Initial Calibration




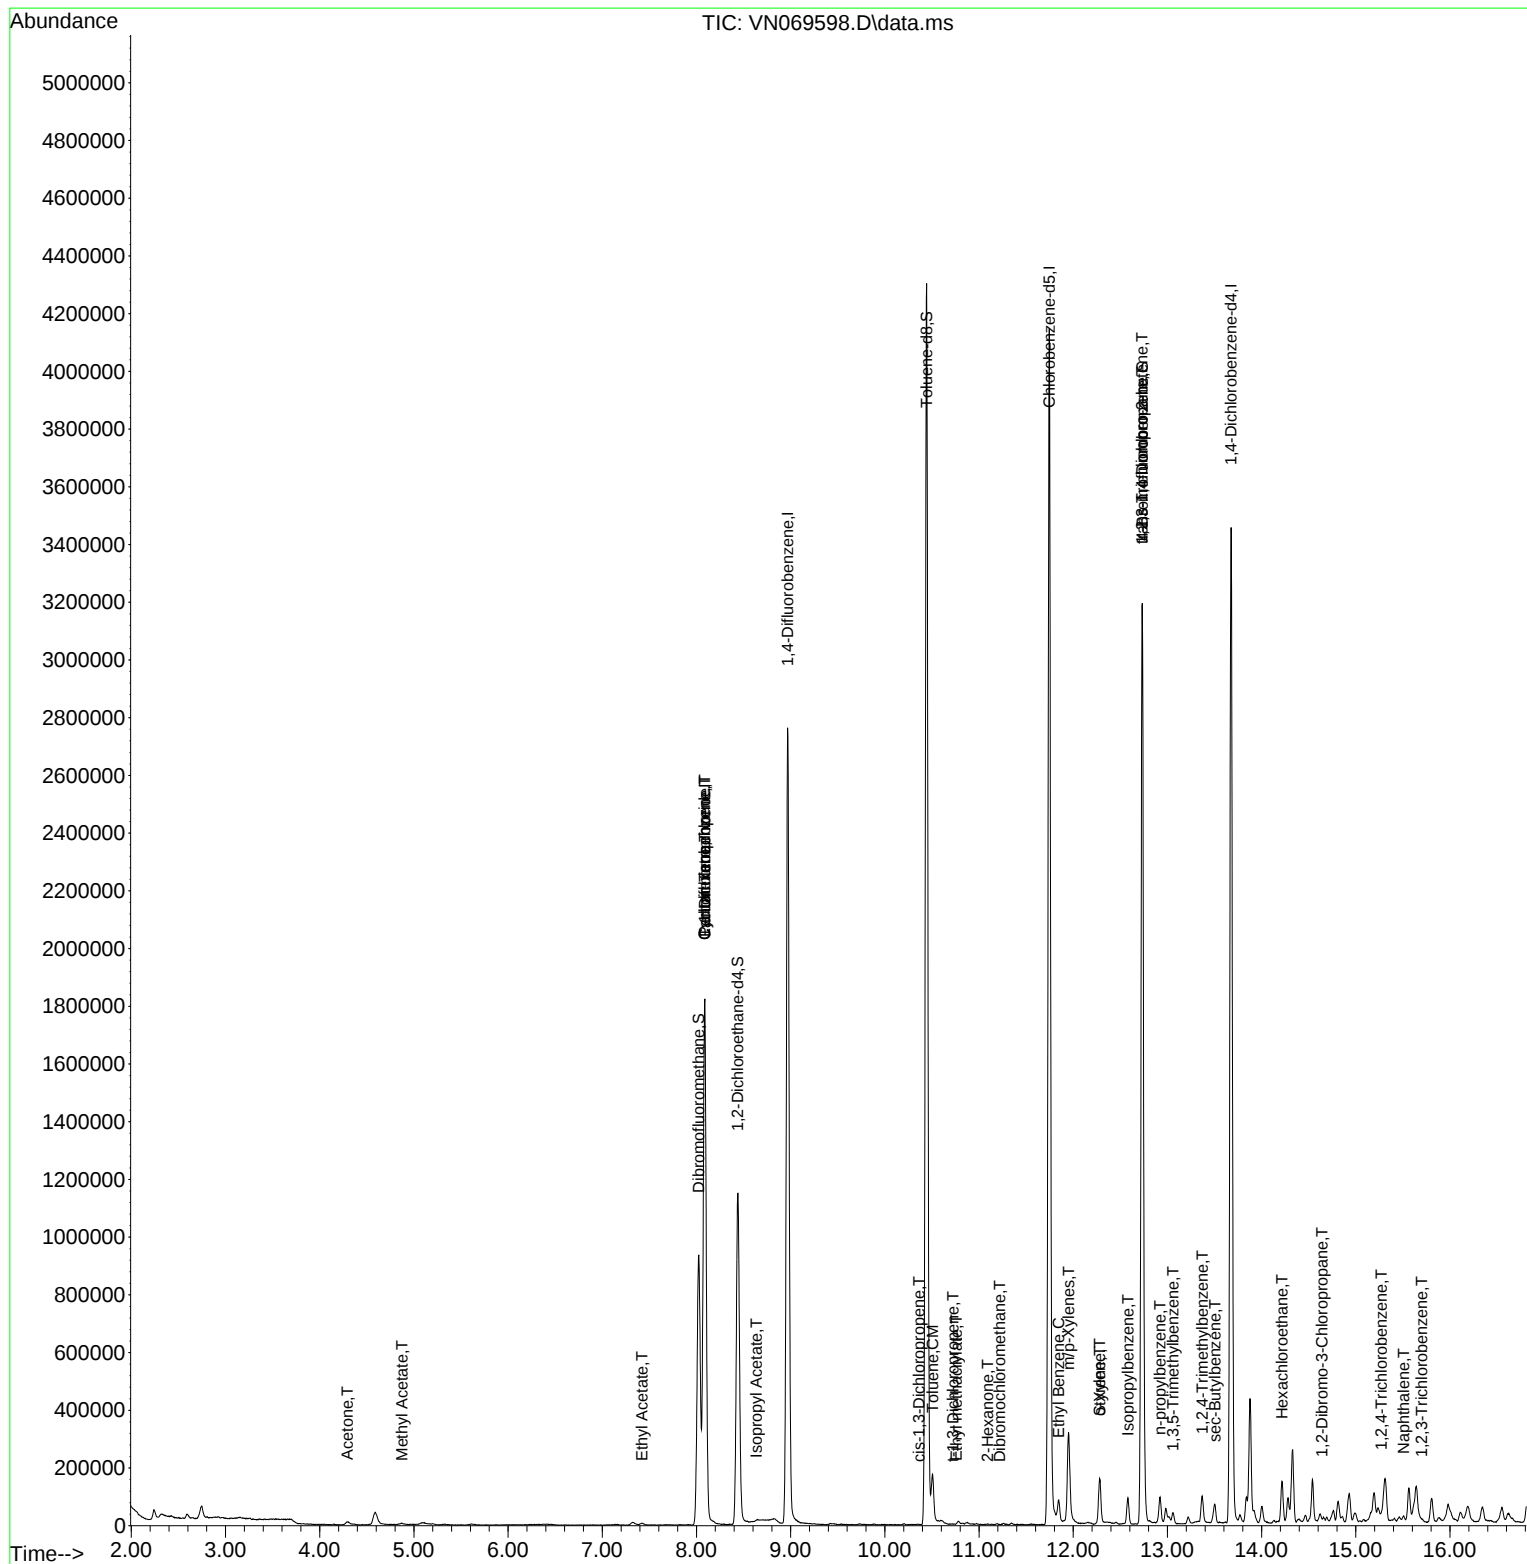




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 21
Delta R.T. 0.002 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 1341998
Ion Ratio Lower Upper
168 100
99 59.8 41.3 61.9

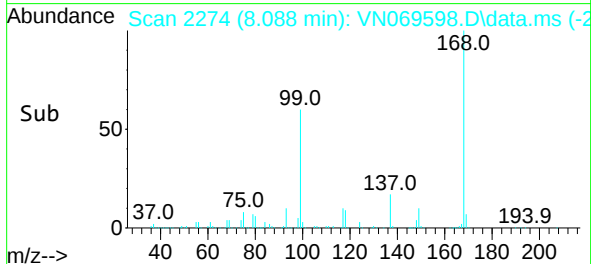

#13
Acrolein
Concen: Below Cal
RT: 4.044 min Scan# 766
Delta R.T. 0.003 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Tgt Ion: 56 Resp: 500
Ion Ratio Lower Upper
56 100
55 162.8 56.6 85.0#


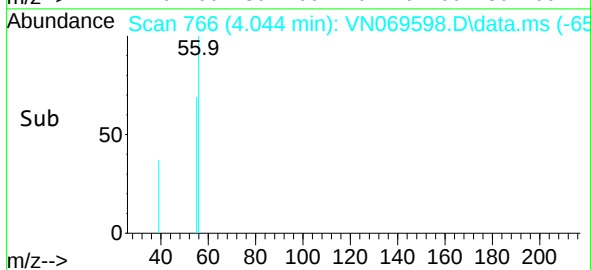






#16
Acetone
Concen: 0.805 ug/l
RT: 4.293 min Scan# 81
Delta R.T. 0.005 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 8454
Ion Ratio Lower Upper
43 100
58 21.2 23.1 34.7#

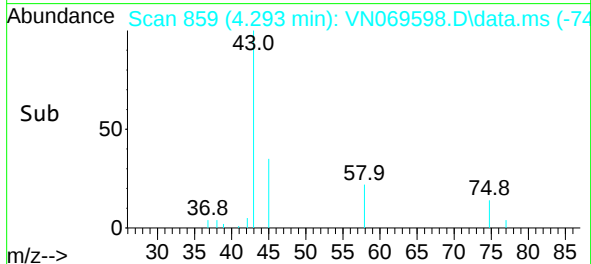

#18
Methyl Acetate
Concen: 0.266 ug/l
RT: 4.873 min Scan# 1075
Delta R.T. 0.016 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46


Tgt Ion: 43 Resp: 9090
Ion Ratio Lower Upper
43 100
74 11.5 19.4 29.2#

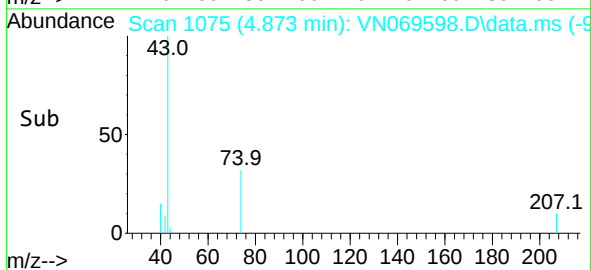






#31
Cyclohexane
Concen: 1.385 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.008 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 56 Resp: 36812
Ion Ratio Lower Upper
56 100
69 151.6 27.1 40.7#
84 123.9 73.4 110.0#

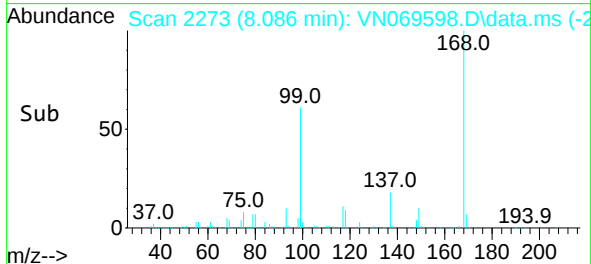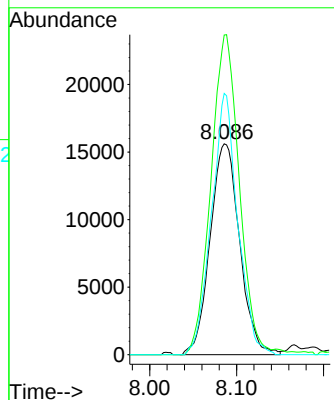

#33
1,2-Dichloroethane-d4
Concen: 50.736 ug/l
RT: 8.437 min Scan# 2404
Delta R.T. -0.003 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46


Tgt Ion: 65 Resp: 987230
Ion Ratio Lower Upper
65 100
67 51.4 0.0 103.0

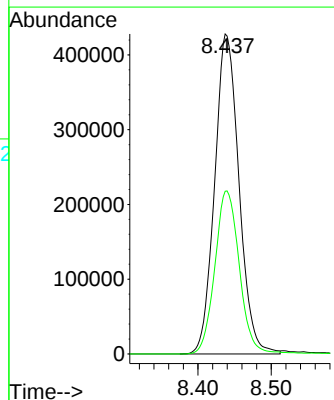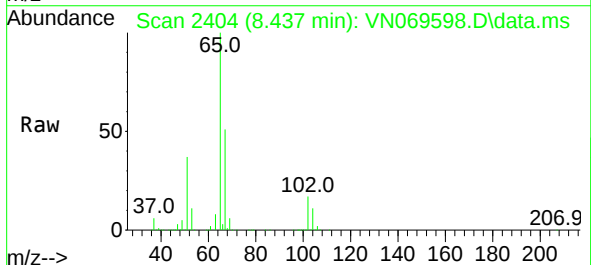






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 21
Delta R.T. 0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Instrument :
MSVOA_N
ClientSampleId :



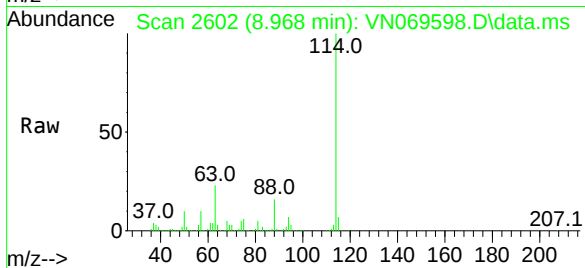



Tgt Ion:114 Resp: 2325883
Ion Ratio Lower Upper
114 100
63 23.4 0.0 37.8
88 15.6 0.0 27.4

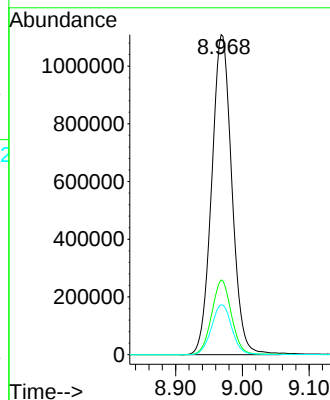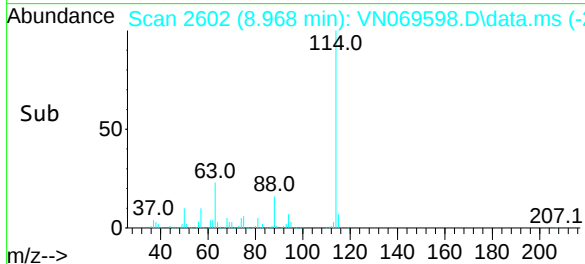

#35
Dibromofluoromethane
Concen: 48.770 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46


Tgt Ion:113 Resp: 680329
Ion Ratio Lower Upper
113 100
111 103.3 82.2 123.2
192 18.6 16.9 25.3

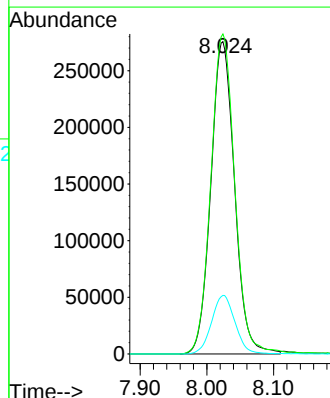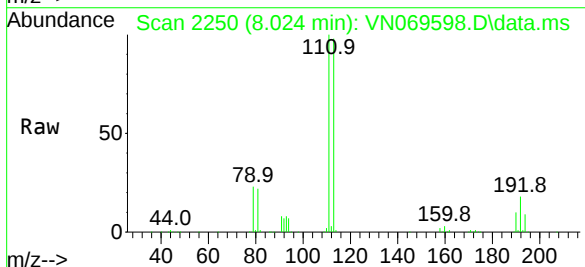






#36
1,1-Dichloropropene
Concen: 5.829 ug/l
RT: 8.088 min Scan# 21
Delta R.T. -0.135 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Instrument :
MSVOA_N
ClientSampleId :



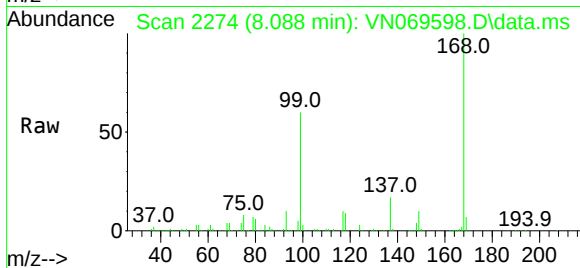



Tgt Ion: 75 Resp: 114079
Ion Ratio Lower Upper
75 100
110 9.2 18.4 55.2#
77 0.1 24.4 36.6#

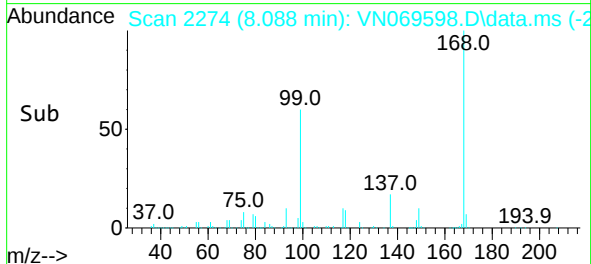

#37
Ethyl Acetate
Concen: 0.339 ug/l
RT: 7.421 min Scan# 2025
Delta R.T. 0.006 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46


Tgt Ion: 43 Resp: 8975
Ion Ratio Lower Upper
43 100
61 5.8 11.5 17.3#
70 5.0 7.9 11.9#

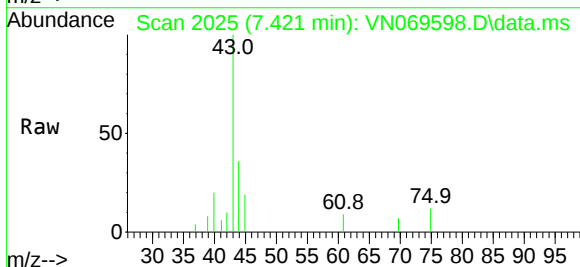






#38
Carbon Tetrachloride
Concen: 7.408 ug/l
RT: 8.086 min Scan# 21
Delta R.T. -0.120 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion:117 Resp: 139978
Ion Ratio Lower Upper
117 100
119 4.6 76.1 114.1#
121 0.0 24.2 36.2#

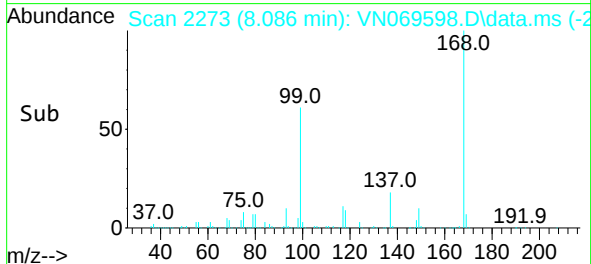

#43
Isopropyl Acetate
Concen: 0.216 ug/l
RT: 8.636 min Scan# 2478
Delta R.T. 0.072 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Tgt Ion: 43 Resp: 9184
Ion Ratio Lower Upper
43 100
61 0.0 20.4 30.6#
87 0.0 11.2 16.8#









#50
Toluene-d8
Concen: 53.842 ug/l
RT: 10.443 min Scan# 3151
Delta R.T. 0.002 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 98 Resp: 2953966
Ion Ratio Lower Upper
98 100
100 63.9 50.4 75.6

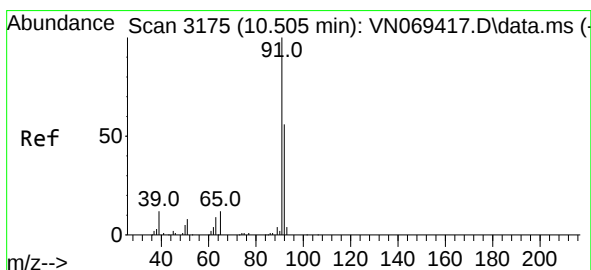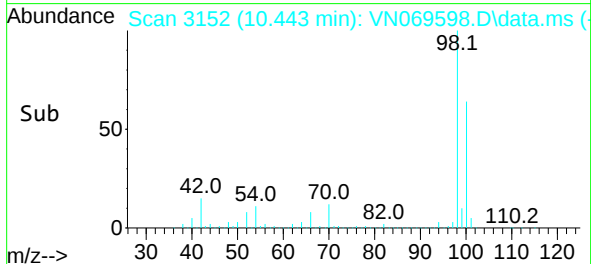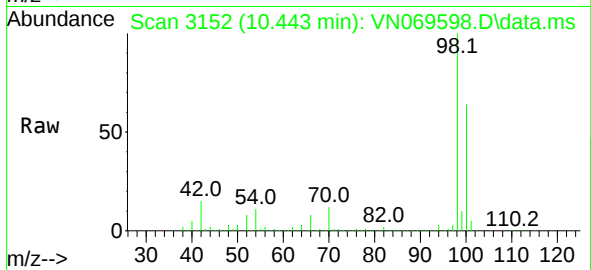

#52
Toluene
Concen: 1.611 ug/l
RT: 10.508 min Scan# 3176
Delta R.T. 0.003 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Tgt Ion: 92 Resp: 60621
Ion Ratio Lower Upper
92 100
91 170.6 142.0 213.0









#53
 t-1,3-Dichloropropene
 Concen: 2.642 ug/l
 RT: 10.722 min Scan# 3111
 Delta R.T. 0.003 min
 Lab File: VN069598.D
 Acq: 19 Nov 2021 20:46




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 110
 Ion Ratio Lower Upper
 75 100
 77 9.6 25.6 38.4#

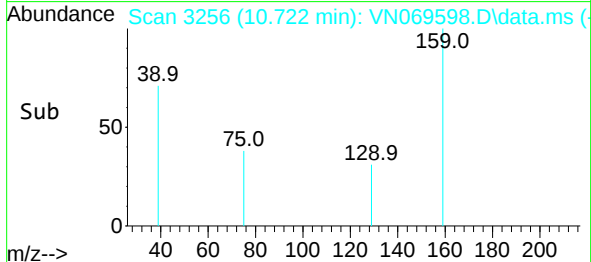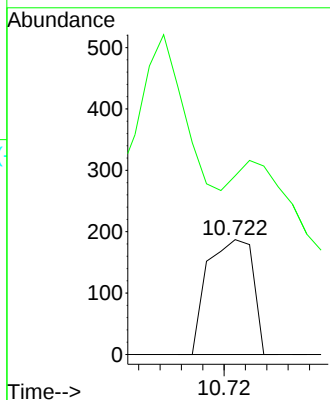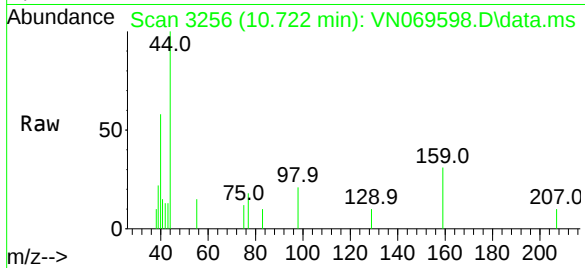

#54
 cis-1,3-Dichloropropene
 Concen: 1.735 ug/l
 RT: 10.363 min Scan# 3122
 Delta R.T. 0.175 min
 Lab File: VN069598.D
 Acq: 19 Nov 2021 20:46


Tgt Ion: 75 Resp: 58
 Ion Ratio Lower Upper
 75 100
 77 0.0 26.4 39.6#
 39 38.0 42.5 63.7#

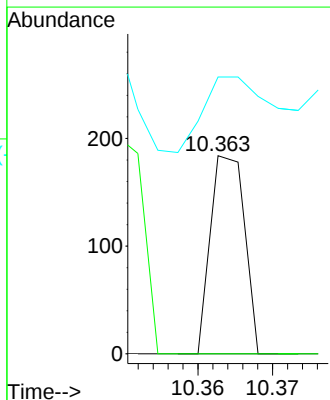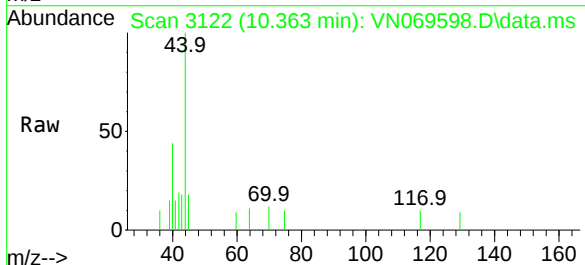



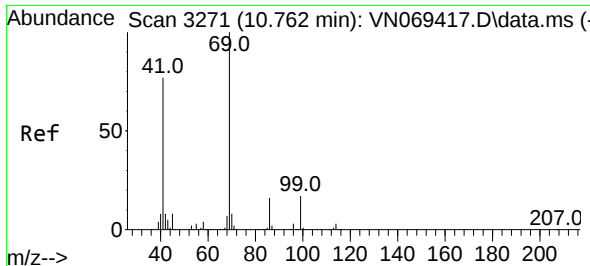


#56
Ethyl methacrylate
Concen: 2.063 ug/l
RT: 10.760 min Scan# 31
Delta R.T. -0.002 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46


Instrument :
MSVOA_N
ClientSampleId :

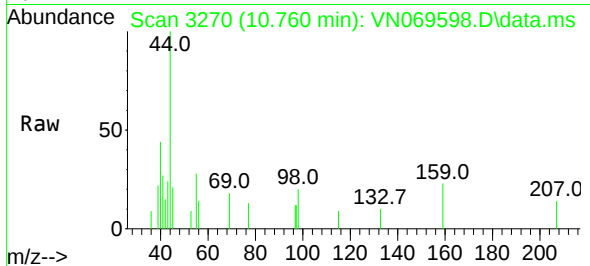



Tgt Ion: 69 Resp: 297
Ion Ratio Lower Upper
69 100
41 0.0 51.4 77.0#
39 0.0 34.6 52.0#

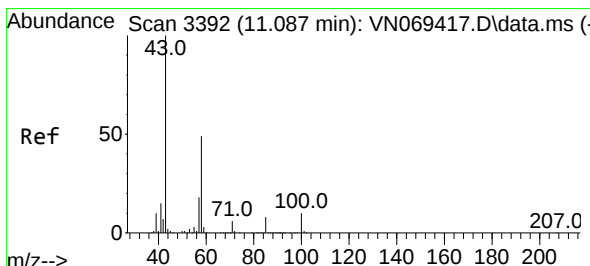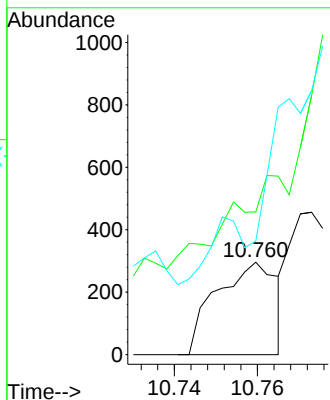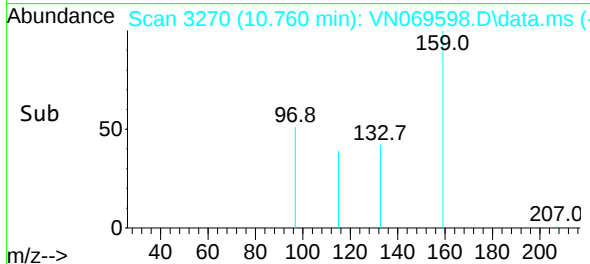


#59
2-Hexanone
Concen: 8.033 ug/l
RT: 11.092 min Scan# 3394
Delta R.T. 0.005 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

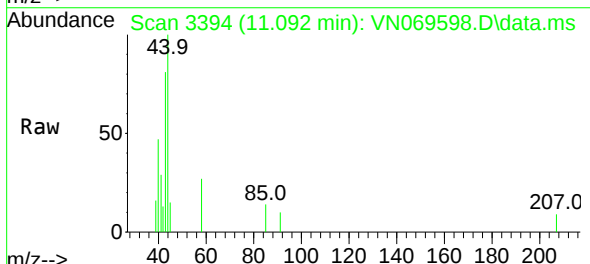

Tgt Ion: 43 Resp: 2182
Ion Ratio Lower Upper
43 100
58 37.4 26.9 80.7



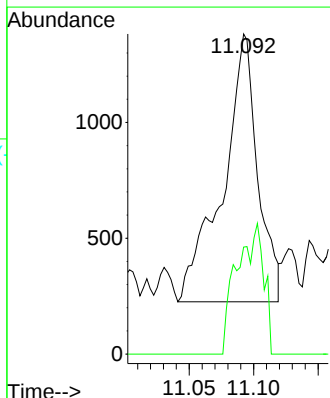
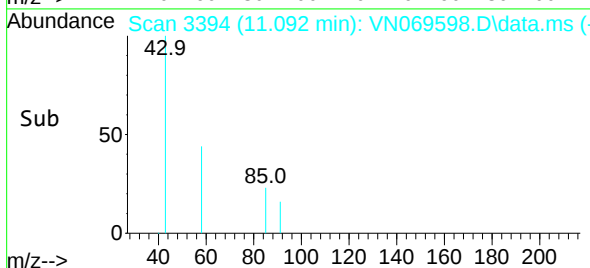




#60
Dibromochloromethane
Concen: 2.420 ug/l
RT: 11.218 min Scan# 3441
Delta R.T. -0.022 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:129 Resp: 54
Ion Ratio Lower Upper
129 100
127 0.0 38.6 116.0#

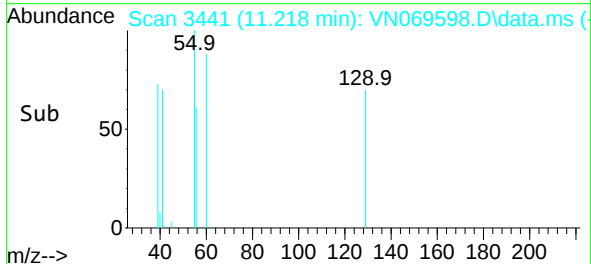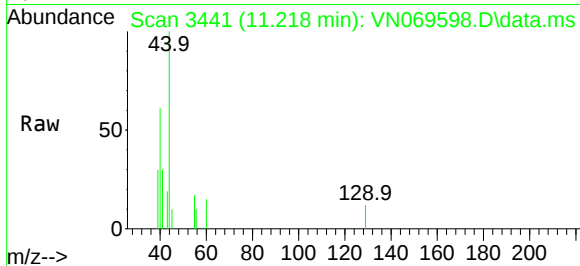

#62
4-Bromofluorobenzene
Concen: 55.048 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Tgt Ion: 95 Resp: 1109478
Ion Ratio Lower Upper
95 100
174 75.5 0.0 187.2
176 72.7 0.0 181.4









#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 2342810
Ion Ratio Lower Upper
117 100
82 58.1 42.4 63.6
119 31.8 25.4 38.2

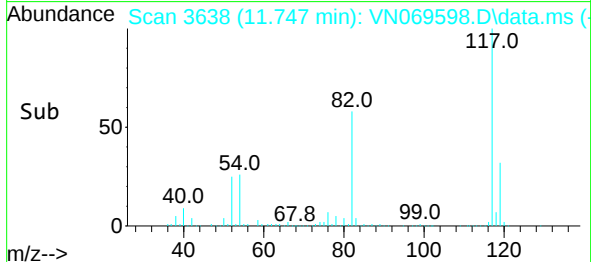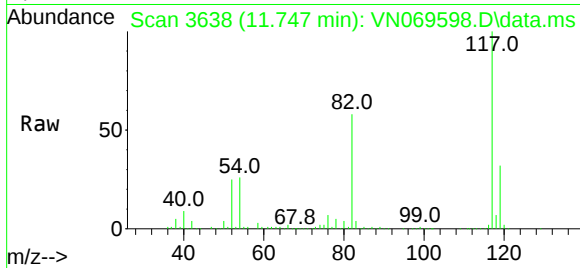

#67
Ethyl Benzene
Concen: 0.663 ug/l
RT: 11.846 min Scan# 3675
Delta R.T. -0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Tgt Ion: 91 Resp: 53300
Ion Ratio Lower Upper
91 100
106 26.4 25.7 38.5




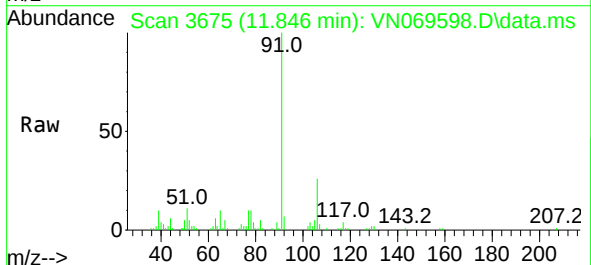




#68
m/p-Xylenes
Concen: 3.082 ug/l
RT: 11.950 min Scan# 3715
Delta R.T. -0.003 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:106 Resp: 91175
Ion Ratio Lower Upper
106 100
91 217.5 160.6 240.8

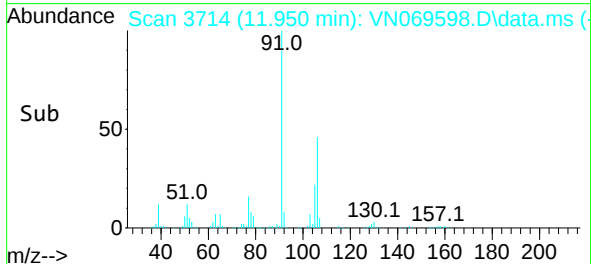

#69
o-Xylene
Concen: 1.428 ug/l
RT: 12.280 min Scan# 3837
Delta R.T. 0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Tgt Ion:106 Resp: 42124
Ion Ratio Lower Upper
106 100
91 226.7 105.8 317.3


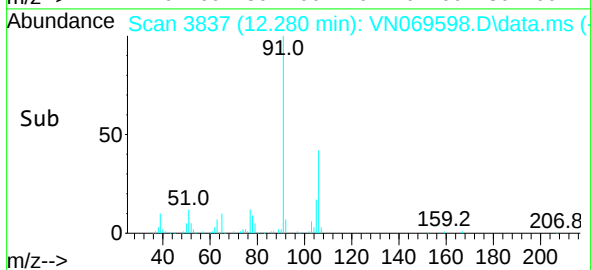






#70
Styrene
Concen: 1.576 ug/l
RT: 12.280 min Scan# 3842
Delta R.T. -0.014 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:104 Resp: 3057
Ion Ratio Lower Upper
104 100
78 254.4 38.7 58.1#
103 217.6 45.0 67.6#

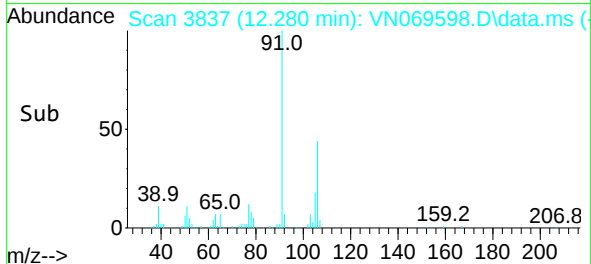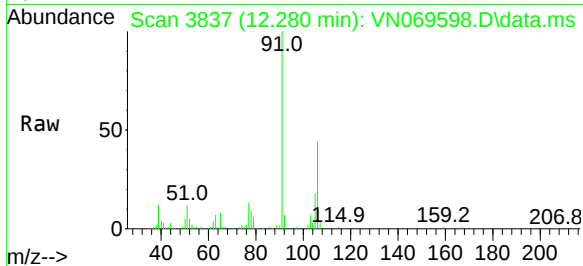

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.675 min Scan# 4357
Delta R.T. -0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Tgt Ion:152 Resp: 929008
Ion Ratio Lower Upper
152 100
115 61.1 27.5 82.5
150 156.0 0.0 344.4


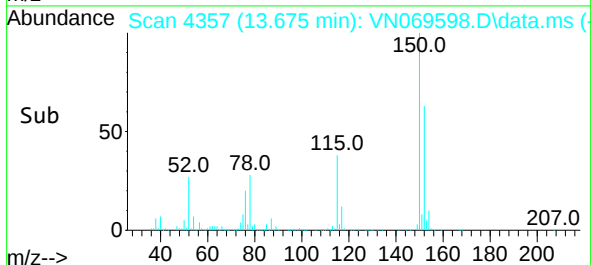

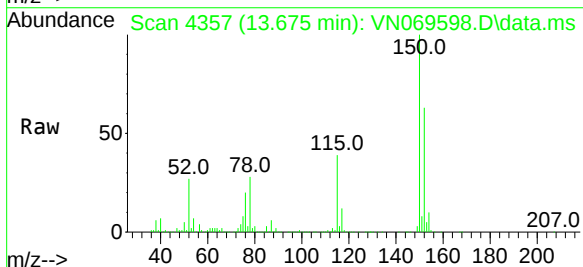


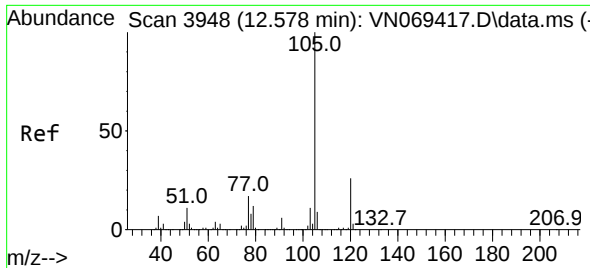

#73
Isopropylbenzene
Concen: 0.778 ug/l
RT: 12.581 min Scan# 3949
Delta R.T. 0.003 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:105 Resp: 57550
Ion Ratio Lower Upper
105 100
120 23.6 13.4 40.1

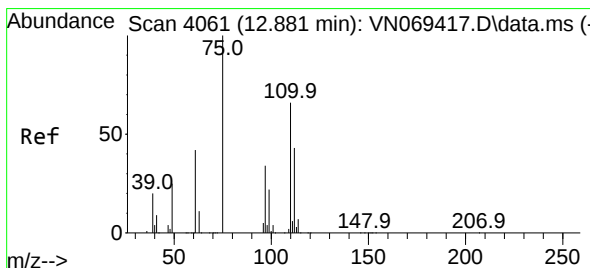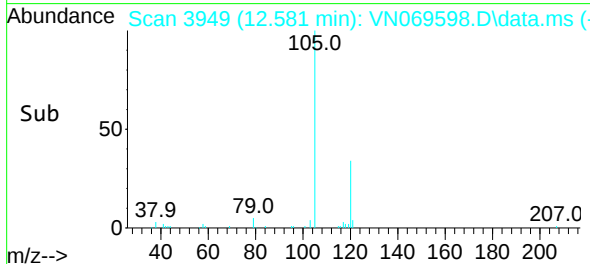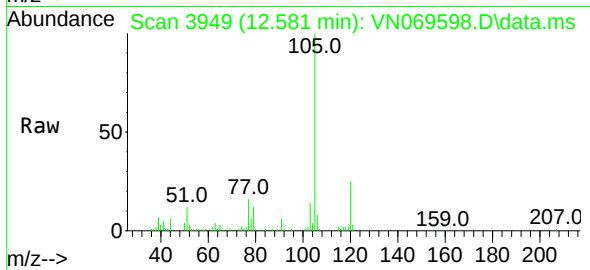

#76
1,2,3-Trichloropropane
Concen: 28.962 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. -0.150 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46


Tgt Ion: 75 Resp: 620921
Ion Ratio Lower Upper
75 100
77 1.1 82.6 247.8#

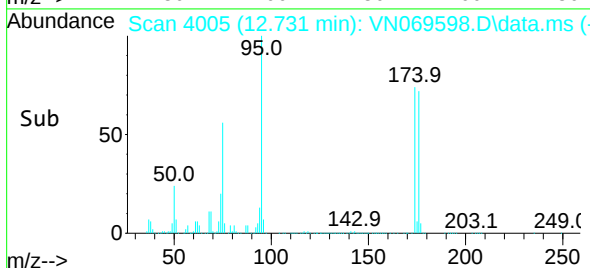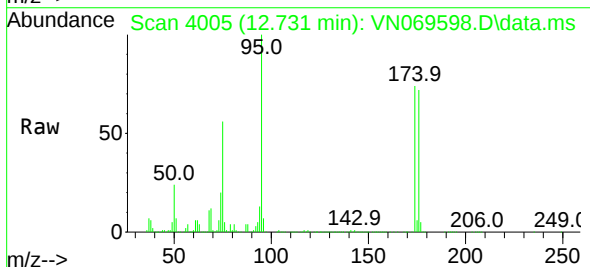






#78
n-propylbenzene
Concen: 0.837 ug/l
RT: 12.921 min Scan# 4076
Delta R.T. 0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Instrument :
MSVOA_N
ClientSampleId :







Tgt Ion: 91 Resp: 69666
Ion Ratio Lower Upper
91 100
120 21.3 11.9 35.9

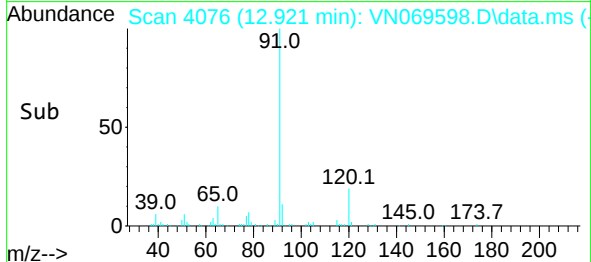

#80
1,3,5-Trimethylbenzene
Concen: 0.249 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. -0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Tgt Ion: 105 Resp: 14917
Ion Ratio Lower Upper
105 100
120 44.1 24.6 73.6




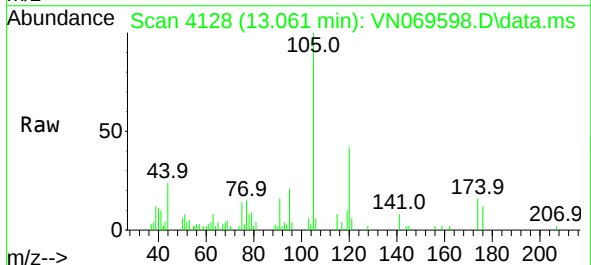




#81
trans-1,4-Dichloro-2-butene
Concen: 82.018 ug/l
RT: 12.731 min Scan# 4005
Delta R.T. 0.105 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 620921
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#



#84
1,2,4-Trimethylbenzene
Concen: 0.915 ug/l
RT: 13.369 min Scan# 4243
Delta R.T. 0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

Tgt Ion:105 Resp: 52826
Ion Ratio Lower Upper
105 100
120 41.6 22.8 68.4


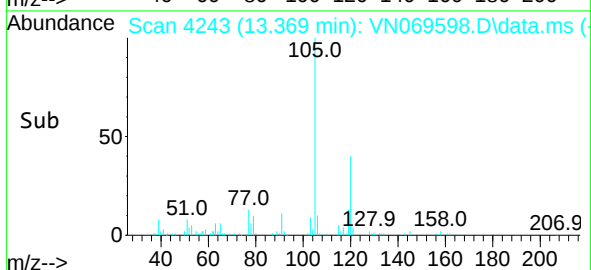

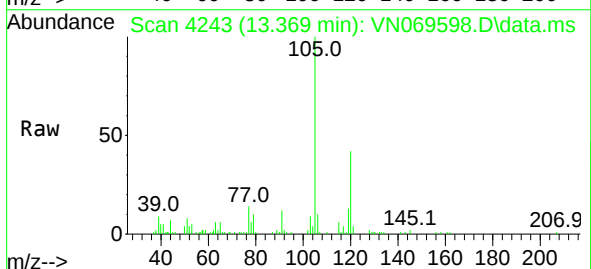


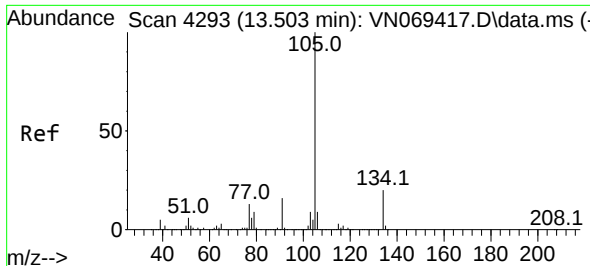

#85
 sec-Butylbenzene
 Concen: 0.593 ug/l
 RT: 13.503 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: VN069598.D
 Acq: 19 Nov 2021 20:46




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:105 Resp: 43404
 Ion Ratio Lower Upper
 105 100
 134 23.9 10.4 31.1

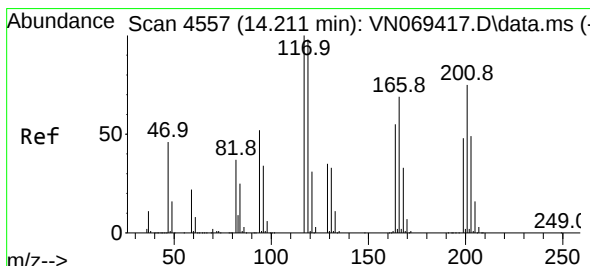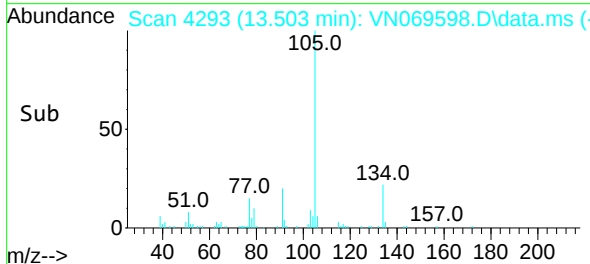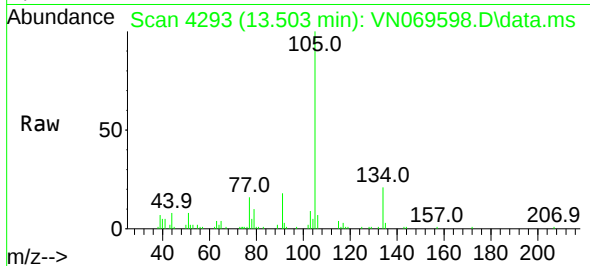

#90
 Hexachloroethane
 Concen: 2.959 ug/l
 RT: 14.217 min Scan# 4559
 Delta R.T. 0.006 min
 Lab File: VN069598.D
 Acq: 19 Nov 2021 20:46

Tgt Ion:117 Resp: 8897
 Ion Ratio Lower Upper
 117 100
 201 0.0 43.9 131.6#


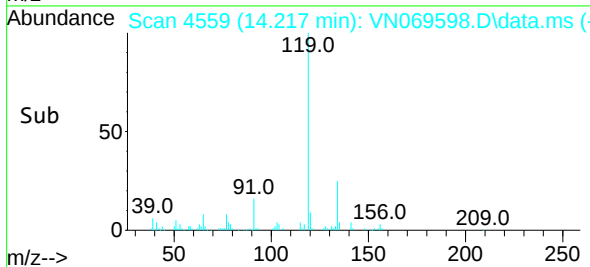

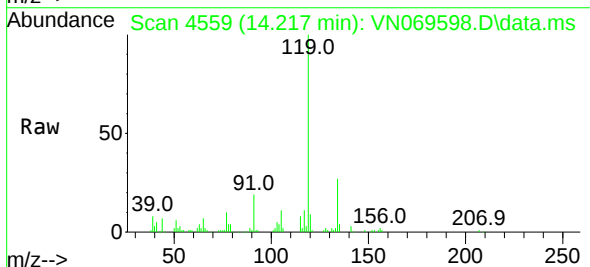


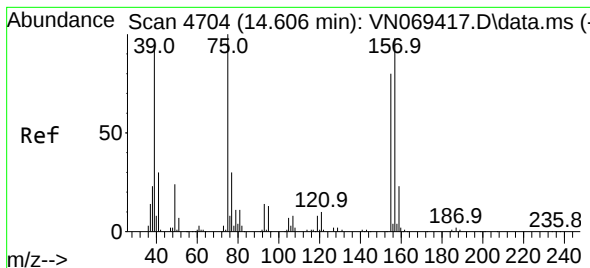

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 1.820 ug/l
 RT: 14.640 min Scan# 41
 Delta R.T. 0.034 min
 Lab File: VN069598.D
 Acq: 19 Nov 2021 20:46




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 109
 Ion Ratio Lower Upper
 75 100
 155 49.5 46.9 140.7
 157 143.1 60.6 181.7

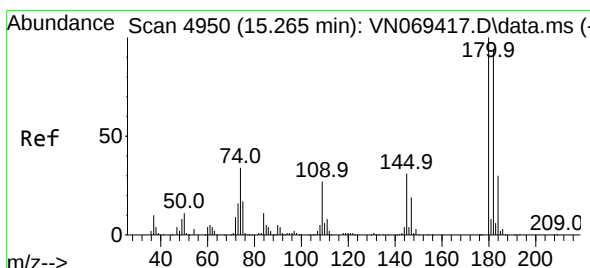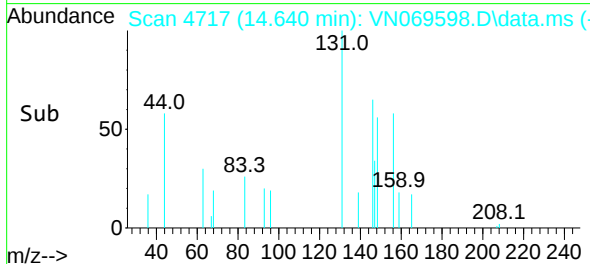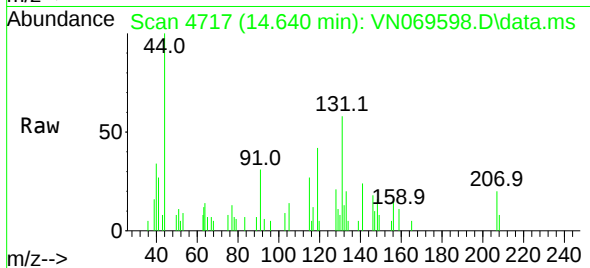

#93
 1,2,4-Trichlorobenzene
 Concen: 3.149 ug/l
 RT: 15.271 min Scan# 4952
 Delta R.T. 0.006 min
 Lab File: VN069598.D
 Acq: 19 Nov 2021 20:46


Tgt Ion: 180 Resp: 552
 Ion Ratio Lower Upper
 180 100
 182 106.5 48.3 144.9
 145 1829.3 14.5 43.5#

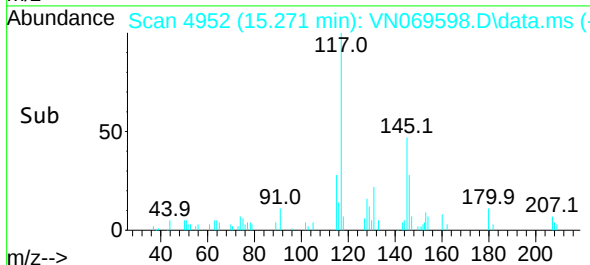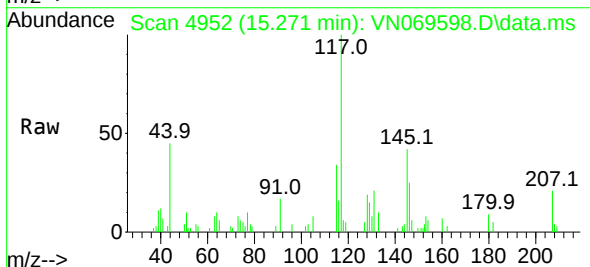






#95
Naphthalene
Concen: 4.877 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46


Instrument :
MSVOA_N
ClientSampleId :



Tgt Ion:128 Resp: 19279
Ion Ratio Lower Upper
128 100
127 9.8 10.5 15.7#
129 12.8 8.7 13.1

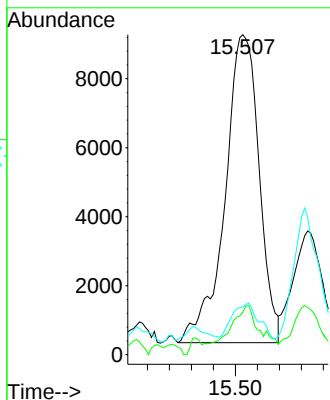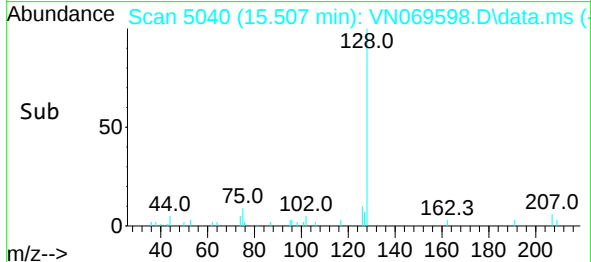

#96
1,2,3-Trichlorobenzene
Concen: 3.222 ug/l
RT: 15.700 min Scan# 5112
Delta R.T. -0.000 min
Lab File: VN069598.D
Acq: 19 Nov 2021 20:46

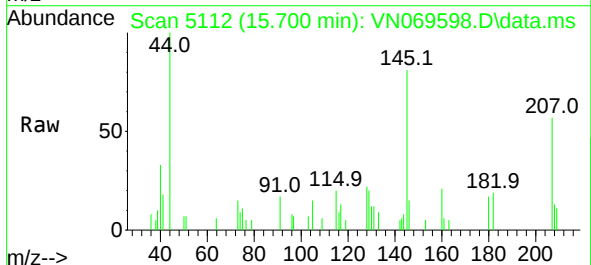

Tgt Ion:180 Resp: 782
Ion Ratio Lower Upper
180 100
182 134.7 47.4 142.2
145 0.0 15.0 45.1#

