
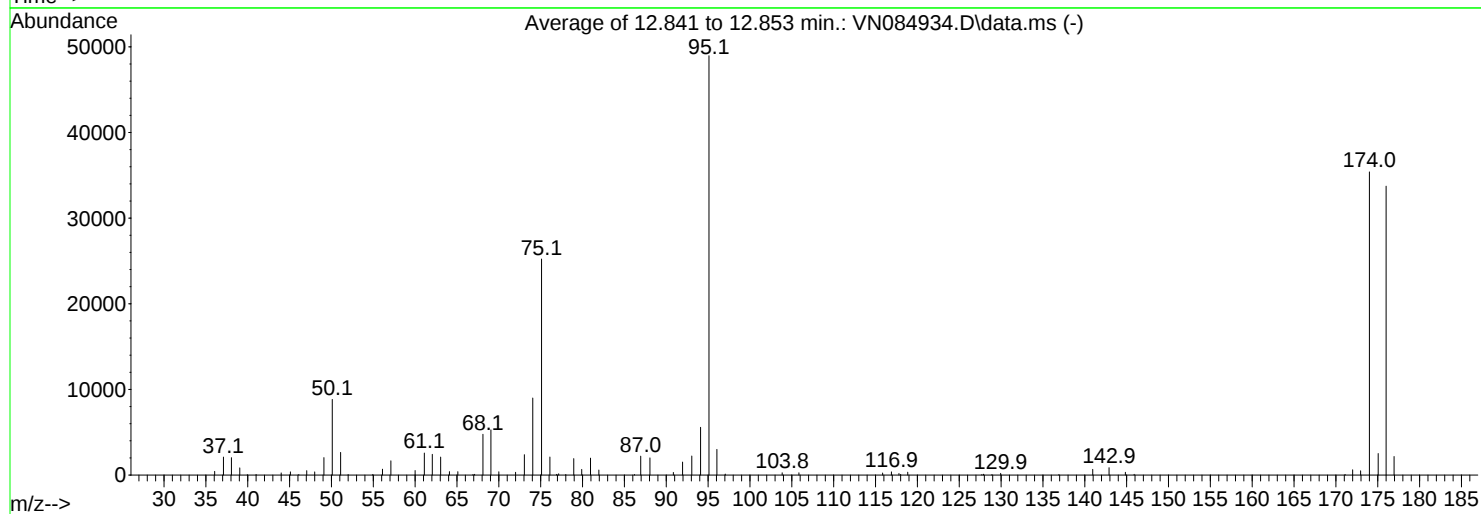


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN111924\
Data File : VN084934.D
Acq On : 19 Nov 2024 08:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N103024W.M
Title : SW846 8260
Last Update : Thu Oct 31 18:45:38 2024

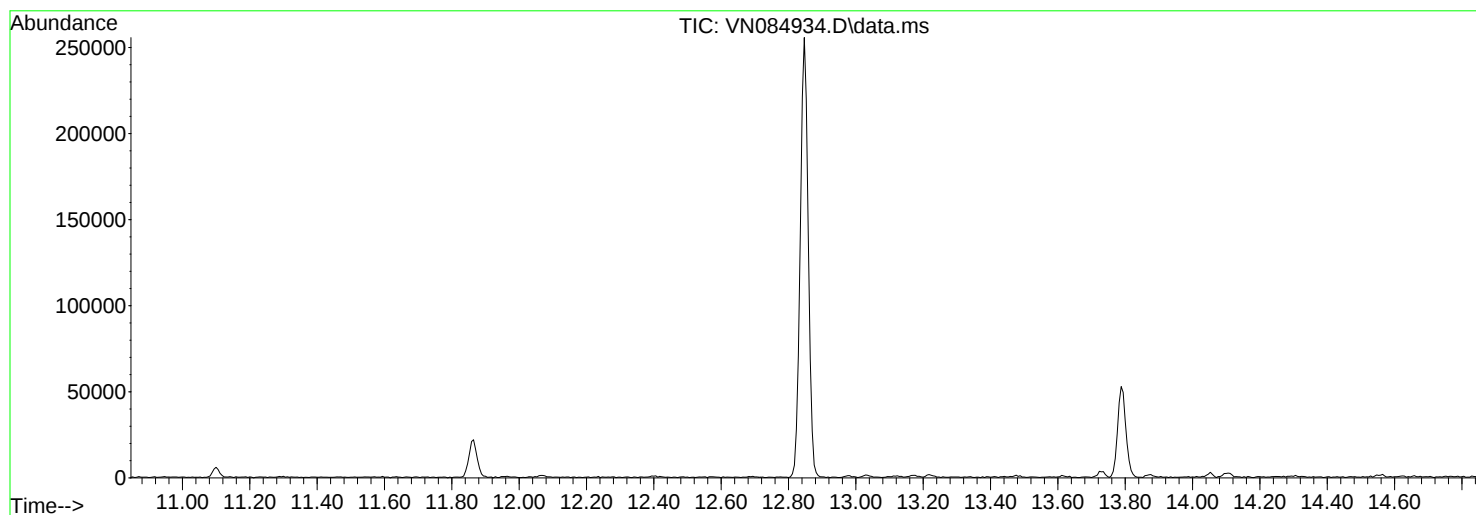

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	8832	PASS
75	95	30	60	51.5	25227	PASS
95	95	100	100	100.0	48965	PASS
96	95	5	9	6.1	2998	PASS
173	174	0.00	2	1.4	500	PASS
174	95	50	100	72.3	35400	PASS
175	174	5	9	7.1	2519	PASS
176	174	95	101	95.3	33736	PASS
177	176	5	9	6.4	2170	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	433	49.10	2042	64.10	404	76.10	2109
37.10	2102	50.10	8832	65.10	401	76.90	86
38.05	2032	51.10	2644	66.90	58	77.15	152
39.05	843	52.00	53	67.10	89	78.00	60
39.95	31	54.90	50	68.10	4763	78.95	1920
41.00	60	56.10	689	69.05	5279	79.90	665
44.00	250	57.10	1665	70.00	387	80.95	1977
45.10	378	60.00	535	72.00	329	81.95	588
46.10	63	61.10	2574	73.05	2385	86.20	67
47.05	518	62.05	2424	74.05	8997	86.95	2210
48.00	370	63.05	2101	75.10	25227	88.05	2008

Average of 12.841 to 12.853 min.: VN084934.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.85	306	117.80	185	145.90	93		
91.95	1519	118.00	73	171.10	72		
93.05	2226	118.85	339	172.00	619		
94.10	5576	127.70	61	172.95	500		
95.10	48965	127.90	102	174.00	35400		
96.05	2998	128.90	50	175.05	2519		
97.05	117	129.95	201	176.00	33736		
103.85	273	136.90	51	176.95	2170		
105.85	269	140.95	668				
115.85	241	142.90	866				
116.90	378	144.85	329				

Instrument :

MSVOA_N

ClientSampleId :

BFB