


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN112018\
 Data File : VN052398.D
 Acq On : 20 Nov 2018 10:48
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 28

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N111418W.M
 Title : SW846 8260
 Last Update : Thu Nov 15 03:02:37 2018

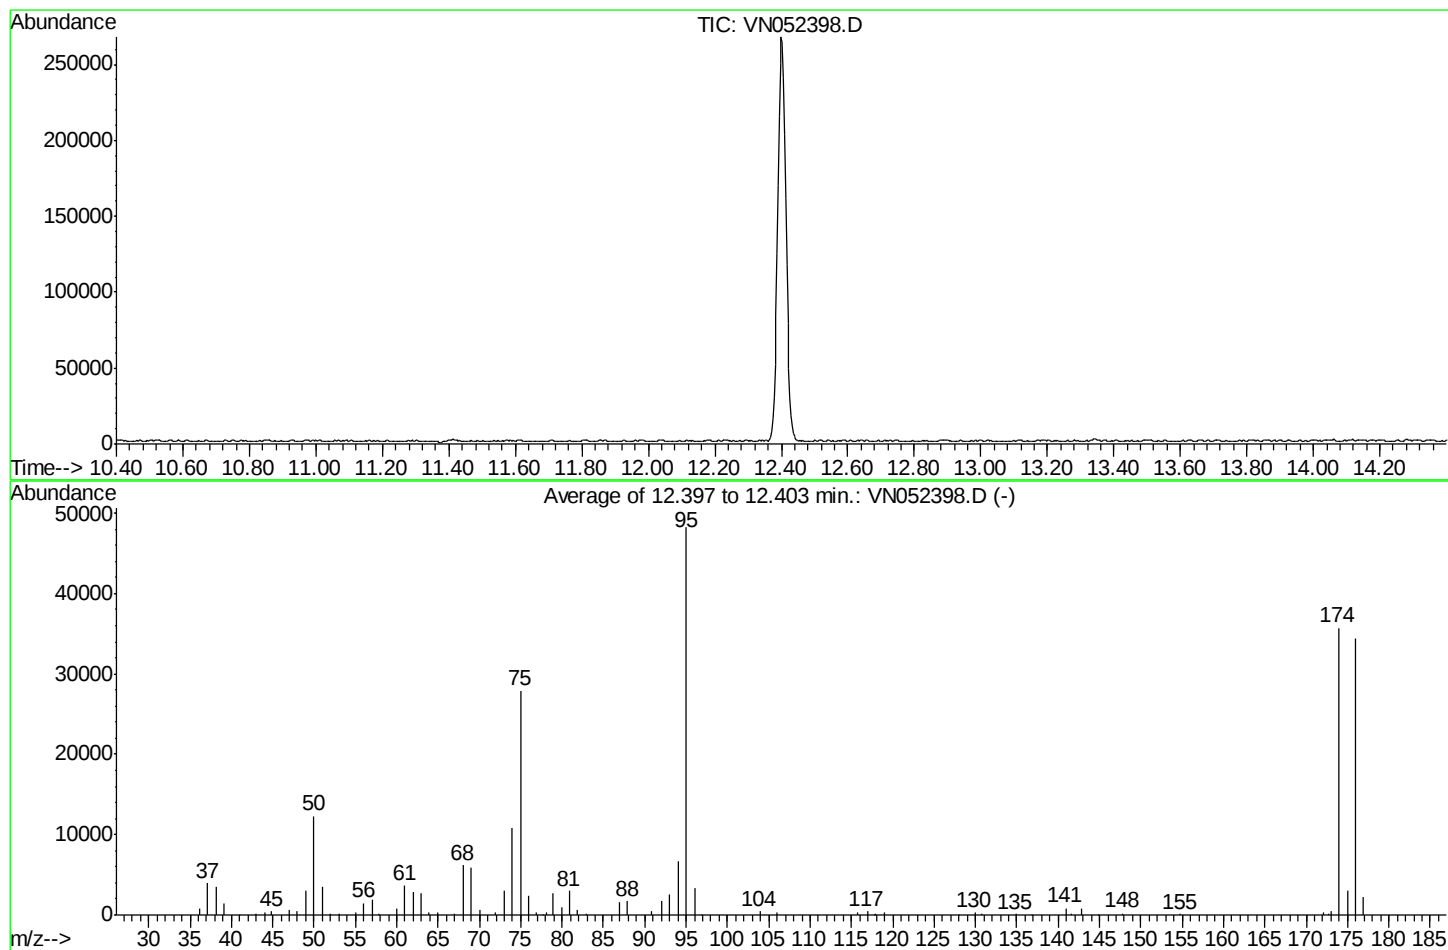

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.5	12321	PASS
75	95	30	60	57.8	27904	PASS
95	95	100	100	100.0	48242	PASS
96	95	5	9	7.1	3424	PASS
173	174	0.00	2	1.2	446	PASS
174	95	50	100	74.1	35736	PASS
175	174	5	9	8.4	3004	PASS
176	174	95	101	96.5	34490	PASS
177	176	5	9	6.6	2273	PASS