


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112019\
Data File : VN059316.D
Acq On : 20 Nov 2019 9:21
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N112019W.M
Title : SW846 8260
Last Update : Thu Nov 07 04:00:41 2019

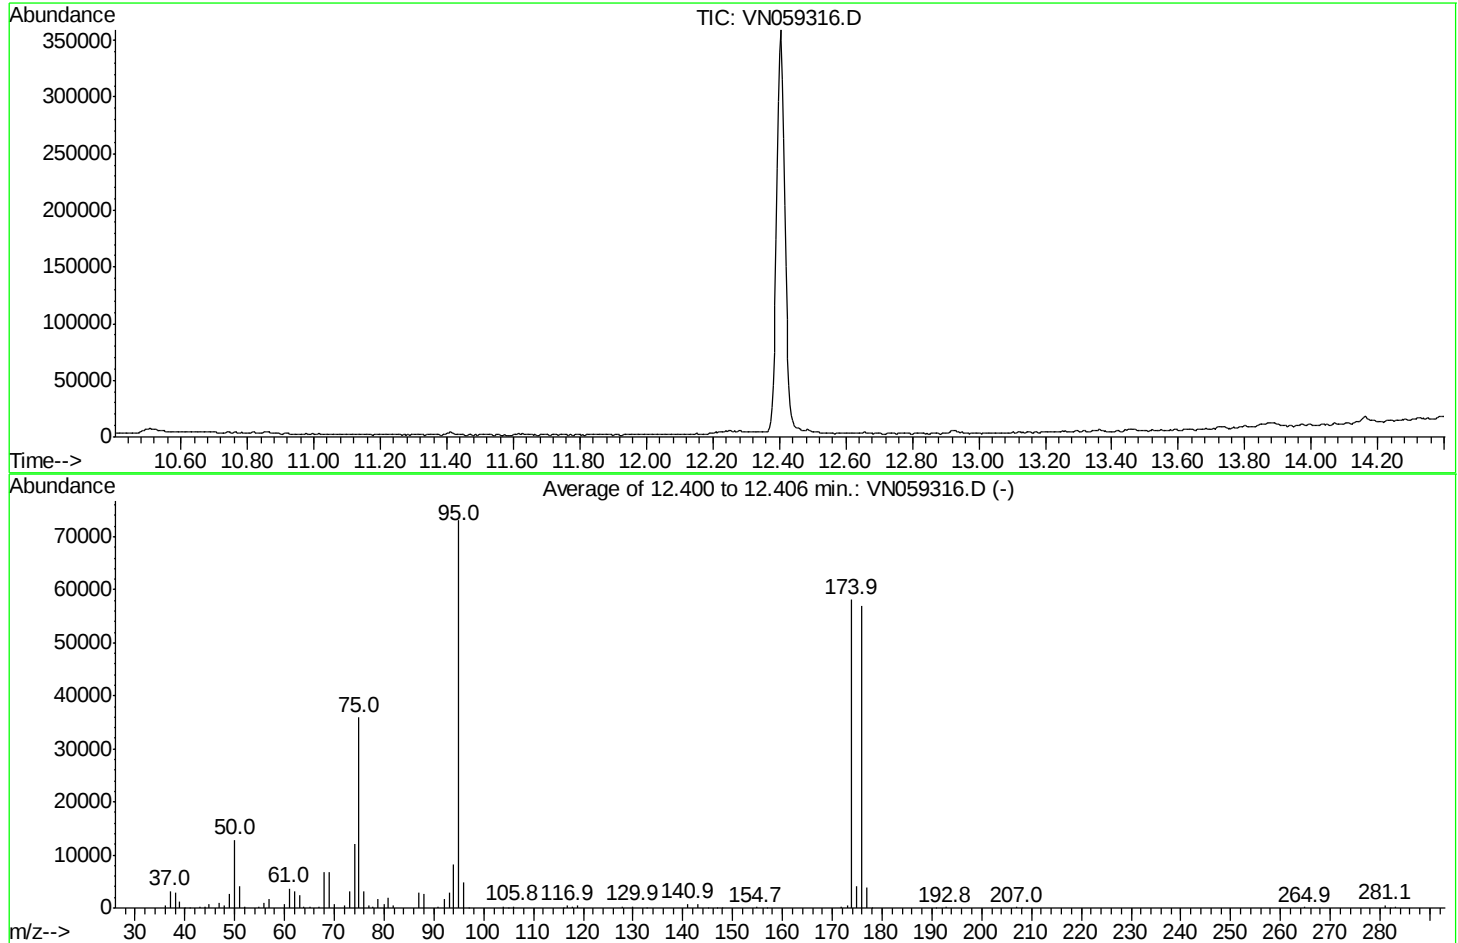

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	12796	PASS
75	95	30	60	49.2	35941	PASS
95	95	100	100	100.0	73114	PASS
96	95	5	9	6.8	4944	PASS
173	174	0.00	2	1.0	571	PASS
174	95	50	100	79.5	58093	PASS
175	174	5	9	7.2	4171	PASS
176	174	95	101	97.9	56872	PASS
177	176	5	9	6.7	3831	PASS