
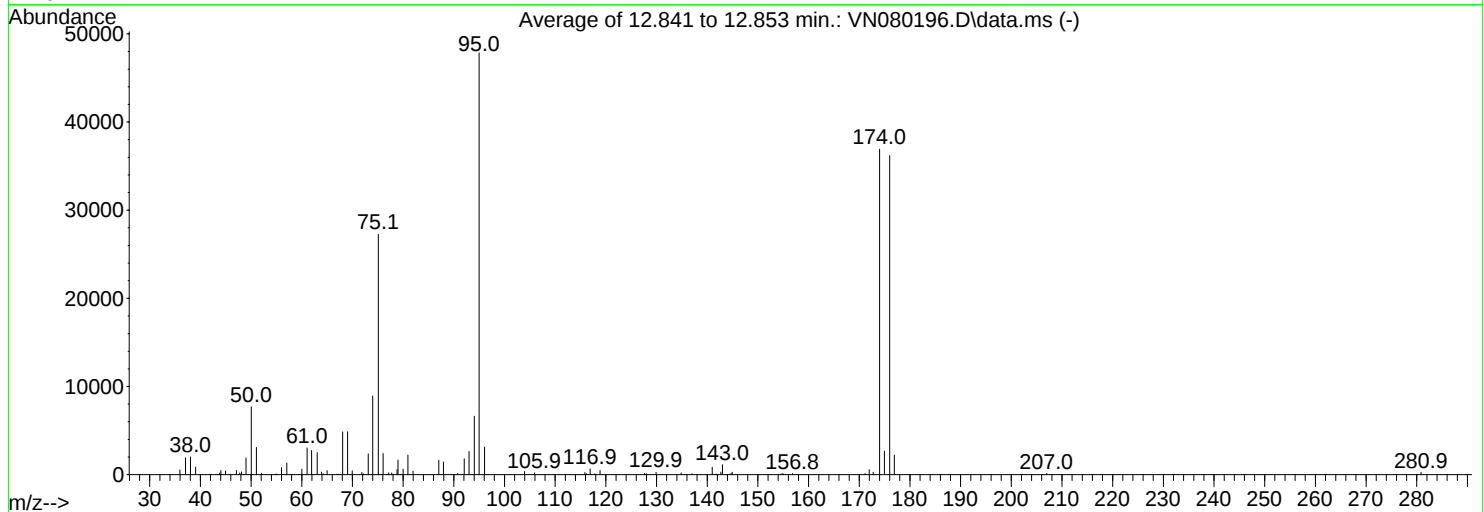


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN112023\
Data File : VN080196.D
Acq On : 20 Nov 2023 09:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N111623W.M
Title : SW846 8260
Last Update : Fri Nov 17 01:19:32 2023

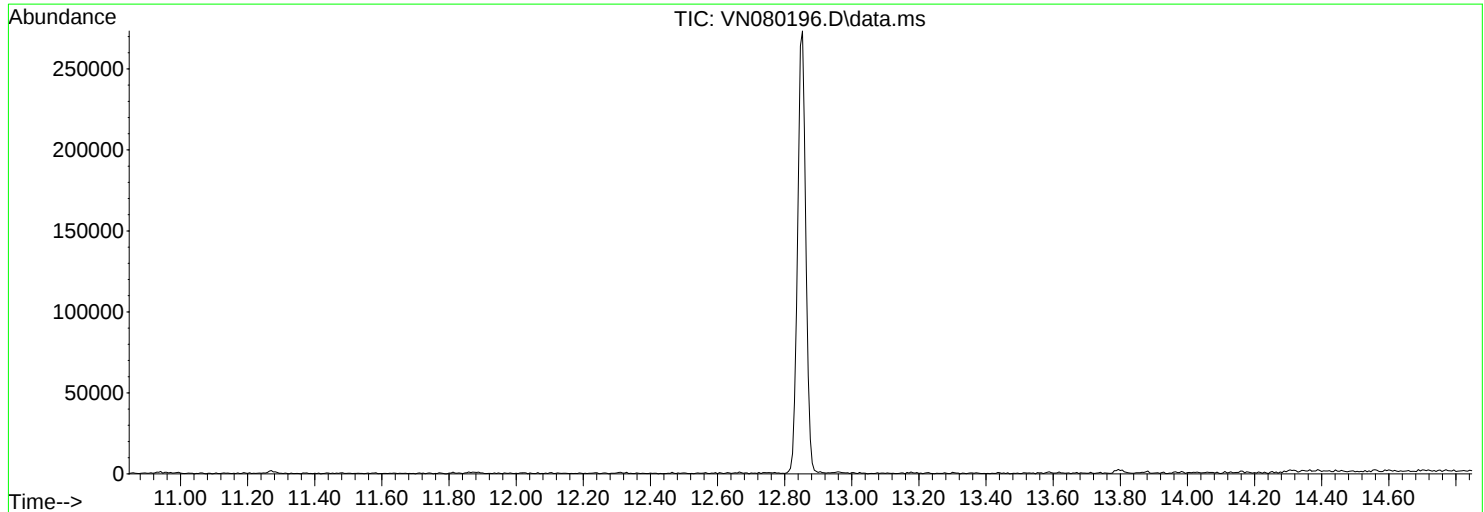

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	7700	PASS
75	95	30	60	57.0	27264	PASS
95	95	100	100	100.0	47848	PASS
96	95	5	9	6.5	3118	PASS
173	174	0.00	2	0.7	269	PASS
174	95	50	100	77.2	36917	PASS
175	174	5	9	7.2	2666	PASS
176	174	95	101	98.1	36200	PASS
177	176	5	9	6.1	2221	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	518	50.05	7700	63.90	296	74.00	892
37.05	1898	51.05	3082	64.20	103	75.10	2726
38.05	2006	52.10	163	65.00	449	76.05	239
39.05	860	54.90	67	66.90	60	76.80	5
43.80	191	55.10	65	67.20	64	77.15	219
44.05	471	56.00	810	68.05	4848	77.75	206
44.95	422	57.05	1326	69.05	4856	78.10	60
47.10	464	60.00	613	69.95	437	78.80	560
47.75	209	61.05	3028	71.85	253	79.00	1645
48.10	316	61.95	2750	72.20	85	80.00	614
49.00	1898	63.05	2506	73.10	2369	80.95	2219

Average of 12.841 to 12.853 min.: VN080196.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.95	397	115.85	233	141.00	837	171.95	572
87.05	1635	116.20	110	141.80	50	172.75	269
87.95	1440	116.90	658	142.70	290	174.00	36917
90.75	147	117.80	68	143.00	1130	174.95	2666
92.05	1796	118.00	80	144.70	160	176.00	36200
93.00	2629	118.85	464	144.95	278	176.90	2221
94.05	6623	127.65	148	154.50	61	207.00	144
95.00	47848	128.00	108	154.80	124	280.85	251
96.05	3118	129.90	280	155.10	75		
103.95	372	134.85	207	156.85	136		
105.90	199	137.00	114	171.15	122		

Instrument :

MSVOA_N

ClientSampleId :

BFB